

Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
 Data File : BE094036.D
 Acq On : 20 Sep 2017 17:42
 Operator : SJ/JU
 Sample : PB102444BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK44

Quant Time: Sep 21 06:27:57 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 21 06:26:27 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	1452	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	7671	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	5308	0.40	ng/ul	-0.02
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.42	240	13968	0.40	ng/ul	-0.01
20) Perylene-d12	23.76	264	1098031	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	4139	0.35	ng/ul	-0.03
14) Fluoranthene-d10	19.27	212	14337	0.00	ng/ul	-0.02
Target Compounds				Ovalue		
9) Fluorene	15.51	166	1472	0.074	ng/ul#	19
17) Pyrene	19.64	202	1954	0.050	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
Data File : BE094036.D
Acq On : 20 Sep 2017 17:42
Operator : SJ/JU
Sample : PB102444BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK44

Quant Time: Sep 21 06:27:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 06:26:27 2017
Response via : Initial Calibration

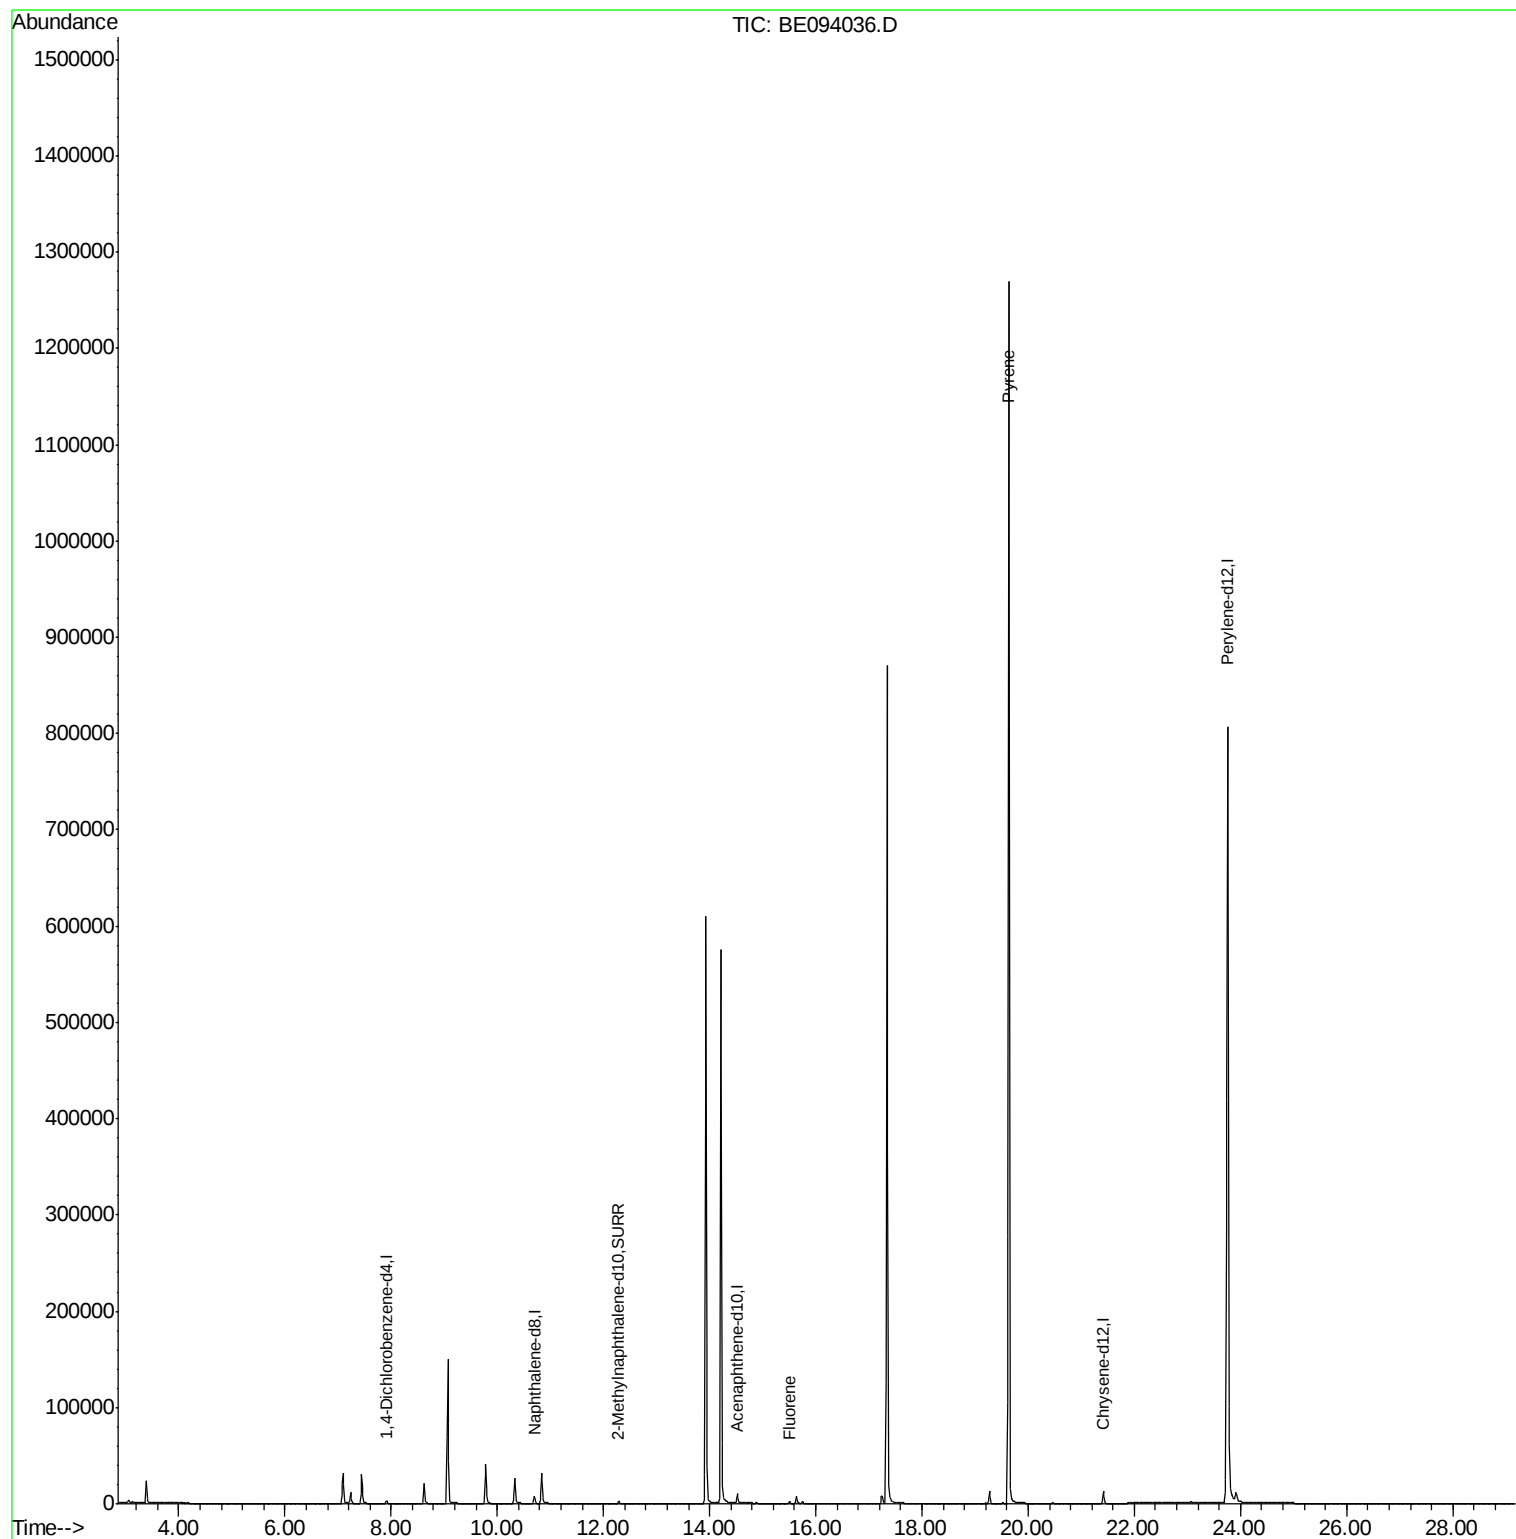

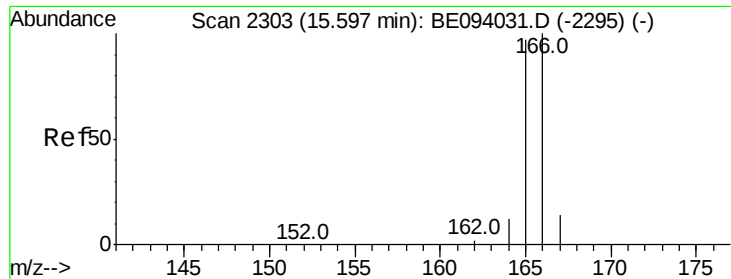

#9

Fluorene

Concen: 0.074 ng/ul

RT: 15.51 min Scan# 2293

Delta R.T. -0.08 min

Lab File: BE094036.D

Acq: 20 Sep 2017 17:42

Instrument :

BNA_E

ClientSampleId :

SBLK44





Tot Ion:166 Resp: 1472

Ion Ratio Lower Upper

166 100

165 8.7 73.4 110.2#

167 40.0 14.6 22.0#

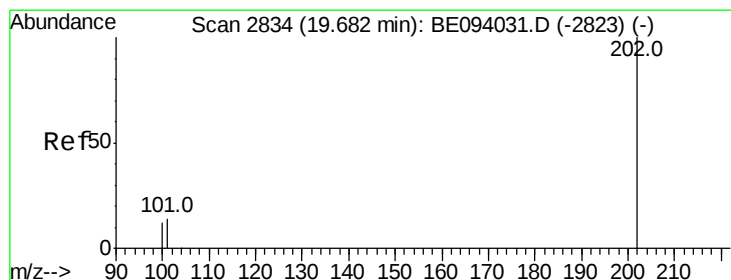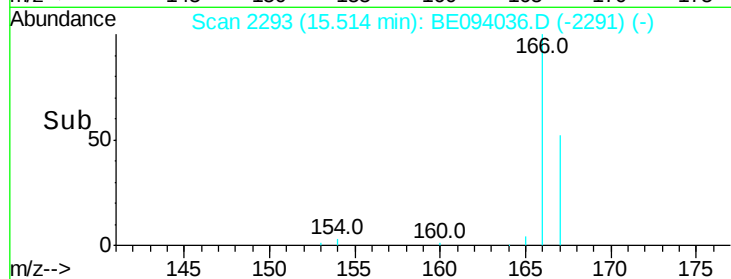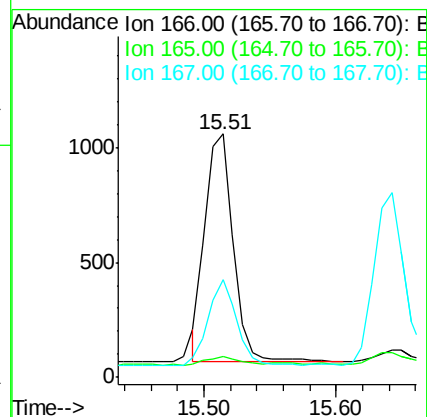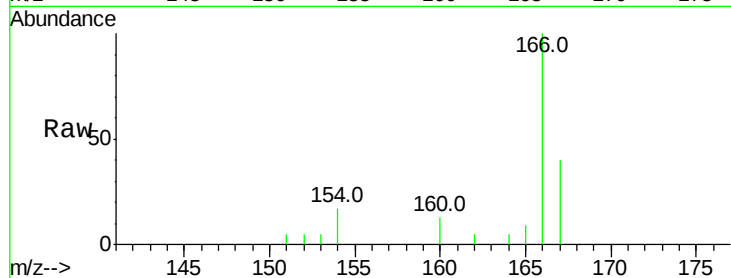

#17

Pyrene

Concen: 0.050 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.05 min

Lab File: BE094036.D

Acq: 20 Sep 2017 17:42

Tgt Ion:202 Resp: 1954

Ion Ratio Lower Upper

202 100

101 182.2 18.2 27.4#

100 1004.3 15.6 23.4#

