

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
Data File : BE094032.D
Acq On : 20 Sep 2017 14:37
Operator : SJ/JU
Sample : PB102446BL
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
SBLK46

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:27 PM

9/22/2017 3:55:27 PM

Quant Time: Sep 20 17:00:34 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 13:07:25 2017
Response via : Initial Calibration

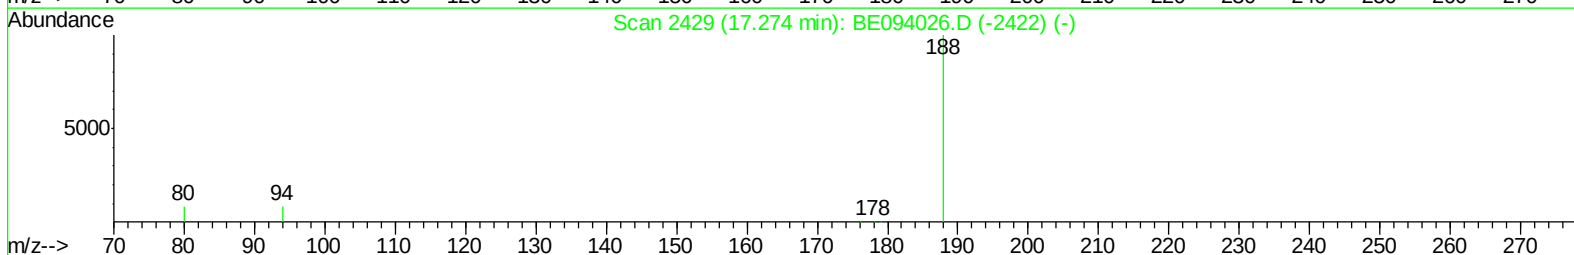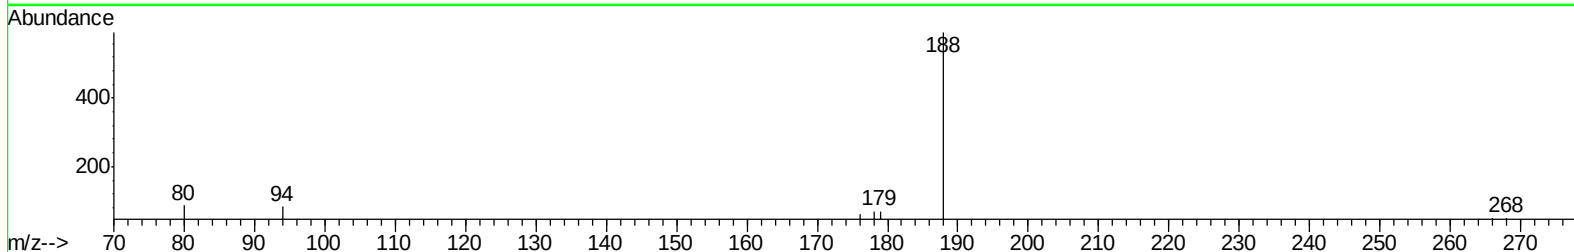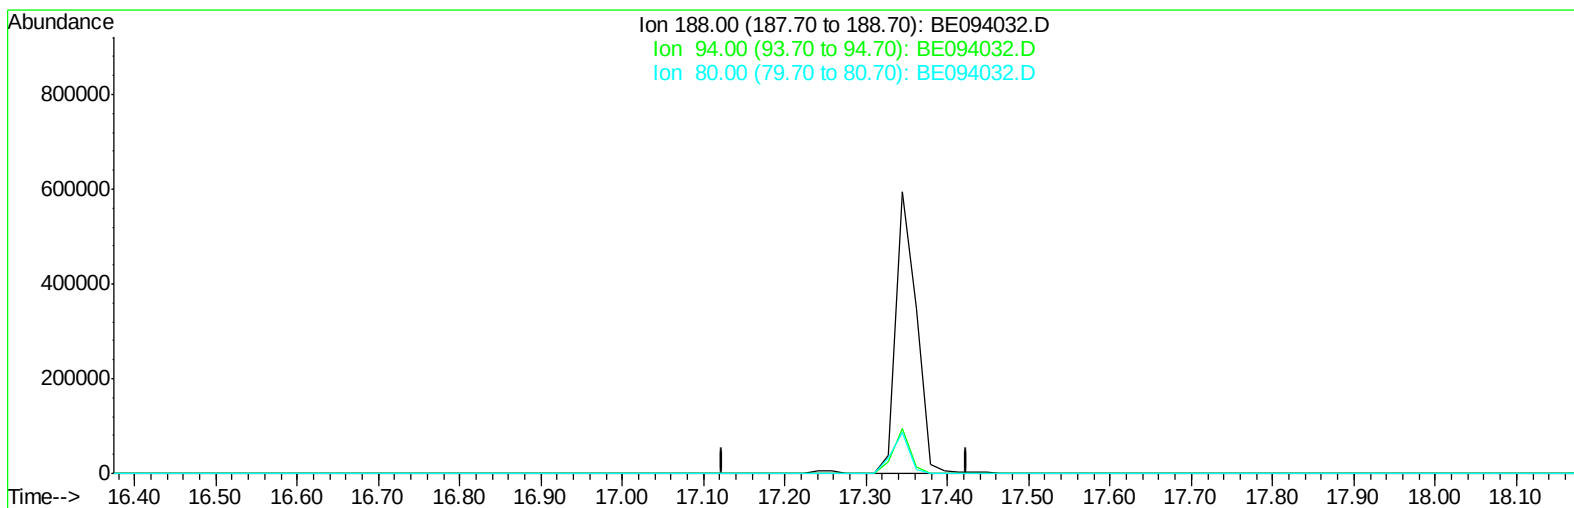

TIC: BE094032.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
Data File : BE094032.D
Acq On : 20 Sep 2017 14:37
Operator : SJ/JU
Sample : PB102446BL
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
SBLK46

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:27 PM

9/22/2017 3:55:27 PM

Quant Time: Sep 20 17:00:34 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 13:07:25 2017
Response via : Initial Calibration

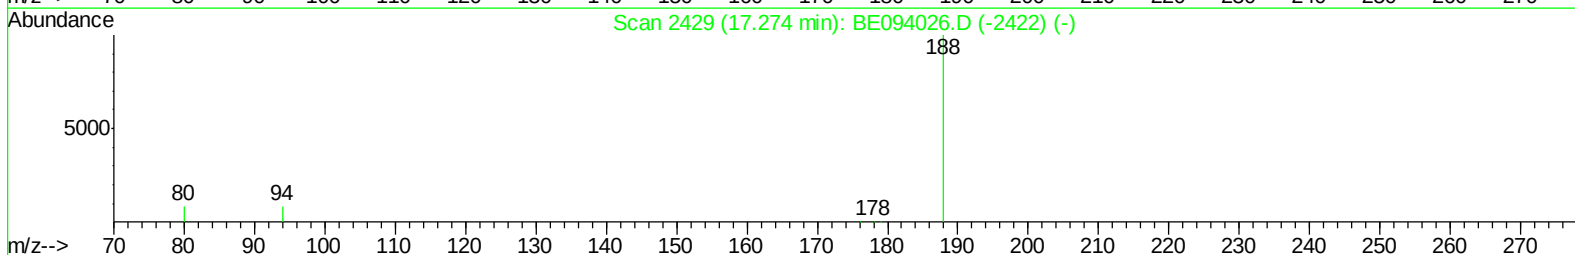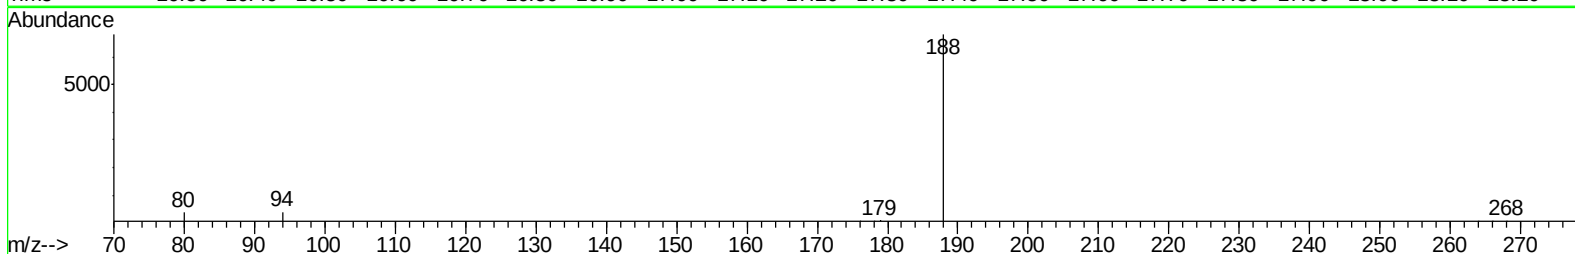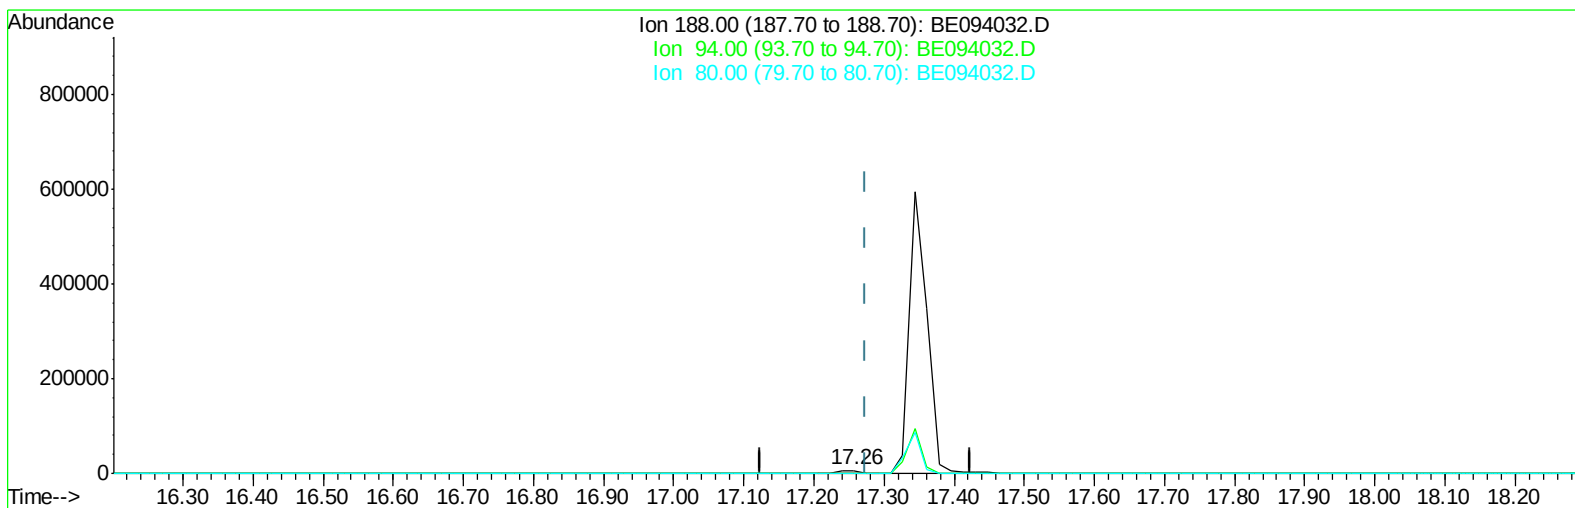

TIC: BE094032.D

(10) Phenanthrene-d10 (I)

17.257min (-0.017) 0.40ng/ul m

response 12688

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.65#
80.00	11.80	5.17#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
Data File : BE094032.D
Acq On : 20 Sep 2017 14:37
Operator : SJ/JU
Sample : PB102446BL
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
SBLK46

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:27 PM

9/22/2017 3:55:27 PM

Quant Time: Sep 20 17:01:44 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 13:07:25 2017
Response via : Initial Calibration

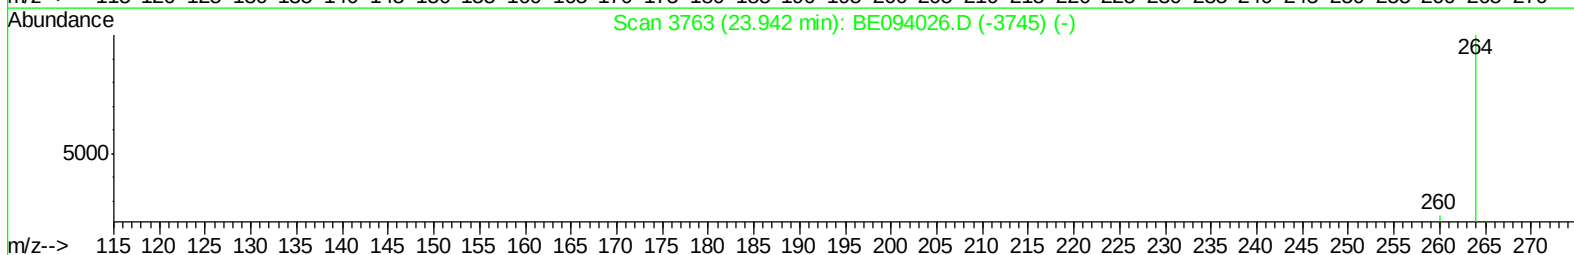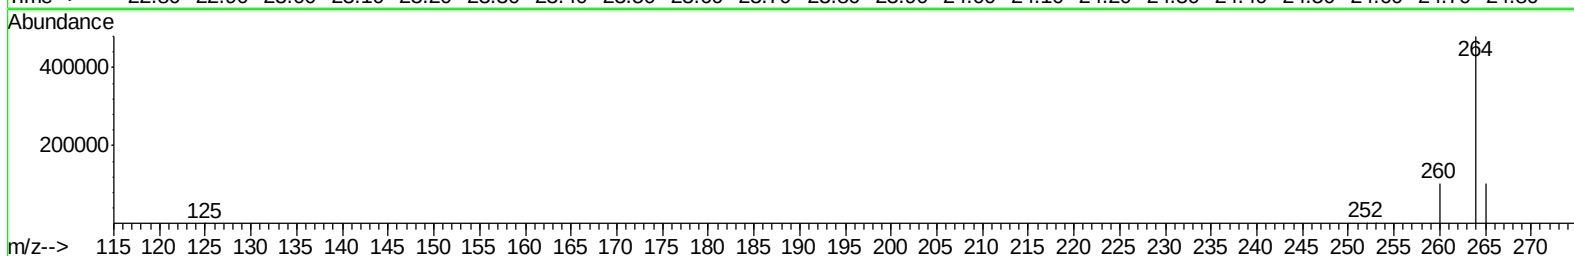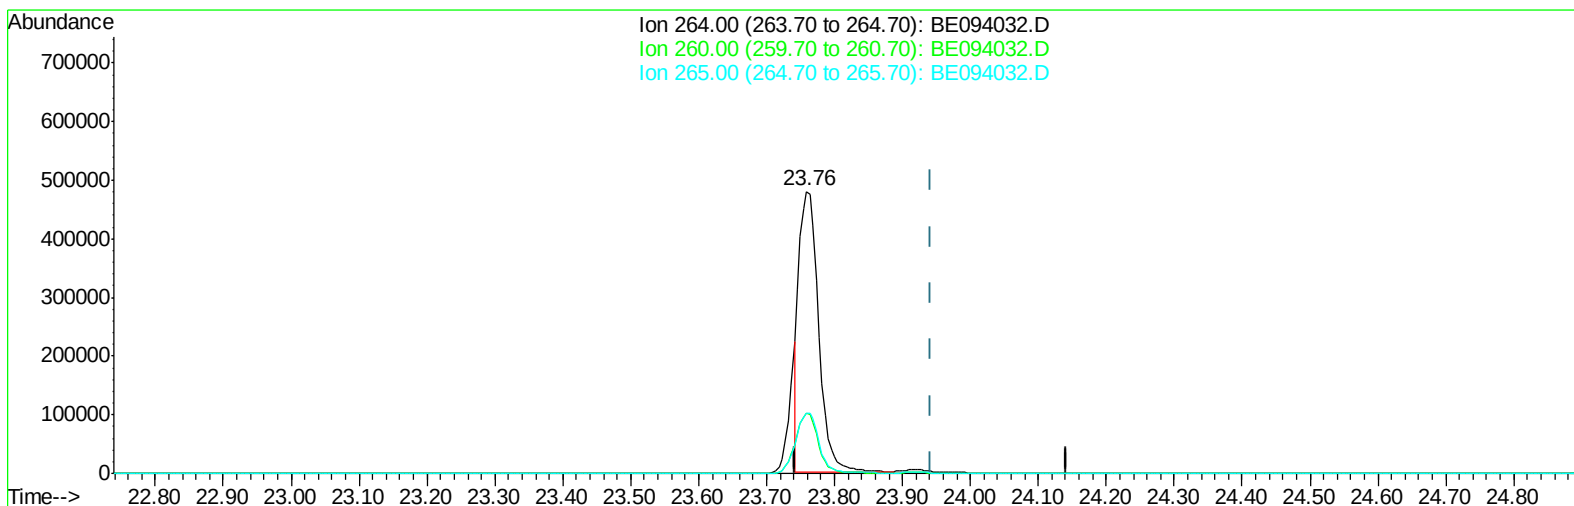

TIC: BE094032.D

(20) Perylene-d12 (I)

23.759min (-0.183) 0.40ng/ul

response 964753

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.16#
265.00	103.50	21.51#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
Data File : BE094032.D
Acq On : 20 Sep 2017 14:37
Operator : SJ/JU
Sample : PB102446BL
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
SBLK46

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:27 PM

9/22/2017 3:55:27 PM

Quant Time: Sep 20 17:01:44 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 13:07:25 2017
Response via : Initial Calibration

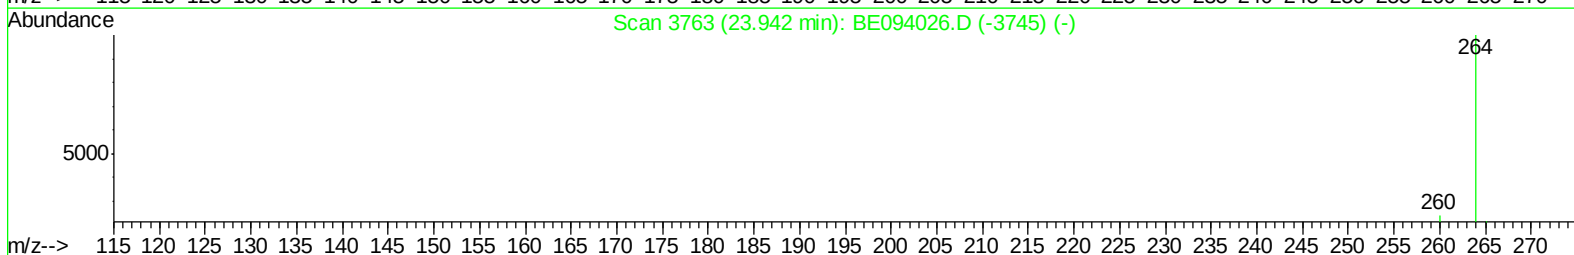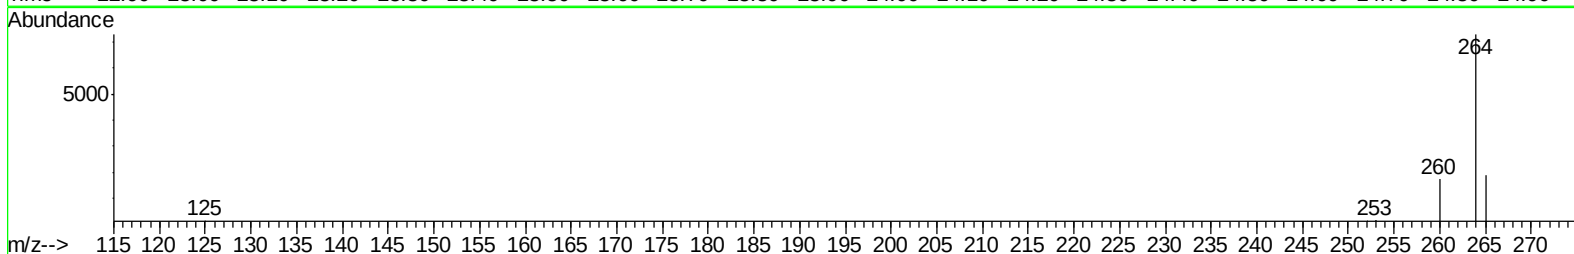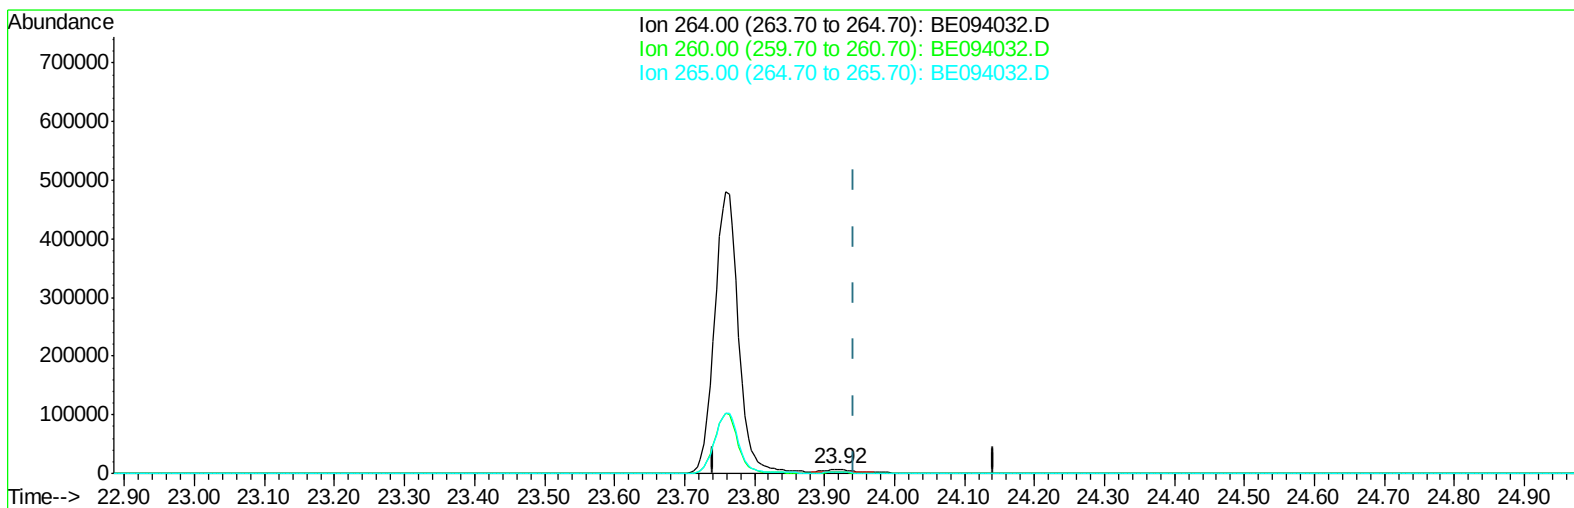

TIC: BE094032.D

(20) Perylene-d12 (I)

23.918min (-0.024) 0.40ng/ul m

response 10413

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.61#
265.00	103.50	25.89#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
 Data File : BE094032.D
 Acq On : 20 Sep 2017 14:37
 Operator : SJ/JU
 Sample : PB102446BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK46

Manual Integrations
 APPROVED

Sohil
 9/22/2017 3:55:27 PM

9/22/2017 3:55:27 PM

Quant Time: Sep 20 17:02:49 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 20 13:07:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1475	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	7702	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	5126	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.26	188	12688m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.42	240	12841	0.40	ng/ul	-0.01
20) Perylene-d12	23.92	264	10413m	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	3778	0.32	ng/ul	-0.03
14) Fluoranthene-d10	19.27	212	12460	0.29	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
Data File : BE094032.D
Acq On : 20 Sep 2017 14:37
Operator : SJ/JU
Sample : PB102446BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK46

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:27 PM

9/22/2017 3:55:27 PM

Quant Time: Sep 20 17:02:49 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 13:07:25 2017
Response via : Initial Calibration

