




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
Data File : BE094035.D
Acq On : 20 Sep 2017 17:03
Operator : SJ/JU
Sample : I5284-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
CB3F5

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:38 PM

Quant Time: Sep 20 17:40:50 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 17:04:41 2017
Response via : Initial Calibration

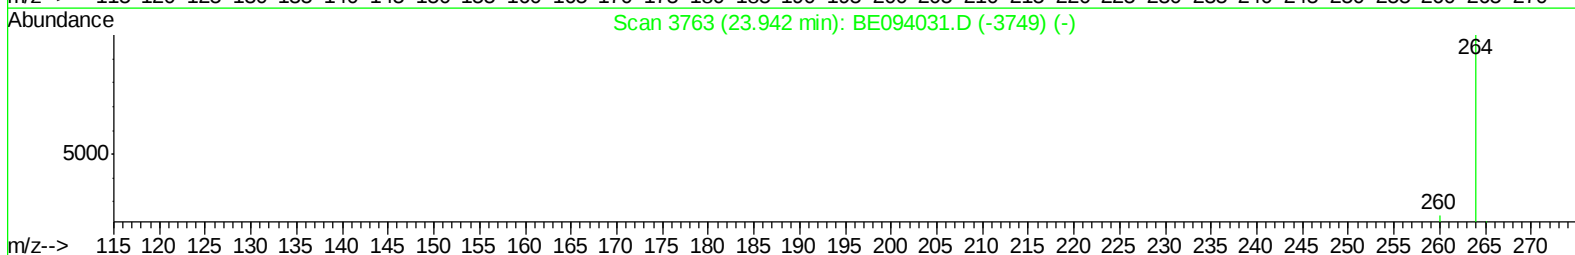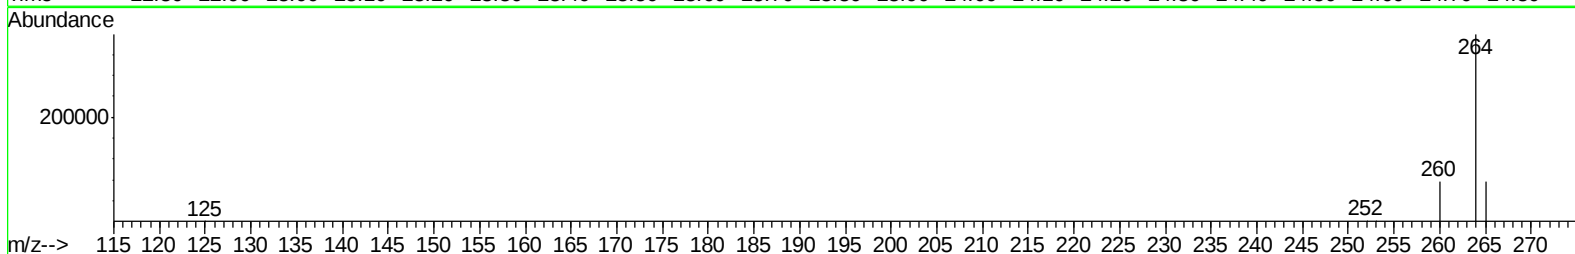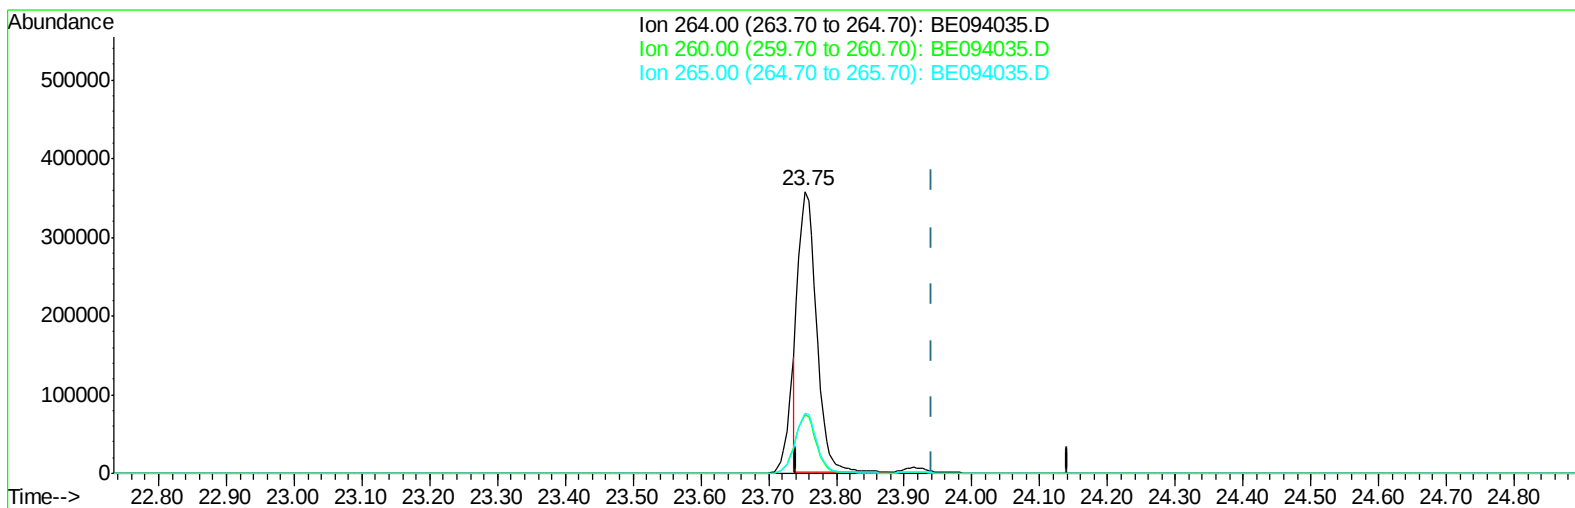

TIC: BE094035.D

(20) Perylene-d12 (I)

23.754min (-0.188) 0.40ng/ul

response 682859

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.13#
265.00	103.50	21.39#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
 Data File : BE094035.D
 Acq On : 20 Sep 2017 17:03
 Operator : SJ/JU
 Sample : I5284-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 CB3F5

Manual Integrations
 APPROVED

Sohil
 9/22/2017 3:55:38 PM

Quant Time: Sep 20 17:40:50 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 20 17:04:41 2017
 Response via : Initial Calibration

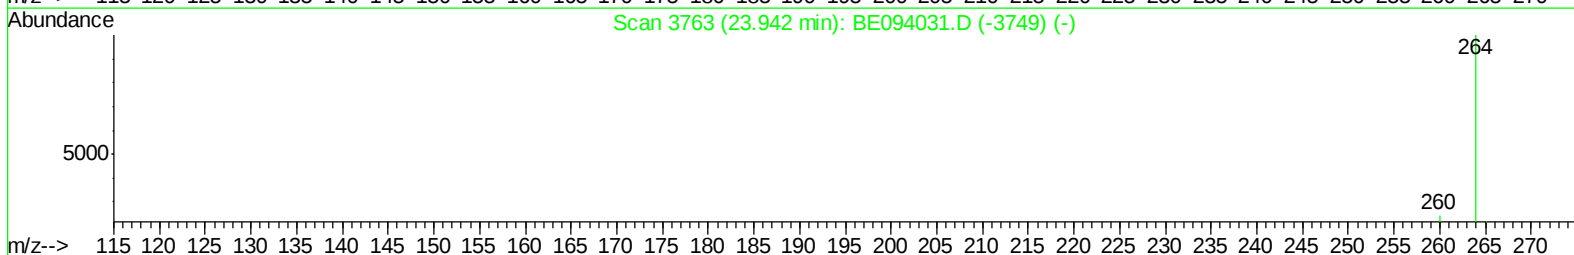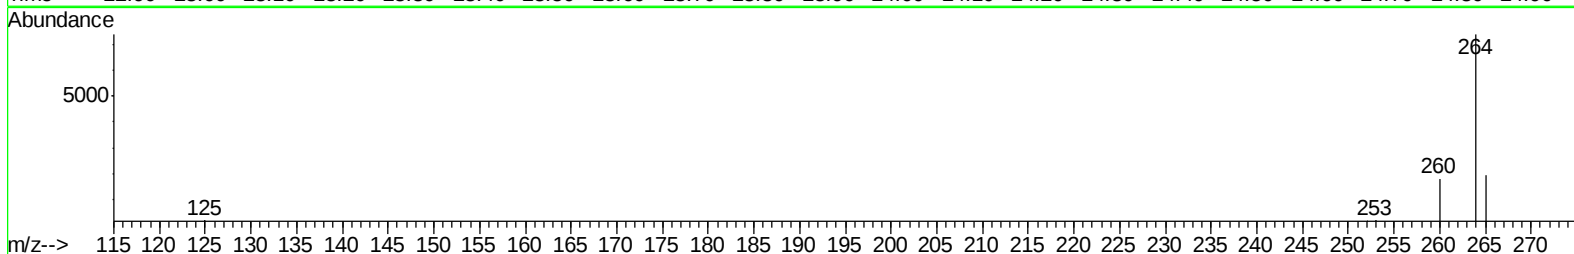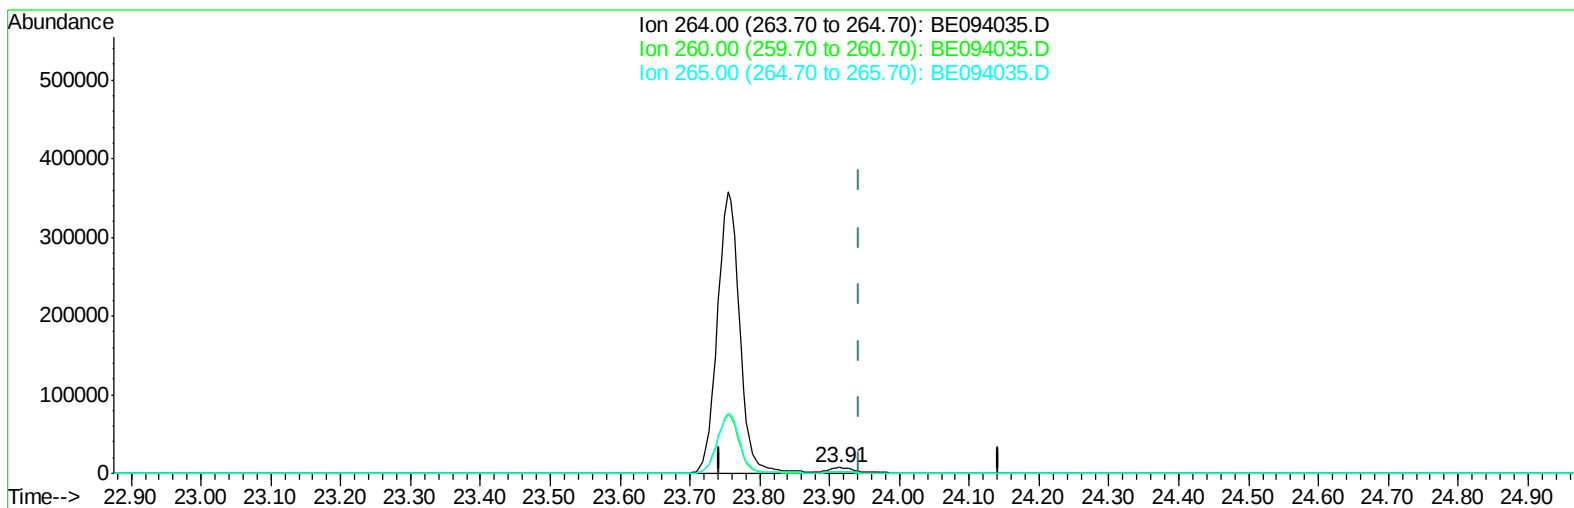

TIC: BE094035.D

(20) Perylene-d12 (I)

23.913min (-0.029) 0.40ng/ul m

response 12616

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.42
265.00	103.50	26.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
 Data File : BE094035.D
 Acq On : 20 Sep 2017 17:03
 Operator : SJ/JU
 Sample : I5284-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 CB3F5

Manual Integrations
 APPROVED

Sohil
 9/22/2017 3:55:38 PM

Quant Time: Sep 20 17:42:55 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 20 17:04:41 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1588	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	8292	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	5564	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.24	188	13916	0.40	ng/ul	-0.03
16) Chrysene-d12	21.41	240	15586	0.40	ng/ul	-0.02
20) Perylene-d12	23.91	264	12616m	0.40	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	2732	0.21	ng/ul	-0.03
14) Fluoranthene-d10	19.27	212	9706	0.21	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092017\
Data File : BE094035.D
Acq On : 20 Sep 2017 17:03
Operator : SJ/JU
Sample : I5284-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
CB3F5

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:38 PM

Quant Time: Sep 20 17:42:55 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 17:04:41 2017
Response via : Initial Calibration

