




Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
Data File : BE094036.D
Acq On : 20 Sep 2017 17:42
Operator : SJ/JU
Sample : PB102444BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK44

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:47 PM

Quant Time: Sep 21 06:27:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 06:26:27 2017
Response via : Initial Calibration

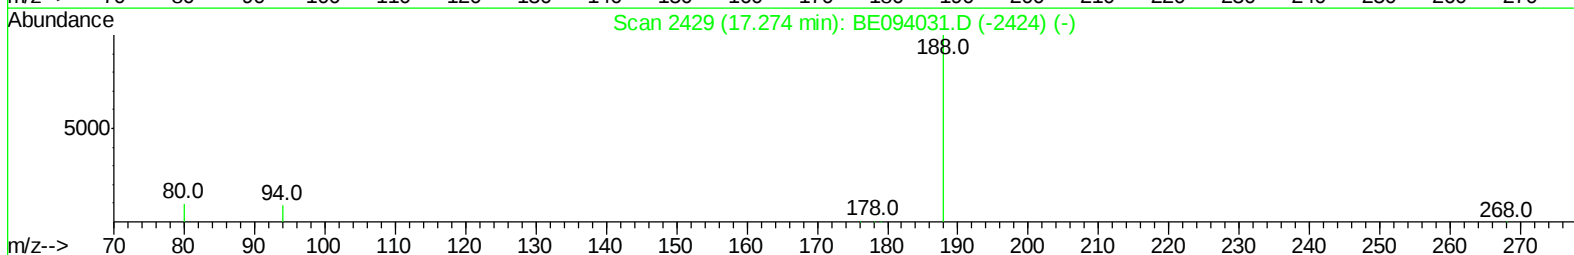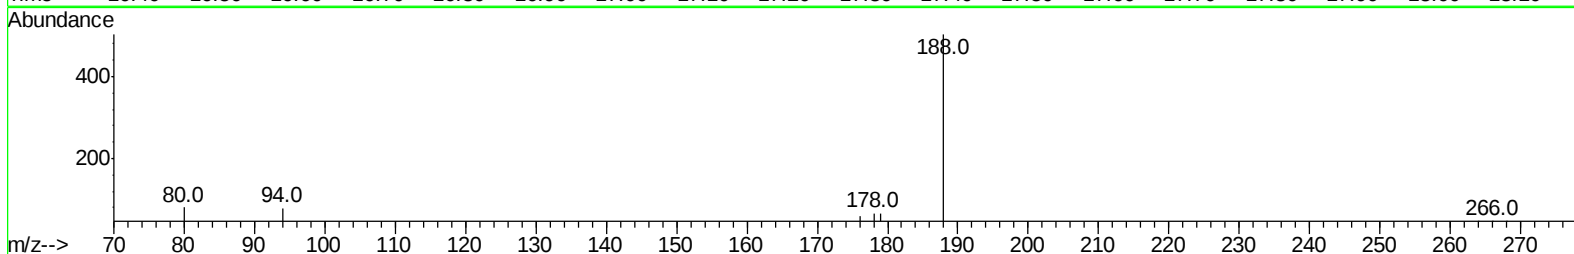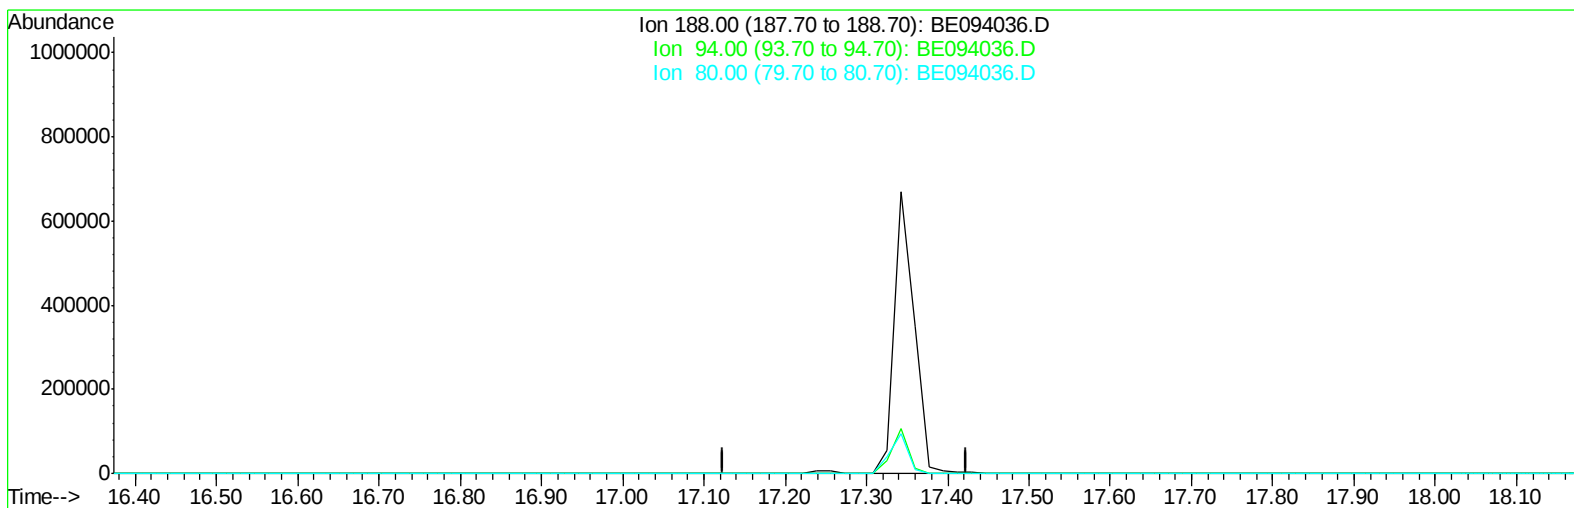

TIC: BE094036.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
Data File : BE094036.D
Acq On : 20 Sep 2017 17:42
Operator : SJ/JU
Sample : PB102444BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK44

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:47 PM

Quant Time: Sep 21 06:27:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 06:26:27 2017
Response via : Initial Calibration

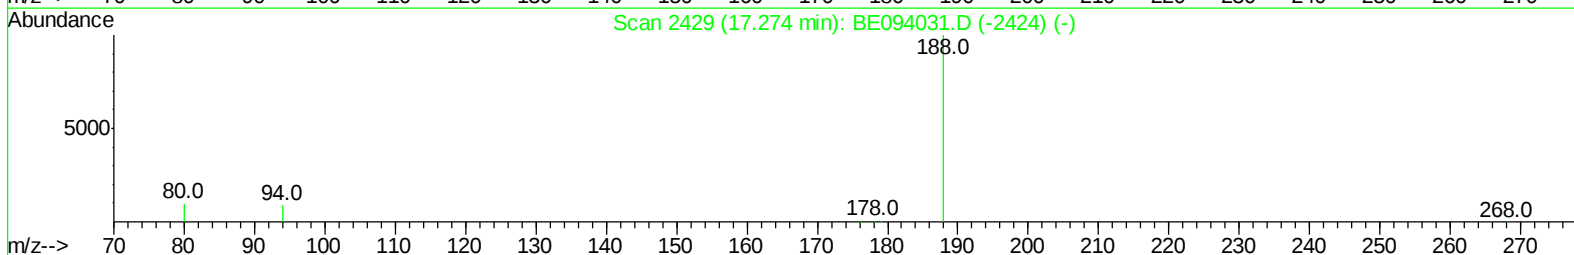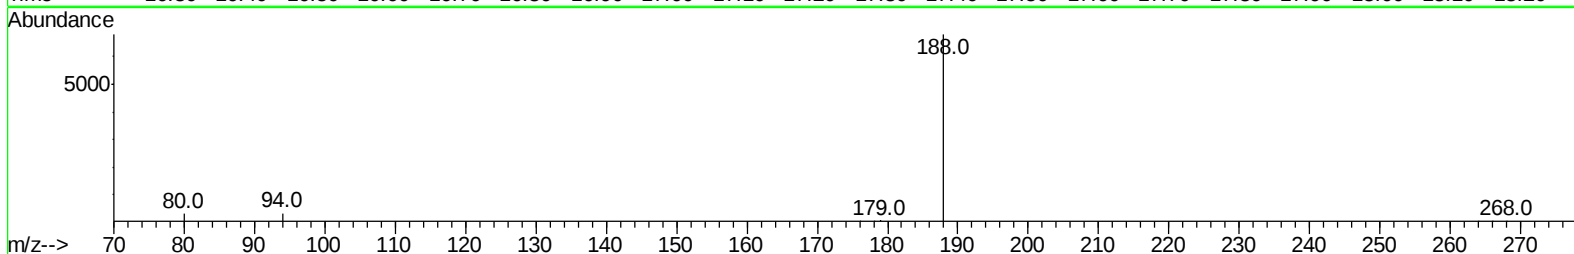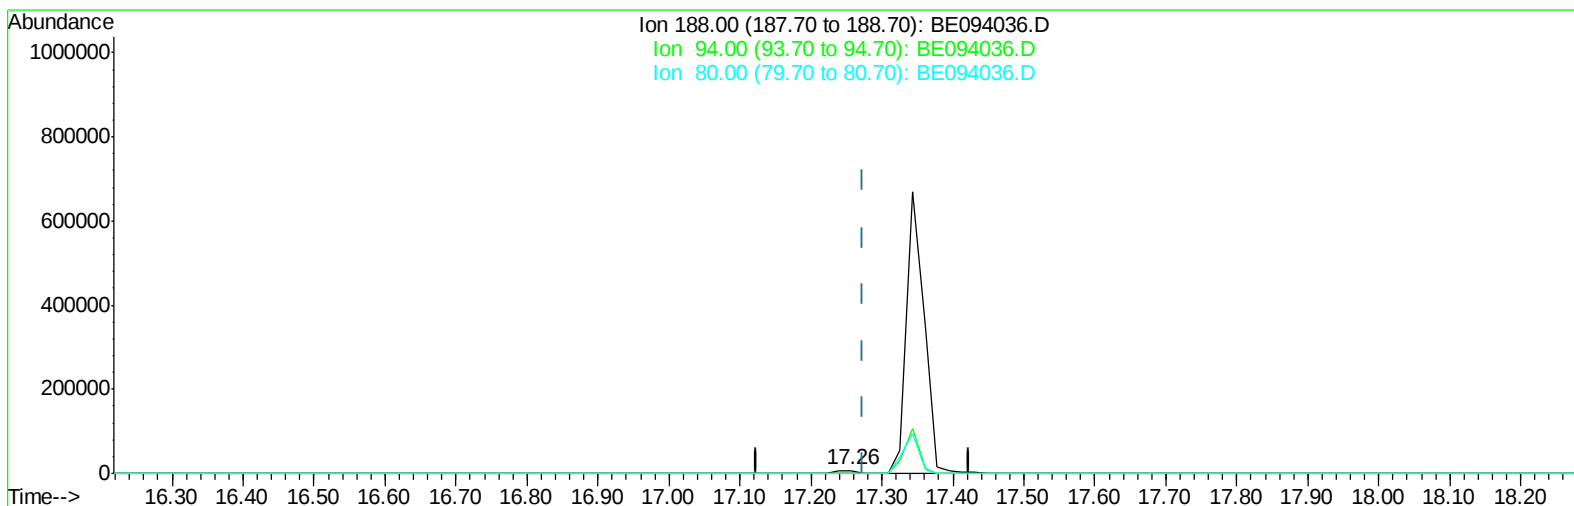

TIC: BE094036.D

(10) Phenanthrene-d10 (I)

17.256min (-0.017) 0.40ng/ul m

response 12847

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.10#
80.00	11.80	4.61#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
Data File : BE094036.D
Acq On : 20 Sep 2017 17:42
Operator : SJ/JU
Sample : PB102444BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK44

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:47 PM

Quant Time: Sep 21 06:33:00 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 06:26:27 2017
Response via : Initial Calibration

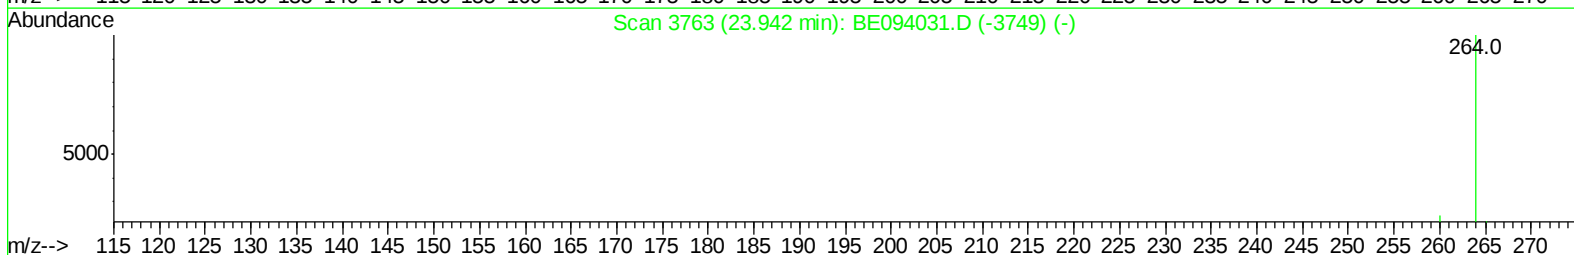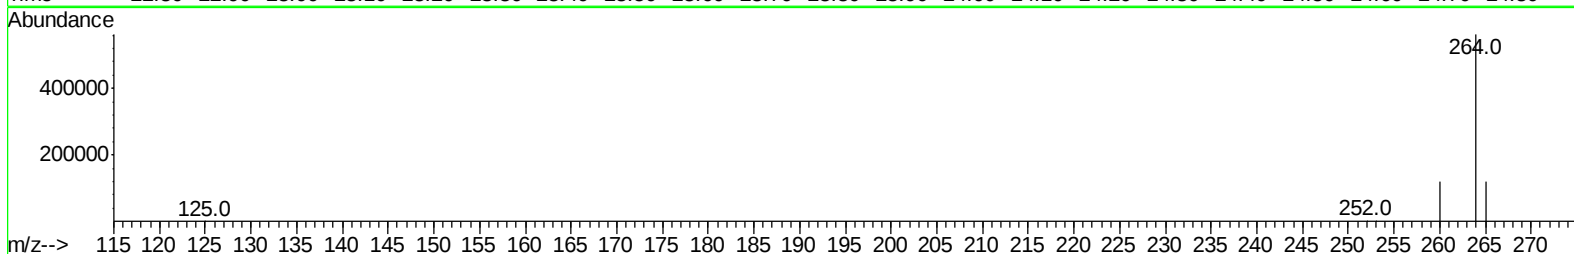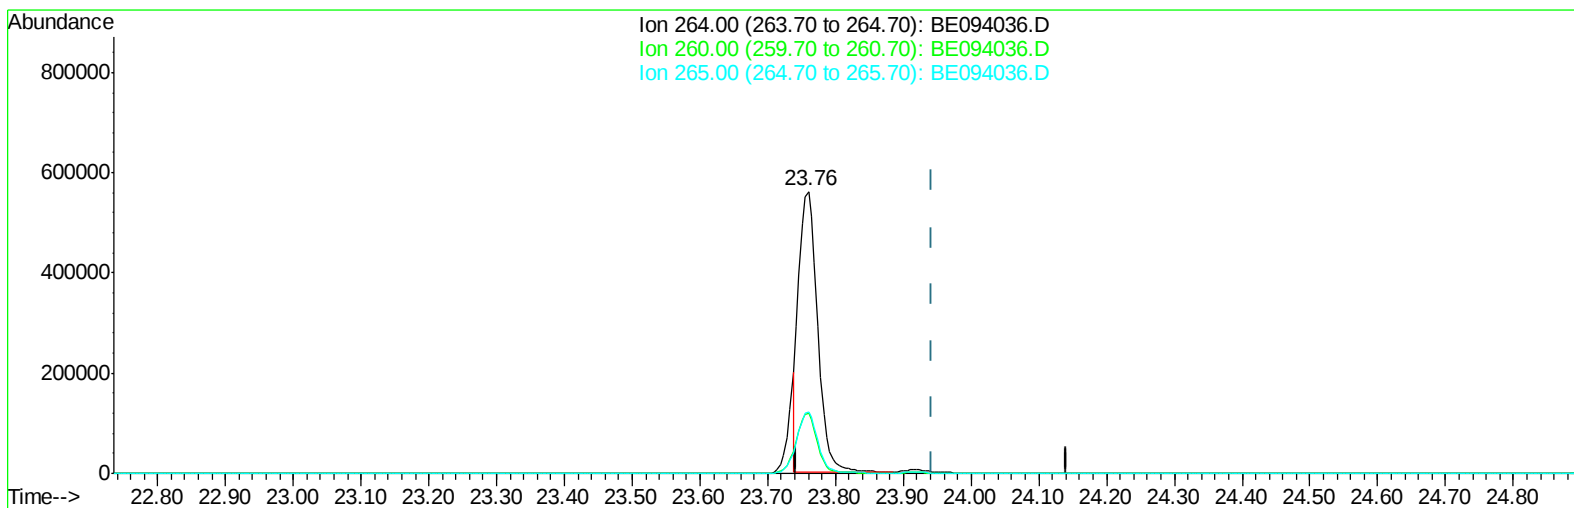

TIC: BE094036.D

(20) Perylene-d12 (I)

23.760min (-0.182) 0.40ng/ul

response 1098031

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.20#
265.00	103.50	21.68#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
Data File : BE094036.D
Acq On : 20 Sep 2017 17:42
Operator : SJ/JU
Sample : PB102444BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK44

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:47 PM

Quant Time: Sep 21 06:33:00 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 06:26:27 2017
Response via : Initial Calibration

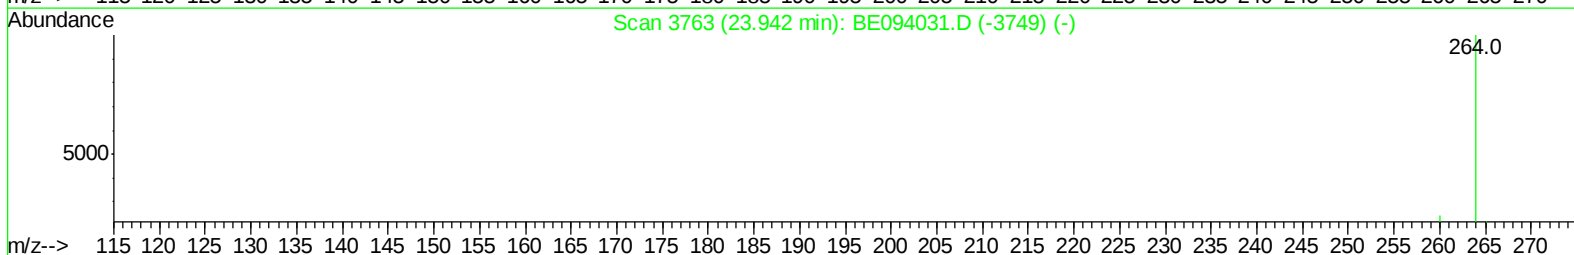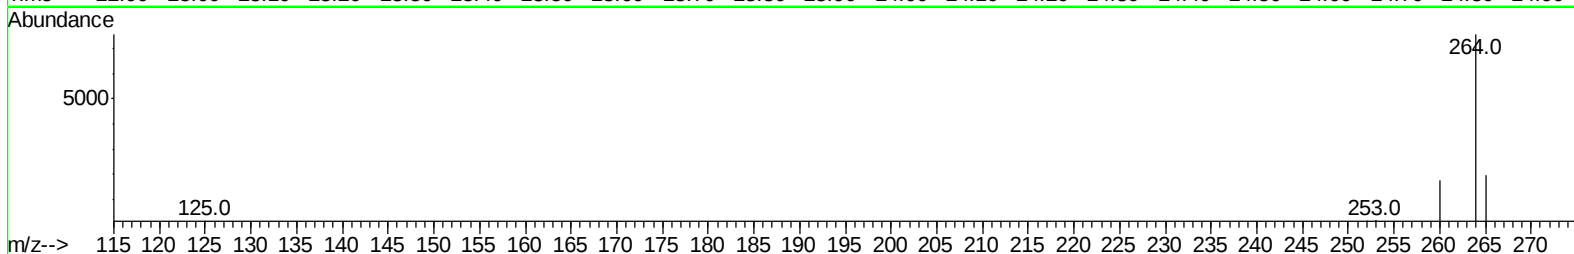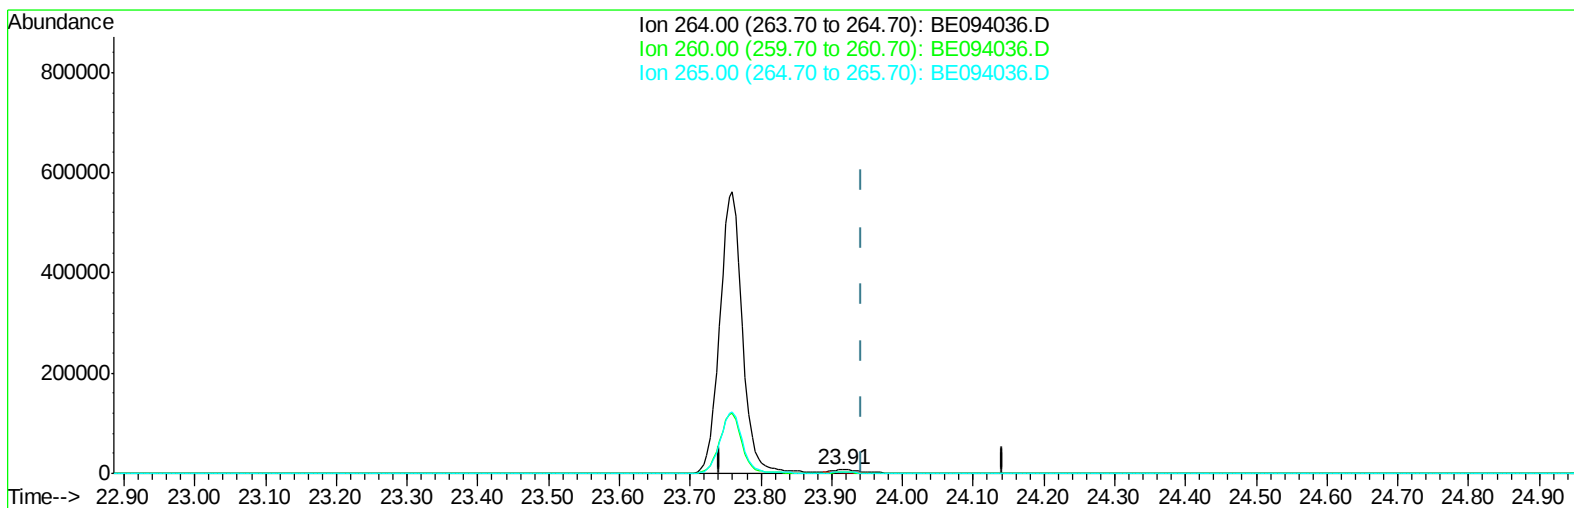

TIC: BE094036.D

(20) Perylene-d12 (I)

23.915min (-0.027) 0.40ng/ul m

response 14615

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.46#
265.00	103.50	26.12#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
 Data File : BE094036.D
 Acq On : 20 Sep 2017 17:42
 Operator : SJ/JU
 Sample : PB102444BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK44

Manual Integrations
 APPROVED

Sohil
 9/22/2017 3:55:47 PM

Quant Time: Sep 21 06:34:28 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 21 06:26:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	1452	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	7671	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	5308	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.26	188	12847m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.42	240	13968	0.40	ng/ul	-0.01
20) Perylene-d12	23.91	264	14615m	0.40	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	4139	0.35	ng/ul	-0.03
14) Fluoranthene-d10	19.27	212	14337	0.33	ng/ul	-0.02

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE092017\
Data File : BE094036.D
Acq On : 20 Sep 2017 17:42
Operator : SJ/JU
Sample : PB102444BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK44

Manual Integrations
APPROVED

Sohil
9/22/2017 3:55:47 PM

Quant Time: Sep 21 06:34:28 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 06:26:27 2017
Response via : Initial Calibration

