
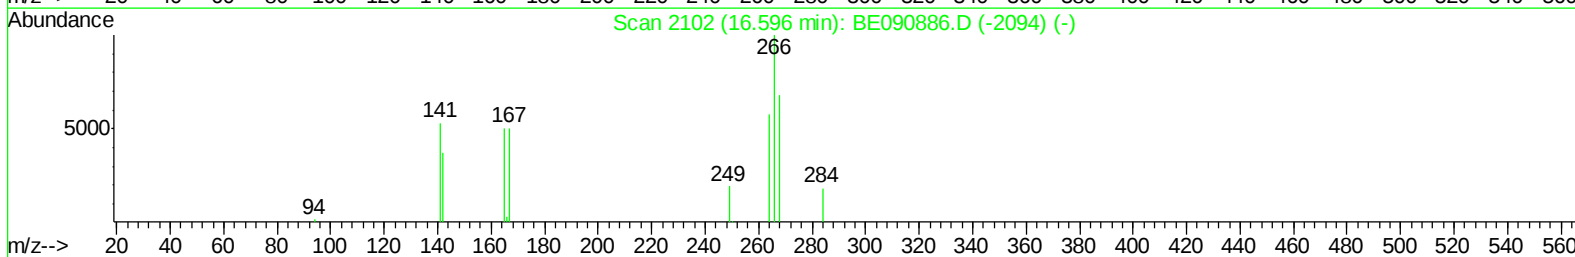
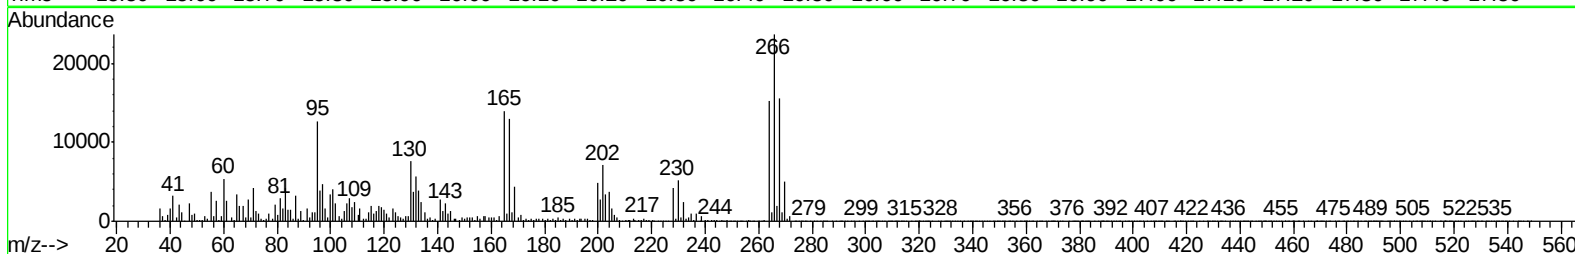


Data Path : Z:\HPCHEM1\BNA E\Data\BE092115\
Data File : BE090909.D
Acq On : 21 Sep 2015 4:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 05:07:33 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE091815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 18:17:34 2015
Response via : Initial Calibration

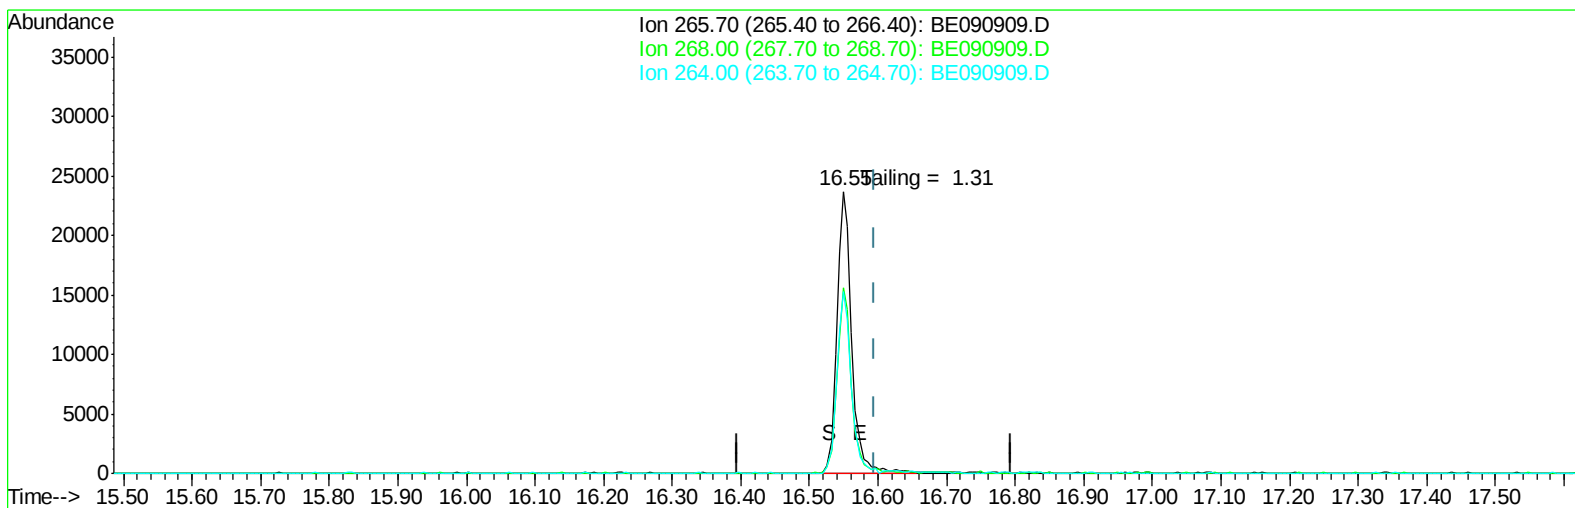

TIC: BE090909.D

(22) Pentachlorophenol

16.549min (-0.046) 24857.84ng

response 35618

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	65.84
264.00	67.40	64.73
0.00	0.00	0.00