

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092115\
 Data File : BE090921.D
 Acq On : 21 Sep 2015 16:50
 Operator : UM/IZ
 Sample : G3745-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 091815-D534-E-D-B

Quant Time: Sep 21 17:31:57 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 18 18:17:34 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	28964	5.00	ng	0.00
7) Naphthalene-d8	10.31	136	119908	5.00	ng	0.00
13) Acenaphthene-d10	14.17	164	65266	5.00	ng	0.00
19) Phenanthrene-d10	16.91	188	161568	5.00	ng	0.00
26) Chrysene-d12	21.07	240	208002	5.00	ng	0.00
33) Perylene-d12	23.35	264	187067	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	14533	2.21	ng	0.00
5) Phenol-d6	6.79	99	10737	1.19	ng	0.03
8) Nitrobenzene-d5	8.72	82	22337	2.70	ng	0.01
14) 2,4,6-Tribromophenol	15.67	330	10161	4.41	ng	-0.02
15) 2-Fluorobiphenyl	12.81	172	53148	2.87	ng	0.00
28) Terphenyl-d14	19.53	244	106318	4.51	ng	0.00
Target Compounds						
31) Bis(2-ethylhexyl)phthalate	21.00	149	1586	0.24	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092115\
Data File : BE090921.D
Acq On : 21 Sep 2015 16:50
Operator : UM/IZ
Sample : G3745-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
091815-D534-E-D-B

Quant Time: Sep 21 17:31:57 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 18:17:34 2015
Response via : Initial Calibration

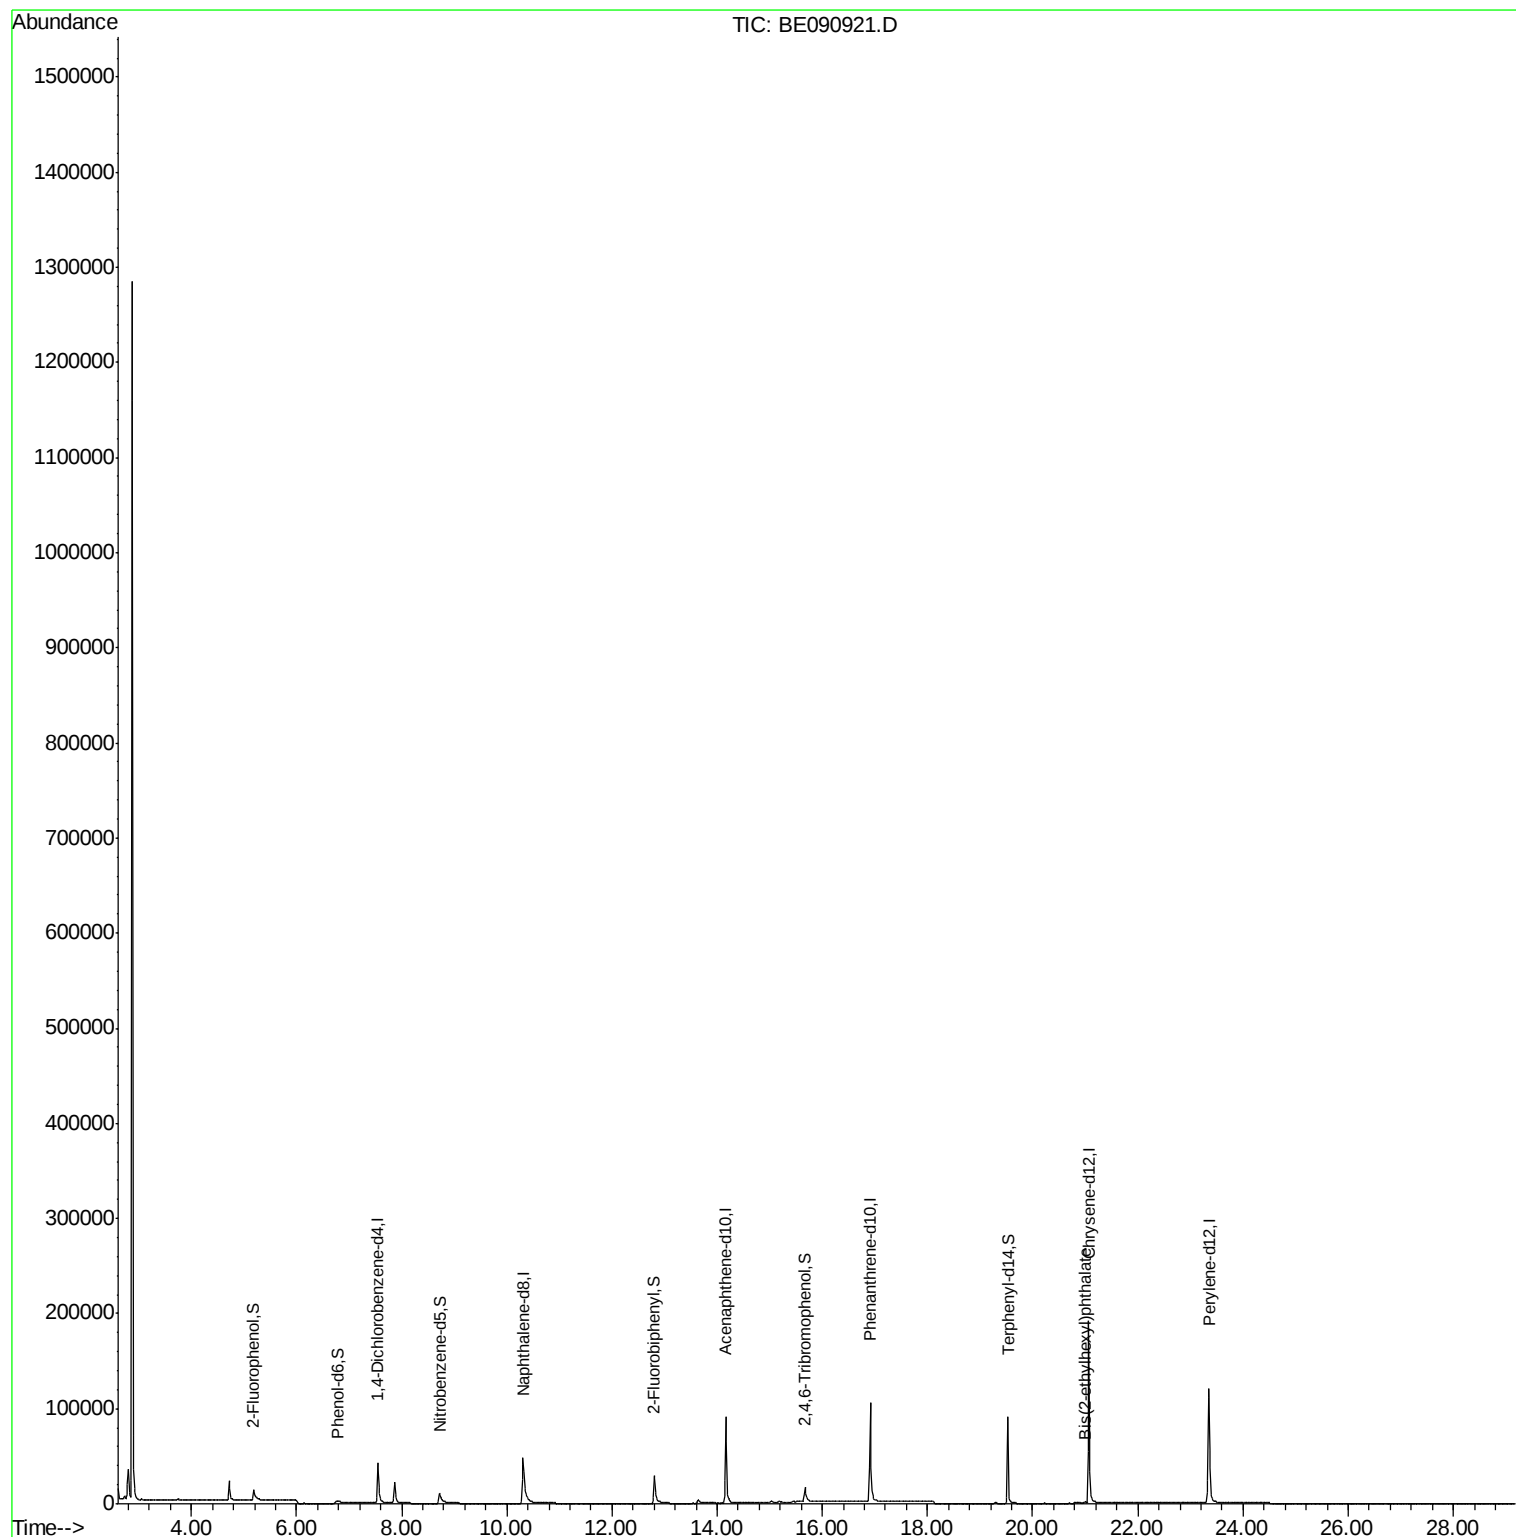


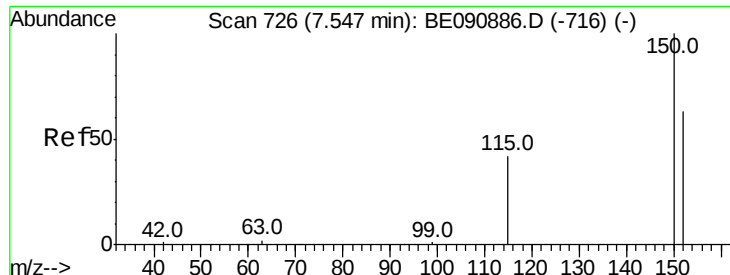




#1
 1,4-Dichlorobenzene-d4
 Concen: 5.00 ng
 RT: 7.55 min Scan# 726
 Delta R.T. -0.00 min
 Lab File: BE090921.D
 Acq: 21 Sep 2015 16:50

Instrument :
 BNA_E
 ClientSampleId :
 091815-D534-E-D-B

Tgt Ion:152 Resp: 28964
 Ion Ratio Lower Upper
 152 100
 150 157.2 122.2 183.4
 115 68.7 51.0 76.4

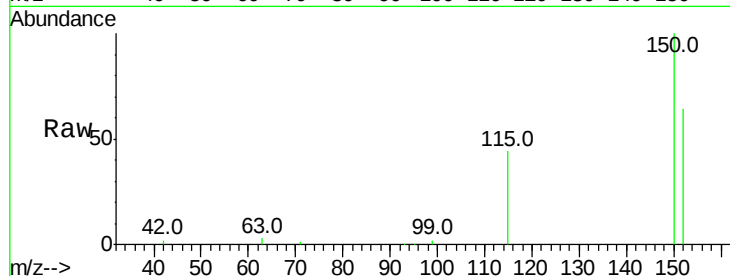


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

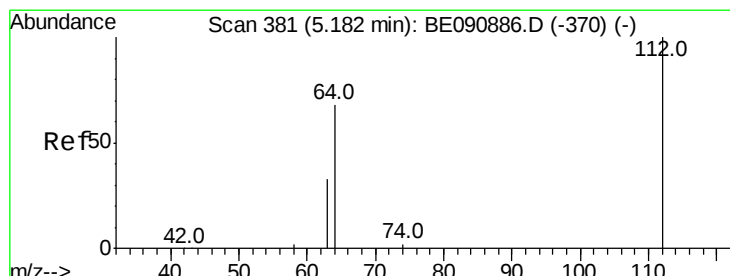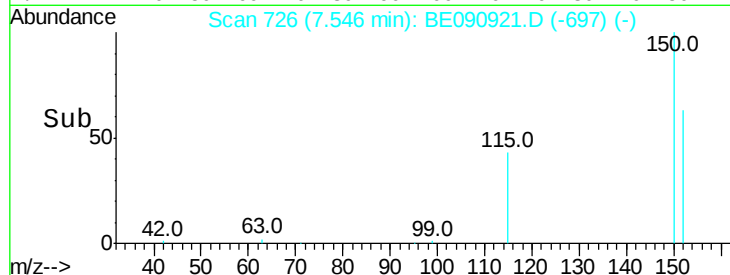
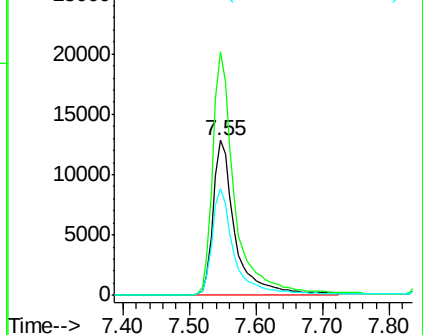



#4
 2-Fluorophenol
 Concen: 2.21 ng
 RT: 5.18 min Scan# 381
 Delta R.T. 0.00 min
 Lab File: BE090921.D
 Acq: 21 Sep 2015 16:50

Tgt Ion:112 Resp: 14533
 Ion Ratio Lower Upper
 112 100
 64 72.7 57.3 85.9
 63 38.0 29.2 43.8

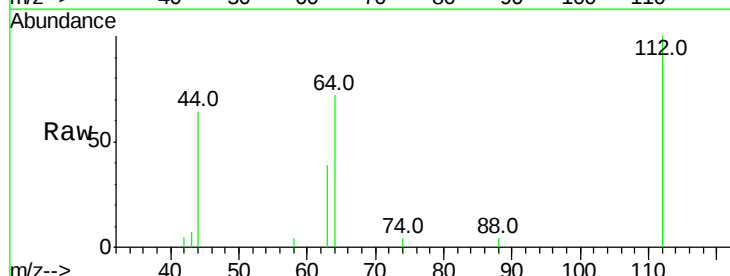

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0

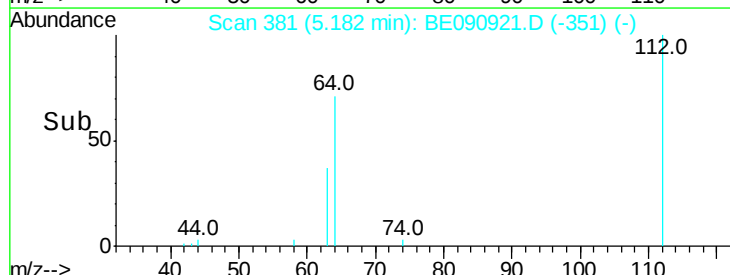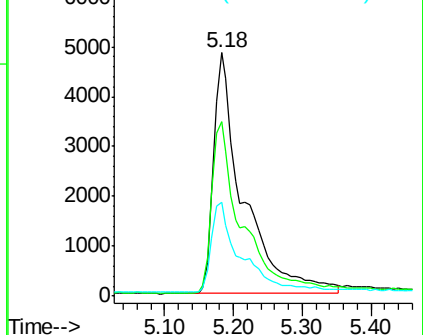

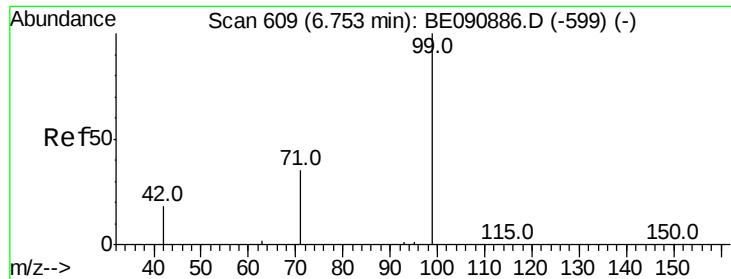

#5

Phenol-d6

Concen: 1.19 ng

RT: 6.79 min Scan# 614

Delta R.T. 0.03 min

Lab File: BE090921.D

Acq: 21 Sep 2015 16:50

Instrument :

BNA_E

ClientSampleId :

091815-D534-E-D-B


Tgt Ion: 99 Resp: 10737

Ion Ratio Lower Upper

99 100

42 23.4 16.8 25.2




71 0.0 28.3 42.5#

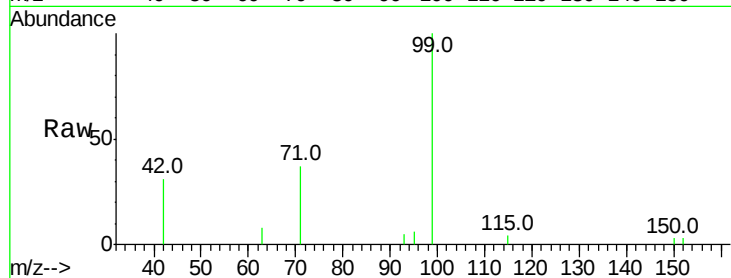

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

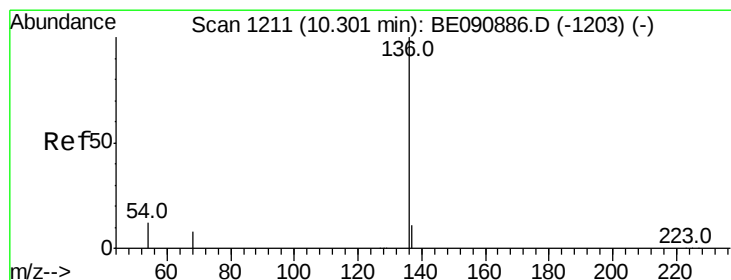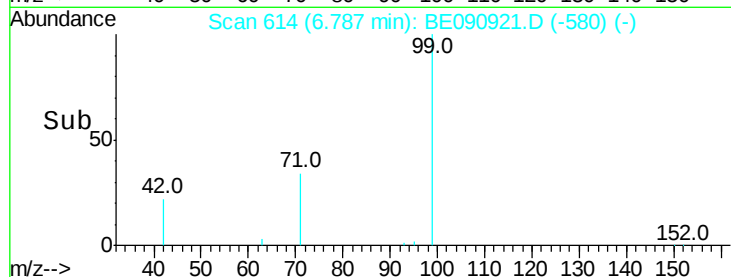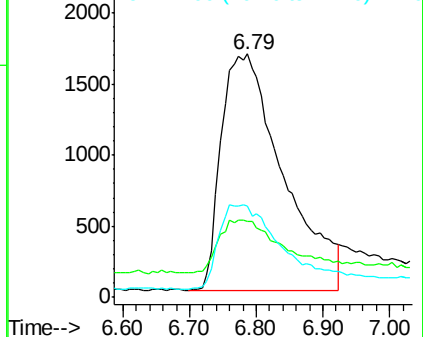

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.31 min Scan# 1212

Delta R.T. 0.01 min

Lab File: BE090921.D

Acq: 21 Sep 2015 16:50

Tgt Ion: 136 Resp: 119908


Ion Ratio Lower Upper

136 100

137 11.1 8.7 13.1

54 12.0 9.0 13.6

68 8.5 6.3 9.5


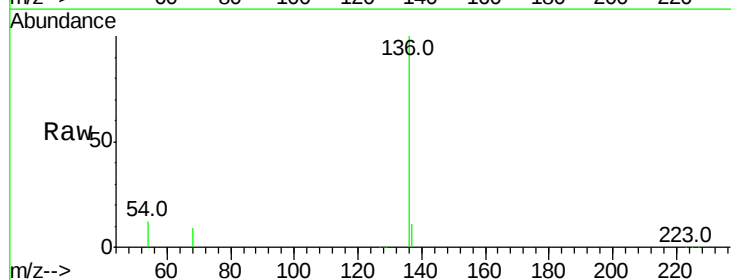



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



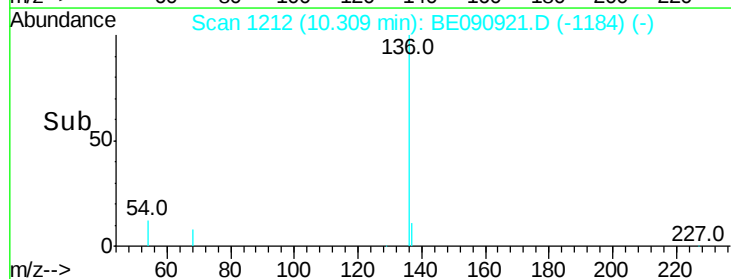
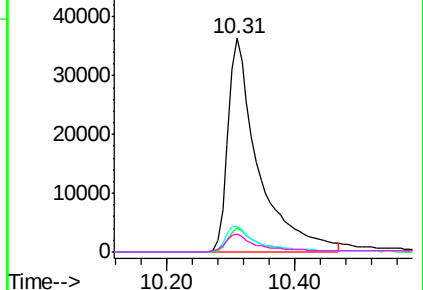


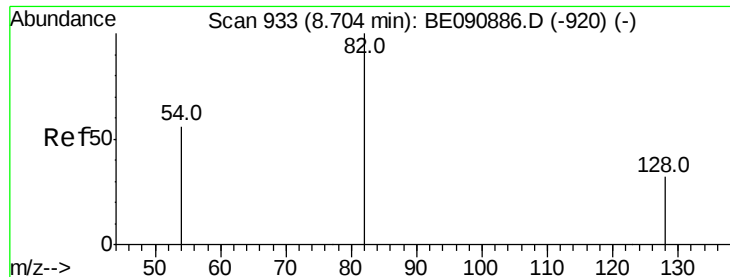

#8
 Nitrobenzene-d5
 Concen: 2.70 ng
 RT: 8.72 min Scan# 936
 Delta R.T. 0.01 min
 Lab File: BE090921.D
 Acq: 21 Sep 2015 16:50




Instrument :
 BNA_E
 ClientSampleId :
 091815-D534-E-D-B


Tgt Ion: 82 Resp: 22337
 Ion Ratio Lower Upper
 82 100
 128 30.2 25.0 37.4
 54 60.2 46.3 69.5

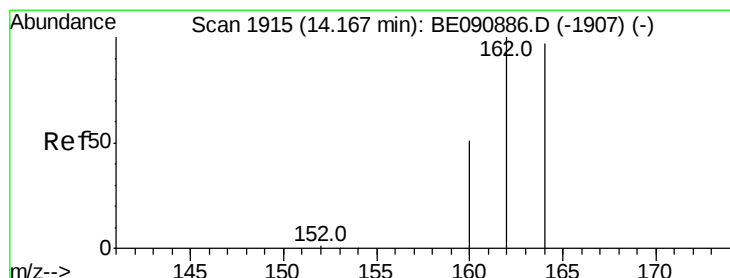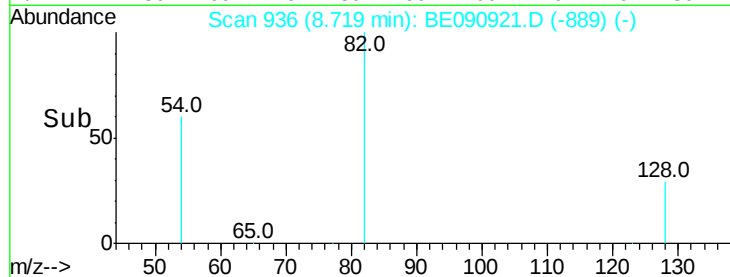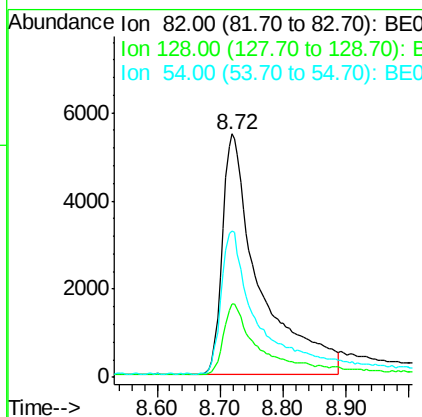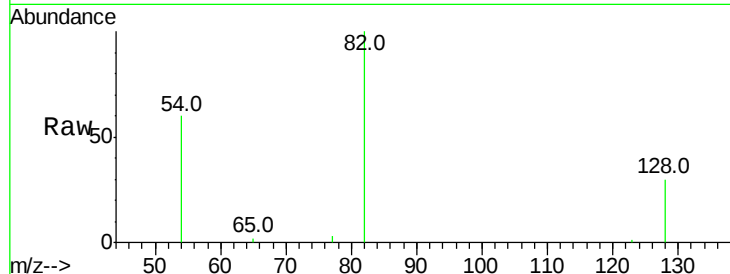

#13
 Acenaphthene-d10
 Concen: 5.00 ng
 RT: 14.17 min Scan# 1916
 Delta R.T. 0.00 min
 Lab File: BE090921.D
 Acq: 21 Sep 2015 16:50

Tgt Ion: 164 Resp: 65266
 Ion Ratio Lower Upper
 164 100
 162 103.5 86.8 130.2
 160 55.9 53.9 80.9

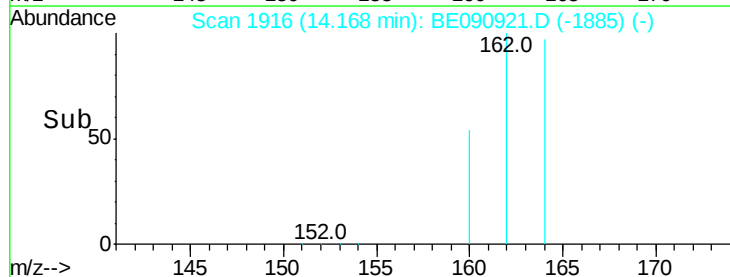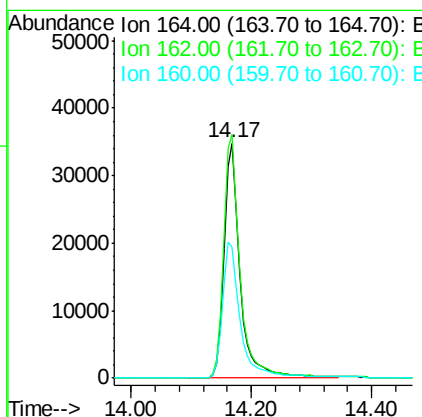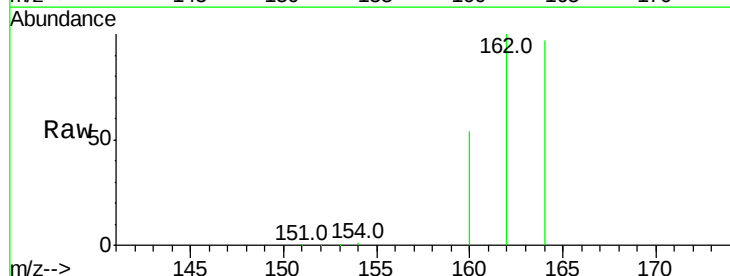


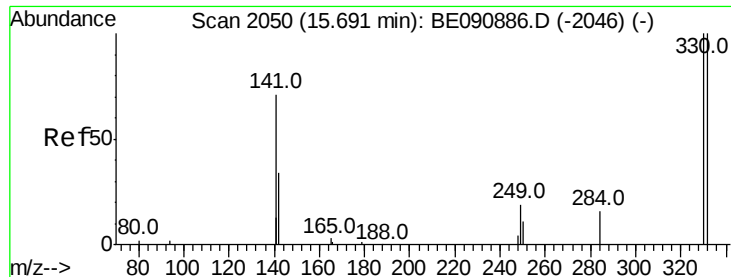




#14
 2,4,6-Tribromophenol
 Concen: 4.41 ng
 RT: 15.67 min Scan# 2050
 Delta R.T. -0.02 min
 Lab File: BE090921.D
 Acq: 21 Sep 2015 16:50

Instrument :
 BNA_E
 ClientSampleId :
 091815-D534-E-D-B

Tgt Ion:330 Resp: 10161
 Ion Ratio Lower Upper
 330 100
 332 95.1 74.9 112.3
 141 172.7 145.2 217.8

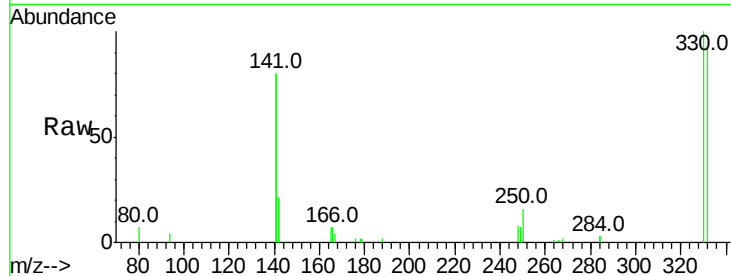


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

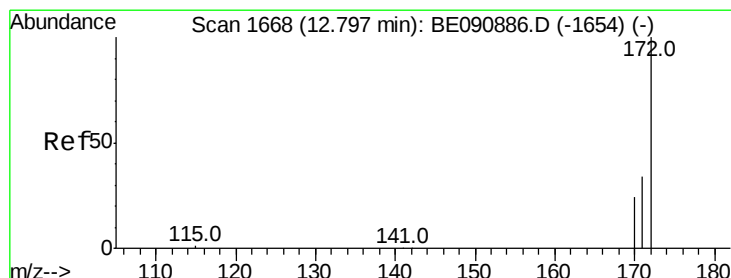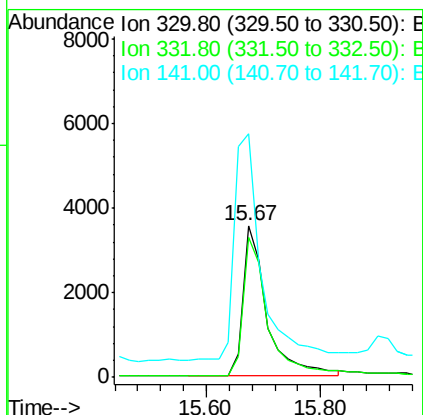
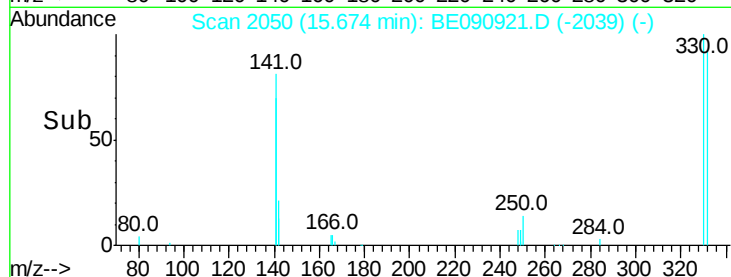



#15
 2-Fluorobiphenyl
 Concen: 2.87 ng
 RT: 12.81 min Scan# 1670
 Delta R.T. 0.01 min
 Lab File: BE090921.D
 Acq: 21 Sep 2015 16:50

Tgt Ion:172 Resp: 53148
 Ion Ratio Lower Upper
 172 100
 171 34.8 27.8 41.8
 170 23.4 19.8 29.6

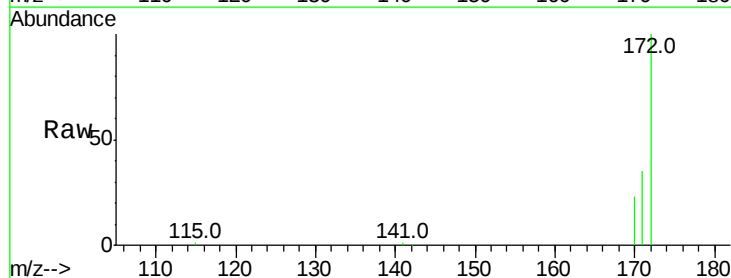

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

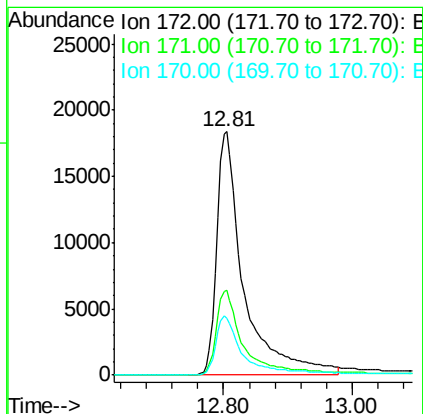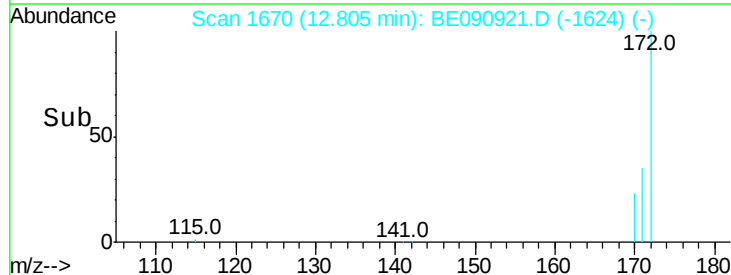

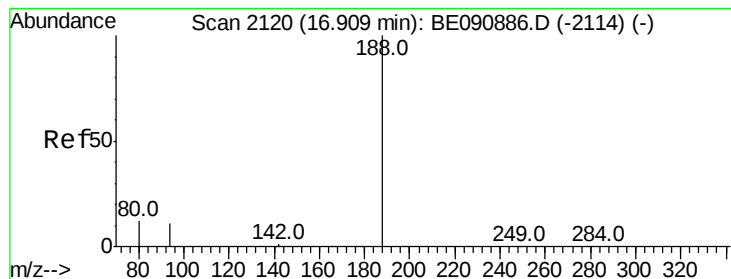

#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.91 min Scan# 2121

Delta R.T. 0.00 min

Lab File: BE090921.D

Acq: 21 Sep 2015 16:50

Instrument :

BNA_E

ClientSampleId :

091815-D534-E-D-B


Tgt Ion:188 Resp: 161568

Ion Ratio Lower Upper

188 100

94 10.0 10.3 15.5#




80 10.8 11.0 16.6#

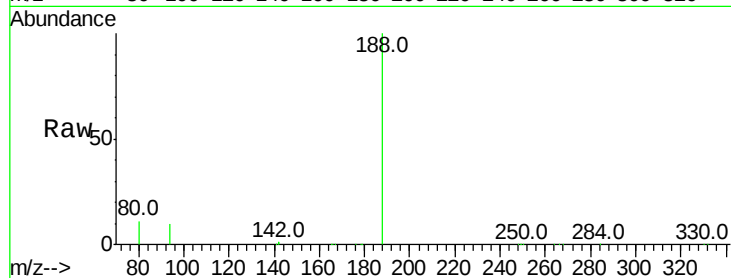

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

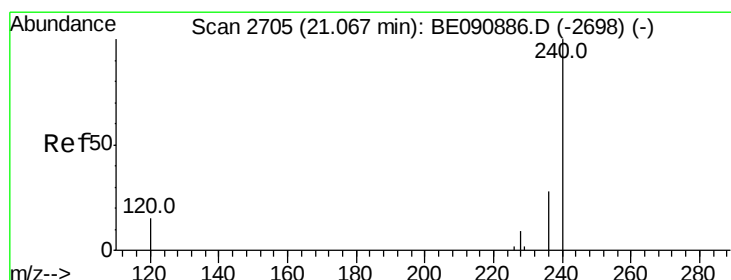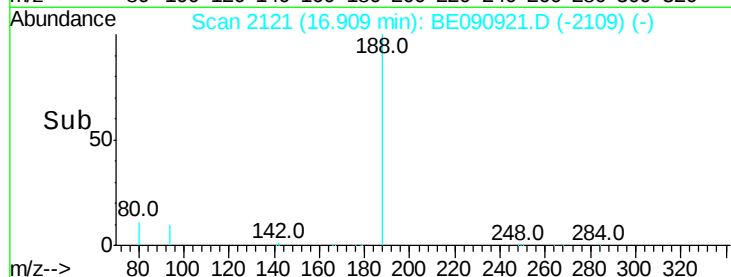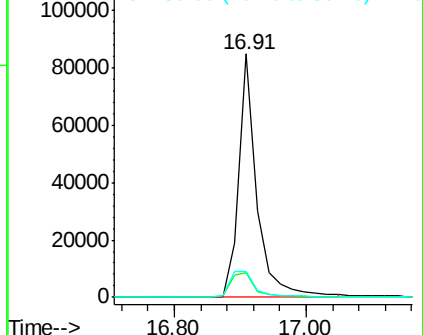

#26

Chrysene-d12

Concen: 5.00 ng

RT: 21.07 min Scan# 2706

Delta R.T. 0.00 min

Lab File: BE090921.D

Acq: 21 Sep 2015 16:50


Tgt Ion:240 Resp: 208002

Ion Ratio Lower Upper

240 100

120 13.5 10.1 15.1



236 27.0 21.9 32.9

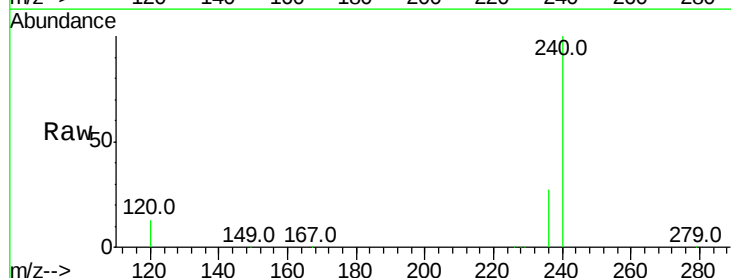


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

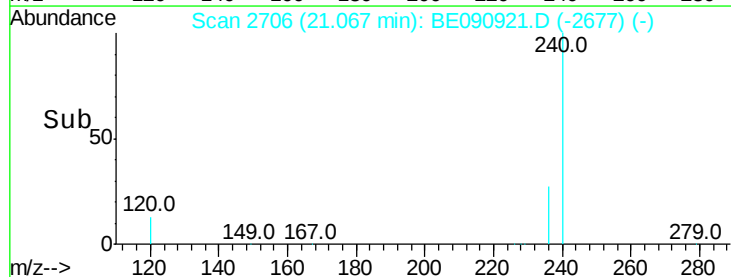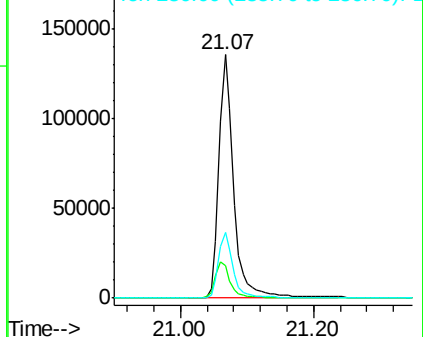

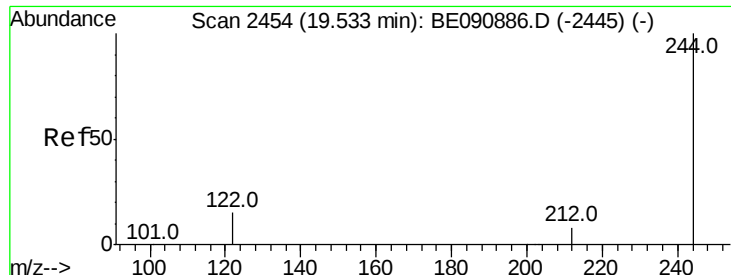

#28

Terphenyl-d14

Concen: 4.51 ng

RT: 19.53 min Scan# 2454

Delta R.T. -0.00 min

Lab File: BE090921.D

Acq: 21 Sep 2015 16:50

Instrument :

BNA_E

ClientSampleId :

091815-D534-E-D-B


Tgt Ion:244 Resp: 106318

Ion Ratio Lower Upper

244 100

212 8.2 6.9 10.3




122 13.5 12.9 19.3

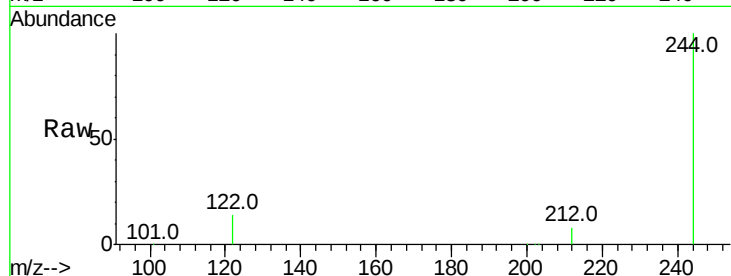

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

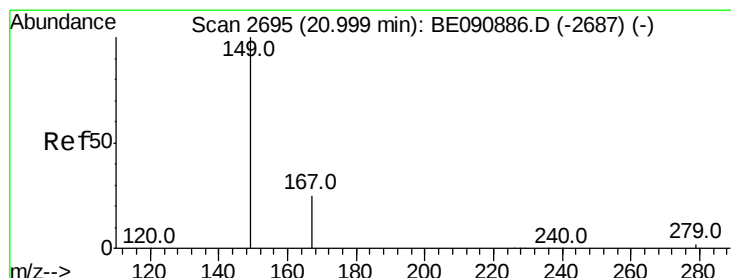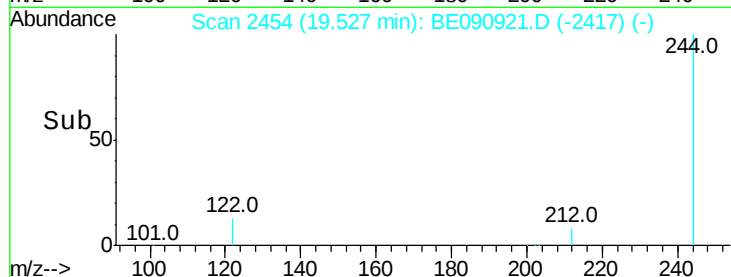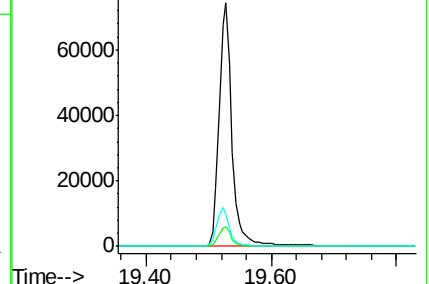

#31

Bis(2-ethylhexyl)phthalate

Concen: 0.24 ng

RT: 21.00 min Scan# 2696

Delta R.T. 0.00 min

Lab File: BE090921.D

Acq: 21 Sep 2015 16:50


Tgt Ion:149 Resp: 1586

Ion Ratio Lower Upper

149 100

167 25.3 20.1 30.1



279 3.2 2.3 3.5

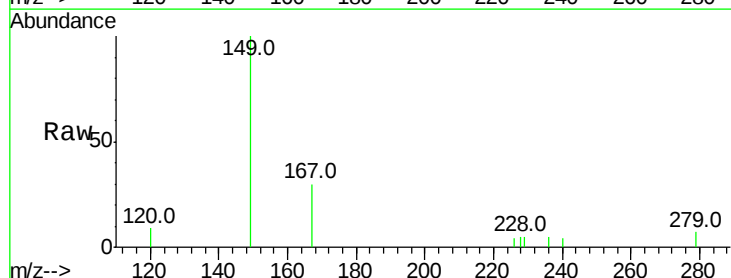


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

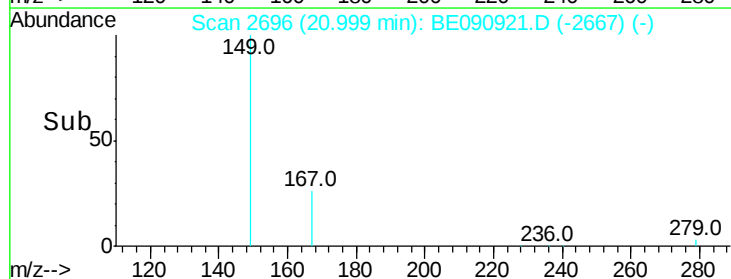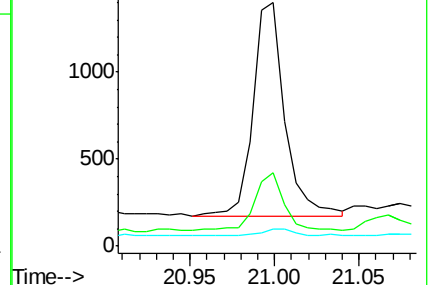

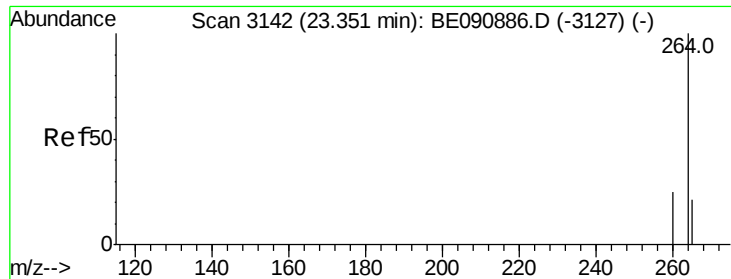

#33

Perylene-d12

Concen: 5.00 ng

RT: 23.35 min Scan# 3143

Delta R.T. 0.00 min

Lab File: BE090921.D


Acq: 21 Sep 2015 16:50

Instrument :

BNA_E

ClientSampleId :

091815-D534-E-D-B

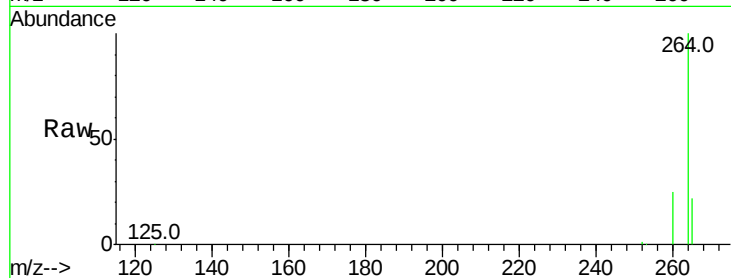


Tgt Ion:264 Resp: 187067

Ion Ratio Lower Upper

264 100

260 25.2 19.7 29.5

265 21.7 17.5 26.3

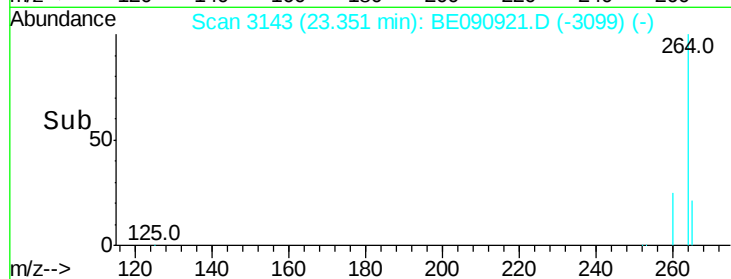

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

