


Data Path : Z:\HPCHEM1\BNA_E\Data\BE092115\
Data File : BE090909.D
Acq On : 21 Sep 2015 4:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 18 18:17:34 2015

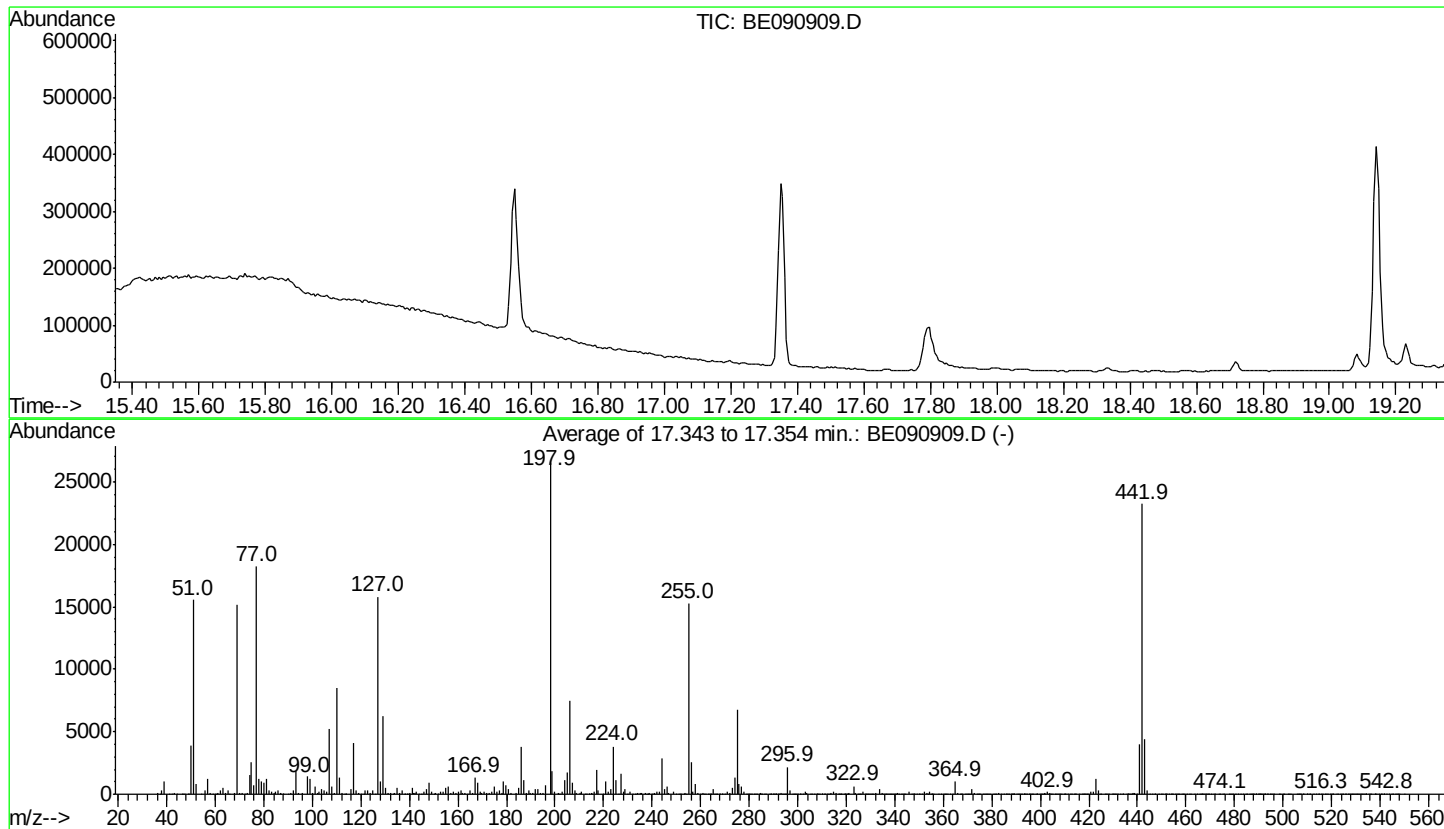

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	15556	PASS
68	69	0.00	2	0.9	136	PASS
69	198	0.00	100	57.3	15191	PASS
70	69	0.00	2	0.5	82	PASS
127	198	10	80	59.5	15791	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26534	PASS
199	198	5	9	7.0	1855	PASS
275	198	10	60	25.5	6766	PASS
365	198	1	100	3.8	1014	PASS
441	442	0.01	24	17.0	3960	PASS
442	198	50	100	87.6	23246	PASS
443	442	15	24	19.0	4415	PASS