


Data Path : Z:\HPCHEM1\BNA_E\Data\BE092115\
 Data File : BE090916.D
 Acq On : 21 Sep 2015 13:45
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 18 18:17:34 2015

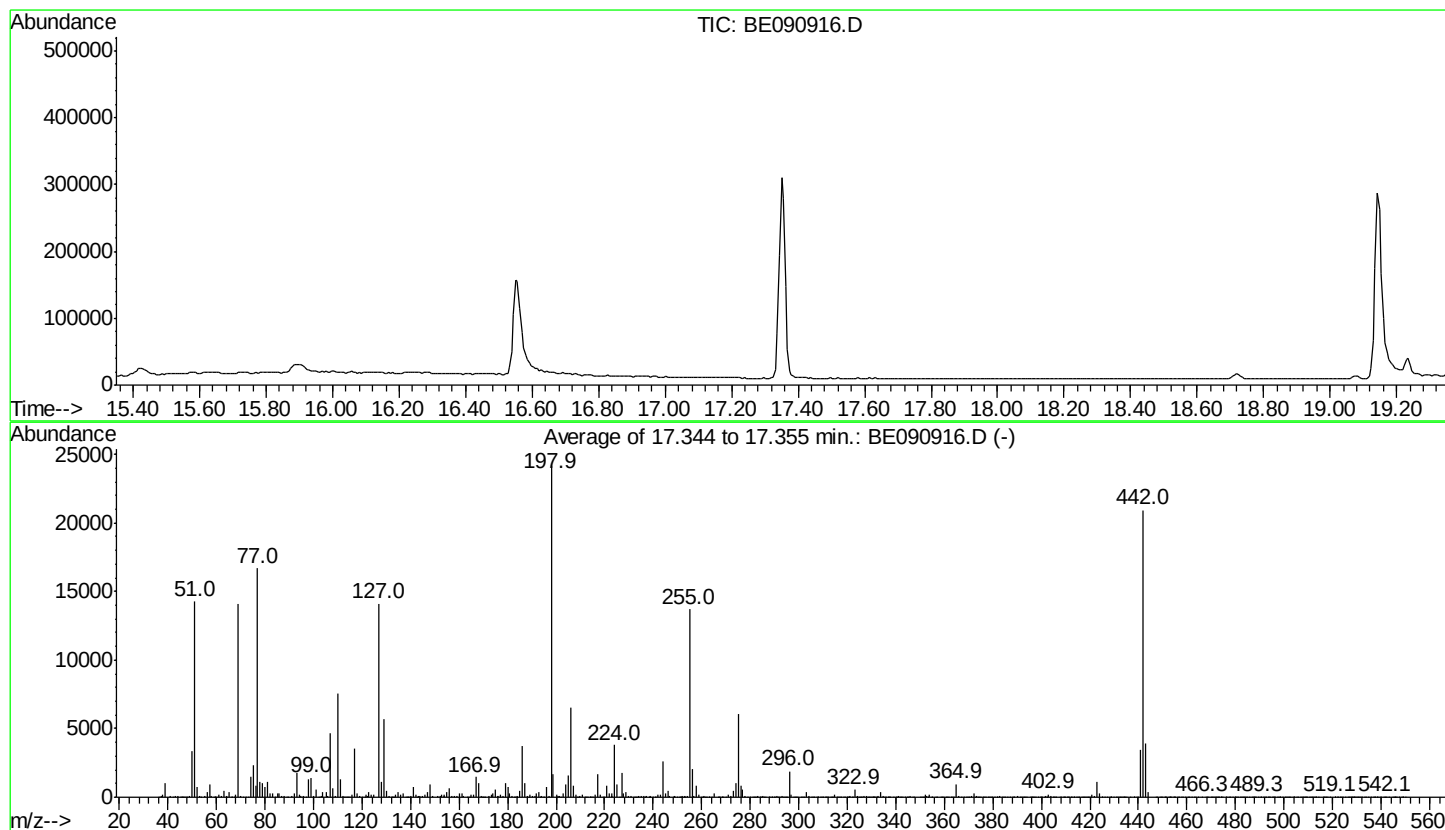

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.9	14244	PASS
68	69	0.00	2	1.6	226	PASS
69	198	0.00	100	58.2	14077	PASS
70	69	0.00	2	0.5	76	PASS
127	198	10	80	58.4	14118	PASS
197	198	0.00	2	0.3	72	PASS
198	198	100	100	100.0	24181	PASS
199	198	5	9	7.1	1710	PASS
275	198	10	60	25.2	6082	PASS
365	198	1	100	4.0	963	PASS
441	442	0.01	24	16.4	3431	PASS
442	198	50	100	86.5	20916	PASS
443	442	15	24	18.8	3924	PASS