


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE092118\
 Data File : BE097608.D
 Acq On : 21 Sep 2018 12:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 20 10:54:43 2018

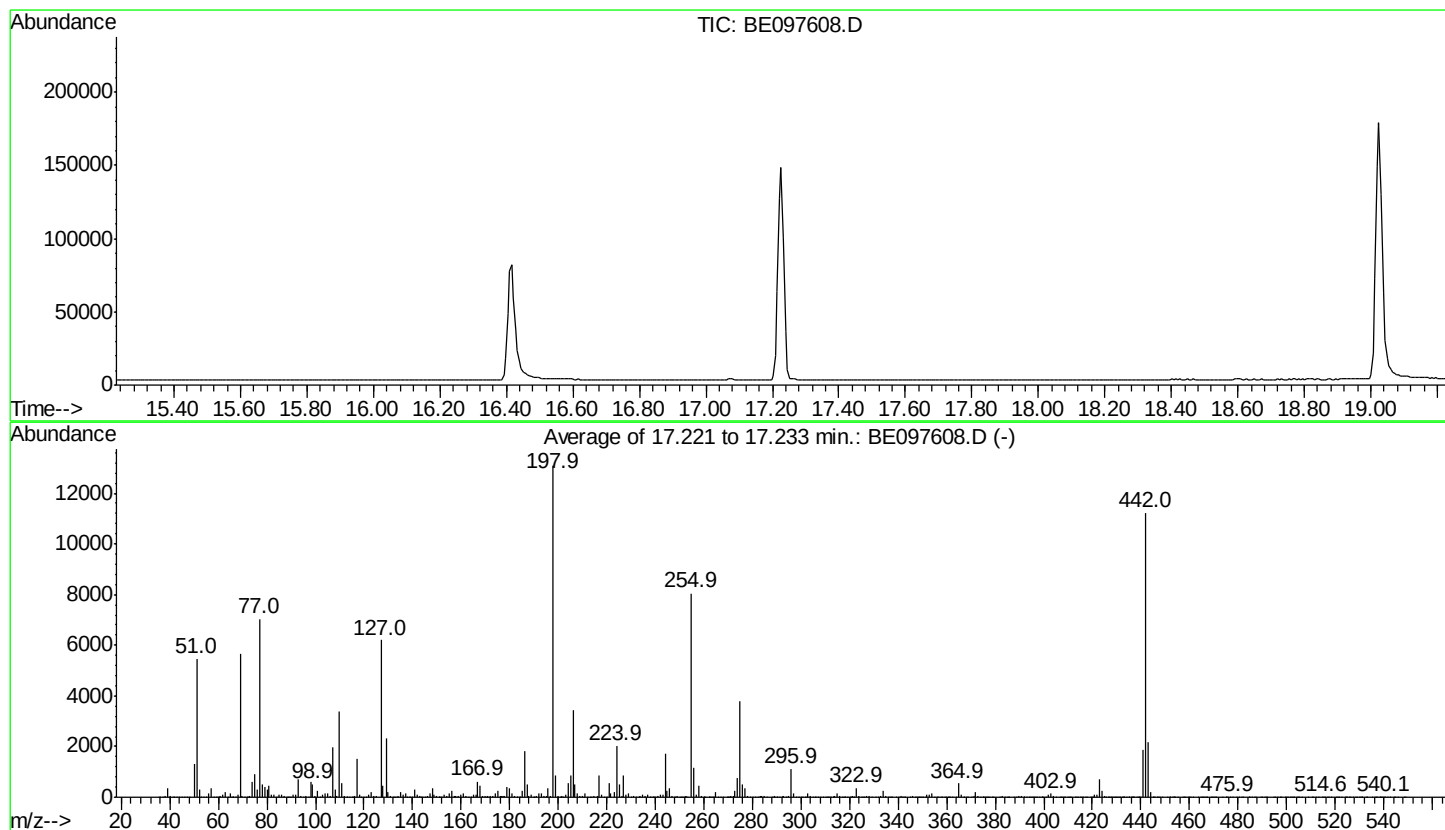

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	5458	PASS
68	69	0.00	2	2.0	115	PASS
69	198	0.00	100	43.3	5673	PASS
70	69	0.00	2	0.5	28	PASS
127	198	10	80	47.3	6195	PASS
197	198	0.00	2	0.4	54	PASS
198	198	100	100	100.0	13090	PASS
199	198	5	9	6.6	865	PASS
275	198	10	60	29.1	3803	PASS
365	198	1	100	4.1	538	PASS
441	198	0.01	100	14.3	1867	PASS
442	198	50	100	85.8	11233	PASS
443	442	15	24	19.2	2160	PASS