


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE092118\
Data File : BE097627.D
Acq On : 22 Sep 2018 1:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 20 10:54:43 2018

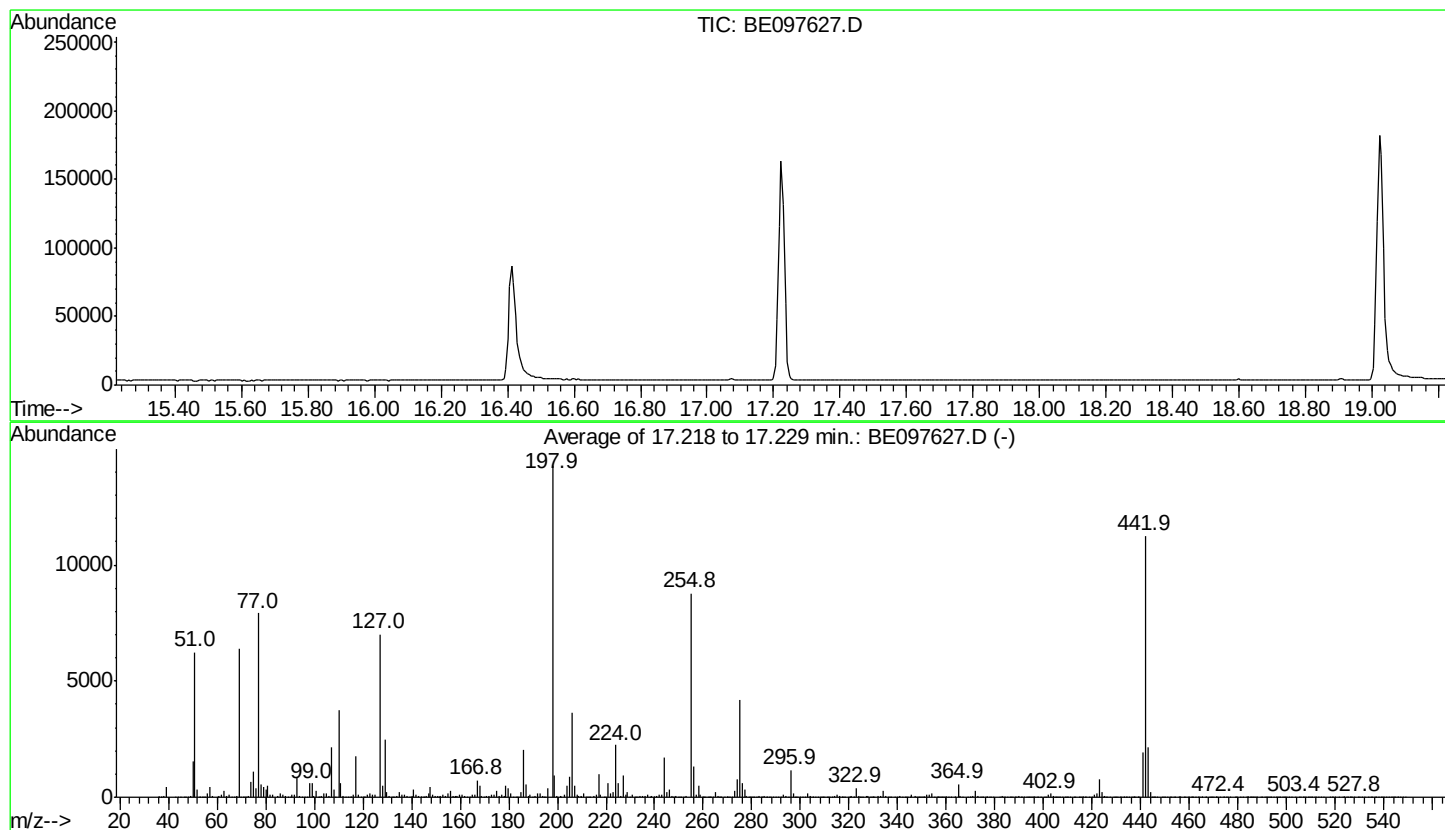

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	6230	PASS
68	69	0.00	2	0.9	56	PASS
69	198	0.00	100	44.8	6391	PASS
70	69	0.00	2	0.5	29	PASS
127	198	10	80	49.1	7003	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14272	PASS
199	198	5	9	6.6	939	PASS
275	198	10	60	29.5	4206	PASS
365	198	1	100	3.9	558	PASS
441	198	0.01	100	13.5	1923	PASS
442	198	50	100	78.9	11259	PASS
443	442	15	24	19.3	2174	PASS