

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092216\
 Data File : BE092398.D
 Acq On : 22 Sep 2016 16:38
 Operator : UM/SJ
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.2

Manual Integrations
 APPROVED

sohil
 9/23/2016 6:48:07 PM

Quant Time: Sep 22 18:06:10 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 16:57:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	8327	5.00	ng	0.00
7) Naphthalene-d8	10.95	136	42474	5.00	ng	0.00
12) Acenaphthene-d10	14.82	164	34287	5.00	ng	0.00
18) Phenanthrene-d10	17.58	188	72123	5.00	ng	0.00
24) Chrysene-d12	21.75	240	88671	5.00	ng	0.00
31) Perylene-d12	24.12	264	81179	5.00	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.69	112	271	0.14	ng	0.00
5) Phenol-d6	7.38	99	305	0.12	ng	0.02
8) Nitrobenzene-d5	9.39	82	412m	0.14	ng	0.02
13) 2,4,6-Tribromophenol	16.33	330	140	0.13	ng	0.00
14) 2-Fluorobiphenyl	13.46	172	1497	0.14	ng	0.01
26) Terphenyl-d14	20.19	244	2134	0.16	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.41	88	224	0.19	ng	99
3) n-Nitrosodimethylamine	3.80	42	128	0.12	ng	# 2
6) bis(2-Chloroethyl)ether	7.61	93	220	0.10	ng	# 83
9) Naphthalene	11.01	128	1837	0.19	ng	# 92
10) Hexachlorobutadiene	11.30	225	304	0.20	ng	100
11) 2-Methylnaphthalene	12.66	142	1161	0.19	ng	97
15) Acenaphthylene	14.54	152	9284	0.16	ng	100
16) Acenaphthene	14.88	154	1617	0.17	ng	95
17) Fluorene	15.88	166	1863	0.16	ng	99
19) Hexachlorobenzene	16.89	284	558	0.16	ng	95
20) Pentachlorophenol	17.28	266	100	0.13	ng	86
21) Phenanthrene	17.63	178	3226	0.16	ng	# 75
22) Anthracene	17.72	178	2919	0.16	ng	99
23) Fluoranthene	19.63	202	14204	0.16	ng	99
25) Pyrene	19.99	202	14976	0.17	ng	99
27) Benzo(a)anthracene	21.72	228	16394m	0.17	ng	
28) Chrysene	21.79	228	16218m	0.16	ng	
29) Bis(2-ethylhexyl)phthalate	21.66	149	1335	0.10	ng	# 73
30) Indeno(1,2,3-cd)pyrene	26.63	276	16152	0.16	ng	99
32) Benzo(b)fluoranthene	23.39	252	3708	0.18	ng	94
33) Benzo(k)fluoranthene	23.44	252	3888	0.18	ng	97
34) Benzo(a)pyrene	24.01	252	3597	0.18	ng	# 94
35) Dibenzo(a,h)anthracene	26.67	278	3181	0.17	ng	# 89
36) Benzo(g,h,i)perylene	27.42	276	14434	0.18	ng	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092216\
Data File : BE092398.D
Acq On : 22 Sep 2016 16:38
Operator : UM/SJ
Sample : SSTDIC0.2
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleID :
SSTDIC0.2

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM

Quant Time: Sep 22 18:06:10 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 16:57:02 2016
Response via : Initial Calibration

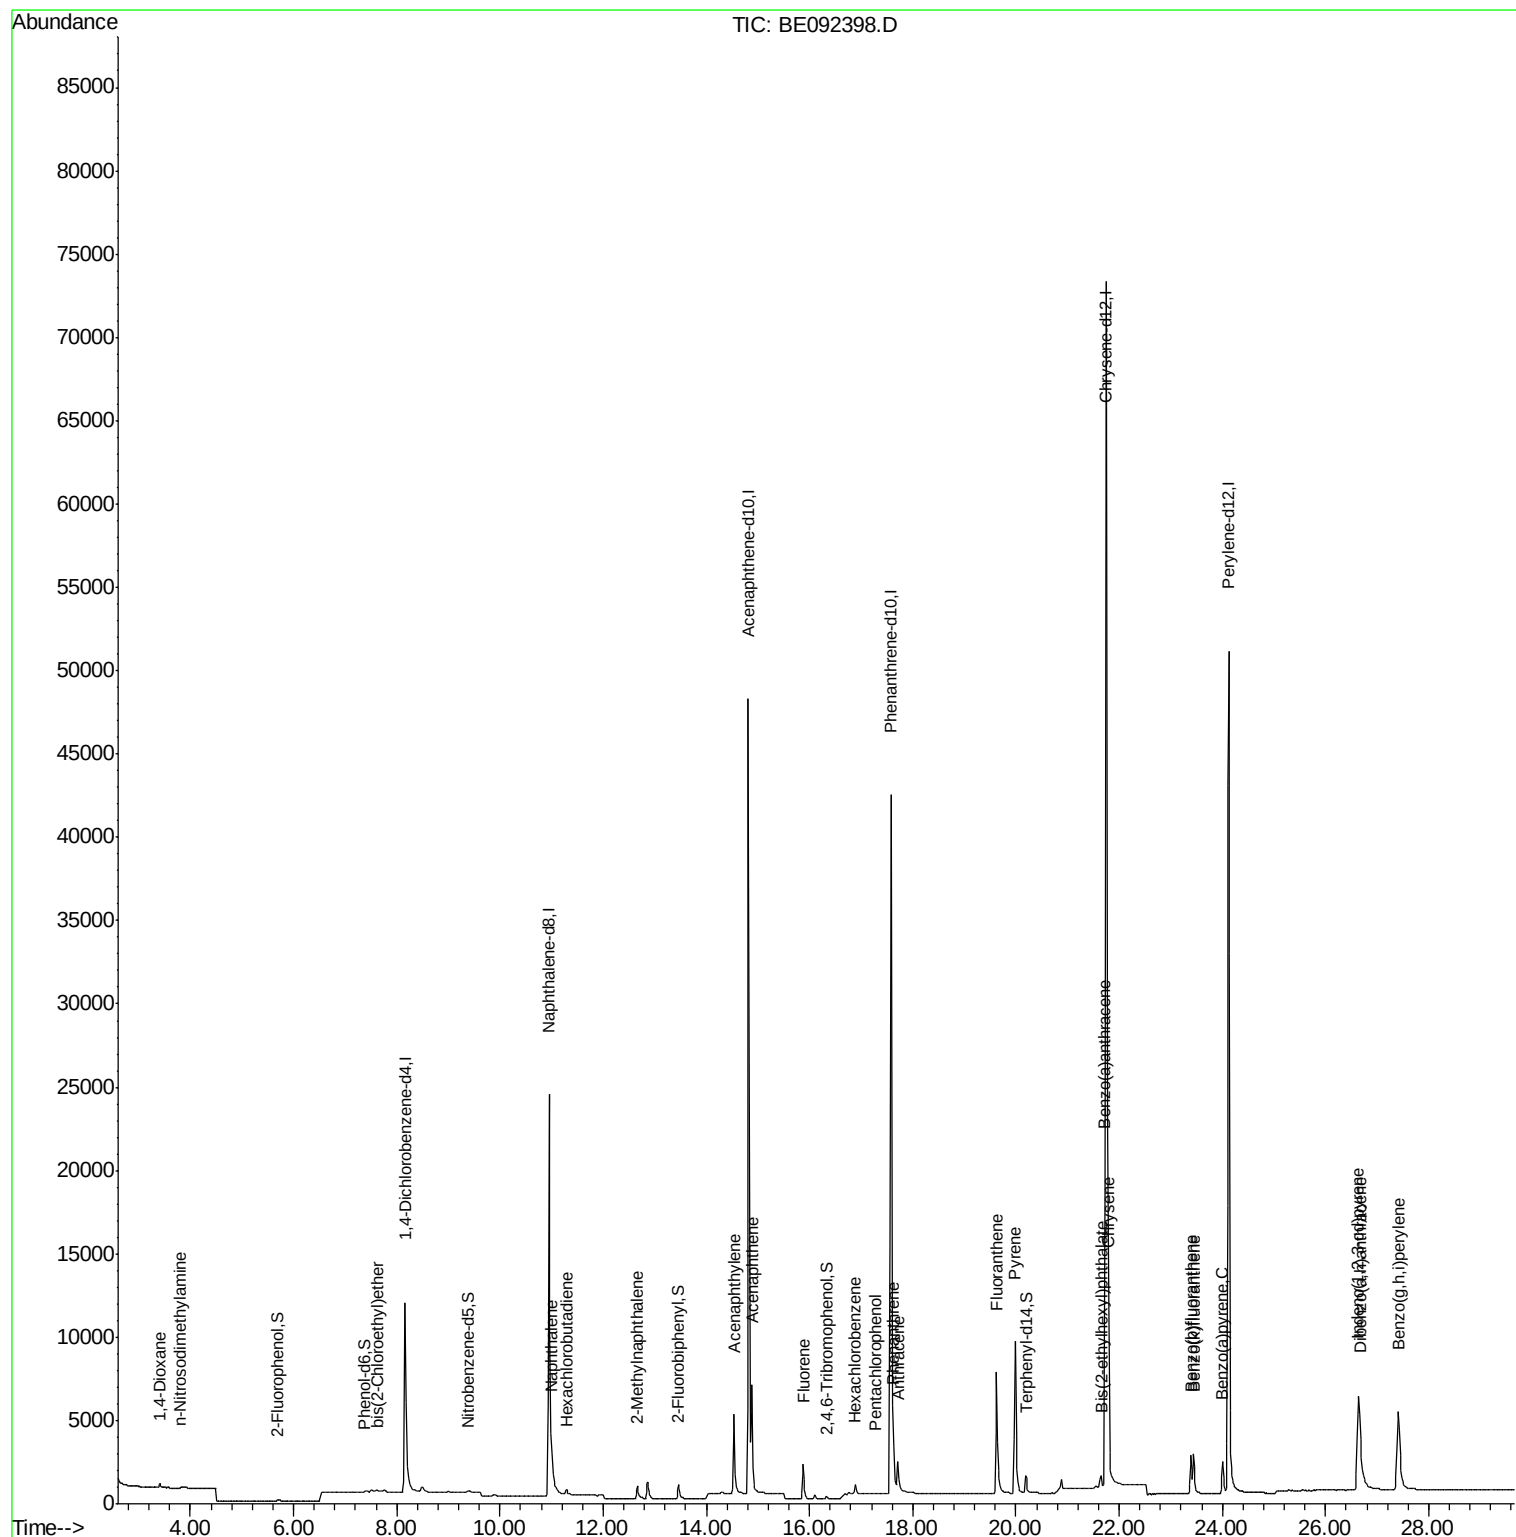

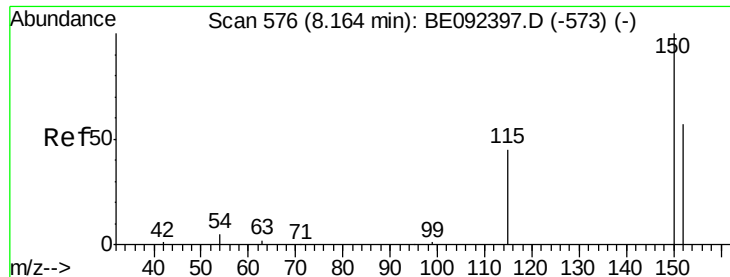

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.16 min Scan# 576

Delta R.T. 0.00 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Instrument :

BNA_E

ClientSampled :

SSTDIC0.2

Tgt Ion: 152 Resp: 8327
Ion Ratio Lower Upper

152 100


150 176.3 106.0 159.0#

115 81.2 31.2 46.8#




Manual Integrations
APPROVED

sohil

9/23/2016 6:48:07 PM

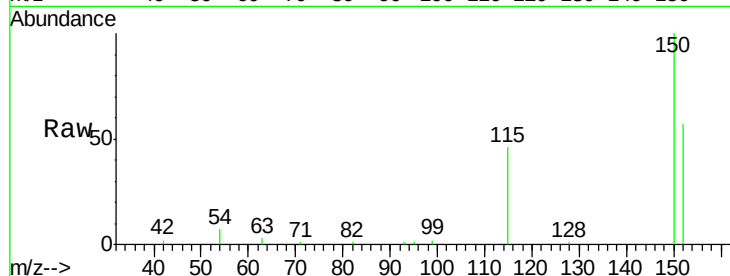

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

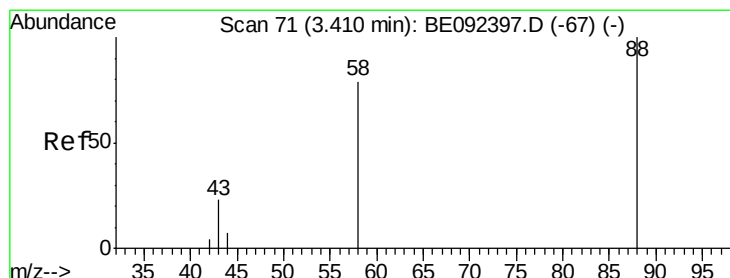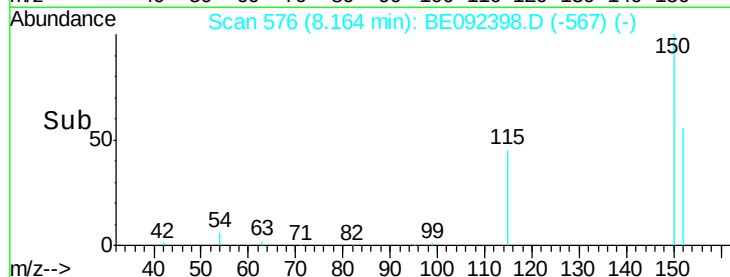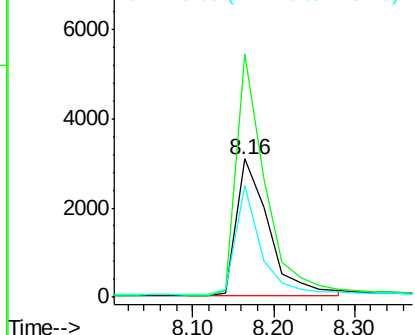

#2

1,4-Dioxane

Concen: 0.19 ng

RT: 3.41 min Scan# 71

Delta R.T. -0.00 min

Lab File: BE092398.D


Acq: 22 Sep 2016 16:38

Tgt Ion: 88 Resp: 224
Ion Ratio Lower Upper



88 100




58 78.1 63.6 95.4

43 35.7 28.0 42.0

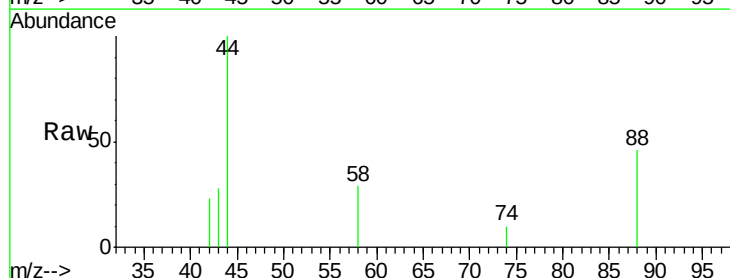

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

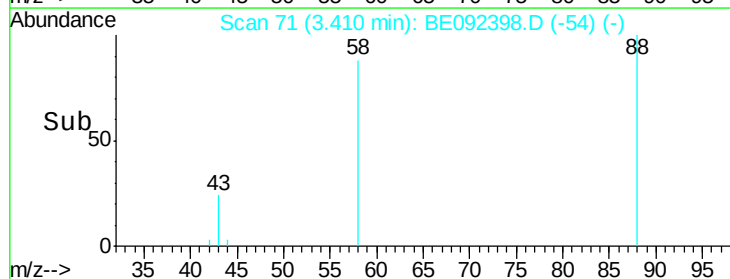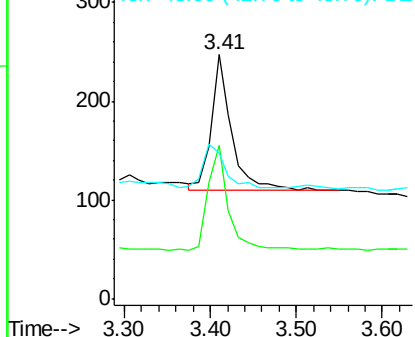



#3

n-Nitrosodimethylamine

Concen: 0.12 ng

RT: 3.80 min Scan# 105

Delta R.T. 0.01 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Tgt Ion:	42	Resp:	128
Ion	Ratio	Lower	Upper
42	100		
74	0.0	86.0	129.0#
44	0.0	5.1	7.7#

Instrument :





BNA_E

ClientSampleId :

SSTDIC0.2

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM

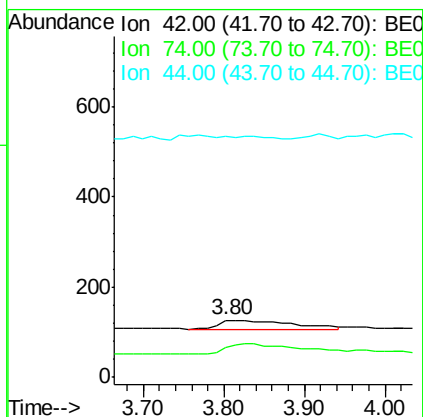

#4

2-Fluorophenol

Concen: 0.14 ng


RT: 5.69 min Scan# 367


Delta R.T. 0.01 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Tgt Ion:	112	Resp:	271
Ion	Ratio	Lower	Upper
112	100		
64	67.2	53.5	80.3
63	29.2	27.9	41.9

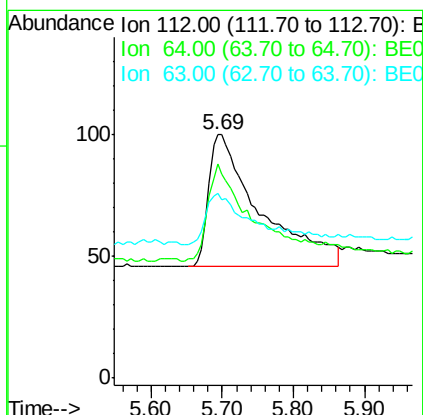

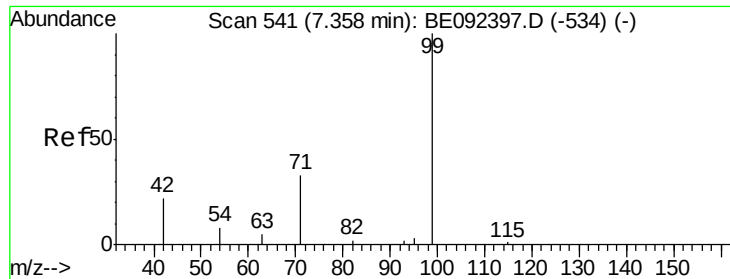

#5

Phenol-d6

Concen: 0.12 ng

RT: 7.38 min Scan# 542

Delta R.T. 0.02 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Instrument :

BNA_E

ClientSampled :





SSTDICC0.2

Tgt Ion: 99 Resp: 305

Ion	Ratio	Lower	Upper
99	100		
42	25.2	16.0	24.0#
71	34.4	30.6	45.8

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM

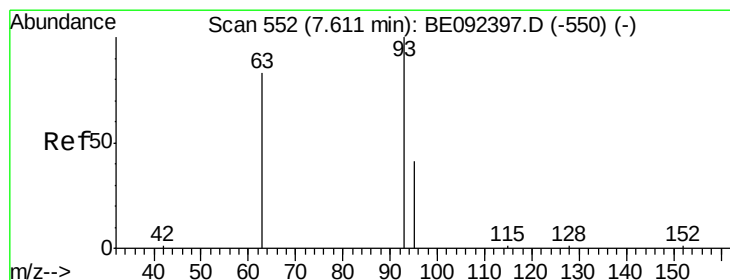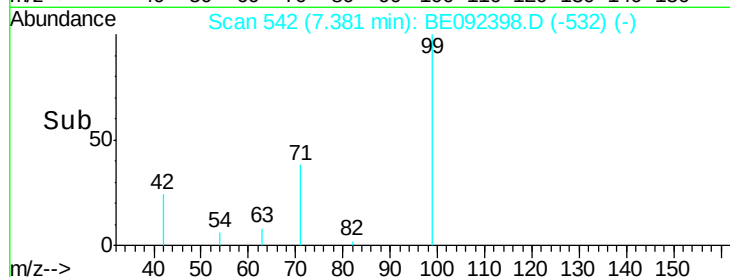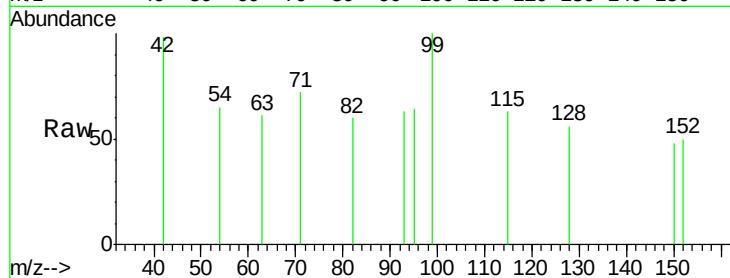

#6

bis(2-Chloroethyl)ether

Concen: 0.10 ng

RT: 7.61 min Scan# 552




Delta R.T. 0.00 min


Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Tgt Ion: 93 Resp: 220

Ion	Ratio	Lower	Upper
93	100		
63	104.1	71.6	107.4
95	42.3	24.0	36.0#

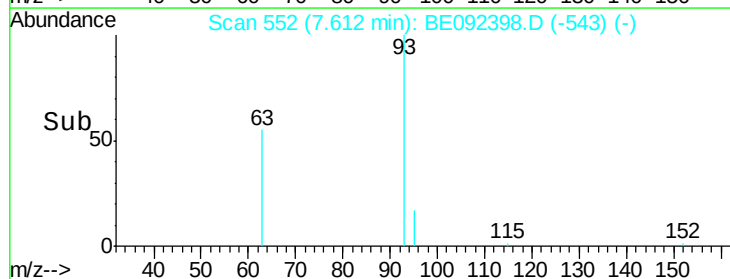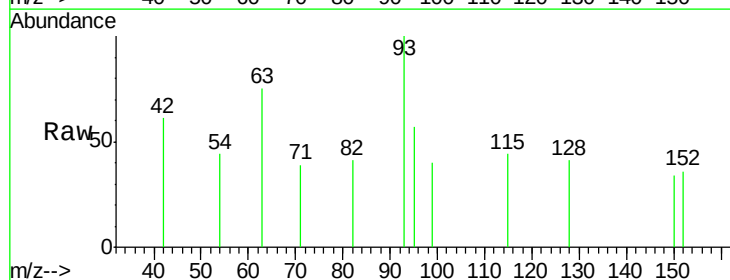



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.95 min Scan# 708

Delta R.T. -0.00 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Instrument :

BNA_E





ClientSampleId :

SSTDICC0.2

Tgt Ion	Ratio	Resp	Lower	Upper
136	100	42474		
137	10.8	8.2	12.4	
54	8.7	9.6	14.4	
68	6.5	6.7	10.1	

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM

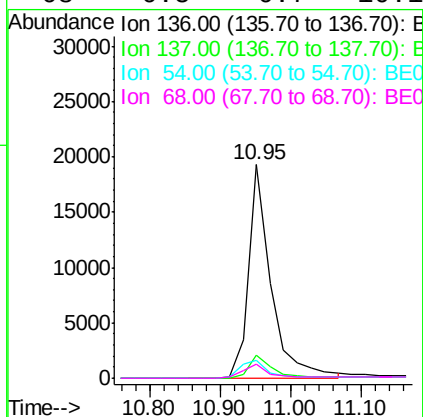

#8

Nitrobenzene-d5

Concen: 0.14 ng m




RT: 9.39 min Scan# 629


Delta R.T. 0.02 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Resp	Lower	Upper
82	100	412		
128	64.7	39.0	58.4	
54	75.6	44.8	67.2	

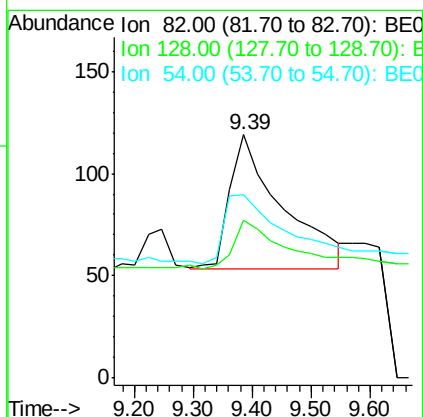



#9

Naphthalene

Concen: 0.19 ng

RT: 11.01 min Scan# 711

Delta R.T. -0.00 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Instrument :

BNA_E





ClientSampleId :

SSTDIC0.2

Tgt Ion:	128	Resp:	1837
Ion Ratio	Lower	Upper	
128	100		
129	17.9	11.2	16.8#
127	17.6	11.6	17.4#

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM

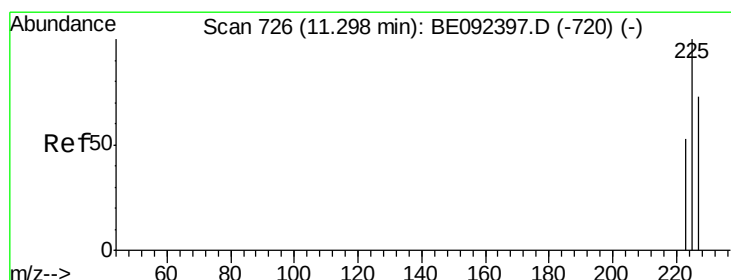

#10

Hexachlorobutadiene

Concen: 0.20 ng




RT: 11.30 min Scan# 726


Delta R.T. -0.00 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Tgt Ion:	225	Resp:	304
Ion Ratio	Lower	Upper	
225	100		
223	62.8	50.6	76.0
227	64.1	51.4	77.0



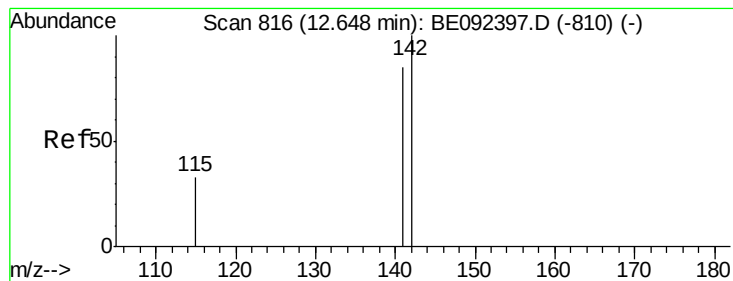

#11

2-Methylnaphthalene

Concen: 0.19 ng

RT: 12.66 min Scan# 817

Delta R.T. 0.01 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Instrument :

BNA_E





ClientSampleId :

SSTDICC0.2

Tgt Ion:	142	Resp:	1161
Ion Ratio	Lower	Upper	
142	100		
141	89.5	73.7	110.5
115	44.8	34.0	51.0

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM

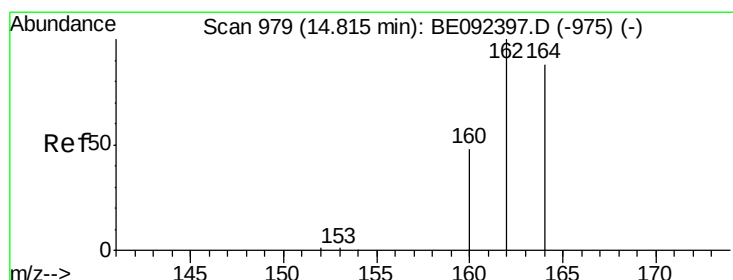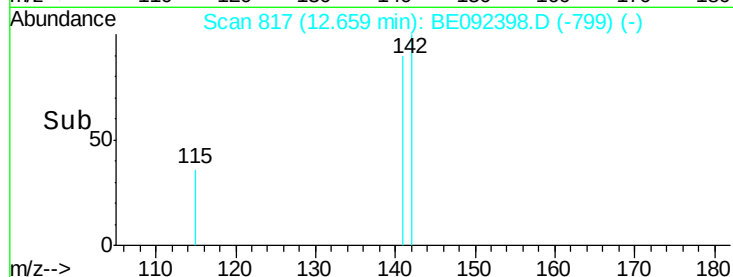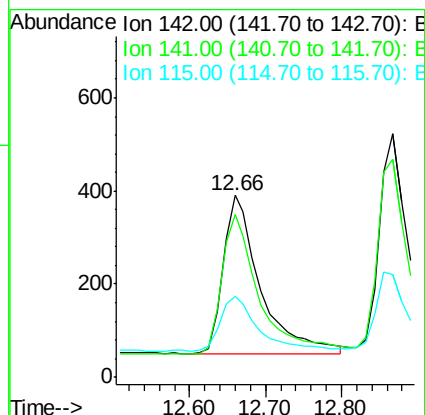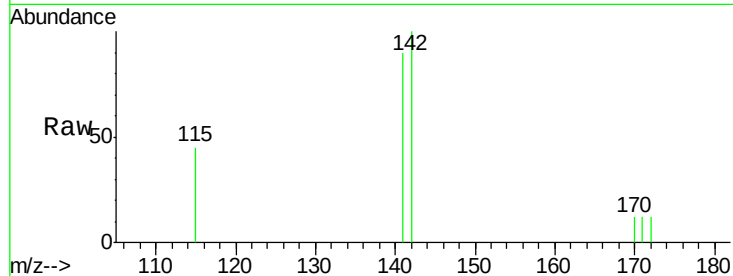

#12

Acenaphthene-d10

Concen: 5.00 ng




RT: 14.82 min Scan# 980


Delta R.T. 0.00 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38


Tgt Ion:	164	Resp:	34287
Ion Ratio	Lower	Upper	
164	100		
162	112.3	71.4	107.0#
160	53.0	27.4	41.2#

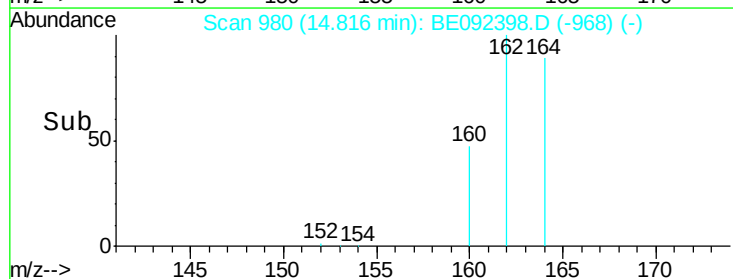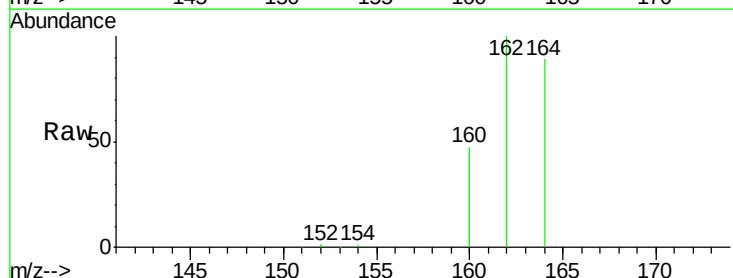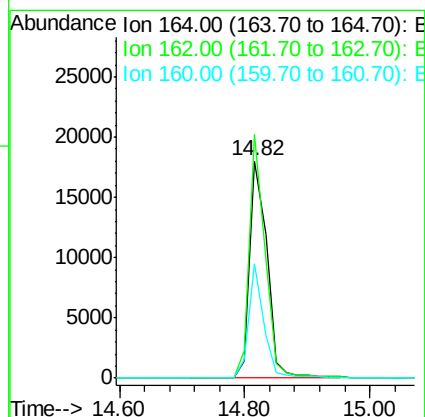

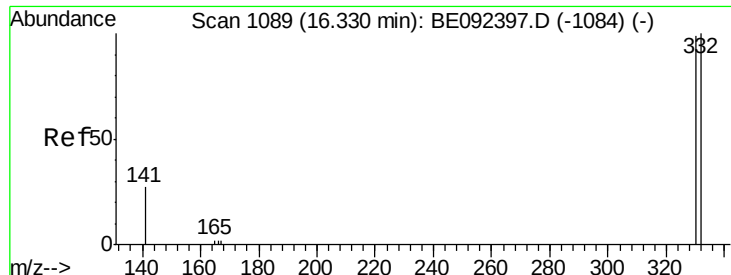

#13
 2,4,6-Tribromophenol
 Concen: 0.13 ng
 RT: 16.33 min Scan# 1090
 Delta R.T. -0.00 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.2






Tgt Ion: 330 Resp: 140

Ion	Ratio	Lower	Upper
330	100		
332	107.9	75.4	113.0
141	45.0	31.0	46.6

Manual Integrations
 APPROVED




sohil
 9/23/2016 6:48:07 PM

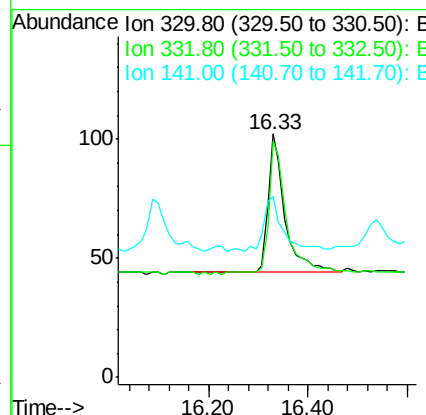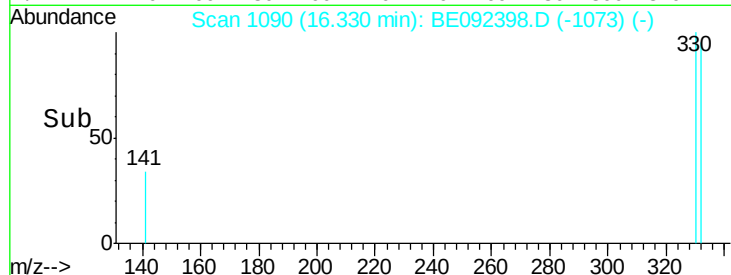


#14
 2-Fluorobiphenyl
 Concen: 0.14 ng
 RT: 13.46 min Scan# 886
 Delta R.T. 0.01 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Tgt Ion: 172 Resp: 1497

Ion	Ratio	Lower	Upper
172	100		
171	39.3	30.1	45.1
170	29.7	21.8	32.6

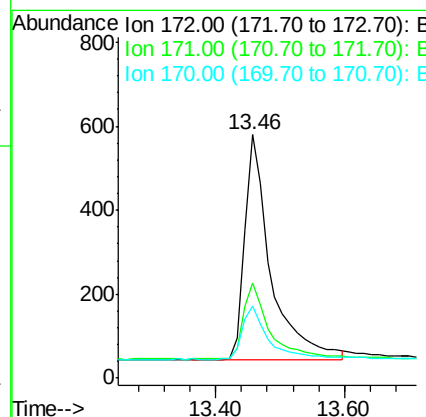







#15
Acenaphthylene
Concen: 0.16 ng
RT: 14.54 min Scan# 964
Delta R.T. 0.00 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Instrument :
BNA_E
ClientSampleId :
SSTDIC0.2

Tgt Ion	Ratio	Lower	Upper
152	100		
151	5.0	3.9	5.9
153	12.8	10.4	15.6




Manual Integrations
APPROVED


sohil
9/23/2016 6:48:07 PM

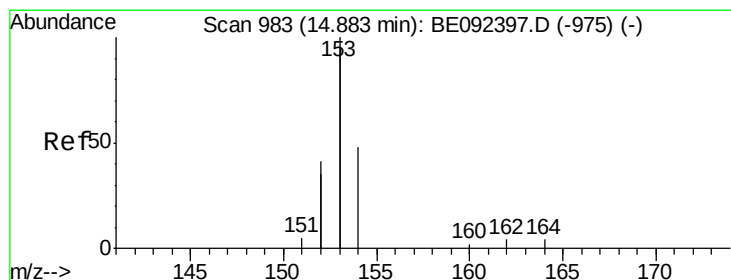

#16
Acenaphthene
Concen: 0.17 ng
RT: 14.88 min Scan# 984
Delta R.T. 0.00 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Lower	Upper
154	100		
153	421.7	350.8	526.2
152	210.6	171.1	256.7









#17
Fluorene
 Concen: 0.16 ng
 RT: 15.88 min Scan# 1051
 Delta R.T. 0.01 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
166	100		
165	98.4	78.2	117.4
167	14.3	11.0	16.4




Manual Integrations
 APPROVED


sohil
 9/23/2016 6:48:07 PM

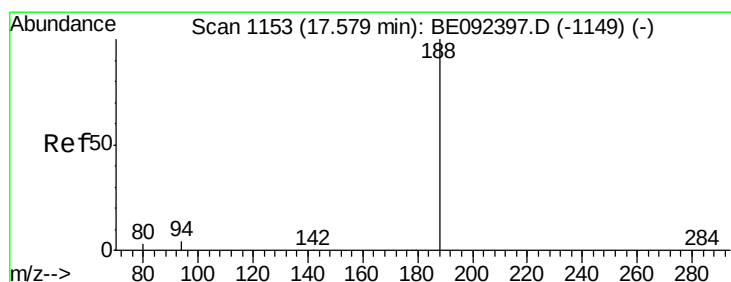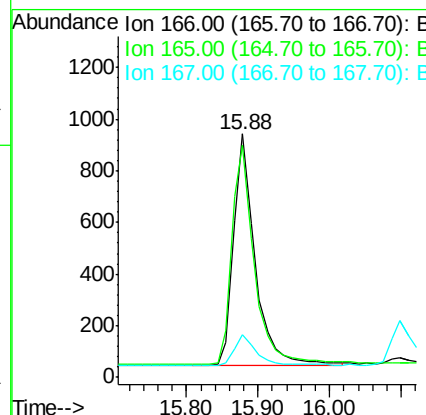

#18
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.58 min Scan# 1154
 Delta R.T. -0.00 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Lower	Upper
188	100		
94	4.4	3.2	4.8
80	3.9	2.6	3.8

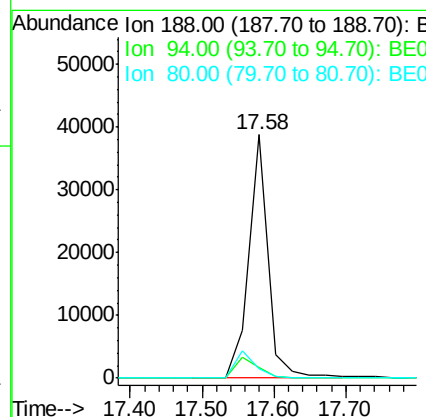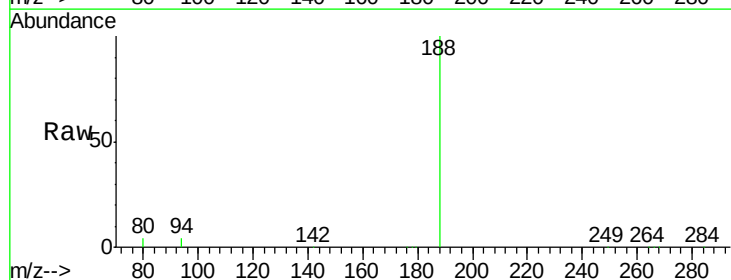







#19
Hexachlorobenzene
Concen: 0.16 ng
RT: 16.89 min Scan# 1124
Delta R.T. -0.00 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Instrument :
BNA_E
ClientSampled :
SSTDIC0.2

Tgt Ion	Ratio	Resp	Lower	Upper
284	100	558		
142	40.0		29.1	43.7
249	36.9		27.9	41.9




Manual Integrations
APPROVED


sohil
9/23/2016 6:48:07 PM

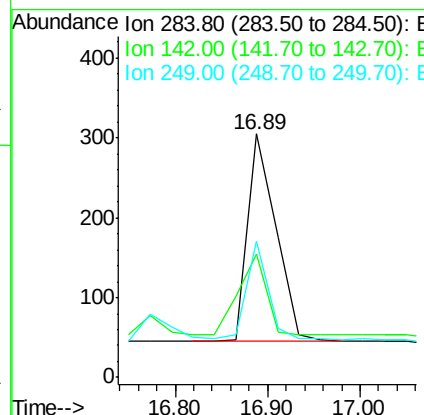

#20
Pentachlorophenol
Concen: 0.13 ng
RT: 17.28 min Scan# 1141
Delta R.T. 0.02 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Resp	Lower	Upper
266	100	100		
268	88.2		62.5	93.7
264	85.3		57.2	85.8

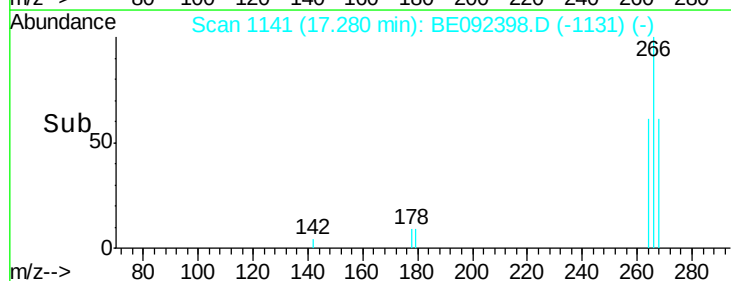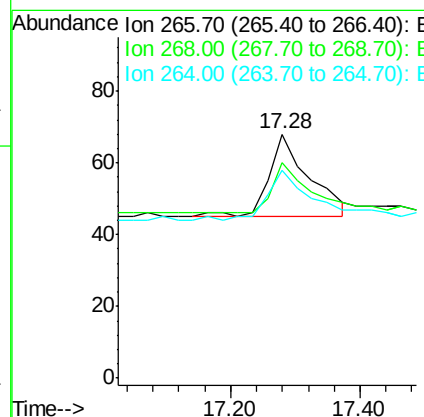







#21
Phenanthrene
Concen: 0.16 ng
RT: 17.63 min Scan# 1156
Delta R.T. 0.02 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Instrument :
BNA_E
ClientSampleId :
SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
178	100		
176	0.0	15.8	23.8#
179	16.9	16.0	24.0




Manual Integrations
APPROVED


sohil
9/23/2016 6:48:07 PM

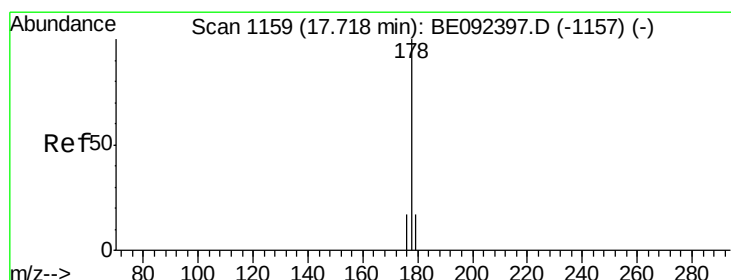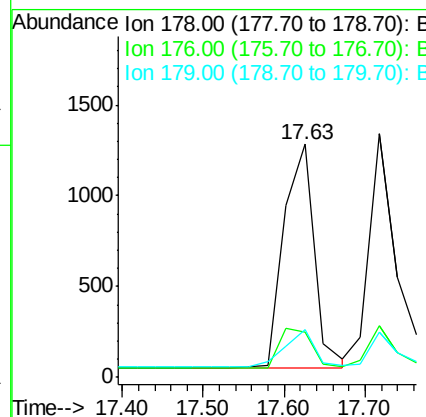

#22
Anthracene
Concen: 0.16 ng
RT: 17.72 min Scan# 1160
Delta R.T. -0.00 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.6	15.0	22.4
179	14.6	12.2	18.2

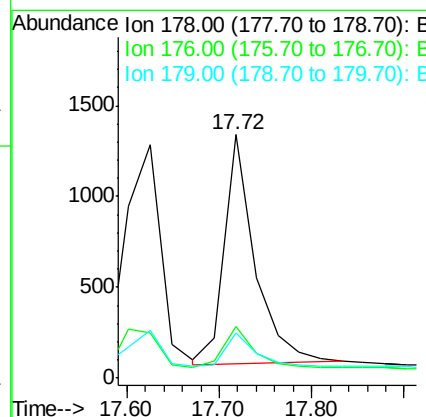



#23

Fluoranthene

Concen: 0.16 ng

RT: 19.63 min Scan# 1267

Delta R.T. 0.02 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Instrument :

BNA_E


ClientSampled :

SSTDIC0.2


Tgt Ion:	202	Resp:	14204
Ion Ratio	Lower	Upper	
202	100		
101	2.9	2.2	3.4
203	17.7	13.7	20.5

Manual Integrations
APPROVED



sohil
9/23/2016 6:48:07 PM



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

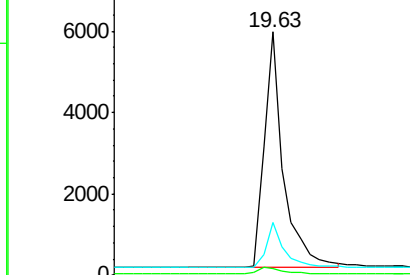

Time-->

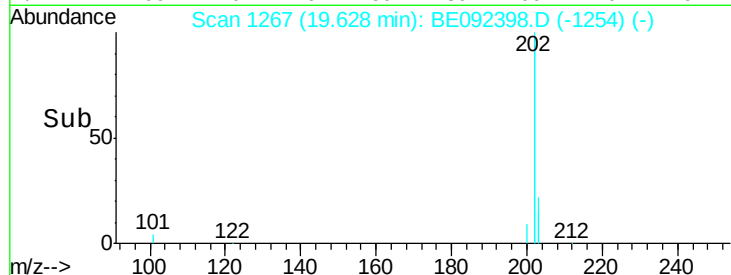

#24

Chrysene-d12

Concen: 5.00 ng


RT: 21.75 min Scan# 1375

Delta R.T. -0.00 min


Lab File: BE092398.D

Acq: 22 Sep 2016 16:38


Tgt Ion:	240	Resp:	88671
Ion Ratio	Lower	Upper	
240	100		
120	4.2	2.6	4.0#
236	30.0	24.6	37.0




Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

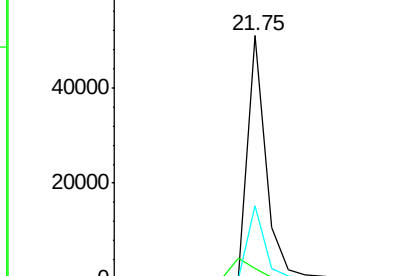

Time-->









#25
 Pyrene
 Concen: 0.17 ng
 RT: 19.99 min Scan# 1288
 Delta R.T. 0.00 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
202	100		
200	5.3	4.2	6.4
203	17.9	13.9	20.9




Manual Integrations
 APPROVED


sohil
 9/23/2016 6:48:07 PM

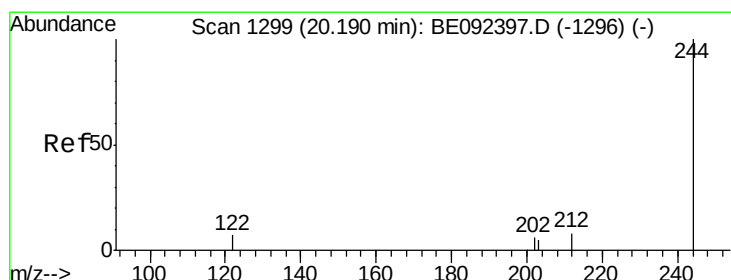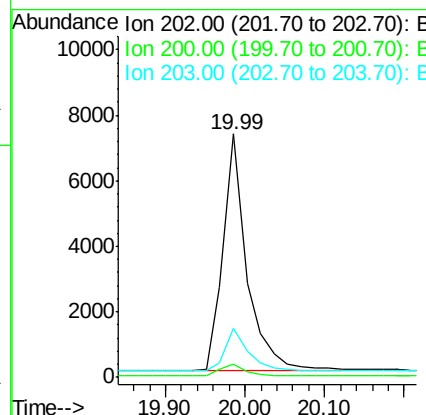

#26
 Terphenyl-d14
 Concen: 0.16 ng
 RT: 20.19 min Scan# 1300
 Delta R.T. 0.00 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Lower	Upper
244	100		
212	13.5	6.7	10.1#
122	19.0	3.6	5.4#

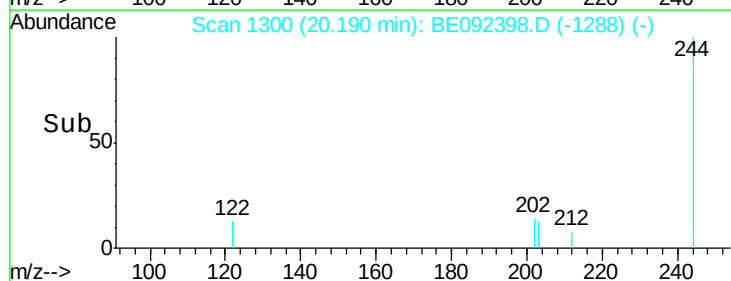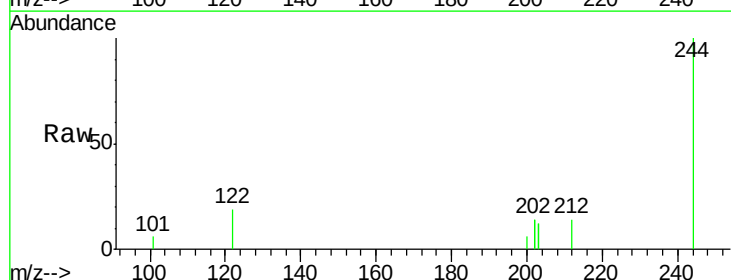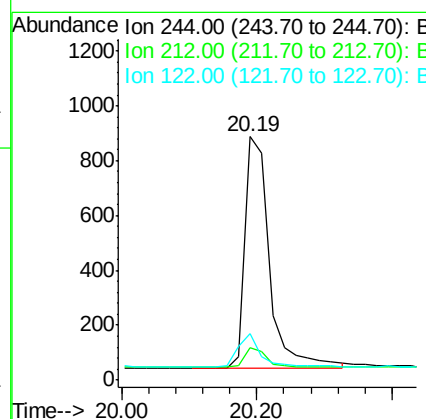







#27
Benzo(a)anthracene
Concen: 0.17 ng m
RT: 21.72 min Scan# 1374
Delta R.T. -0.00 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Instrument :
BNA_E
ClientSampleId :
SSTDICC0.2

Tgt Ion:228 Resp: 16394
Ion Ratio Lower Upper
228 100
226 31.2 23.6 35.4
229 16.4 13.3 19.9




Manual Integrations
APPROVED


sohil
9/23/2016 6:48:07 PM

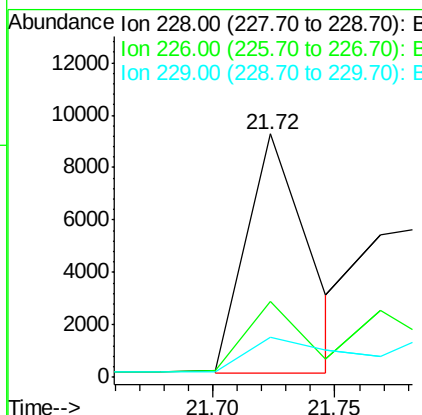

#28
Chrysene
Concen: 0.16 ng m
RT: 21.79 min Scan# 1377
Delta R.T. 0.02 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38


Tgt Ion:228 Resp: 16218
Ion Ratio Lower Upper
228 100
226 22.7 36.3 54.5#
229 30.0 10.6 16.0#

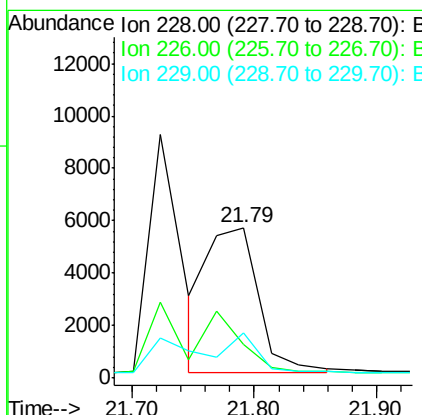



#29
 Bis(2-ethylhexyl)phthalate
 Concen: 0.10 ng
 RT: 21.66 min Scan# 1371
 Delta R.T. 0.02 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC0.2



Tgt Ion: 149 Resp: 1335
 Ion Ratio Lower Upper
 149 100
 167 29.6 16.0 24.0#
 279 4.3 16.0 24.0#




Manual Integrations
 APPROVED


sohil
 9/23/2016 6:48:07 PM

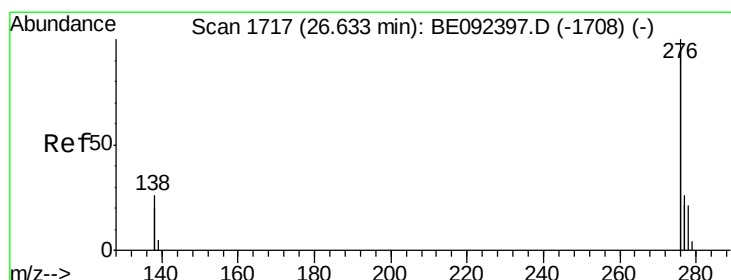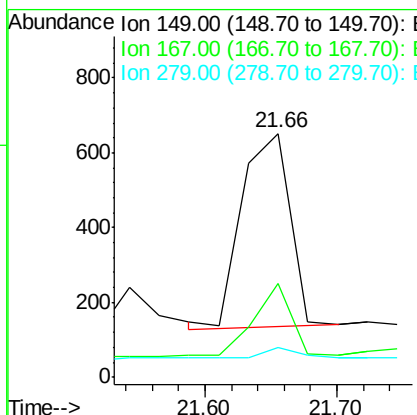

#30
 Indeno(1,2,3-cd)pyrene
 Concen: 0.16 ng
 RT: 26.63 min Scan# 1718
 Delta R.T. -0.00 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Tgt Ion: 276 Resp: 16152
 Ion Ratio Lower Upper
 276 100
 138 25.9 20.3 30.5
 277 24.9 19.7 29.5

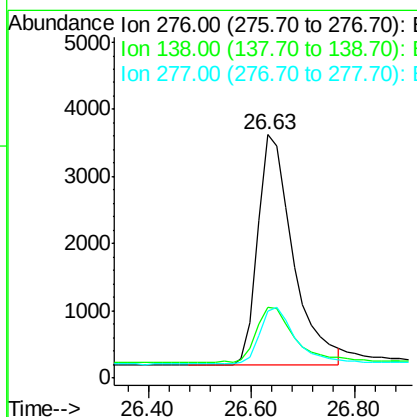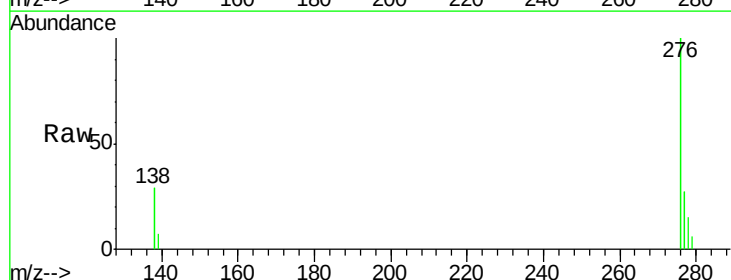

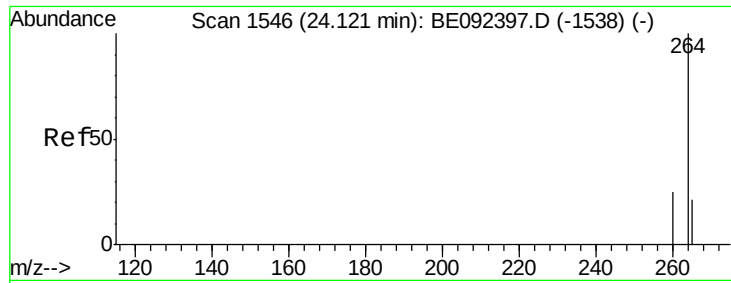





#31
Perylene-d12
 Concen: 5.00 ng
 RT: 24.12 min Scan# 1547
 Delta R.T. 0.00 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.7	20.1	30.1
265	22.3	17.9	26.9




Manual Integrations
 APPROVED


sohil
 9/23/2016 6:48:07 PM

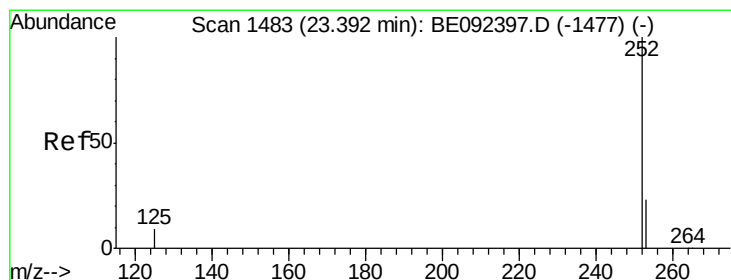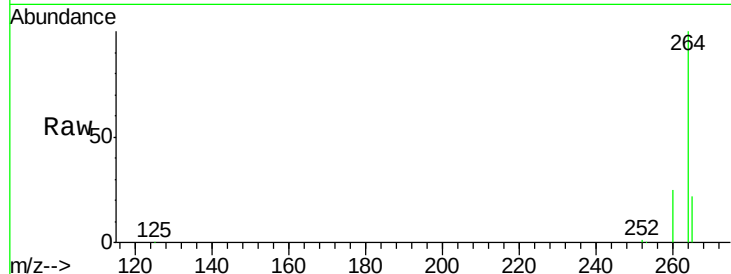

#32
Benzo(b)fluoranthene
 Concen: 0.18 ng
 RT: 23.39 min Scan# 1484
 Delta R.T. 0.00 min
 Lab File: BE092398.D
 Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Lower	Upper
252	100		
253	27.3	18.7	28.1
125	14.2	10.5	15.7





#33

Benzo(k)fluoranthene

Concen: 0.18 ng

RT: 23.44 min Scan# 1488

Delta R.T. 0.00 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Instrument :

BNA_E





ClientSampleId :

SSTDIC0.2

Tgt Ion:	252	Resp:	3888
Ion Ratio	Lower	Upper	
252	100		
253	26.5	20.3	30.5
125	14.2	9.6	14.4

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM



#34

Benzo(a)pyrene

Concen: 0.18 ng




RT: 24.01 min Scan# 1537


Delta R.T. 0.00 min

Lab File: BE092398.D

Acq: 22 Sep 2016 16:38

Tgt Ion:	252	Resp:	3597
Ion Ratio	Lower	Upper	
252	100		
253	26.6	19.0	28.6
125	17.8	11.8	17.8#









#35
Dibenzo(a,h)anthracene
Concen: 0.17 ng
RT: 26.67 min Scan# 1720
Delta R.T. 0.02 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Instrument :
BNA_E
ClientSampleId :
SSTDICC0.2

Tgt Ion	Ratio	Resp	Lower	Upper
278	100	3181		
139	23.7	13.8	20.8	
279	31.1	21.4	32.2	

Manual Integrations
APPROVED

sohil
9/23/2016 6:48:07 PM

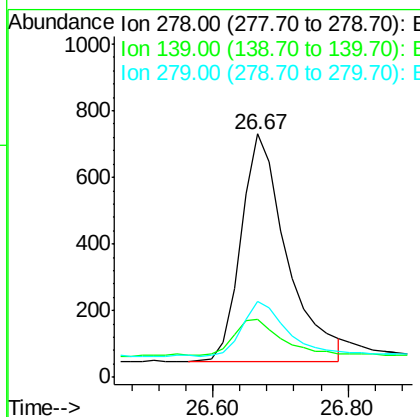

#36
Benzo(g,h,i)perylene
Concen: 0.18 ng
RT: 27.42 min Scan# 1764
Delta R.T. 0.02 min
Lab File: BE092398.D
Acq: 22 Sep 2016 16:38

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	14434		
277	28.1	19.8	29.8	
138	27.1	19.8	29.6	

