


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE092216\  
 Data File : BE092391.D  
 Acq On : 22 Sep 2016 11:24  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE092216.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Sep 22 18:25:56 2016

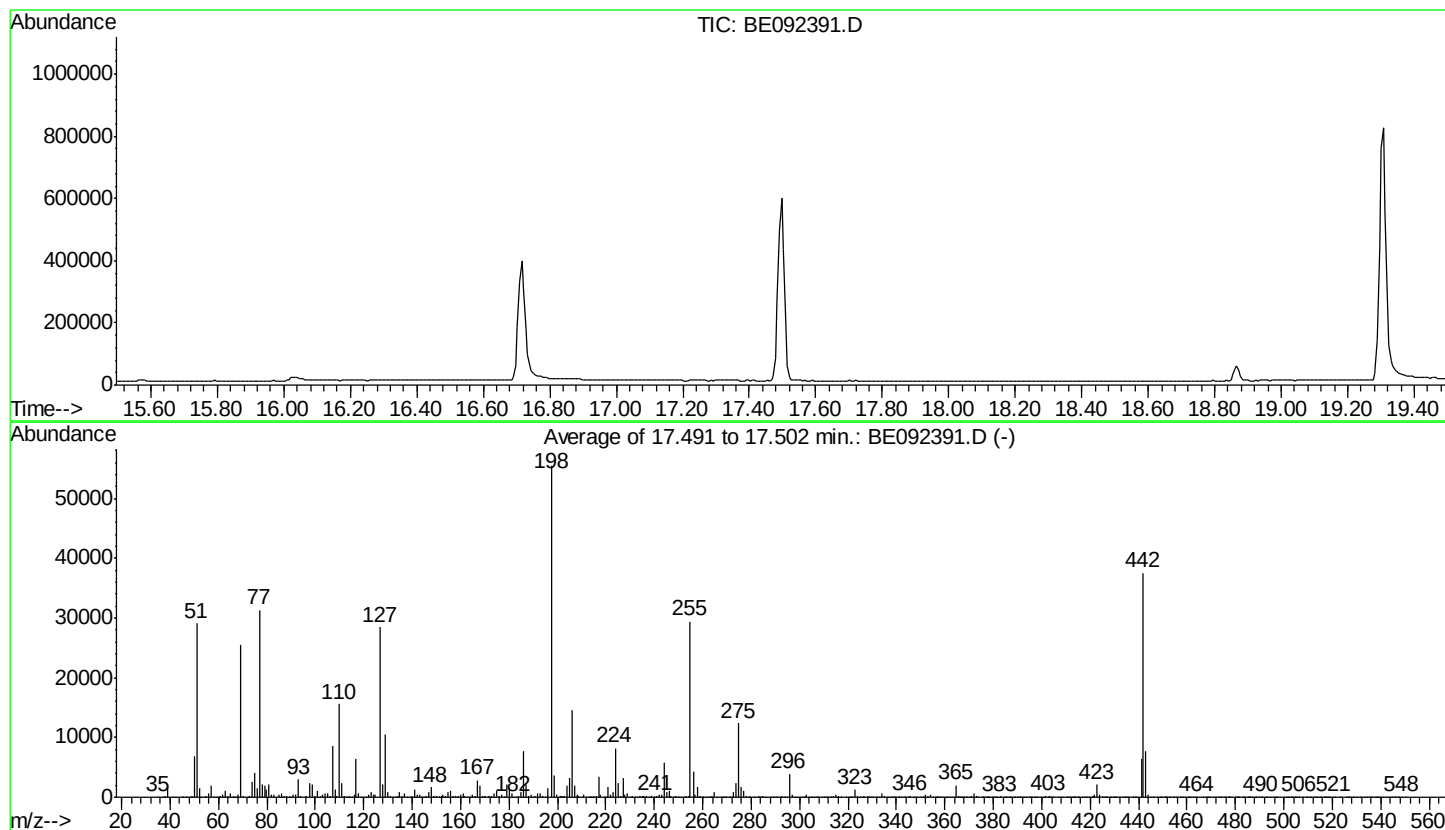

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2526

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 52.5      | 29114   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.9       | 484     | PASS             |
| 69          | 198          | 0.00         | 100          | 46.1      | 25590   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 179     | PASS             |
| 127         | 198          | 10           | 80           | 51.3      | 28467   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 55496   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 3718    | PASS             |
| 275         | 198          | 10           | 60           | 22.3      | 12398   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 2024    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.9      | 6337    | PASS             |
| 442         | 198          | 50           | 100          | 67.7      | 37564   | PASS             |
| 443         | 442          | 15           | 24           | 20.4      | 7667    | PASS             |