


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092315\
 Data File : BE090949.D
 Acq On : 23 Sep 2015 14:47
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 18 18:17:34 2015

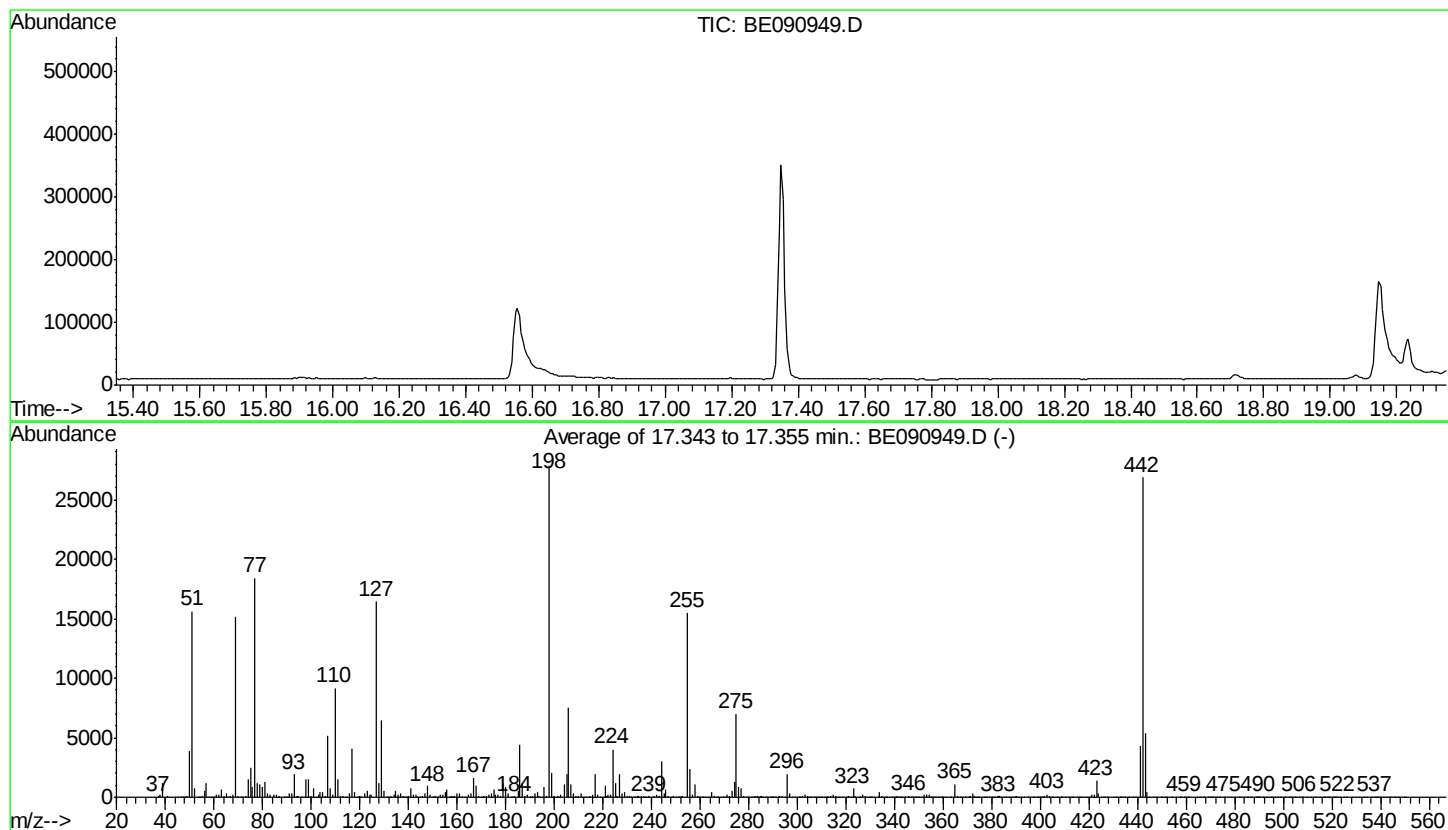

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.1	15625	PASS
68	69	0.00	2	1.6	236	PASS
69	198	0.00	100	54.6	15200	PASS
70	69	0.00	2	0.6	93	PASS
127	198	10	80	59.1	16454	PASS
197	198	0.00	2	0.3	91	PASS
198	198	100	100	100.0	27864	PASS
199	198	5	9	7.3	2028	PASS
275	198	10	60	25.1	6995	PASS
365	198	1	100	4.0	1106	PASS
441	442	0.01	24	16.1	4317	PASS
442	198	50	100	96.4	26871	PASS
443	442	15	24	20.0	5367	PASS