
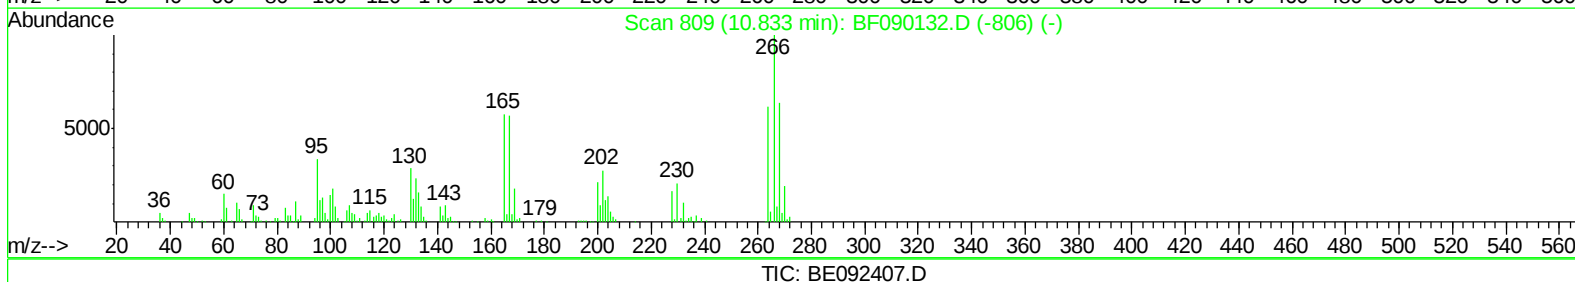
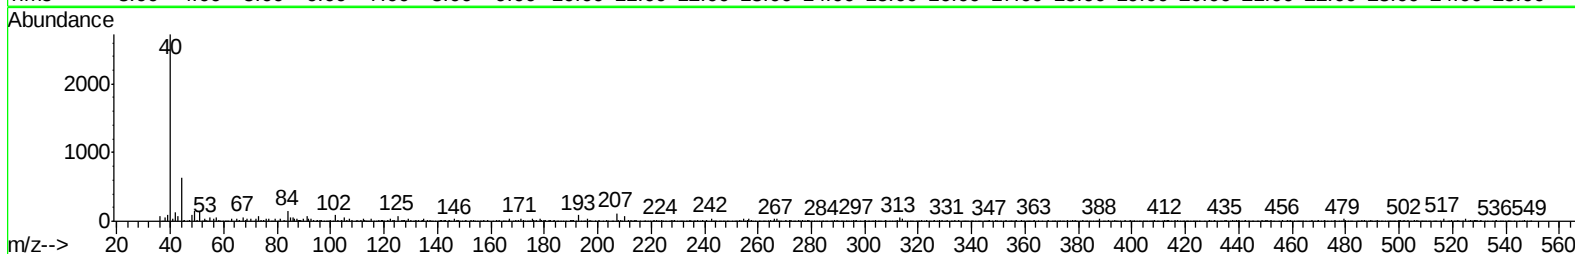


Data Path : Z:\HPCHEM1\BNA_E\Data\BE092316\
Data File : BE092407.D
Acq On : 23 Sep 2016 8:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:54:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

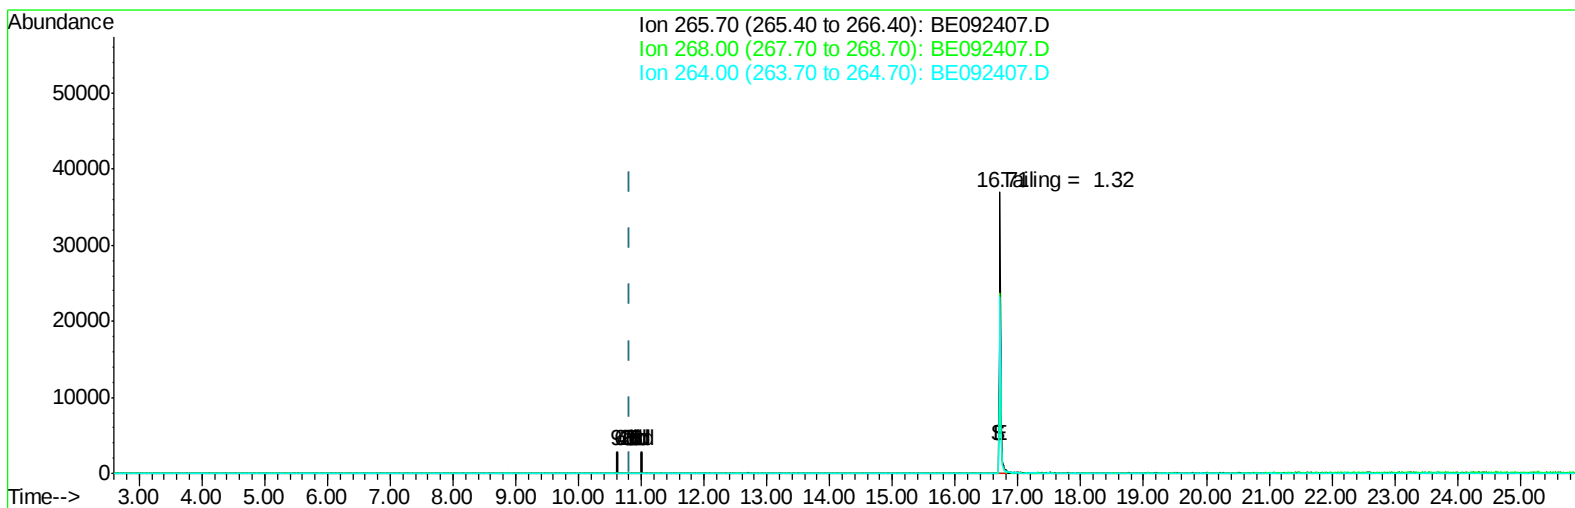

TIC: BE092407.D

(69) Pentachlorophenol (C)




10.874min (+0.040) 320.60ng

response 48

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	34.15#
264.00	62.90	46.34#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE092316\
 Data File : BE092407.D
 Acq On : 23 Sep 2016 8:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:54:01 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 17:58:29 2016
 Response via : Initial Calibration

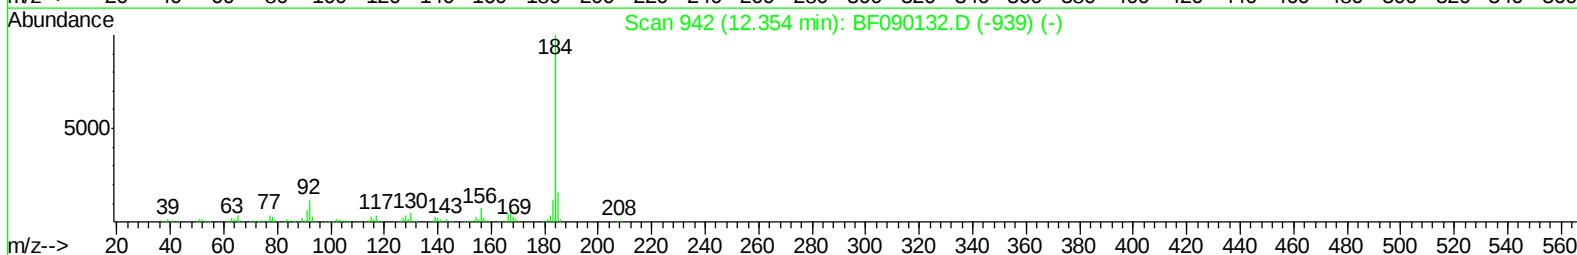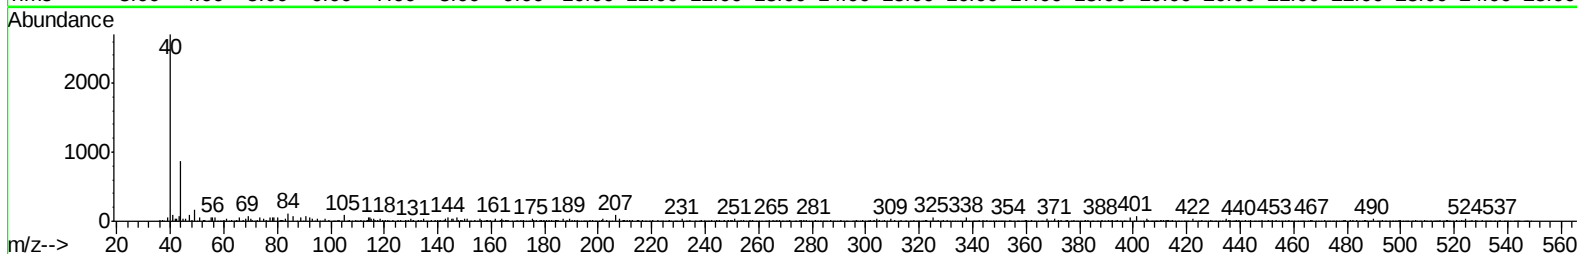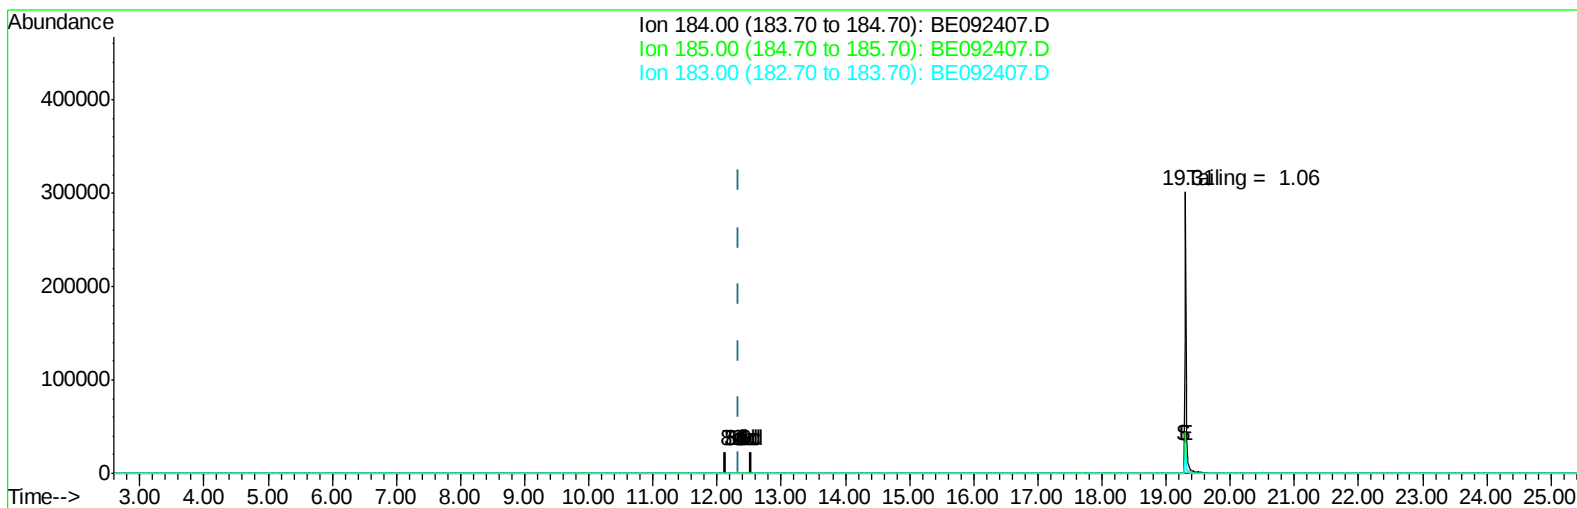

TIC: BE092407.D

(76) Benzidine

12.384min (+0.031) 23.73ng

response 27

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	55.56#
183.00	11.50	74.07#
0.00	0.00	0.00