


Data Path : Z:\HPCHEM1\BNA E\DATA\BE092316\
Data File : BE092407.D
Acq On : 23 Sep 2016 8:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 22 18:25:56 2016

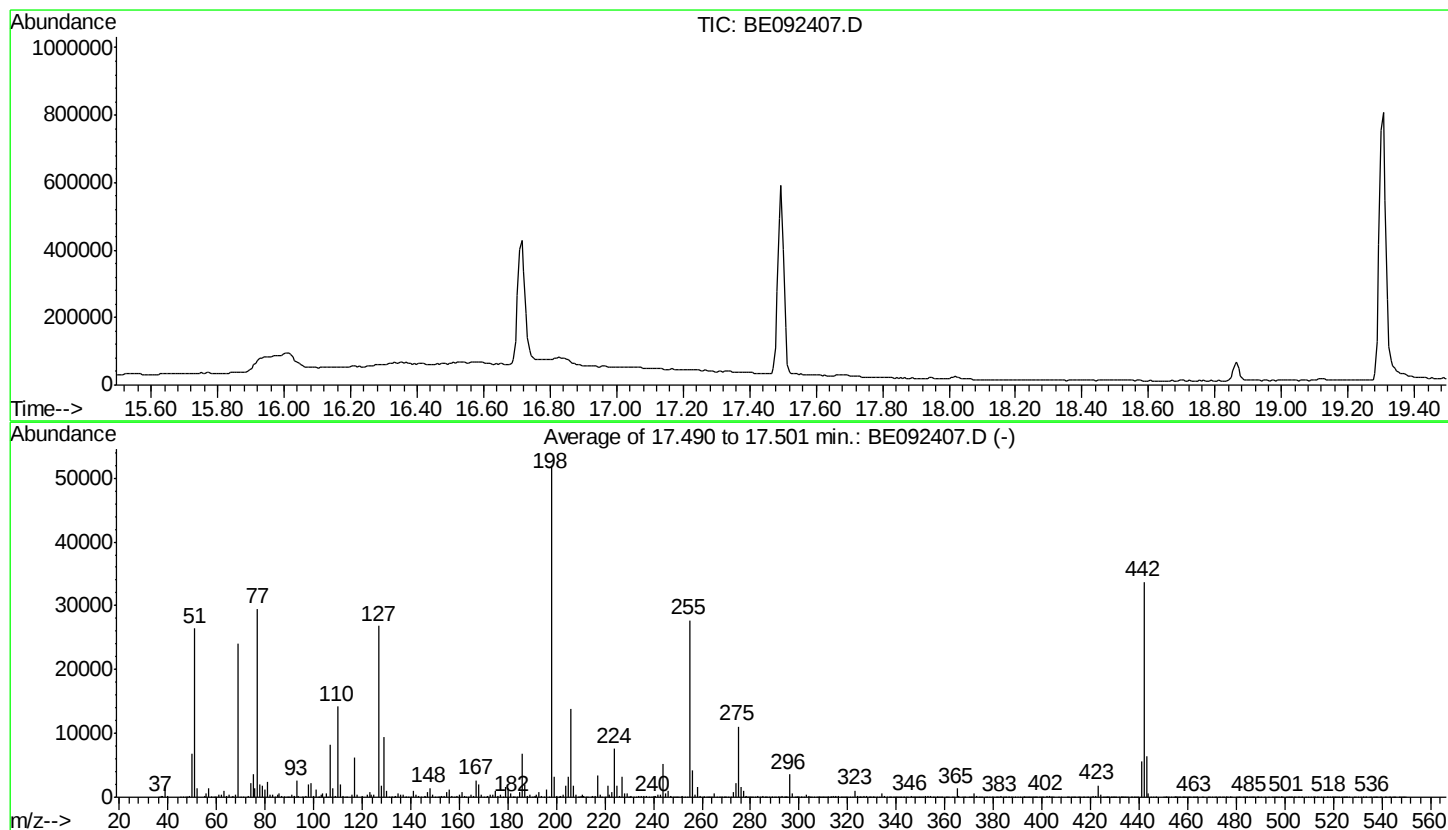

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	26411	PASS
68	69	0.00	2	1.4	348	PASS
69	198	0.00	100	46.3	24056	PASS
70	69	0.00	2	0.3	63	PASS
127	198	10	80	51.6	26794	PASS
197	198	0.00	2	0.2	82	PASS
198	198	100	100	100.0	51942	PASS
199	198	5	9	6.2	3230	PASS
275	198	10	60	21.3	11045	PASS
365	198	1	100	2.6	1362	PASS
441	442	0.01	24	16.6	5601	PASS
442	198	50	100	64.9	33687	PASS
443	442	15	24	18.8	6341	PASS