


Data Path : Z:\HPCHEM1\BNA E\Data\BE092317\
 Data File : BE094072.D
 Acq On : 23 Sep 2017 11:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 25 13:07:29 2017

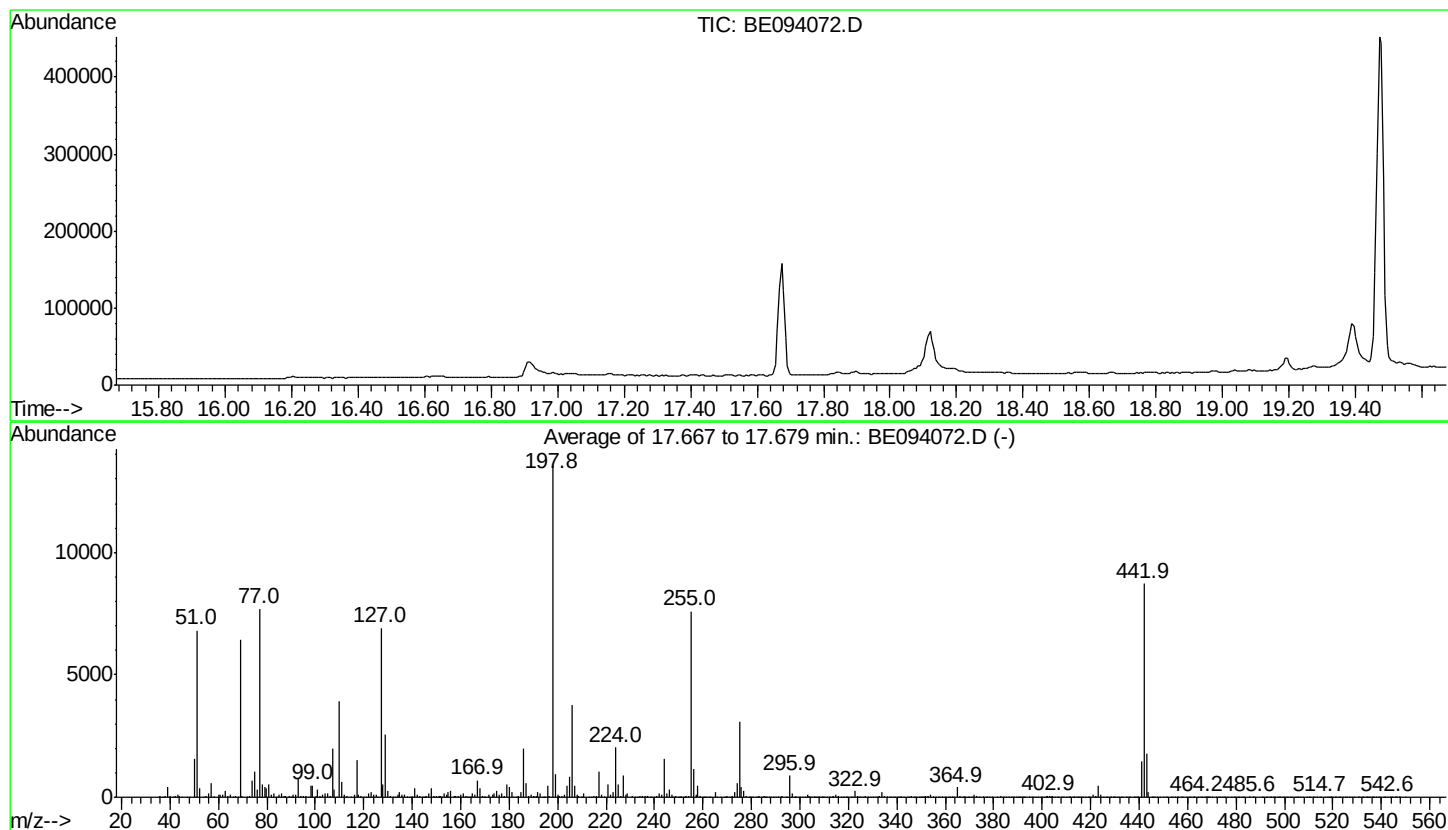

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	6813	PASS
68	69	0.00	2	0.1	5	PASS
69	198	0.00	100	47.5	6430	PASS
70	69	0.00	2	0.8	49	PASS
127	198	10	80	51.1	6916	PASS
197	198	0.00	2	0.4	56	PASS
198	198	100	100	100.0	13547	PASS
199	198	5	9	6.9	941	PASS
275	198	10	60	22.7	3072	PASS
365	198	1	100	2.9	394	PASS
441	442	0.01	24	17.0	1482	PASS
442	198	50	100	64.3	8717	PASS
443	442	15	24	20.3	1768	PASS