


Data Path : Z:\HPCHEM1\BNA E\Data\BE092317\
 Data File : BE094080.D
 Acq On : 23 Sep 2017 16:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 25 13:07:29 2017

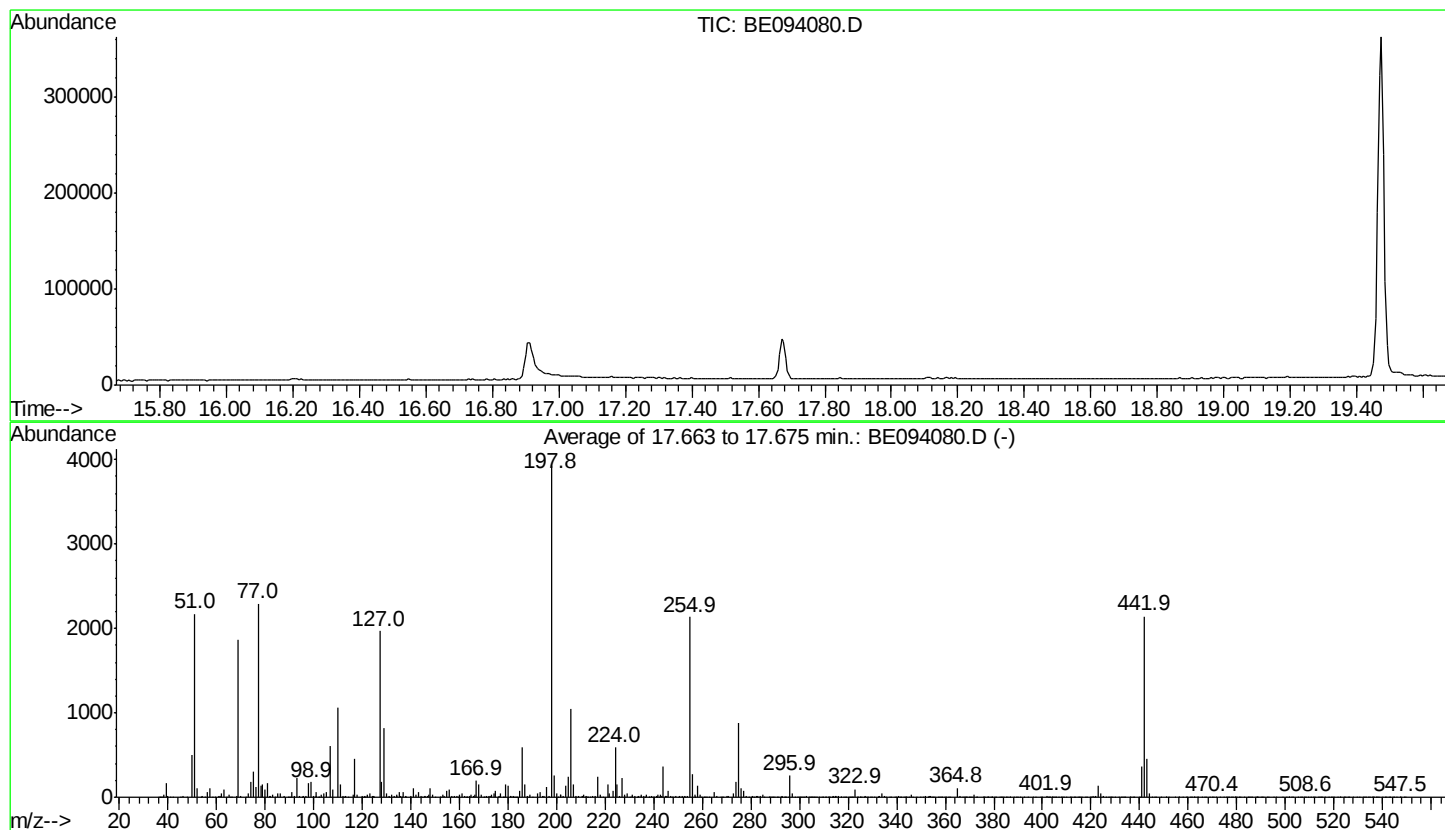

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	2169	PASS
68	69	0.00	2	1.2	23	PASS
69	198	0.00	100	47.4	1864	PASS
70	69	0.00	2	0.5	10	PASS
127	198	10	80	50.1	1968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	3929	PASS
199	198	5	9	6.5	256	PASS
275	198	10	60	22.3	875	PASS
365	198	1	100	2.7	108	PASS
441	442	0.01	24	17.4	372	PASS
442	198	50	100	54.5	2140	PASS
443	442	15	24	21.2	454	PASS