
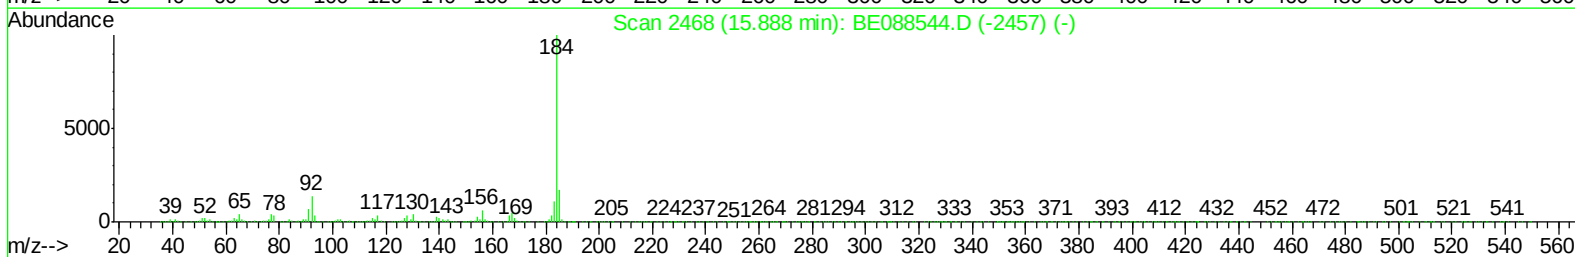
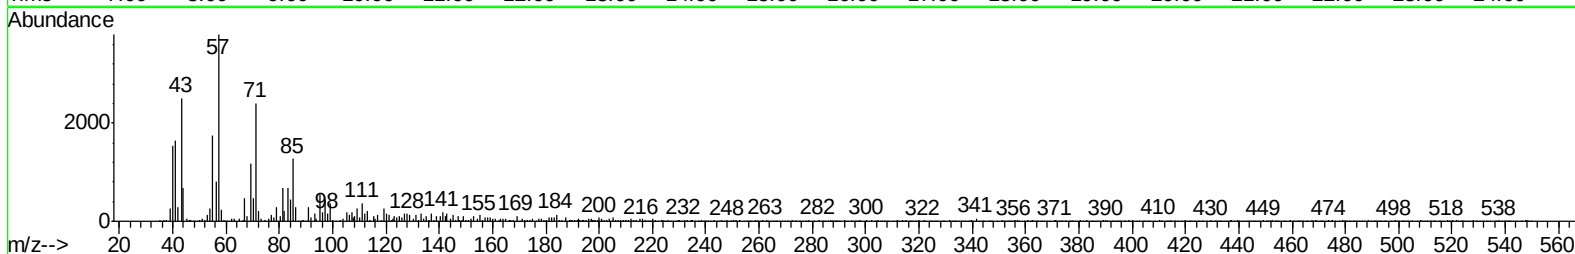


Data Path : Z:\HPCHEM1\BNA E\Data\be092415\
Data File : BE090963.D
Acq On : 24 Sep 2015 3:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 04:17:19 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 06 14:19:16 2014
Response via : Initial Calibration

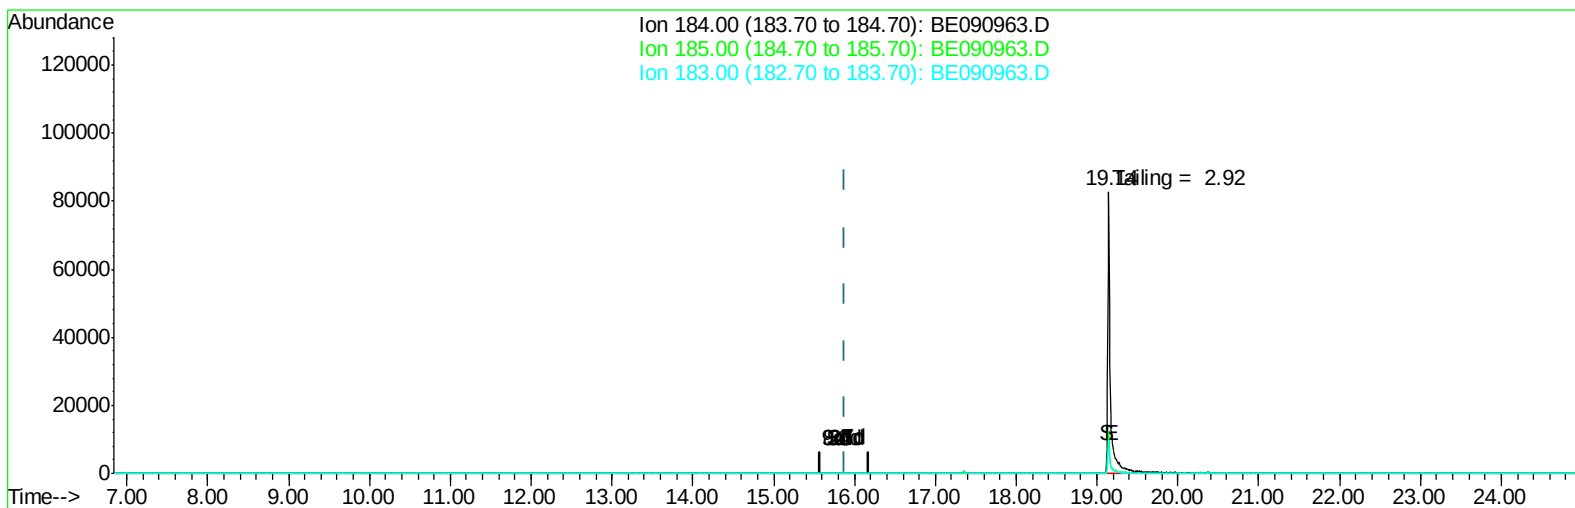

TIC: BE090963.D

(76) Benzidine




15.875min (-0.013) 306.29ng

response 227

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	23.91#
183.00	10.70	63.77#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\be092415\
Data File : BE090963.D
Acq On : 24 Sep 2015 3:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 04:17:19 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 06 14:19:16 2014
Response via : Initial Calibration

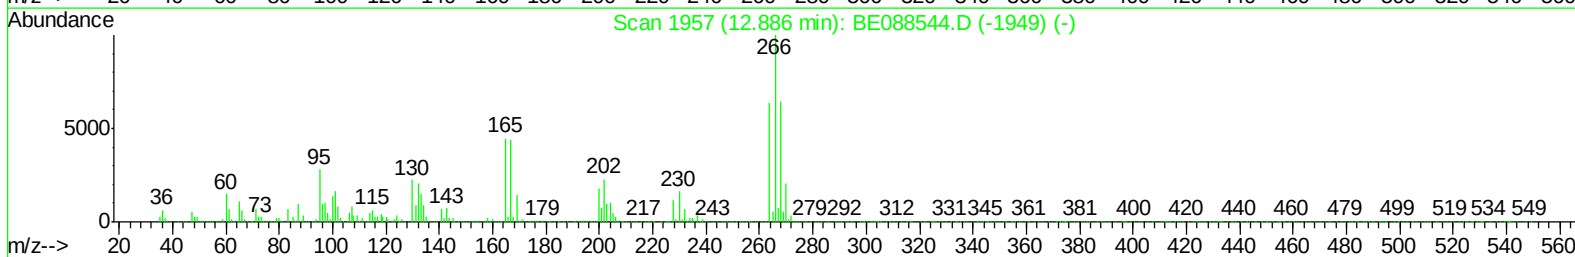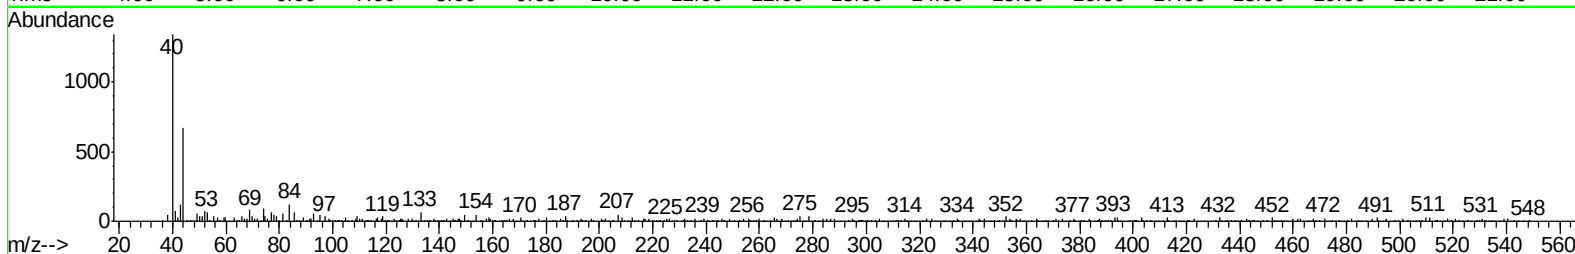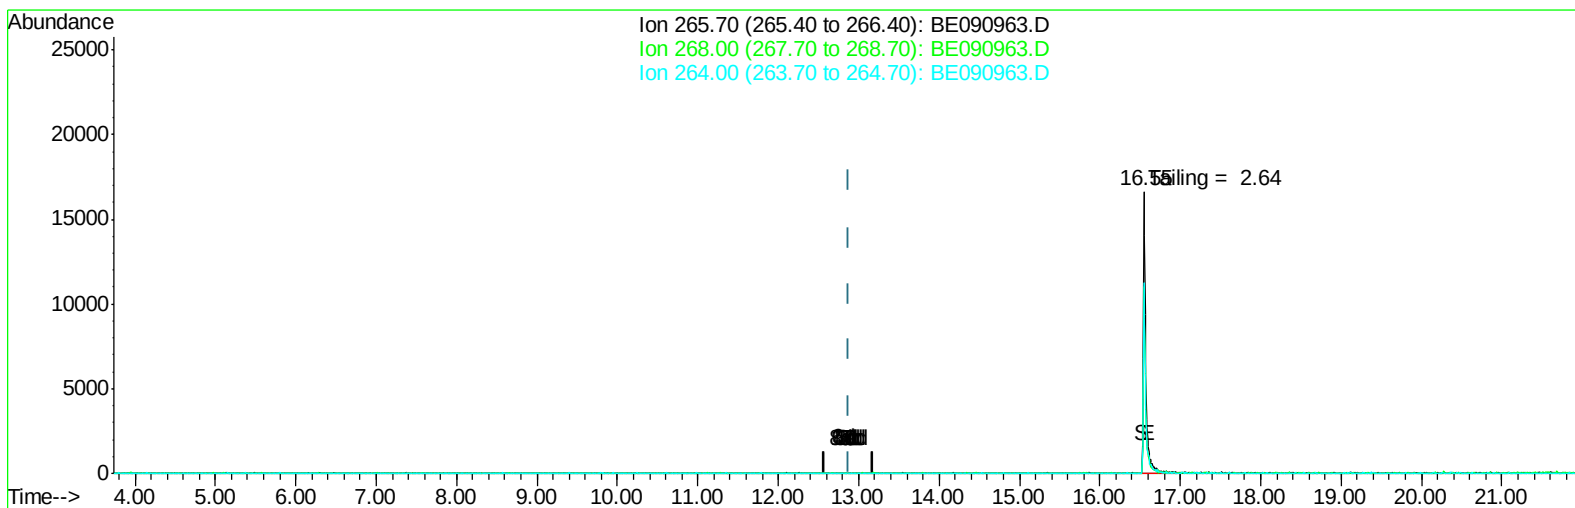

TIC: BE090963.D

(69) Pentachlorophenol (C)

12.744min (-0.142) 87.31ng

response 16

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	68.97
264.00	63.70	68.97
0.00	0.00	0.00