


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE092415\
Data File : BE090963.D
Acq On : 24 Sep 2015 3:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 18 18:17:34 2015

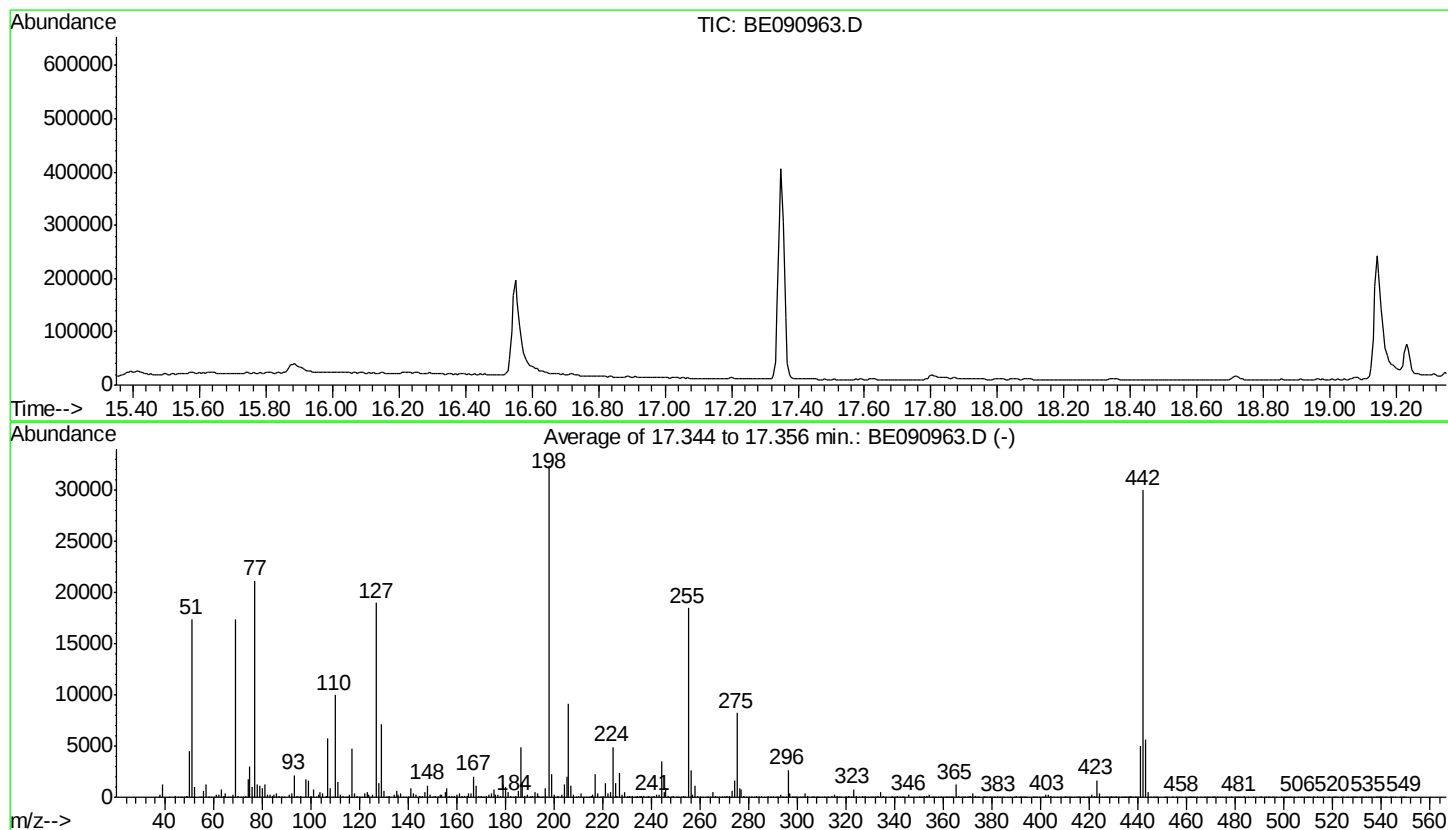

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	17330	PASS
68	69	0.00	2	1.1	197	PASS
69	198	0.00	100	53.7	17386	PASS
70	69	0.00	2	0.6	106	PASS
127	198	10	80	58.6	18964	PASS
197	198	0.00	2	0.1	42	PASS
198	198	100	100	100.0	32360	PASS
199	198	5	9	7.1	2308	PASS
275	198	10	60	25.4	8221	PASS
365	198	1	100	3.8	1230	PASS
441	442	0.01	24	16.7	4993	PASS
442	198	50	100	92.6	29964	PASS
443	442	15	24	18.6	5574	PASS