
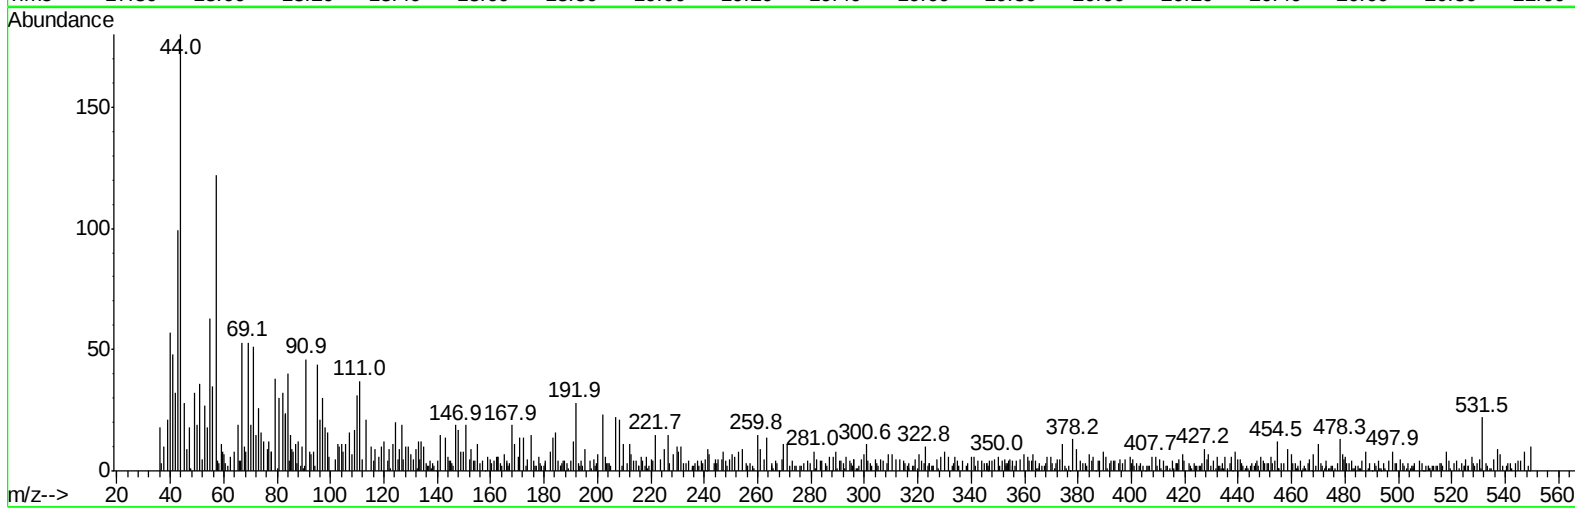


Data Path : Z:\HPCHEM1\BNA E\DATA\BE092517\
Data File : BE094098.D
Acq On : 25 Sep 2017 11:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:32:22 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

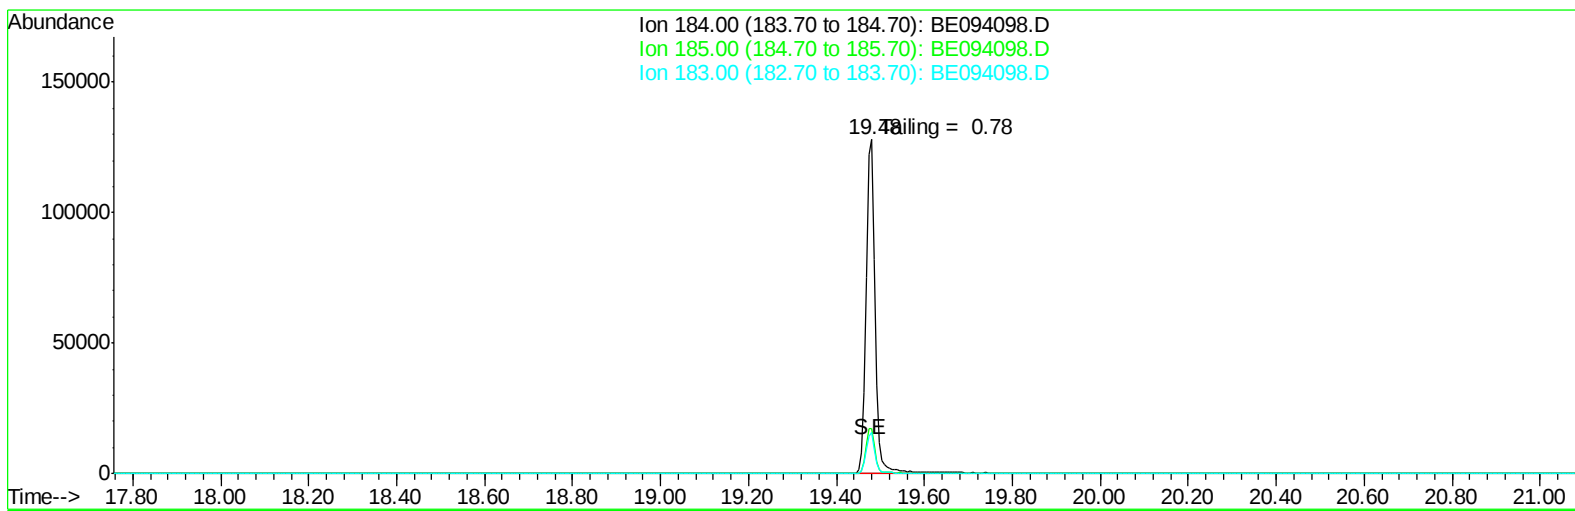

TIC: BE094098.D

(76) Benzidine



12.976min (+0.196) 60.83ng

response 9

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	25.00#
183.00	11.60	87.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE092517\
Data File : BE094098.D
Acq On : 25 Sep 2017 11:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:32:22 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

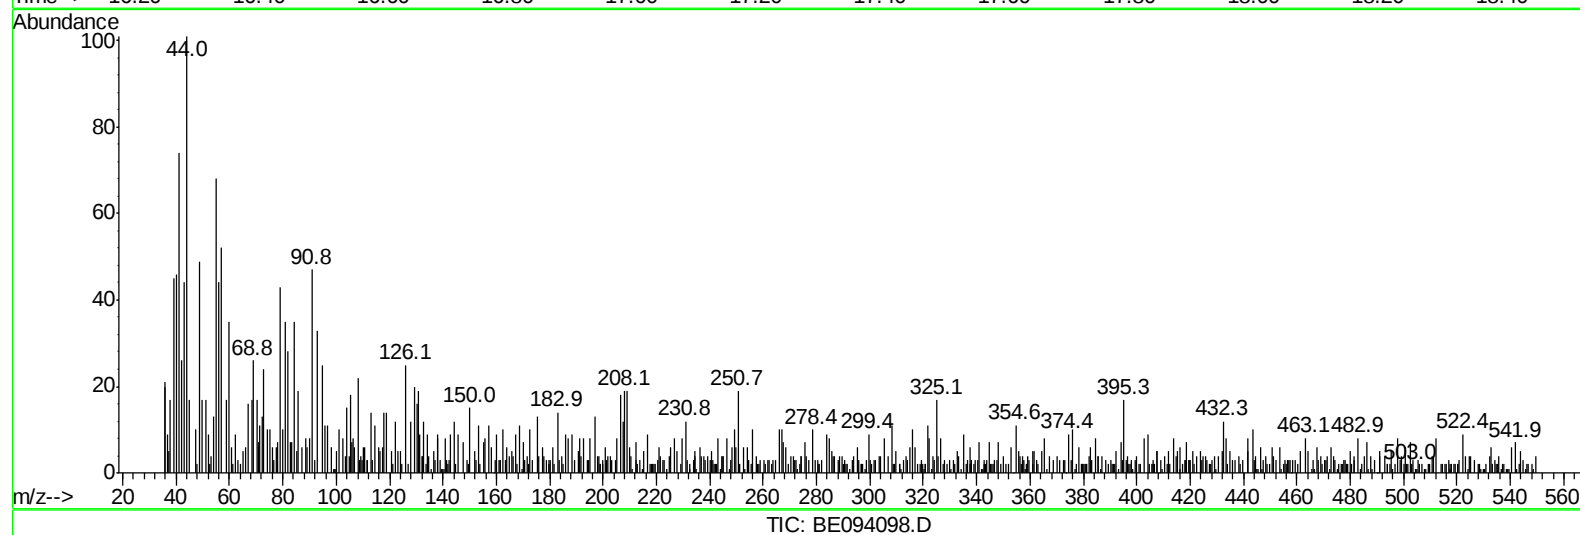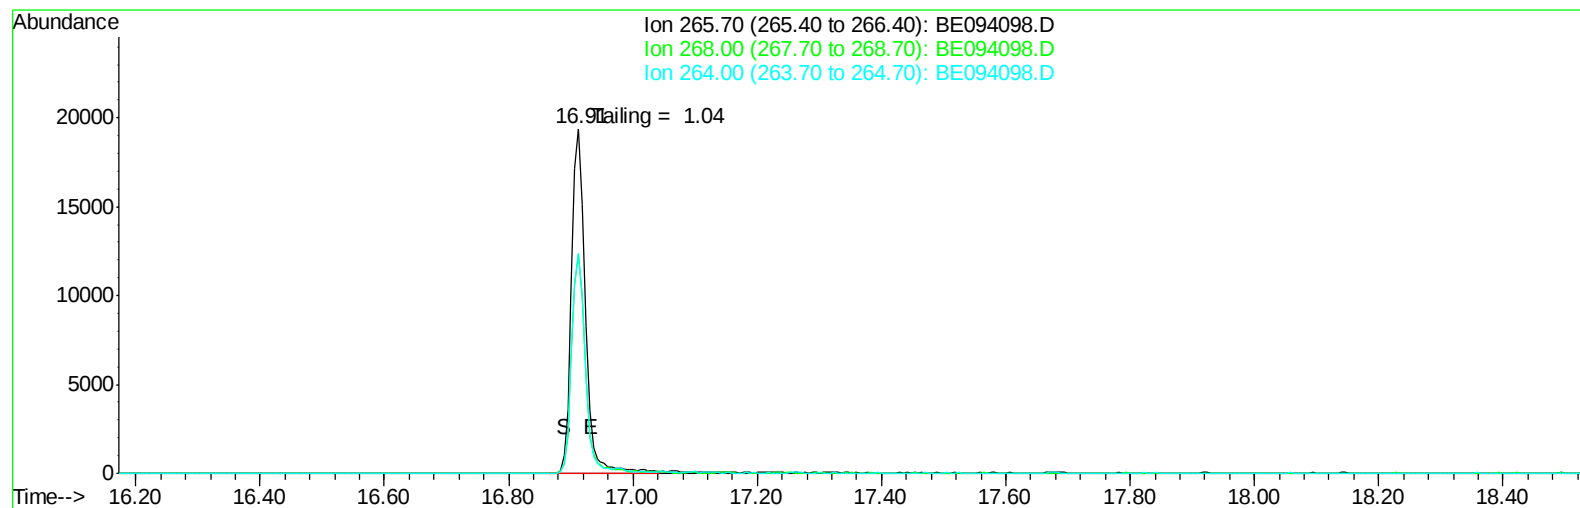

(69) Pentachlorophenol (C)

11.642min (+0.397) 61.48ng

response 2

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.00
264.00	61.90	60.00
0.00	0.00	0.00