
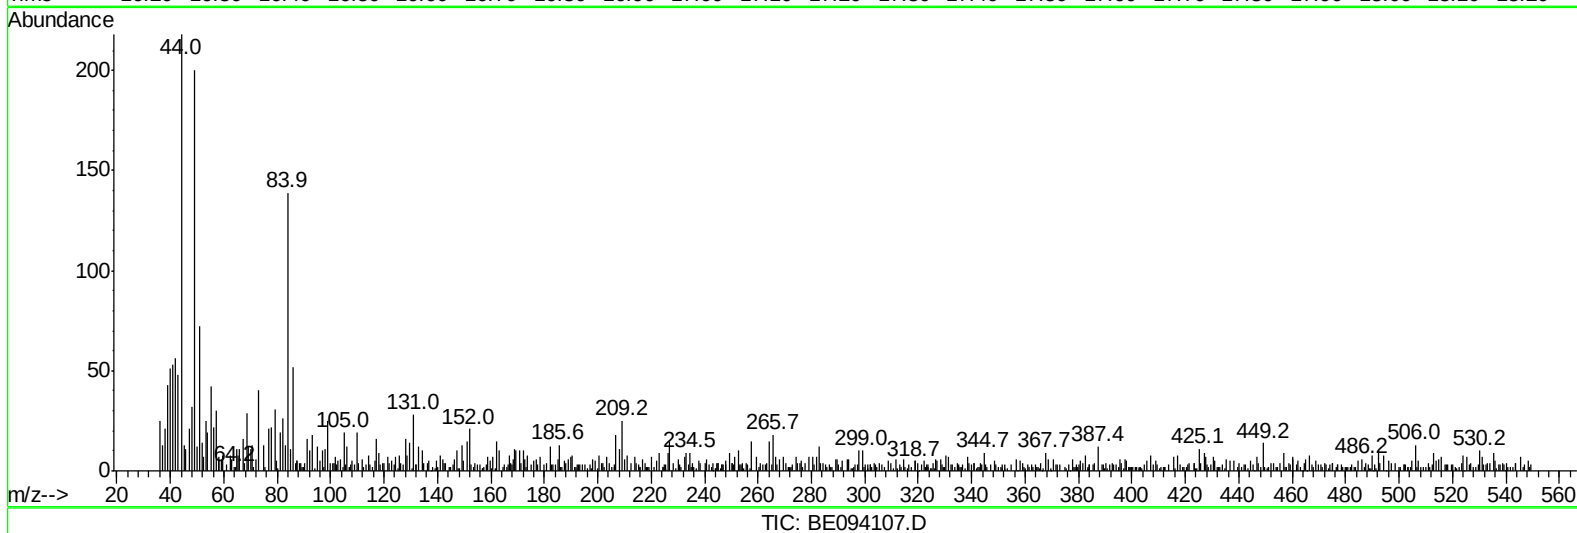


Data Path : Z:\HPCHEM1\BNA E\DATA\BE092517\
Data File : BE094107.D
Acq On : 25 Sep 2017 18:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:34:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

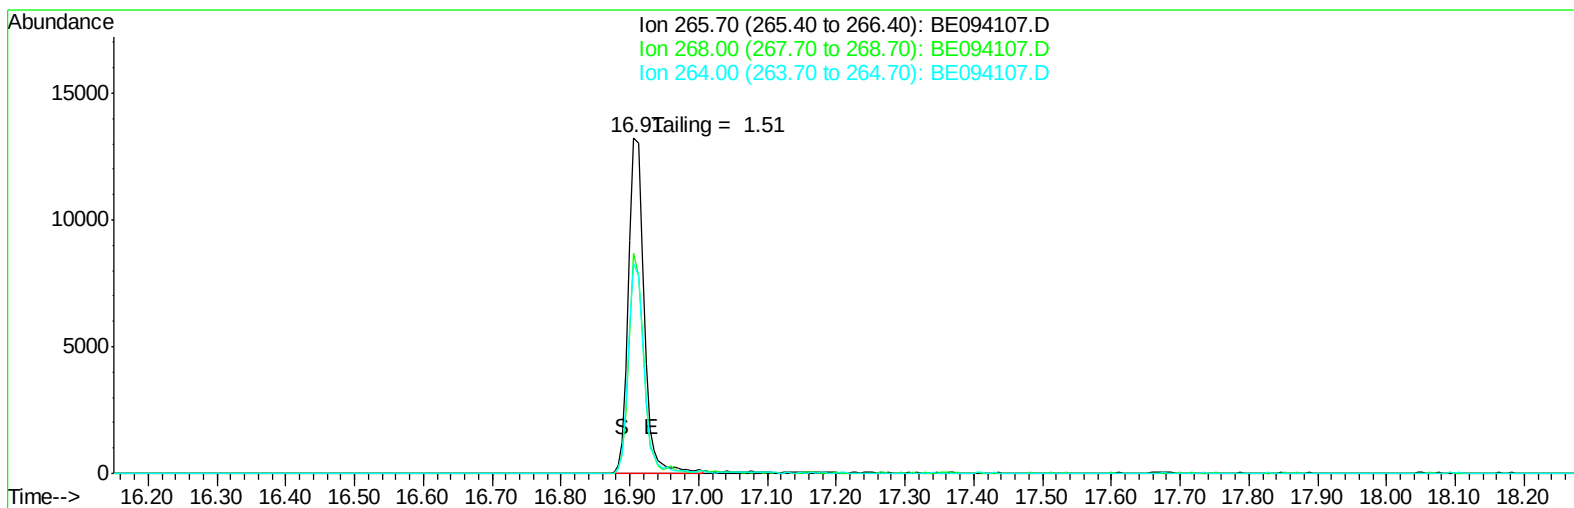

(69) Pentachlorophenol (C)



11.295min (+0.050) 175.65ng

response 8

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	33.33#
264.00	61.90	83.33#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE092517\
Data File : BE094107.D
Acq On : 25 Sep 2017 18:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:34:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

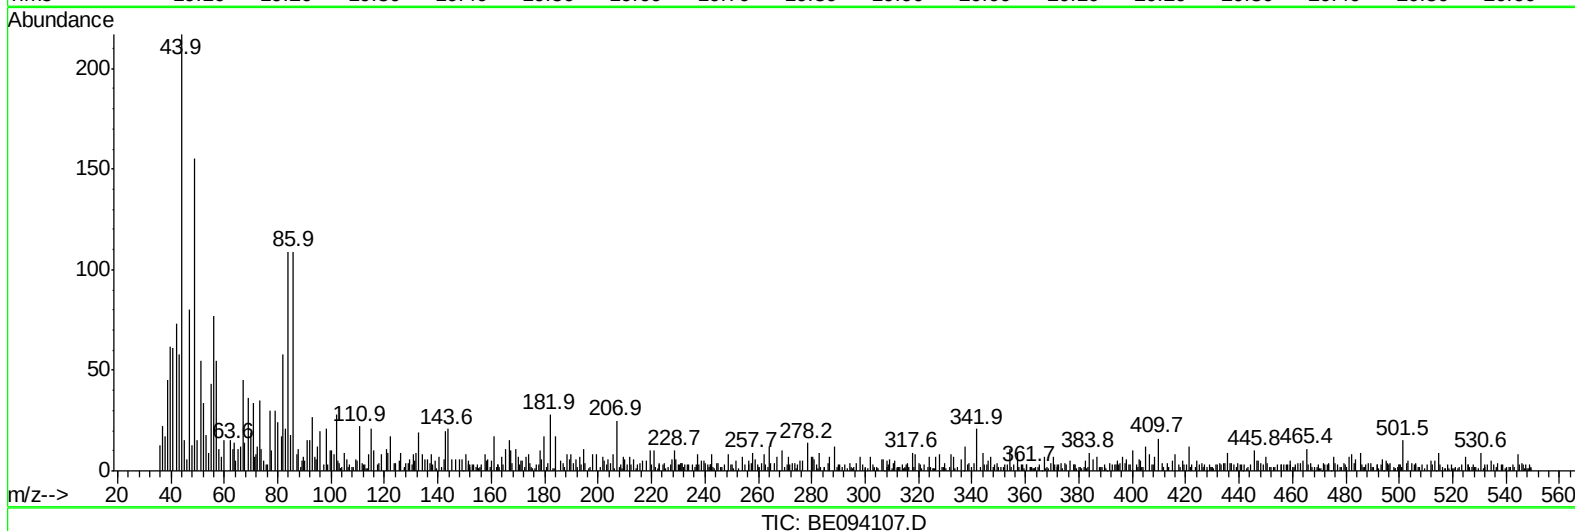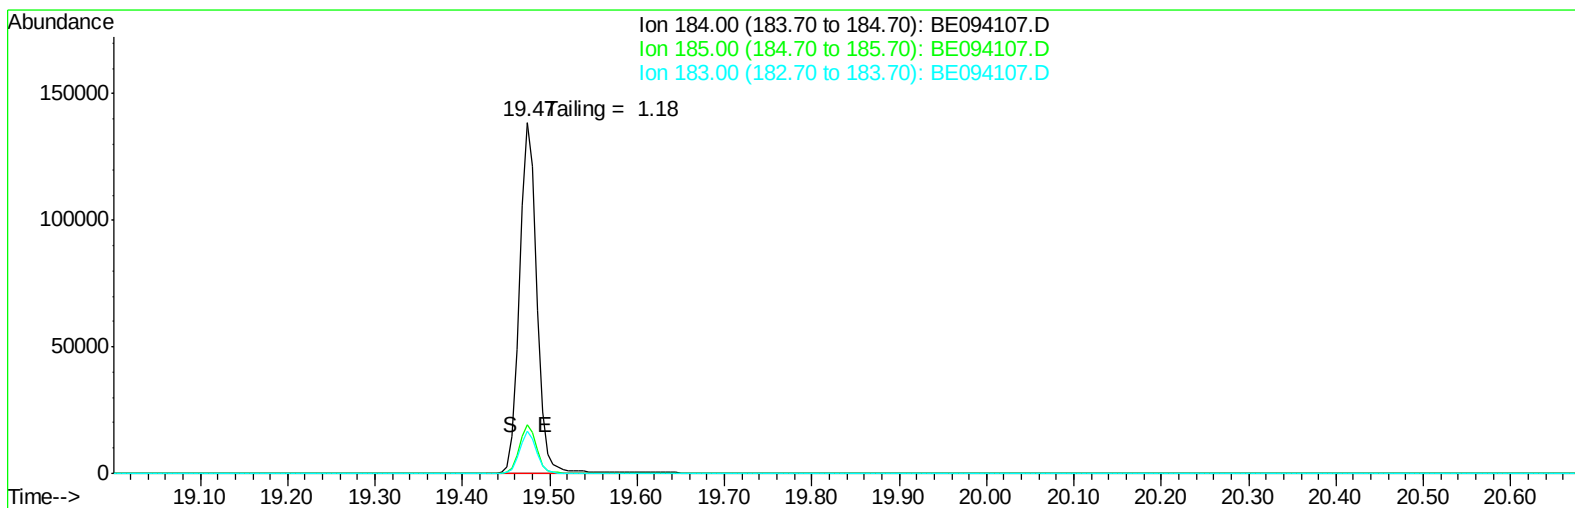

TIC: BE094107.D

(76) Benzidine

12.864min (+0.084) 50.69ng

response 15

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	11.76
0.00	0.00	0.00