


Data Path : Z:\HPCHEM1\BNA E\Data\BE092517\
 Data File : BE094098.D
 Acq On : 25 Sep 2017 11:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 25 17:37:08 2017

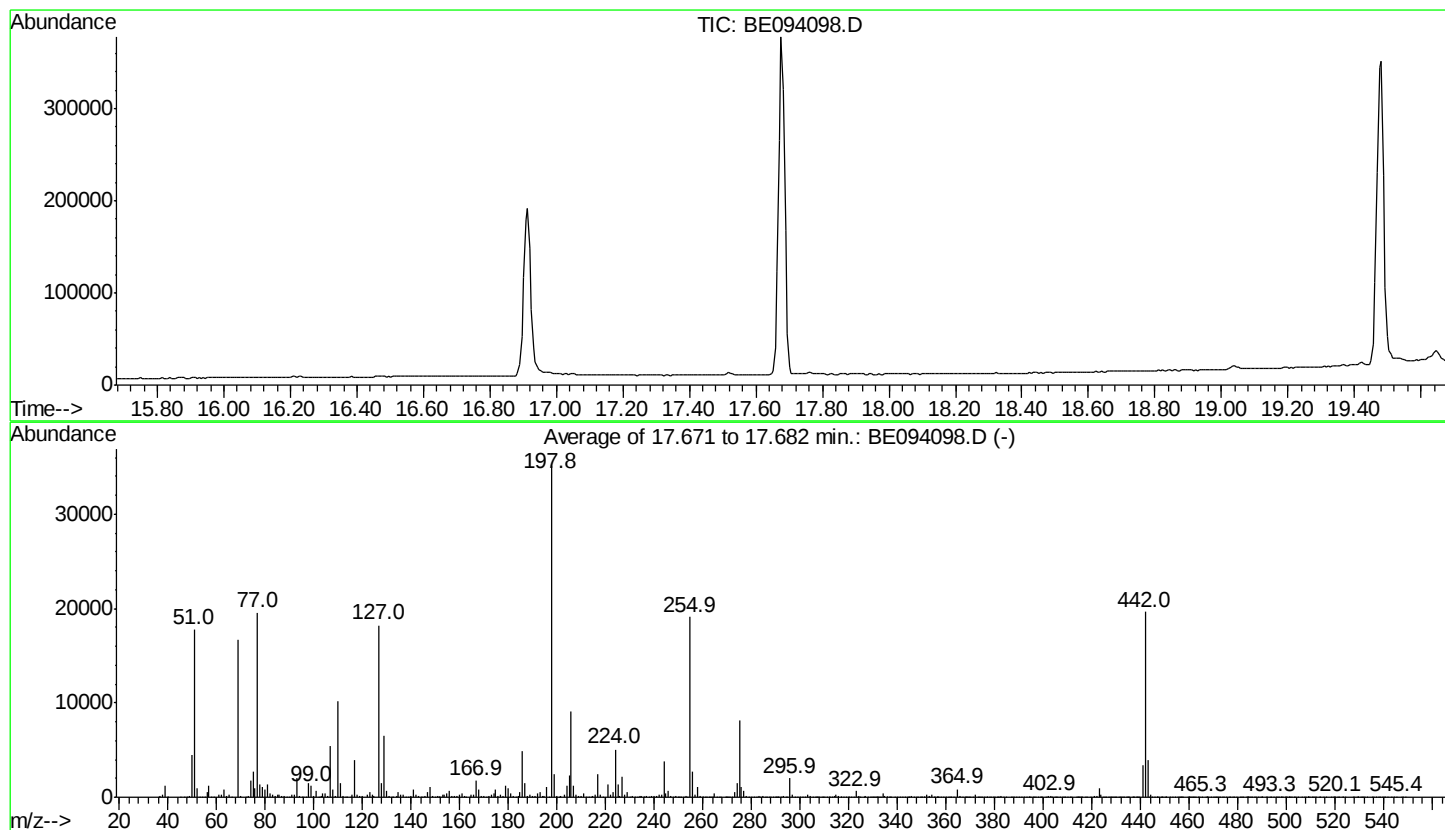

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	17714	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.4	16664	PASS
70	69	0.00	2	0.6	102	PASS
127	198	10	80	51.8	18226	PASS
197	198	0.00	2	0.2	61	PASS
198	198	100	100	100.0	35154	PASS
199	198	5	9	6.9	2428	PASS
275	198	10	60	23.4	8209	PASS
365	198	1	100	2.4	858	PASS
441	442	0.01	24	17.4	3430	PASS
442	198	50	100	56.0	19674	PASS
443	442	15	24	20.4	4004	PASS