


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE092518\
Data File : BE097651.D
Acq On : 25 Sep 2018 9:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092418.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 24 18:40:34 2018

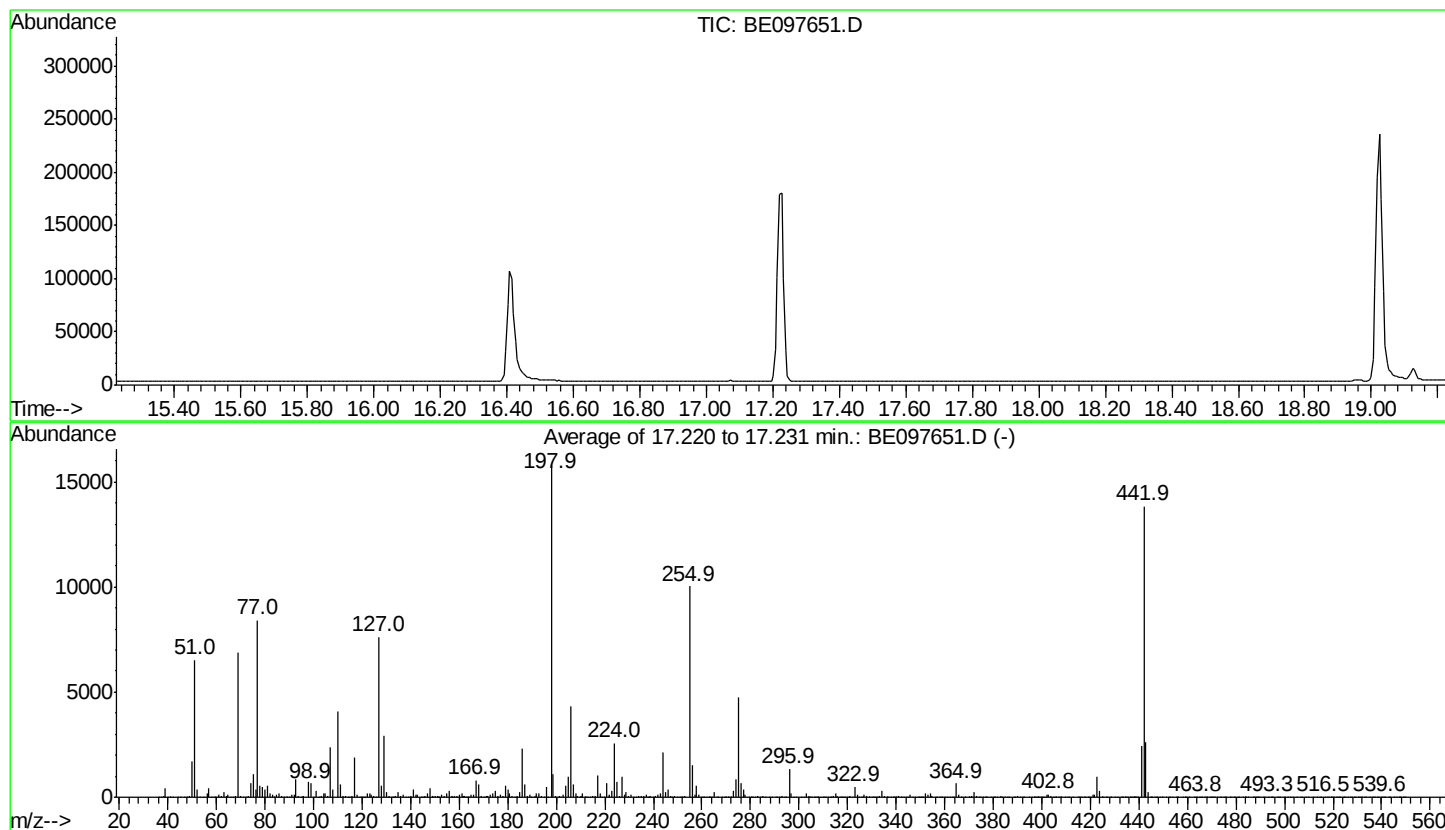

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	6519	PASS
68	69	0.00	2	1.1	74	PASS
69	198	0.00	100	43.5	6864	PASS
70	69	0.00	2	0.7	46	PASS
127	198	10	80	48.4	7631	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15774	PASS
199	198	5	9	6.8	1072	PASS
275	198	10	60	30.0	4735	PASS
365	198	1	100	4.2	656	PASS
441	198	0.01	100	15.3	2419	PASS
442	198	50	100	87.8	13845	PASS
443	442	15	24	18.8	2603	PASS