


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE092518\
 Data File : BE097668.D
 Acq On : 25 Sep 2018 21:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 18:40:34 2018

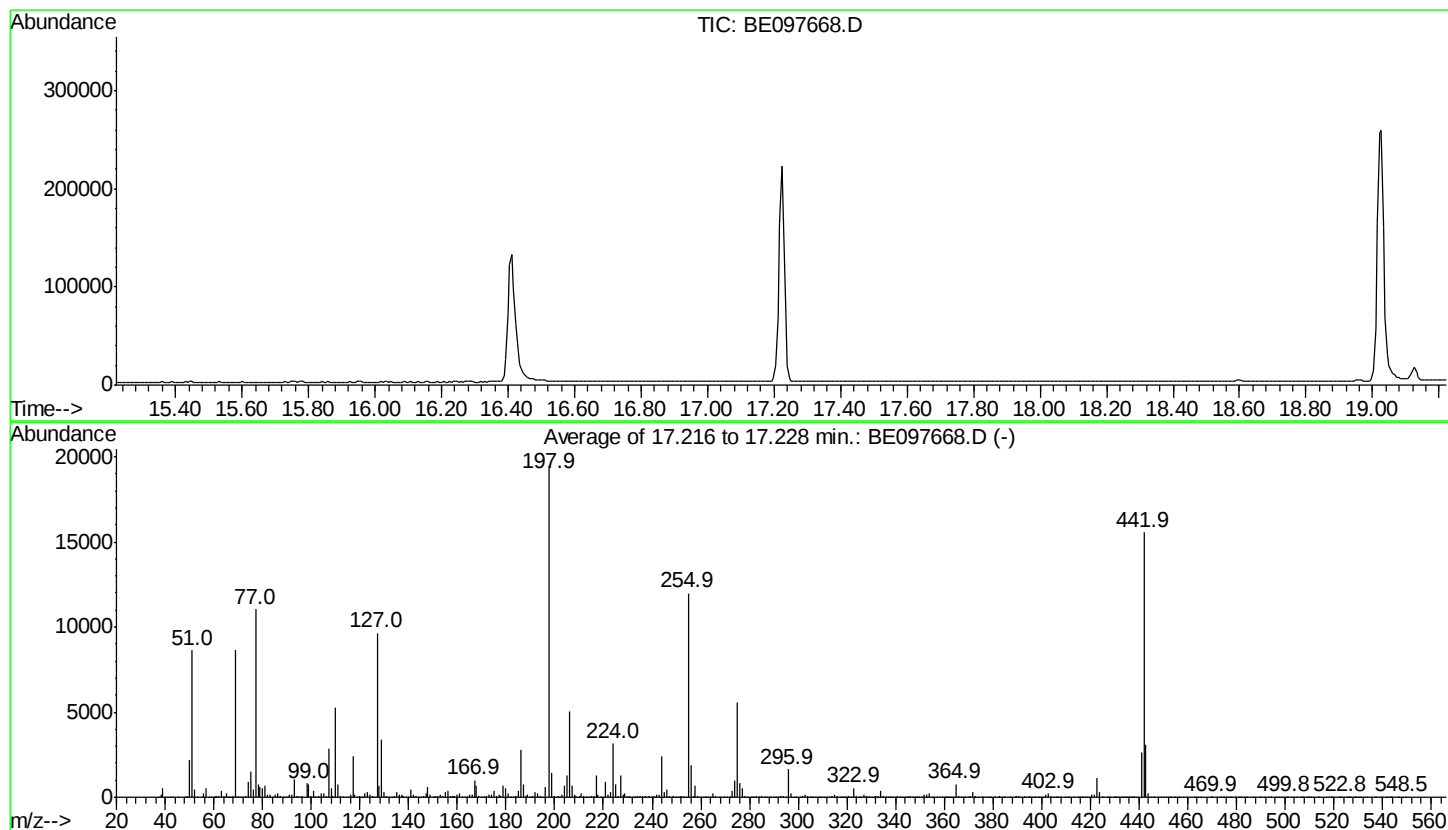

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	8635	PASS
68	69	0.00	2	0.8	67	PASS
69	198	0.00	100	44.4	8661	PASS
70	69	0.00	2	0.5	47	PASS
127	198	10	80	49.6	9659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19485	PASS
199	198	5	9	7.2	1405	PASS
275	198	10	60	28.6	5575	PASS
365	198	1	100	4.1	792	PASS
441	198	0.01	100	13.6	2654	PASS
442	198	50	100	79.9	15565	PASS
443	442	15	24	19.7	3061	PASS