


Data Path : Z:\HPCHEM1\BNA_E\Data\BE092616\
Data File : BE092424.D
Acq On : 26 Sep 2016 12:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 22 18:25:56 2016

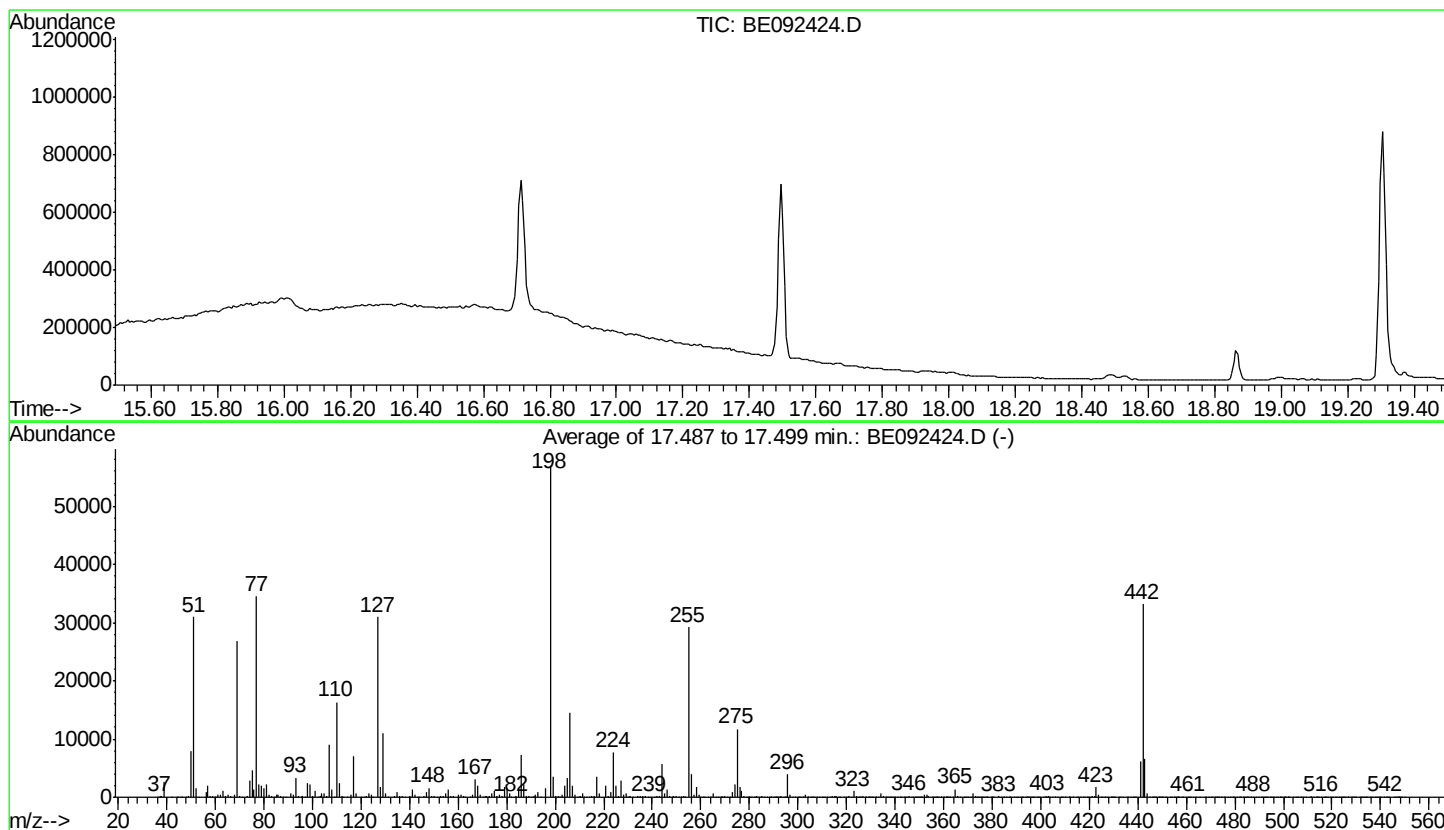

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	30933	PASS
68	69	0.00	2	1.5	398	PASS
69	198	0.00	100	47.2	26890	PASS
70	69	0.00	2	0.6	149	PASS
127	198	10	80	54.4	30988	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56981	PASS
199	198	5	9	6.1	3482	PASS
275	198	10	60	20.5	11686	PASS
365	198	1	100	2.5	1429	PASS
441	442	0.01	24	18.3	6058	PASS
442	198	50	100	58.2	33164	PASS
443	442	15	24	20.0	6642	PASS