


Data Path : Z:\HPCHEM1\BNA E\Data\BE092617\
 Data File : BE094122.D
 Acq On : 26 Sep 2017 8:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 25 17:37:08 2017

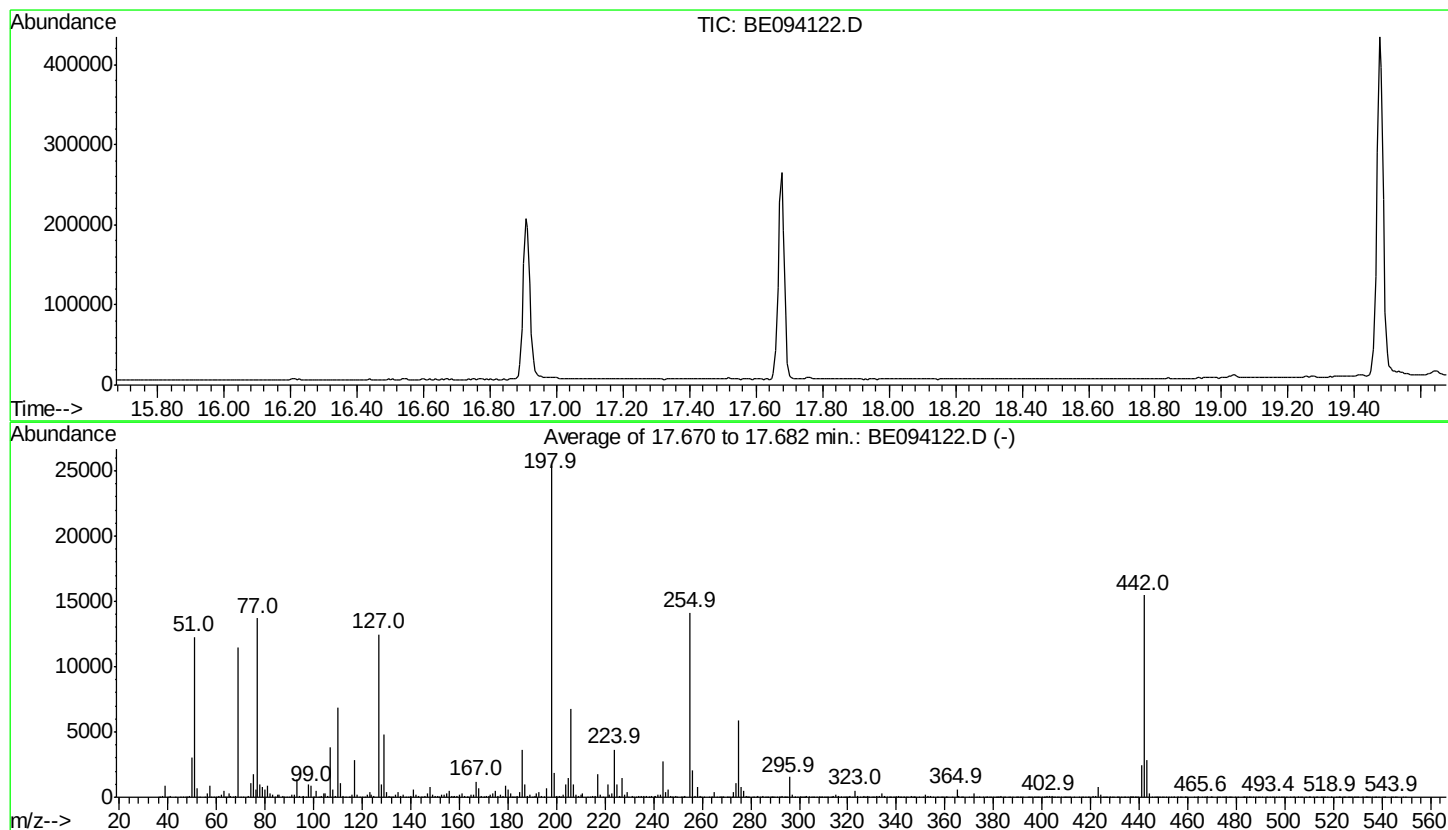

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	12272	PASS
68	69	0.00	2	1.0	119	PASS
69	198	0.00	100	45.0	11426	PASS
70	69	0.00	2	0.4	45	PASS
127	198	10	80	49.1	12458	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25383	PASS
199	198	5	9	7.2	1817	PASS
275	198	10	60	23.3	5926	PASS
365	198	1	100	2.4	621	PASS
441	442	0.01	24	16.0	2479	PASS
442	198	50	100	60.9	15464	PASS
443	442	15	24	18.5	2862	PASS