


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE092618\
 Data File : BE097680.D
 Acq On : 26 Sep 2018 9:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 18:40:34 2018

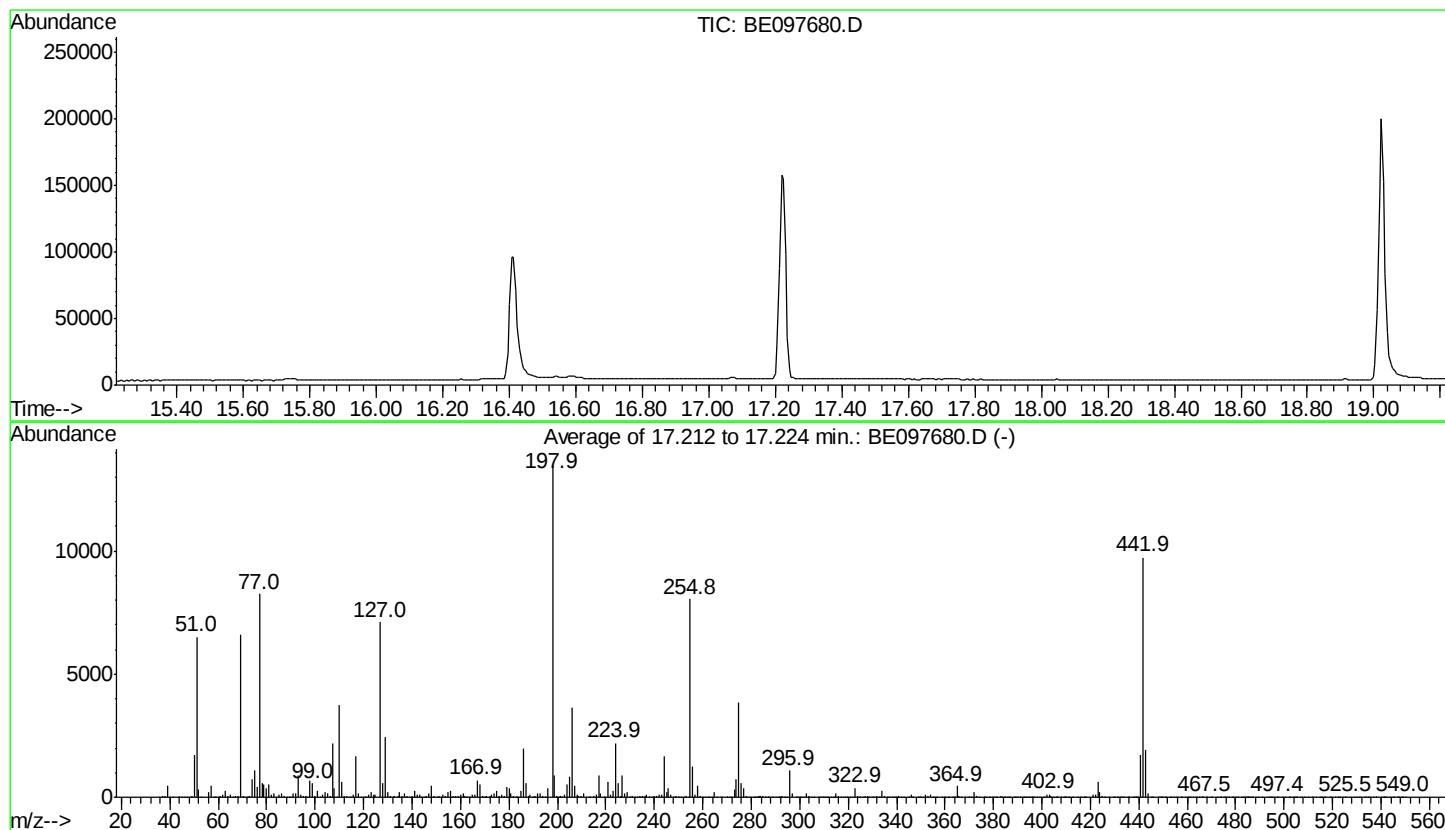

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	6499	PASS
68	69	0.00	2	0.5	35	PASS
69	198	0.00	100	48.9	6587	PASS
70	69	0.00	2	0.5	30	PASS
127	198	10	80	52.7	7102	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13464	PASS
199	198	5	9	6.6	895	PASS
275	198	10	60	28.7	3867	PASS
365	198	1	100	3.5	467	PASS
441	198	0.01	100	12.9	1736	PASS
442	198	50	100	72.2	9727	PASS
443	442	15	24	19.9	1934	PASS