


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092619\
 Data File : BE100564.D
 Acq On : 26 Sep 2019 11:49
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 26 18:21:08 2019

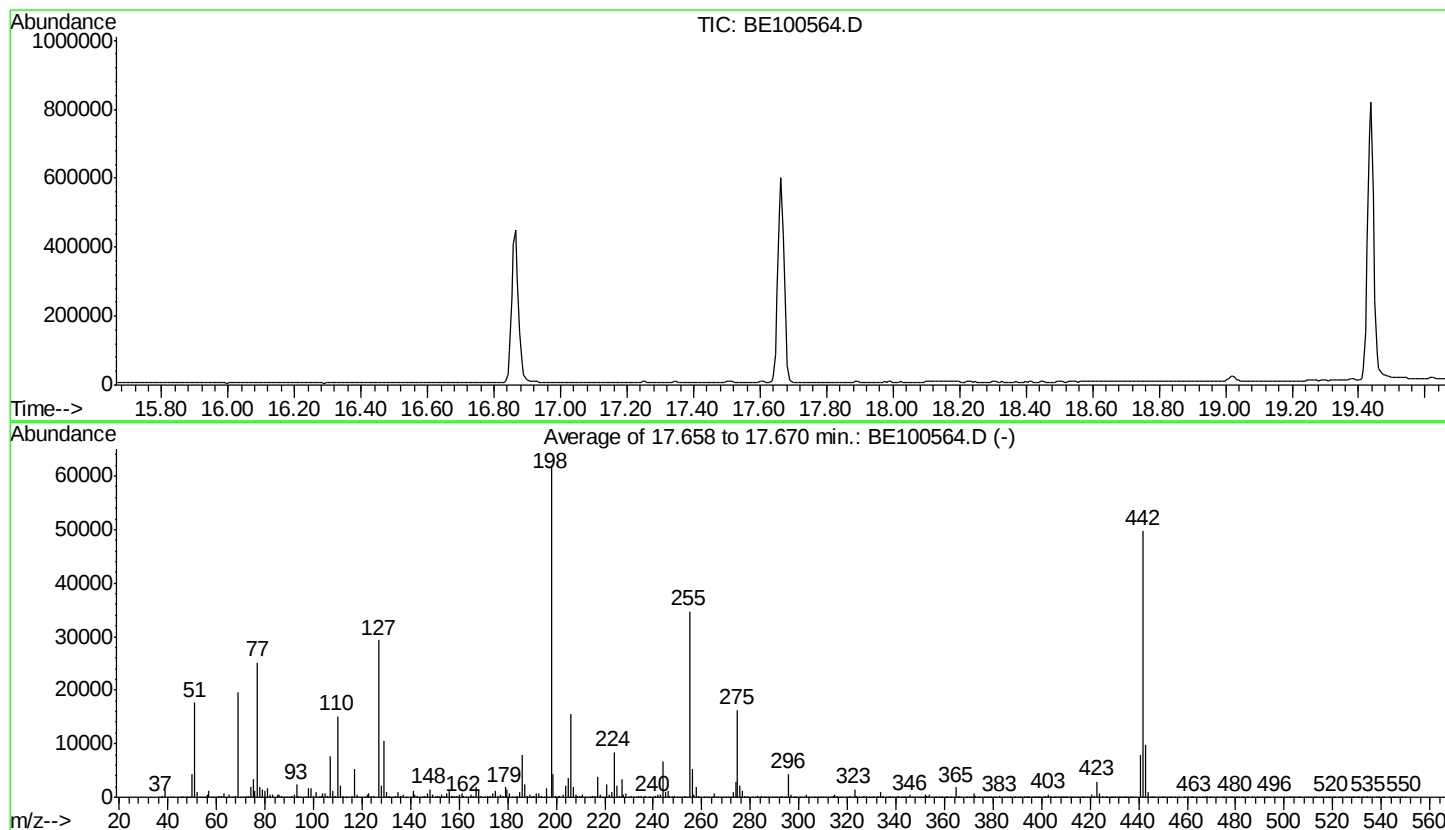

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	17691	PASS
68	69	0.00	2	1.4	283	PASS
69	198	0.00	100	31.8	19679	PASS
70	69	0.00	2	0.3	68	PASS
127	198	10	80	47.4	29373	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61932	PASS
199	198	5	9	7.0	4315	PASS
275	198	10	60	26.3	16309	PASS
365	198	1	100	3.0	1866	PASS
441	198	0.01	100	12.6	7797	PASS
442	198	50	100	80.3	49728	PASS
443	442	15	24	19.5	9693	PASS