




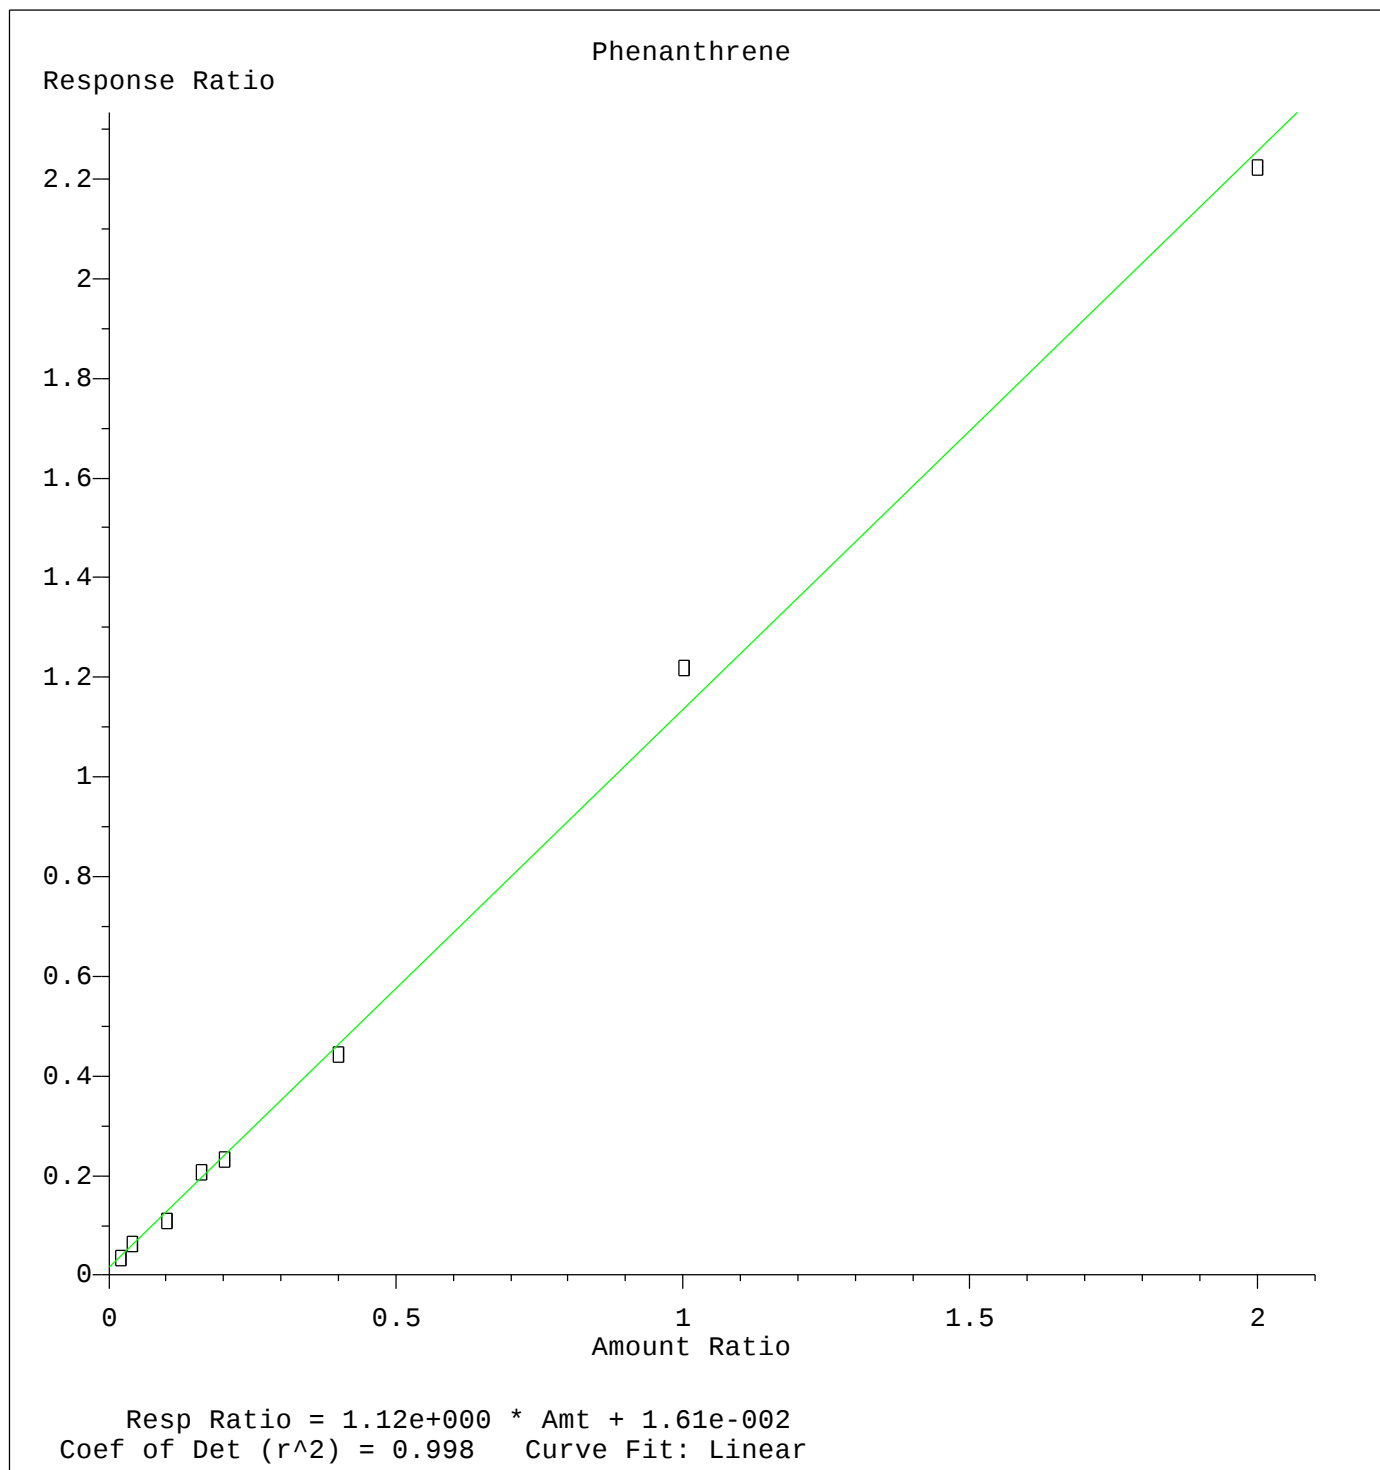


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

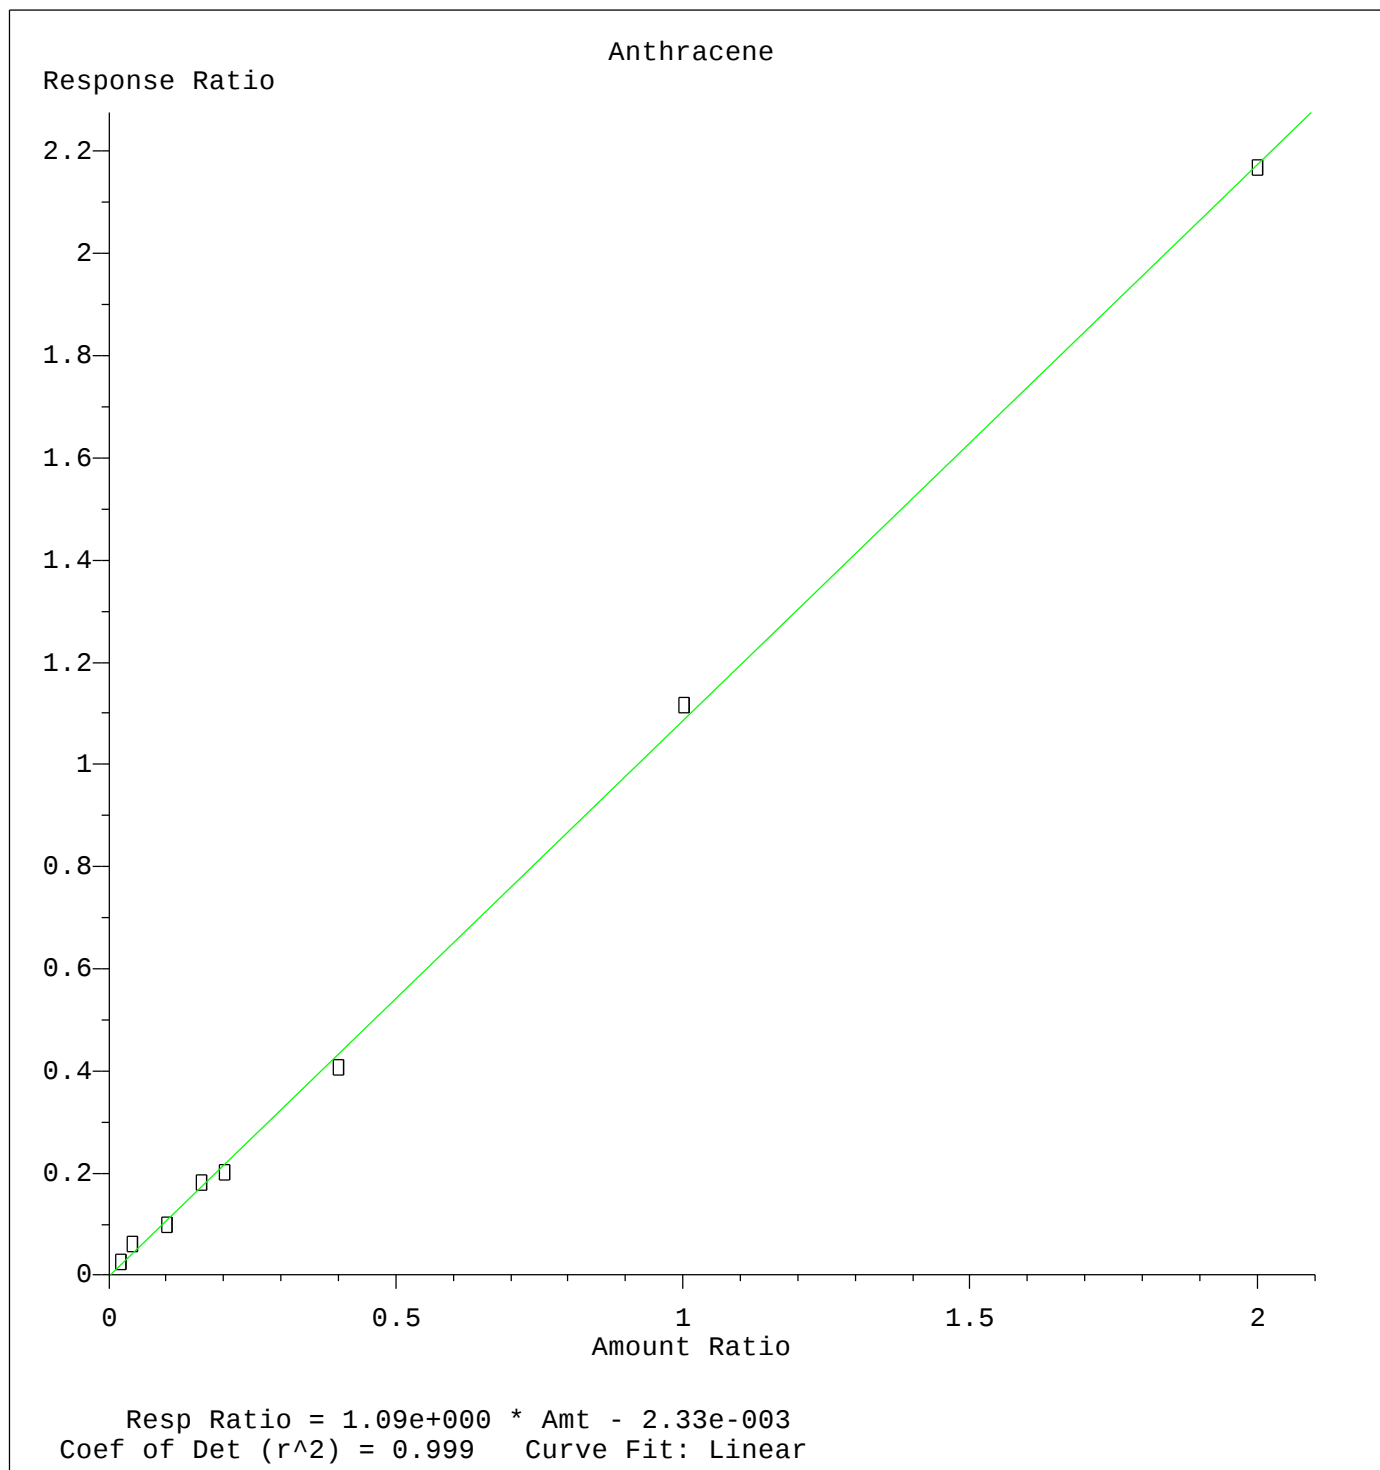


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

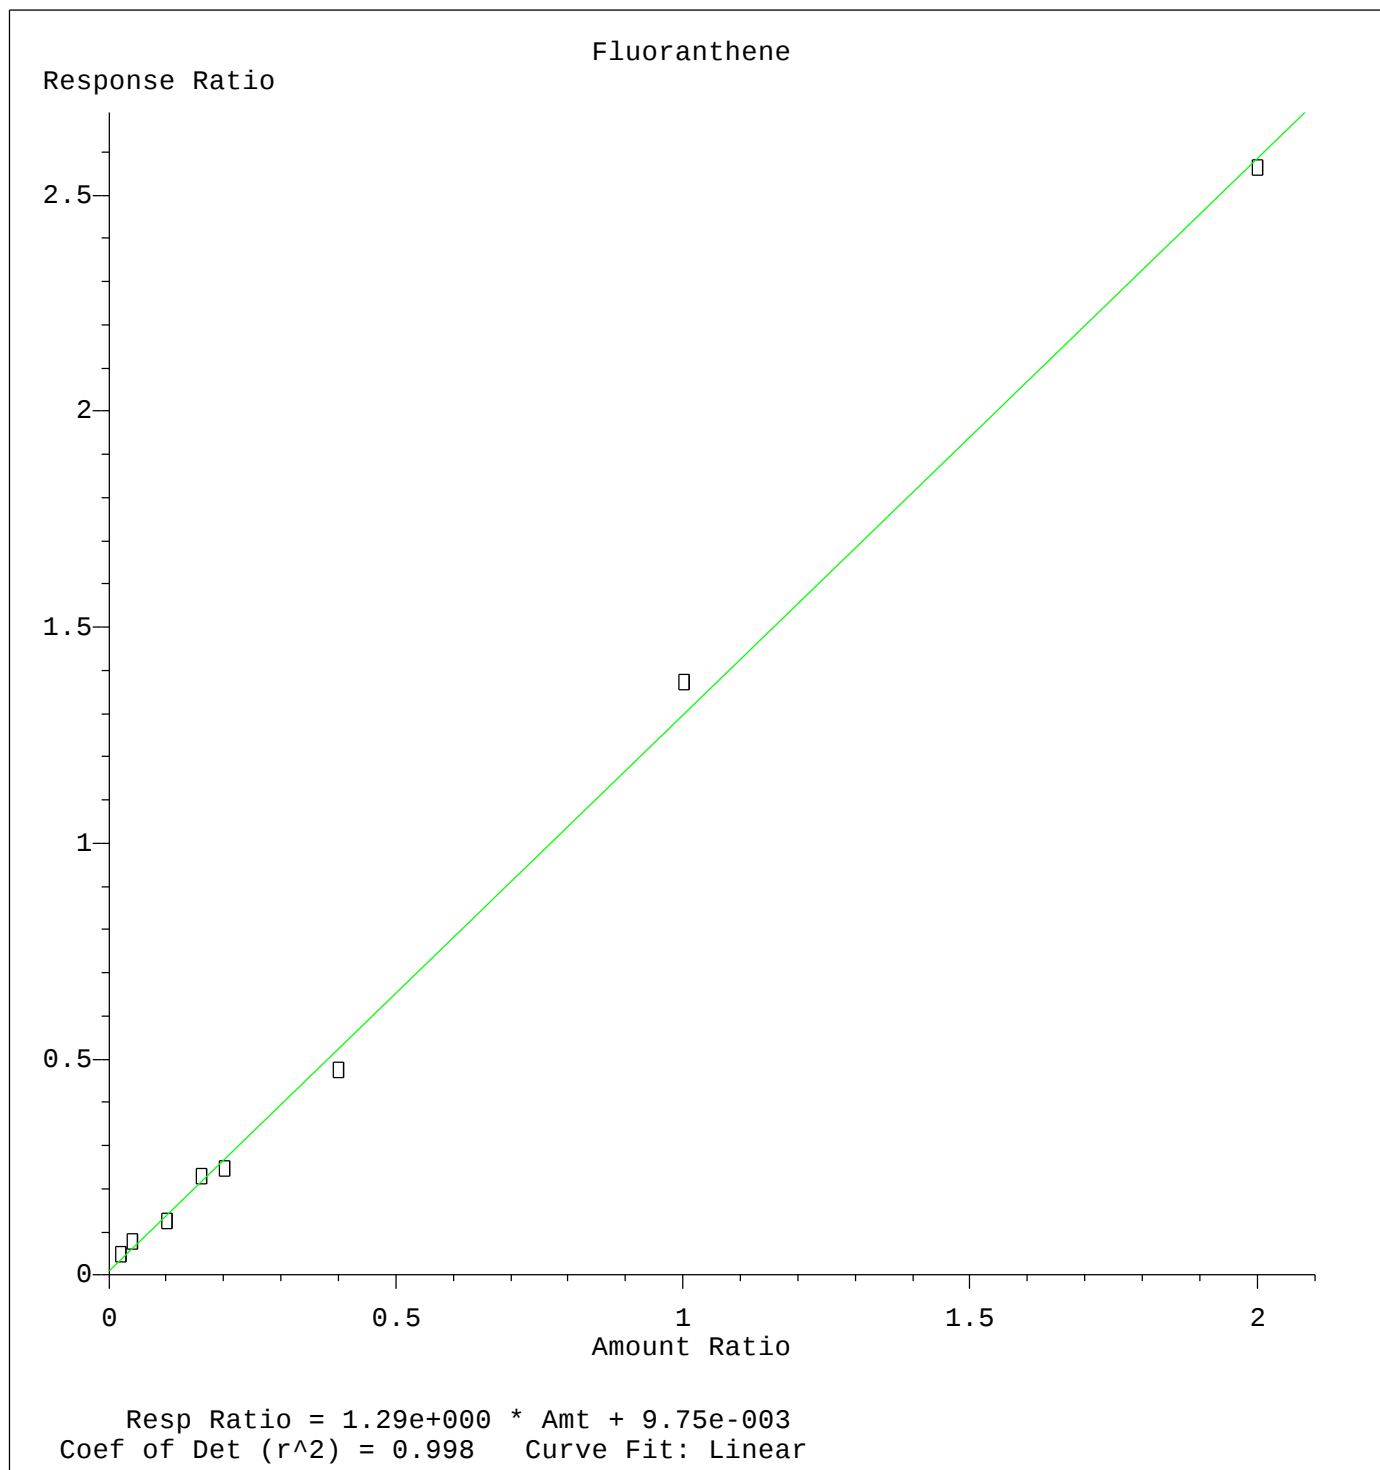


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

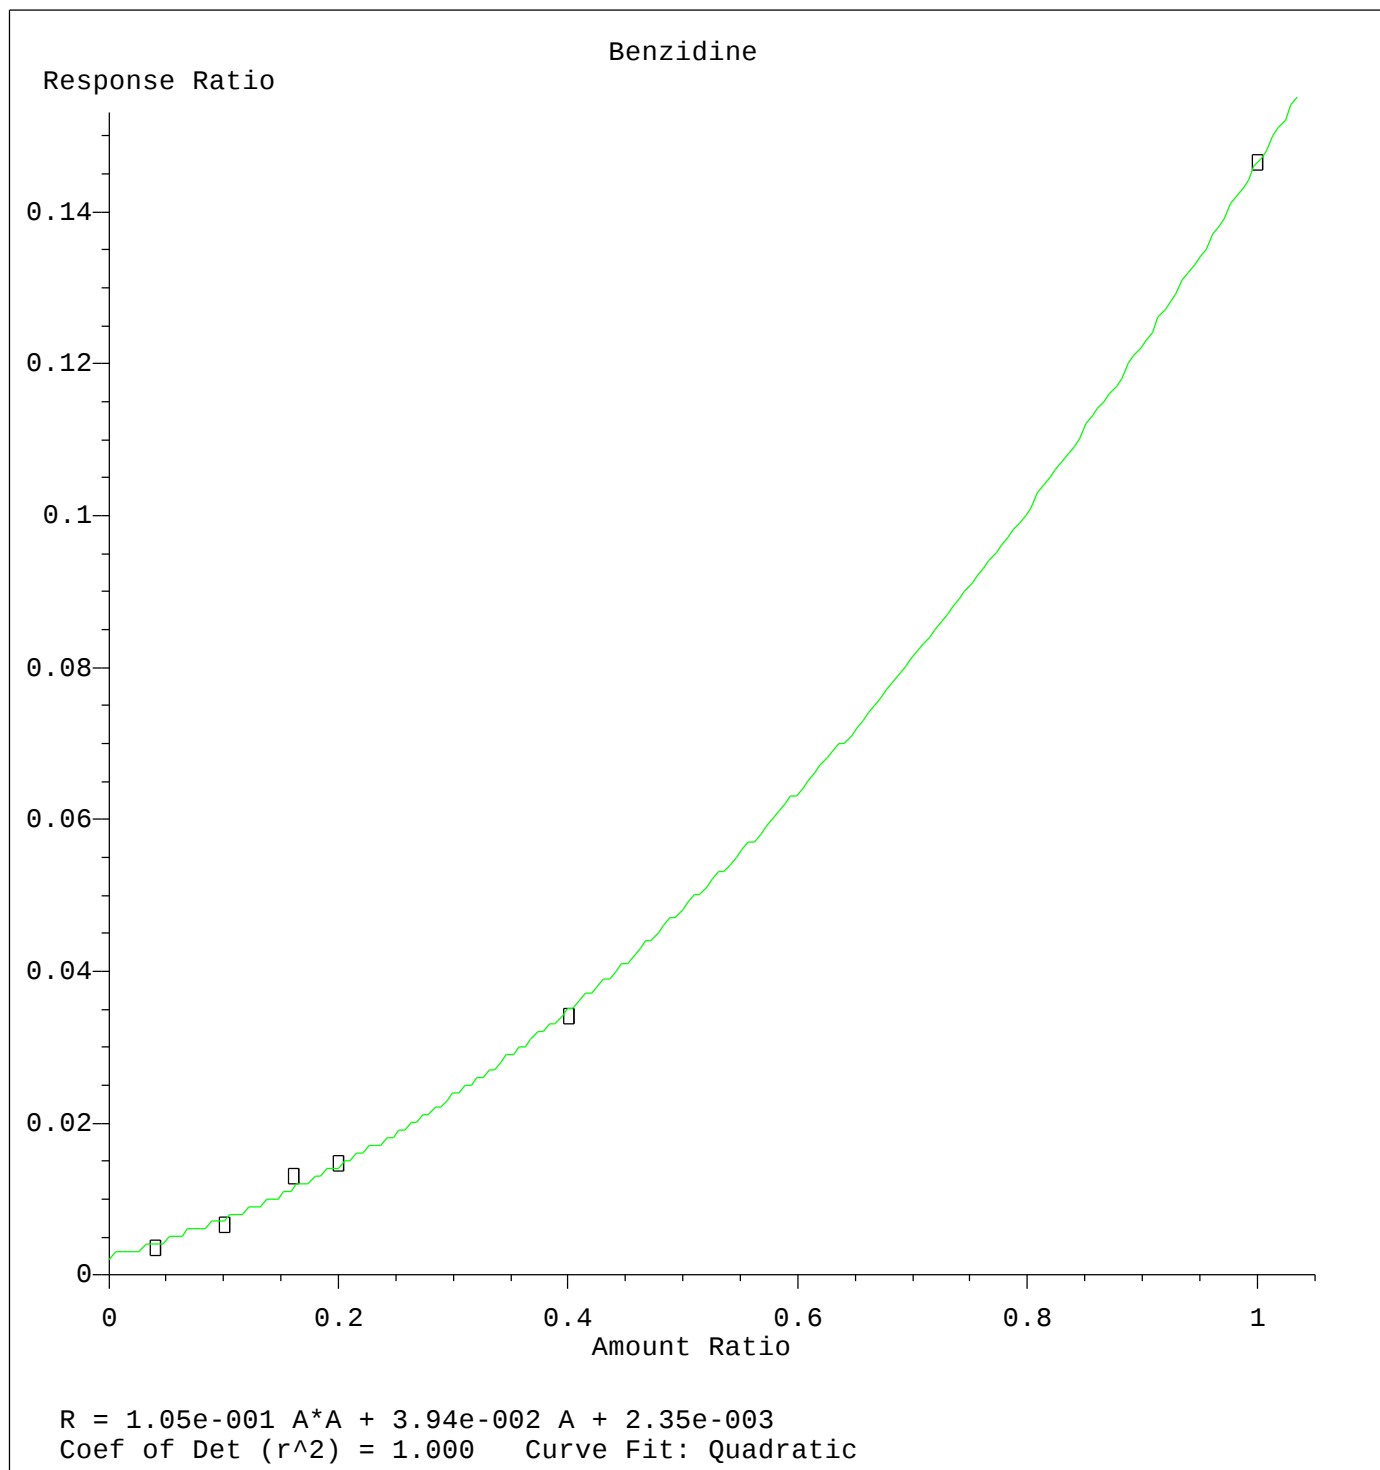


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

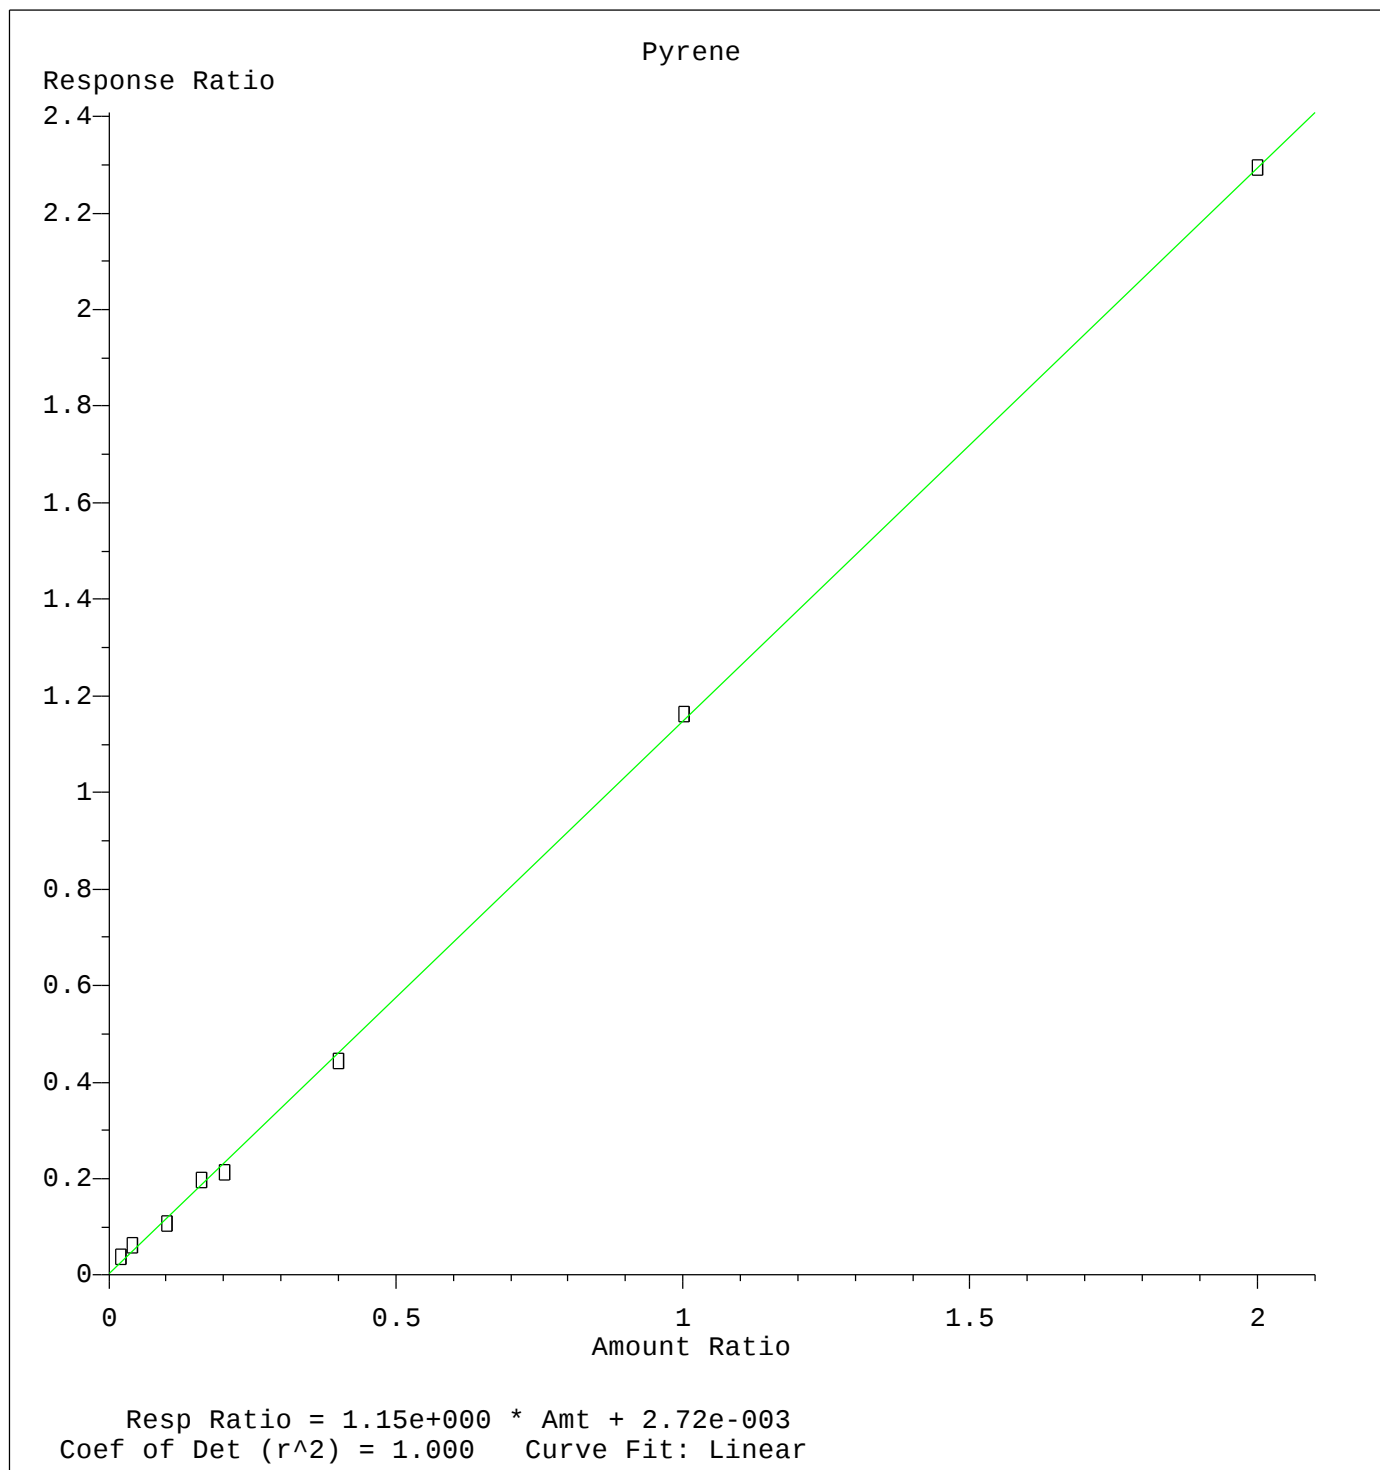


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

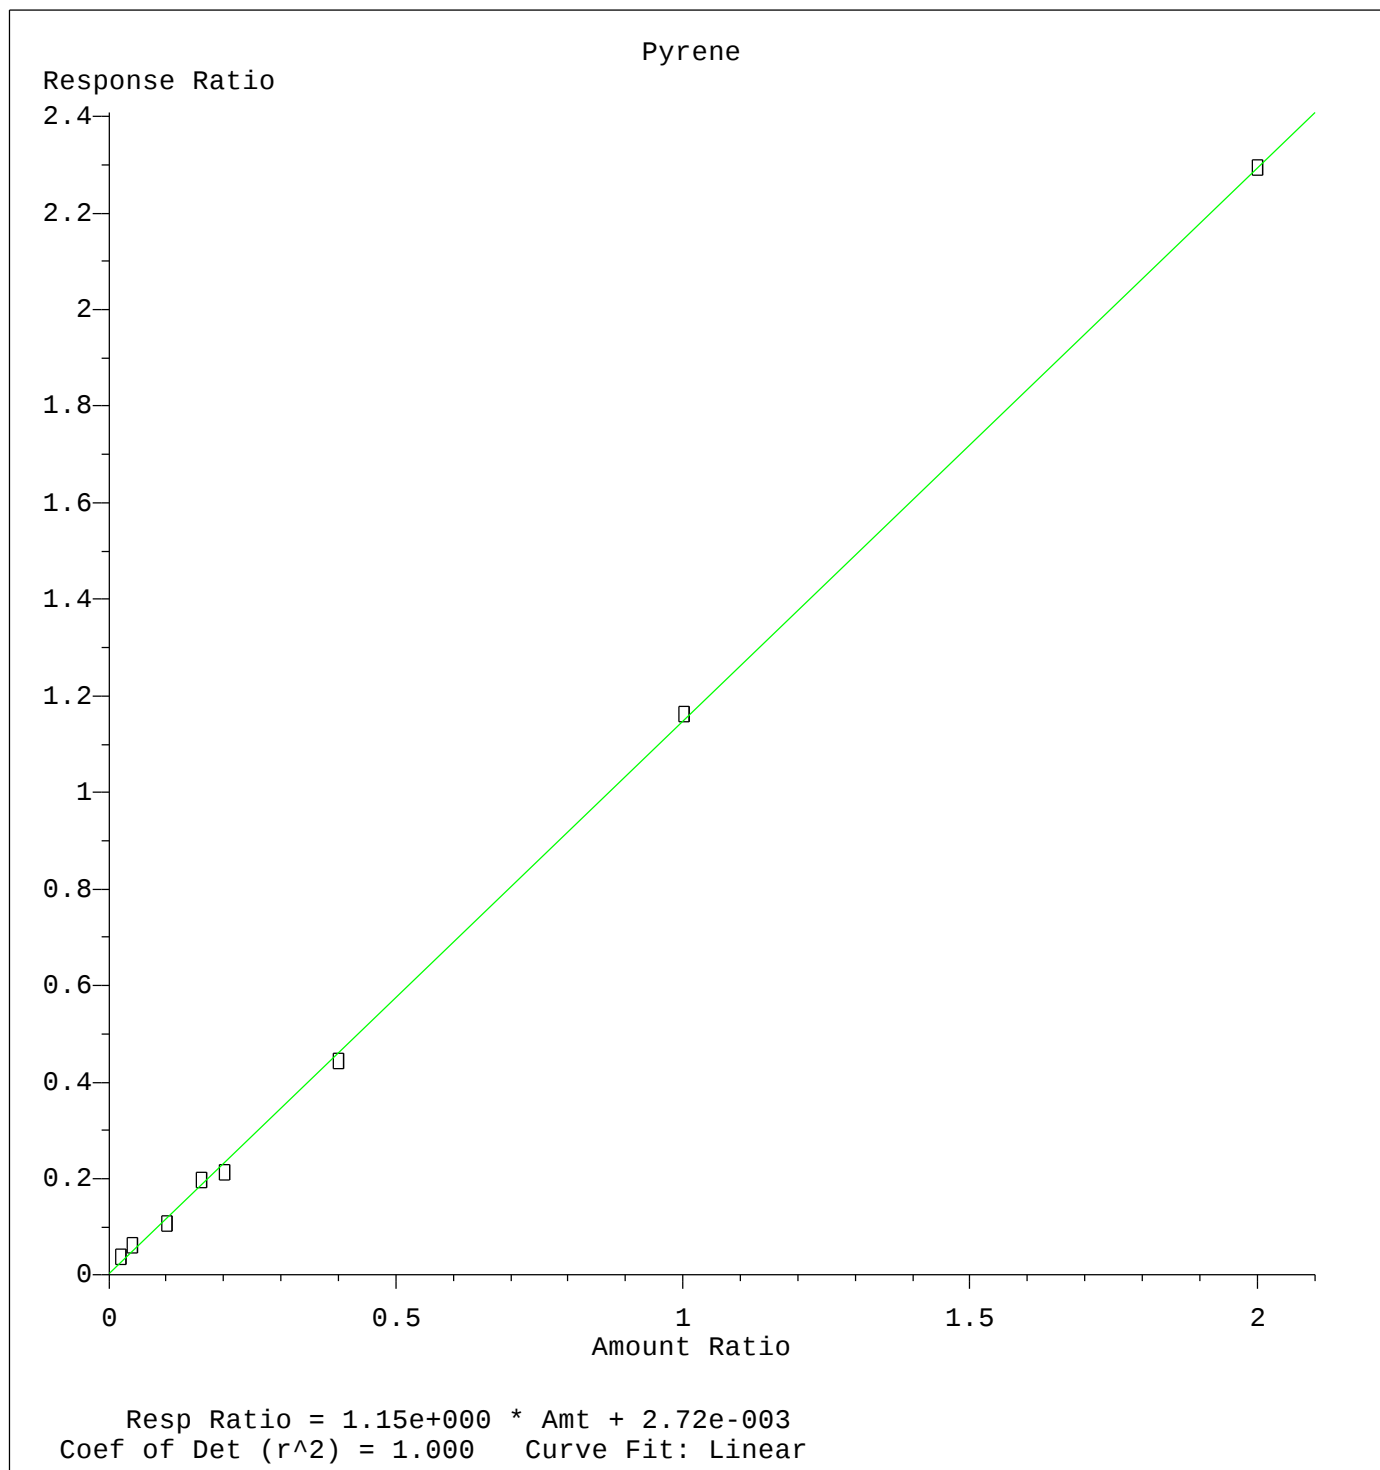

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

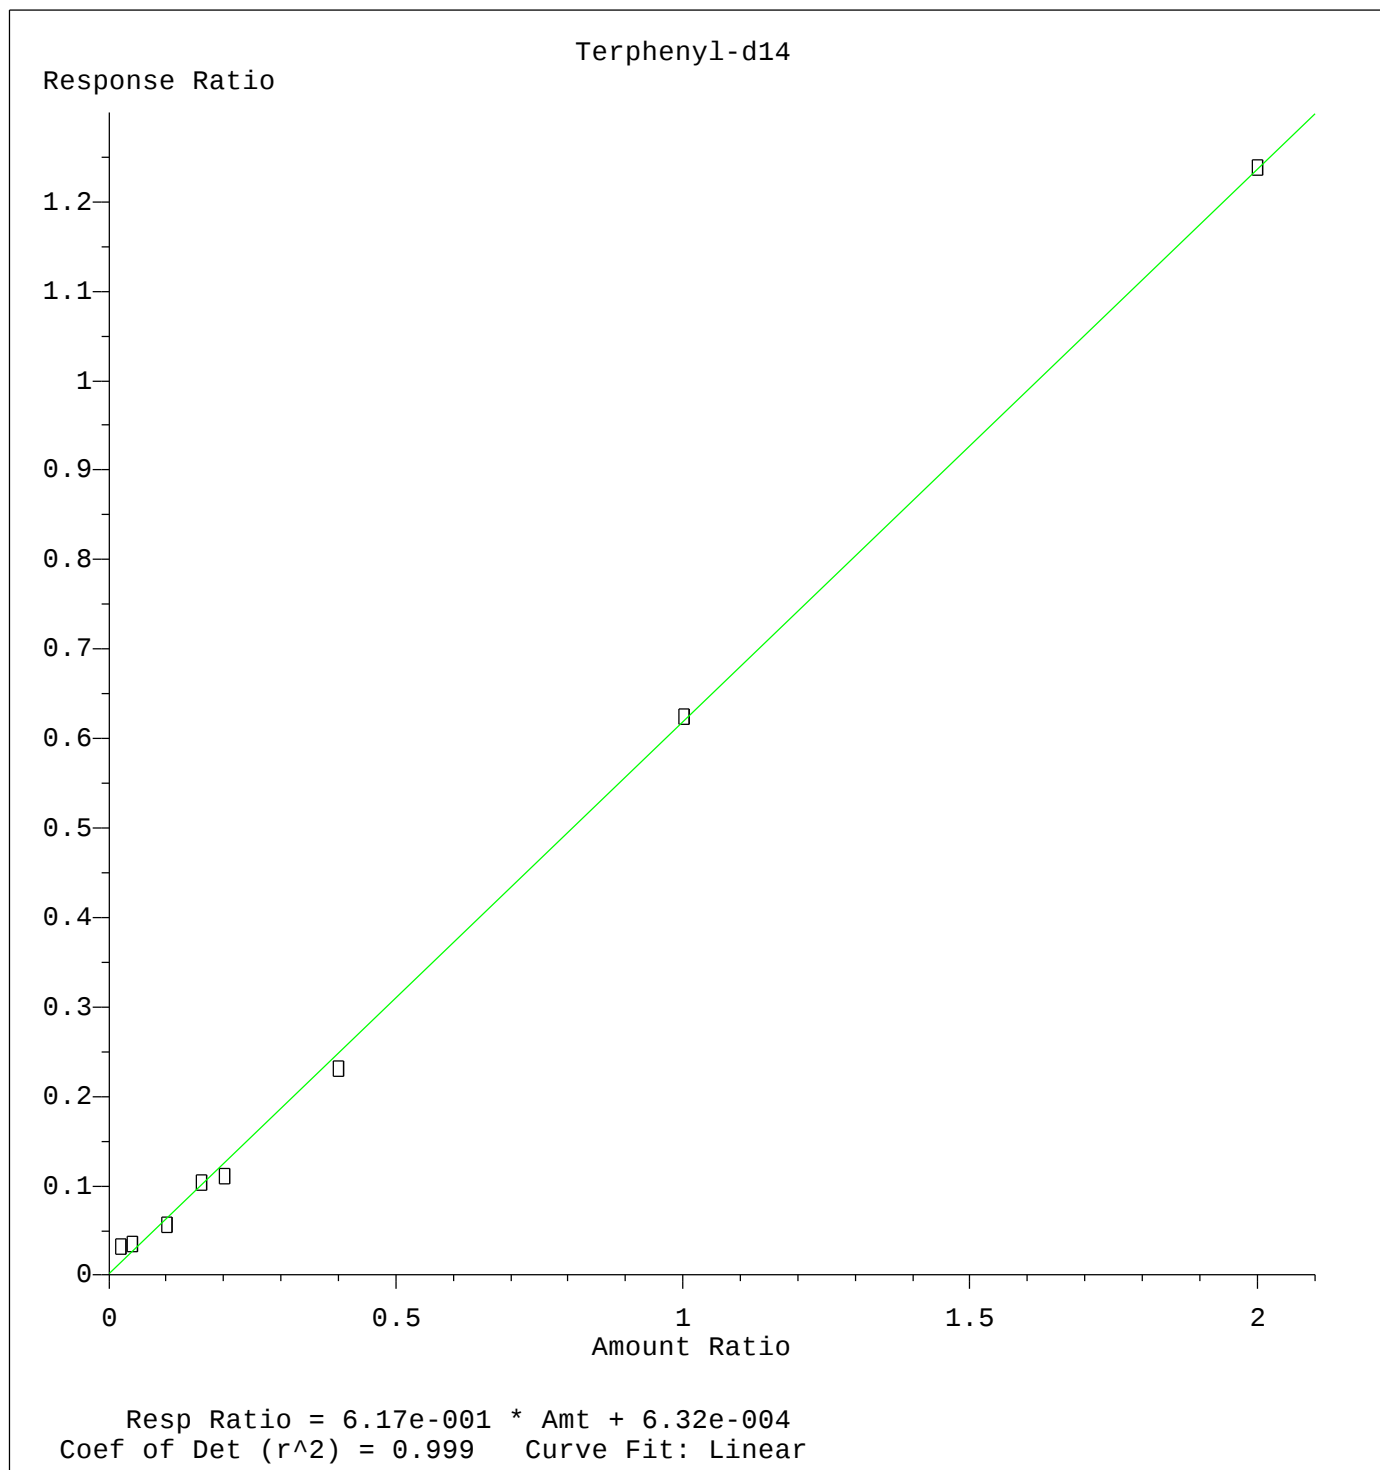


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

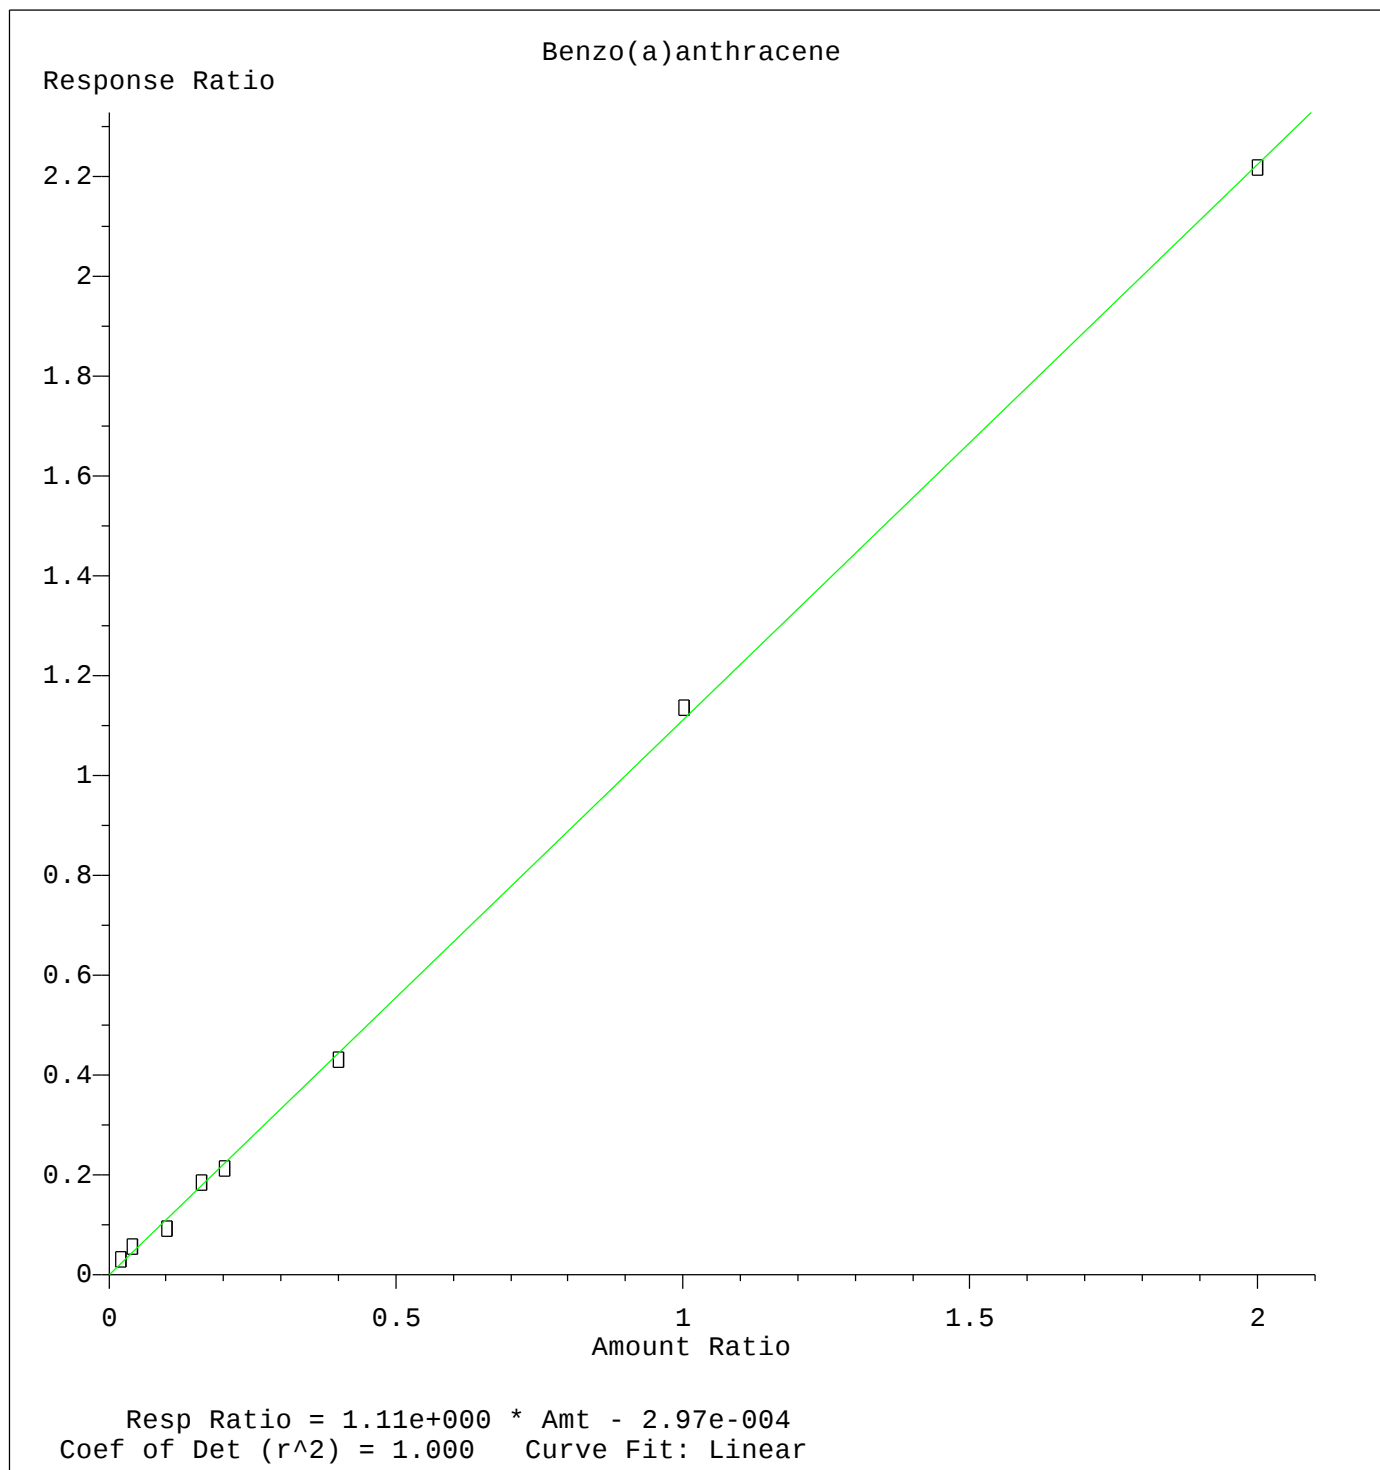


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

3,3'-Dichlorobenzidine

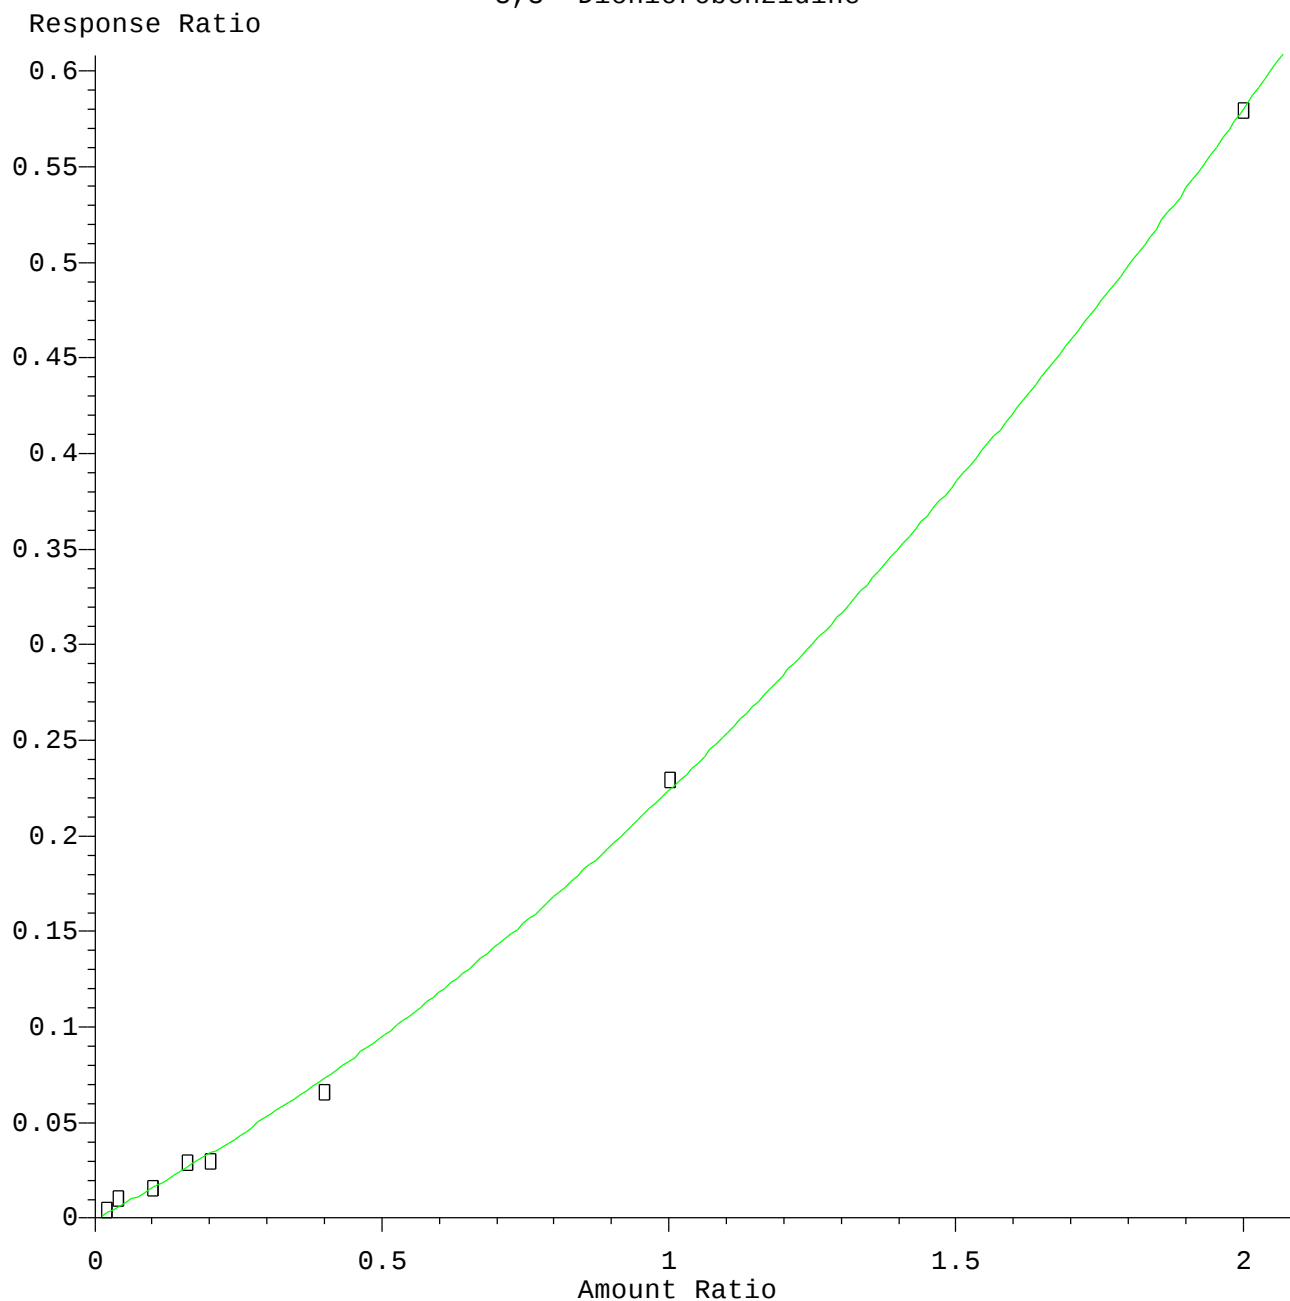

$R = 6.60e-002 A^2 + 1.58e-001 A - 6.99e-004$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

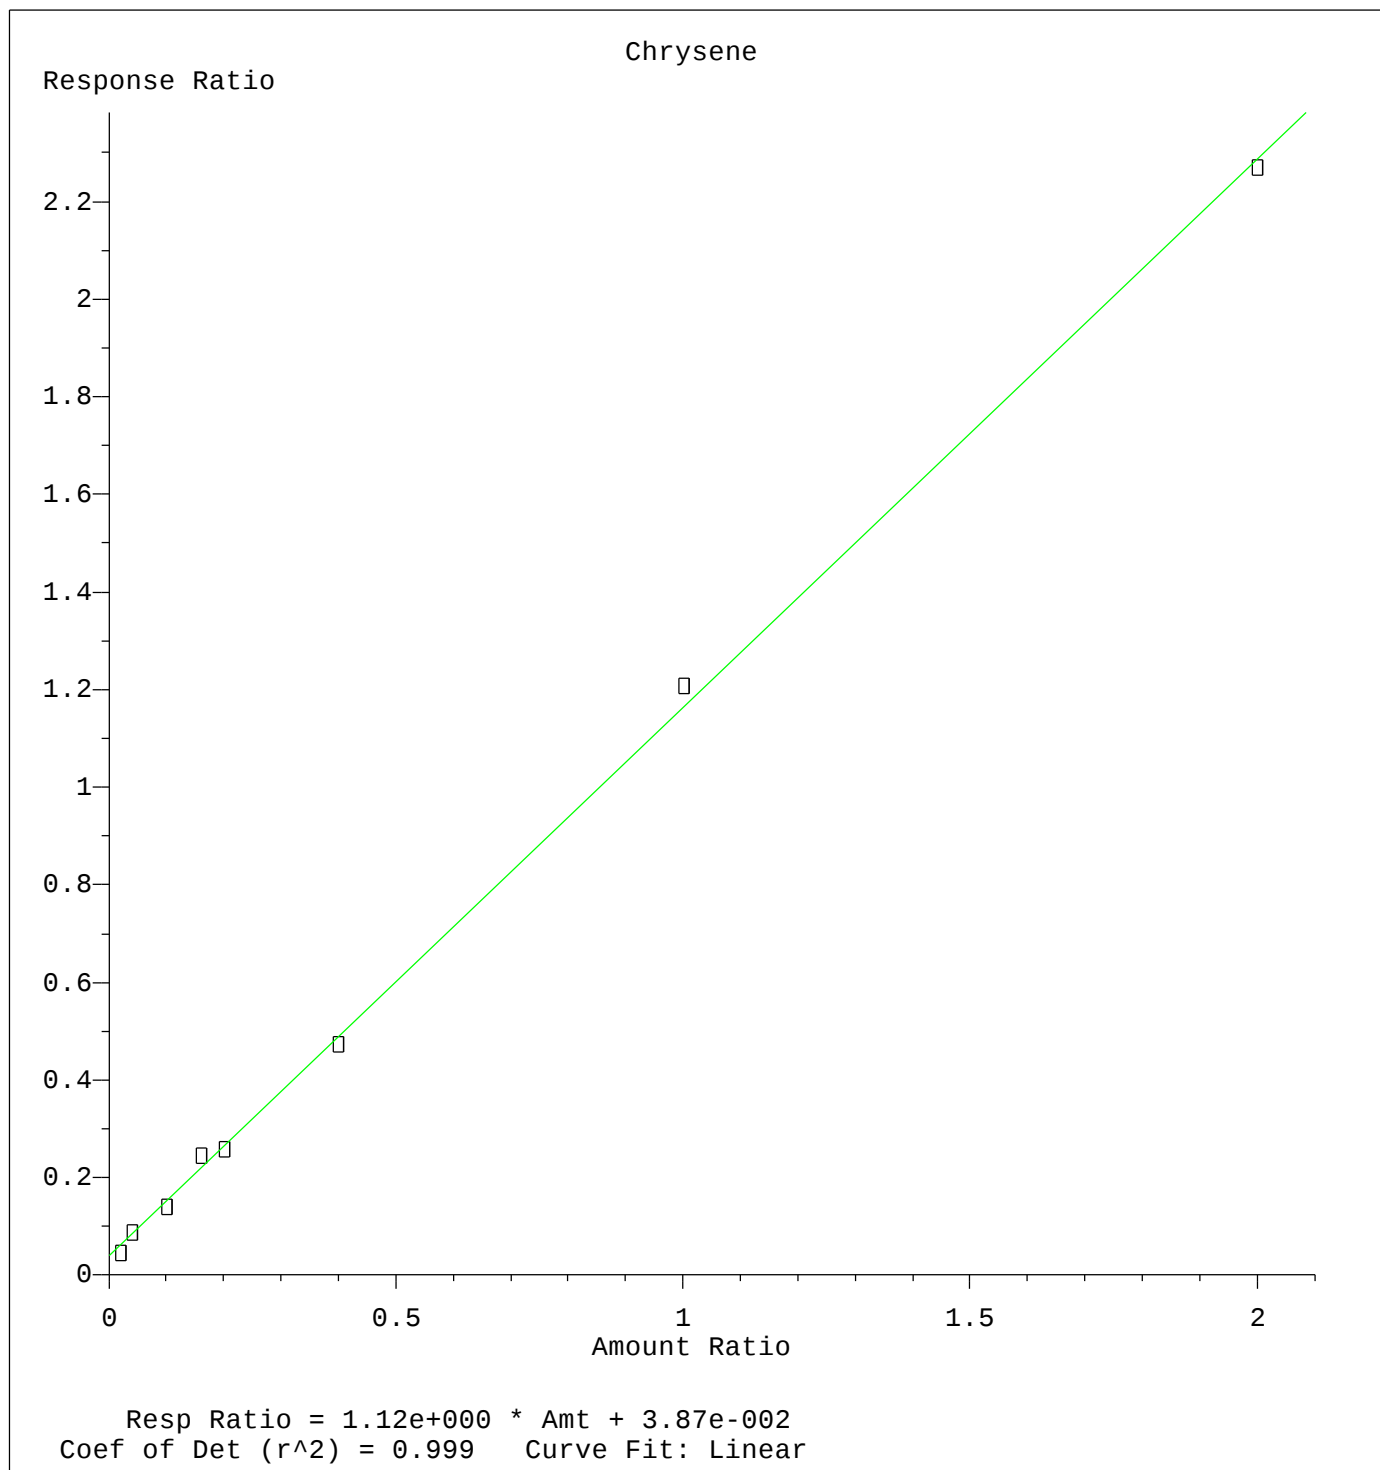

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

Bis(2-ethylhexyl)phthalate

Response Ratio

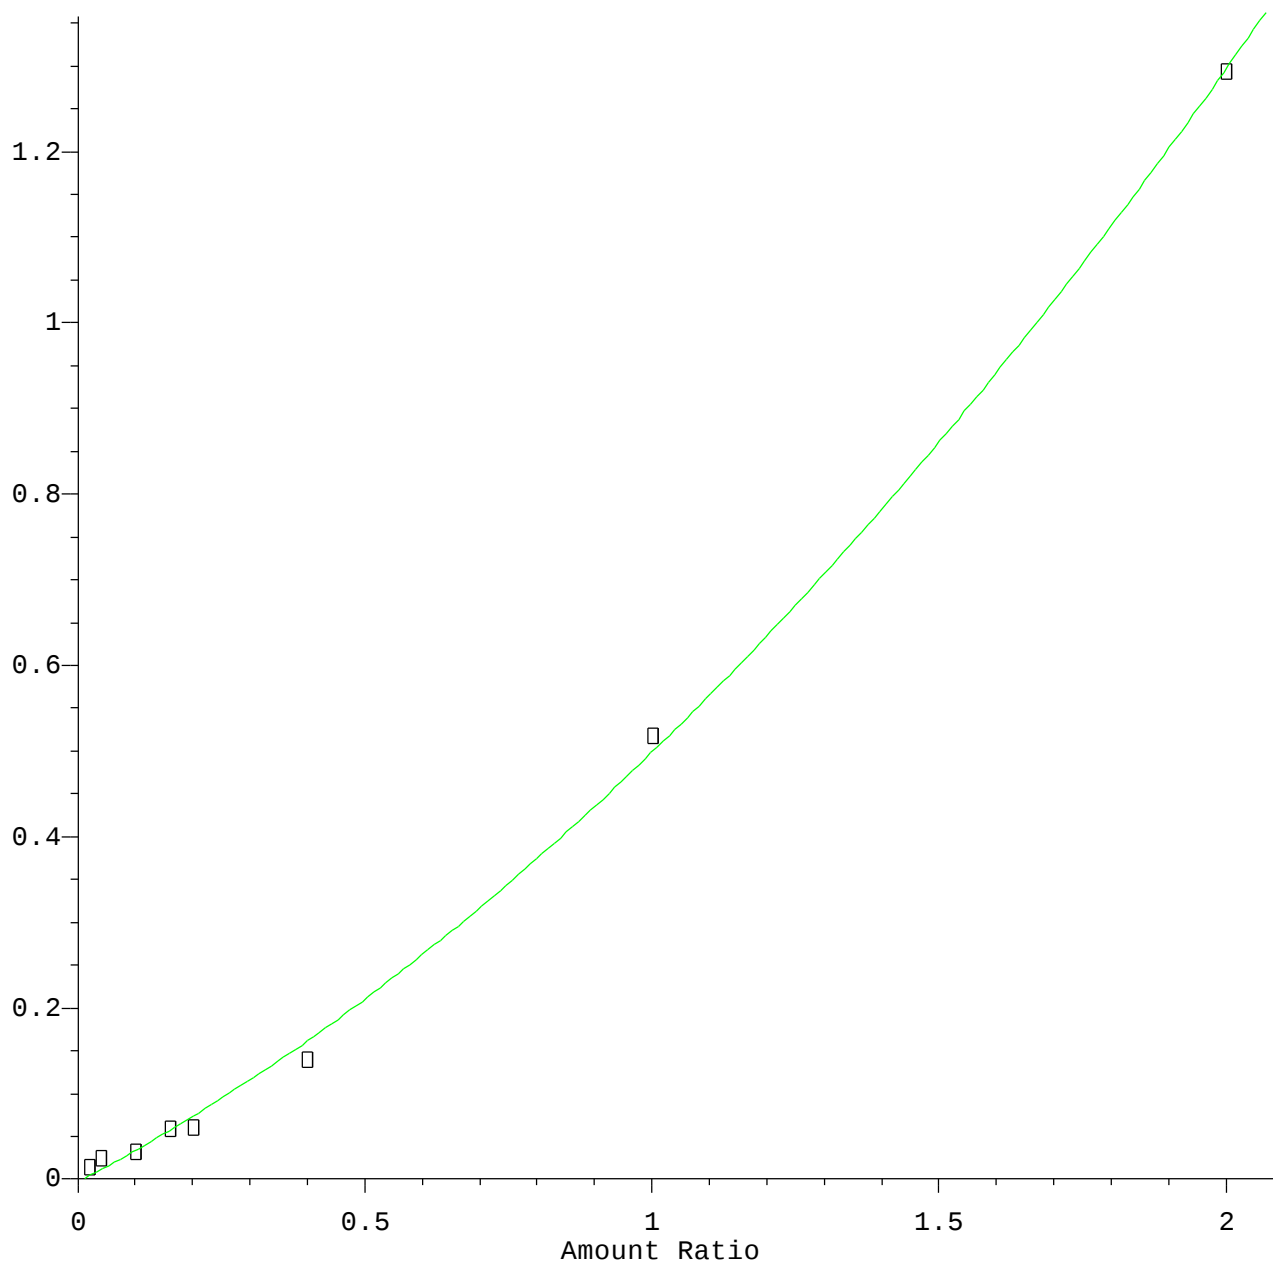


$R = 1.48e-001 A^2 + 3.54e-001 A - 3.56e-003$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015


Indeno(1,2,3-cd)pyrene

Response Ratio

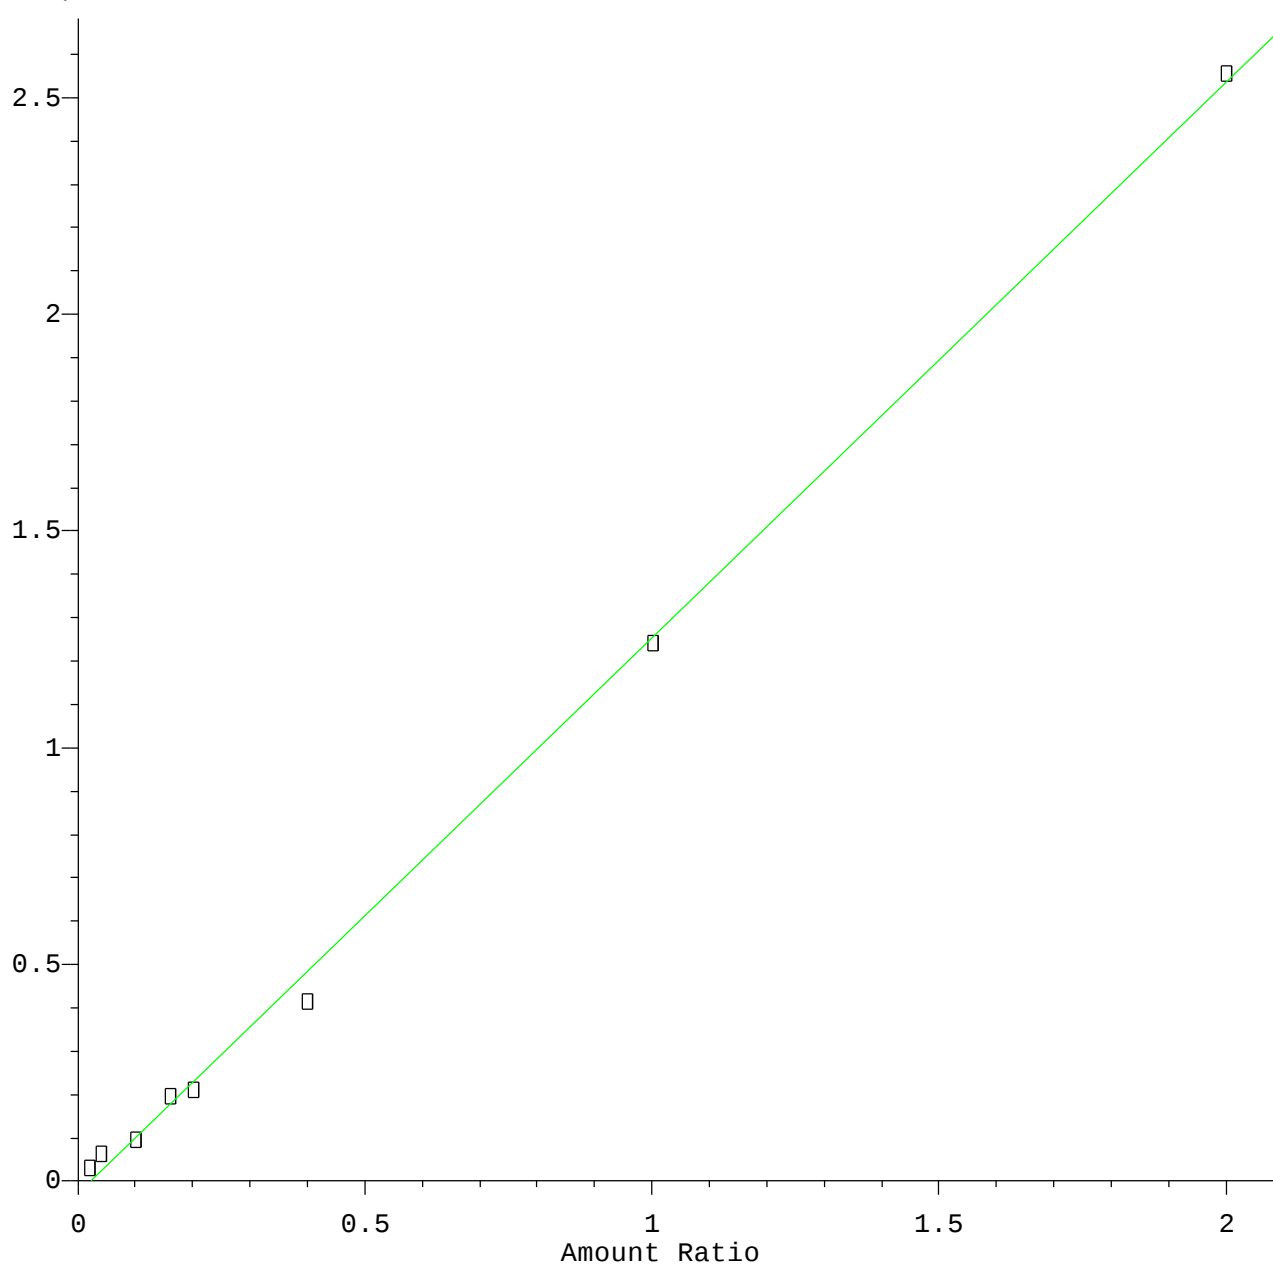


Resp Ratio = 1.28e+000 * Amt - 2.83e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

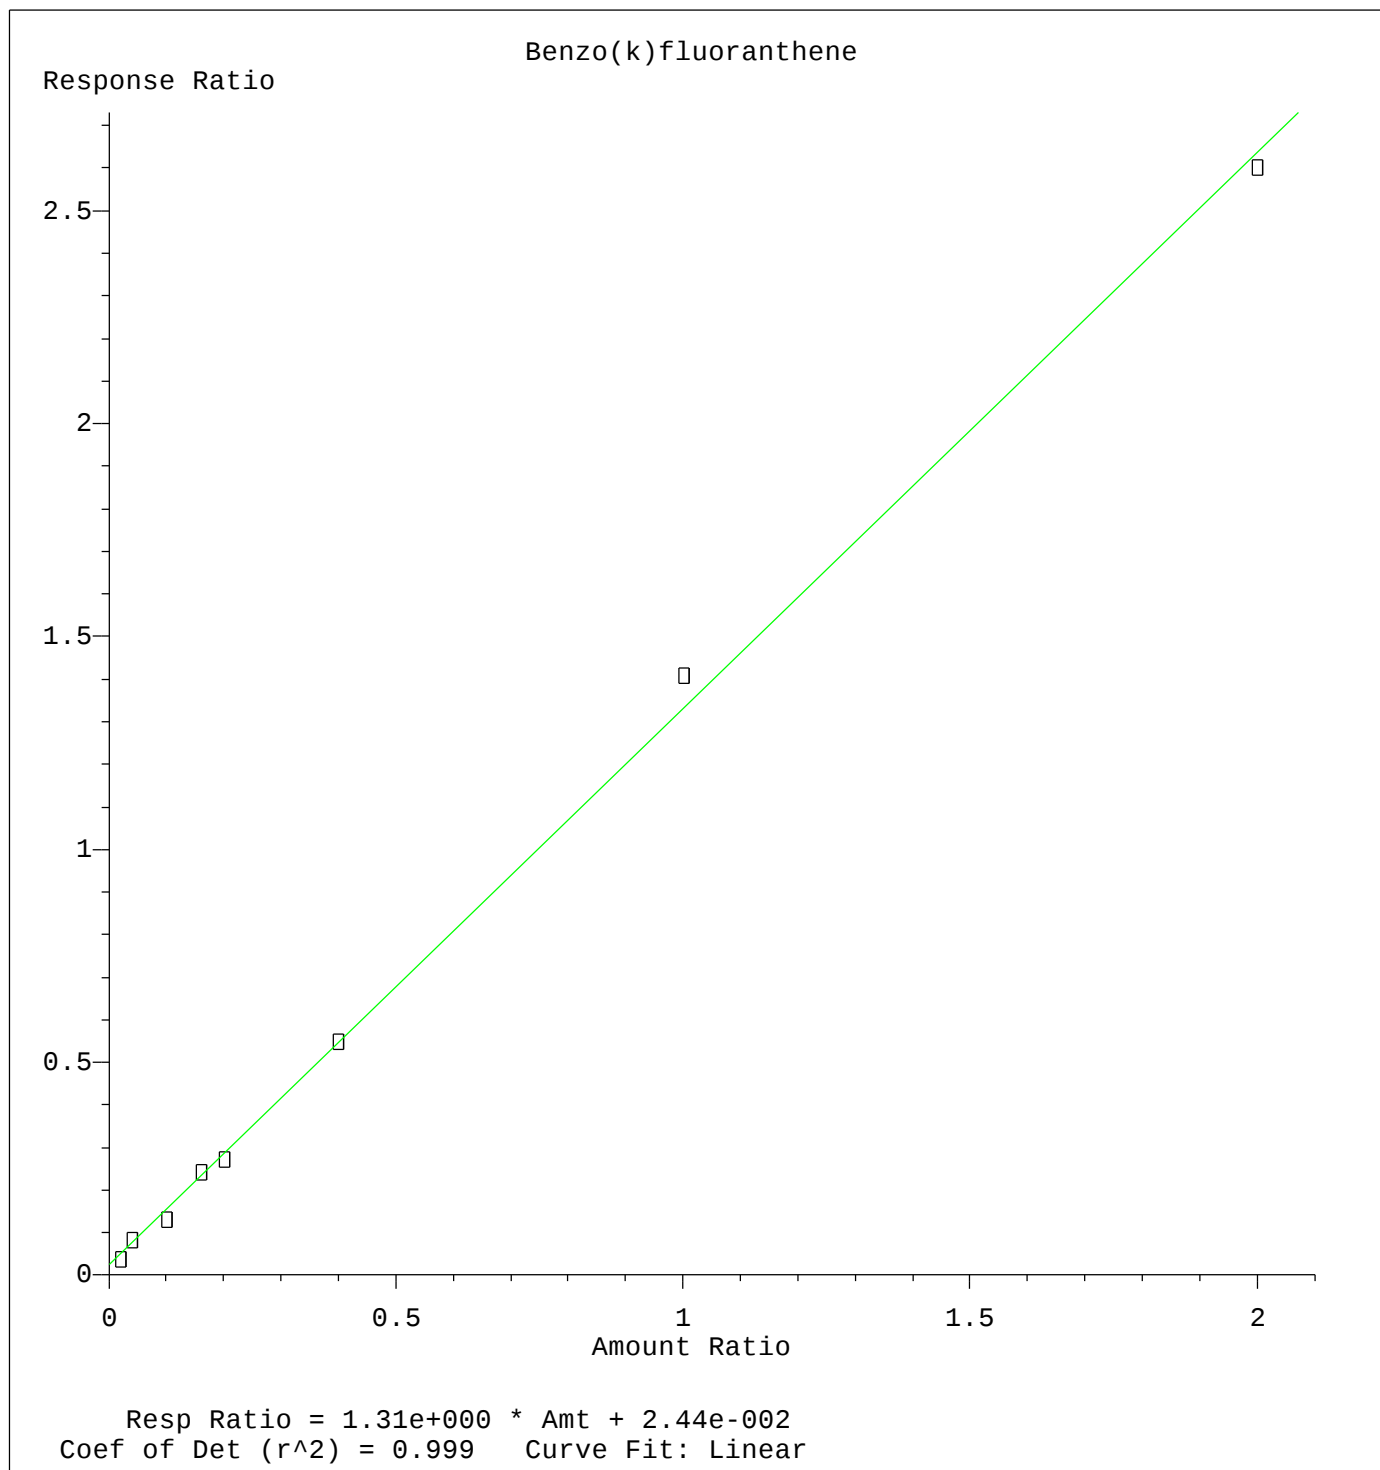


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

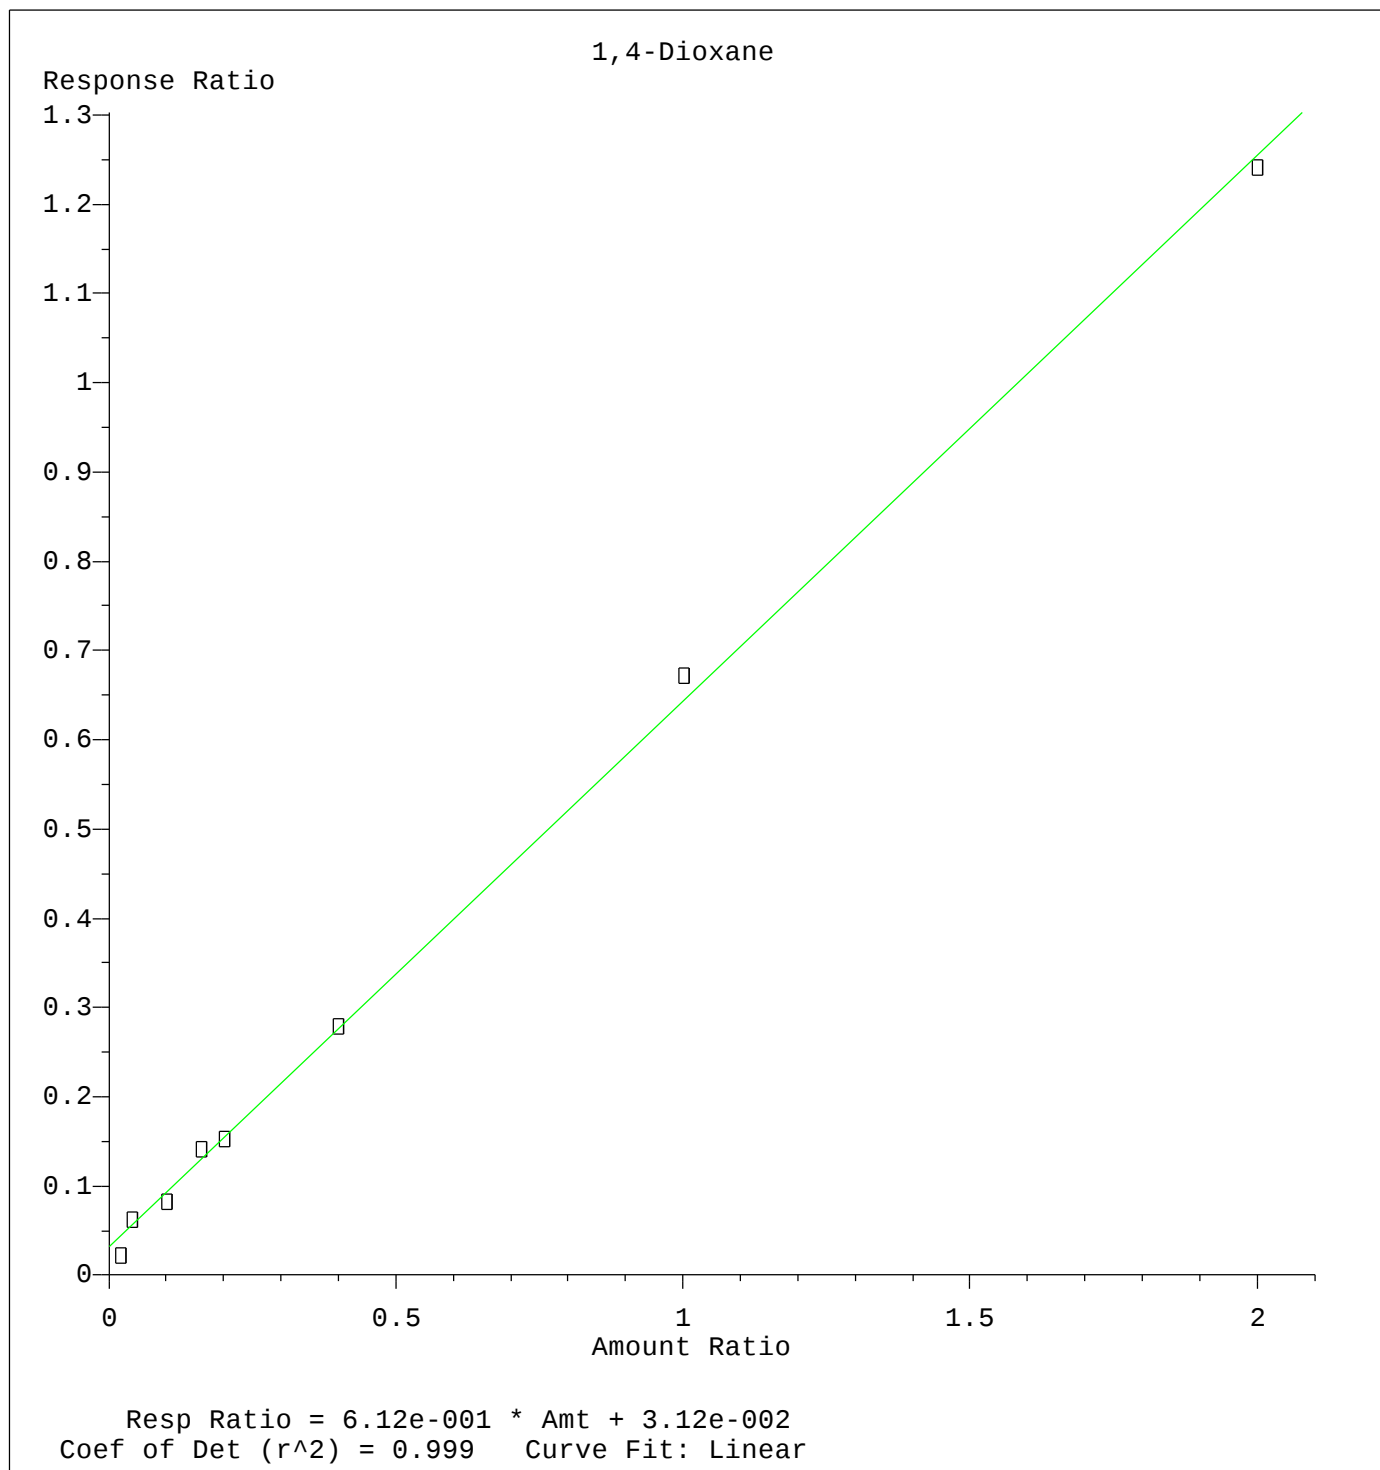

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

n-Nitrosodimethylamine

Response Ratio

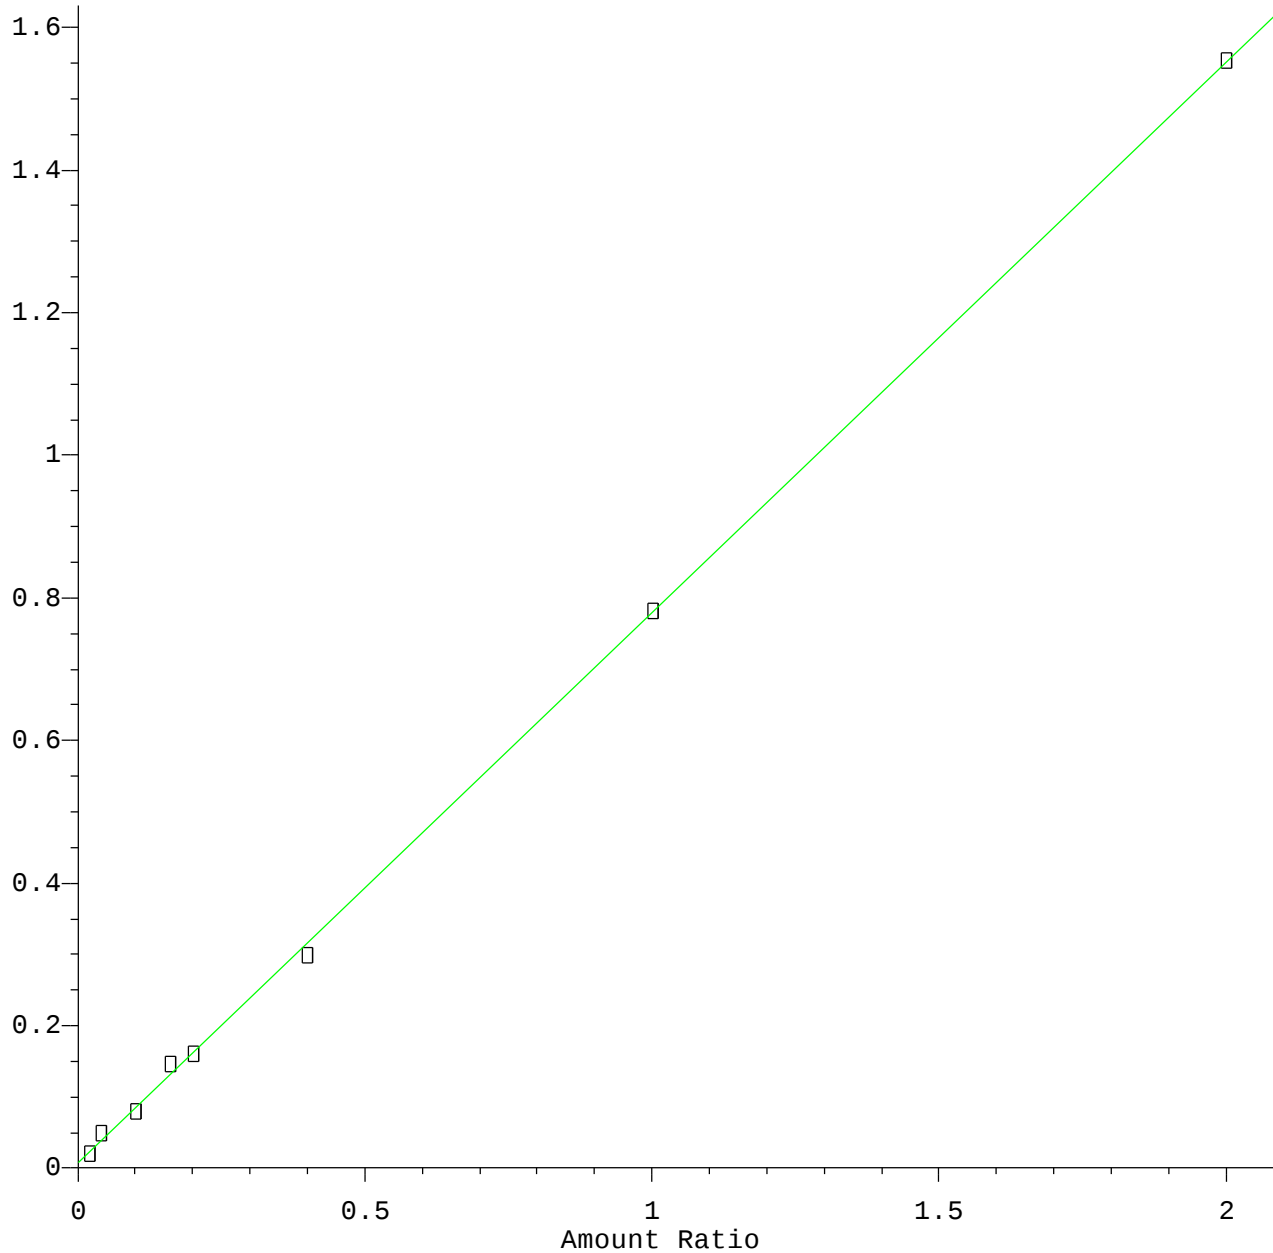


Resp Ratio = $7.72 \times 10^{-1} \times \text{Amt} + 7.44 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

2-Fluorophenol

Response Ratio

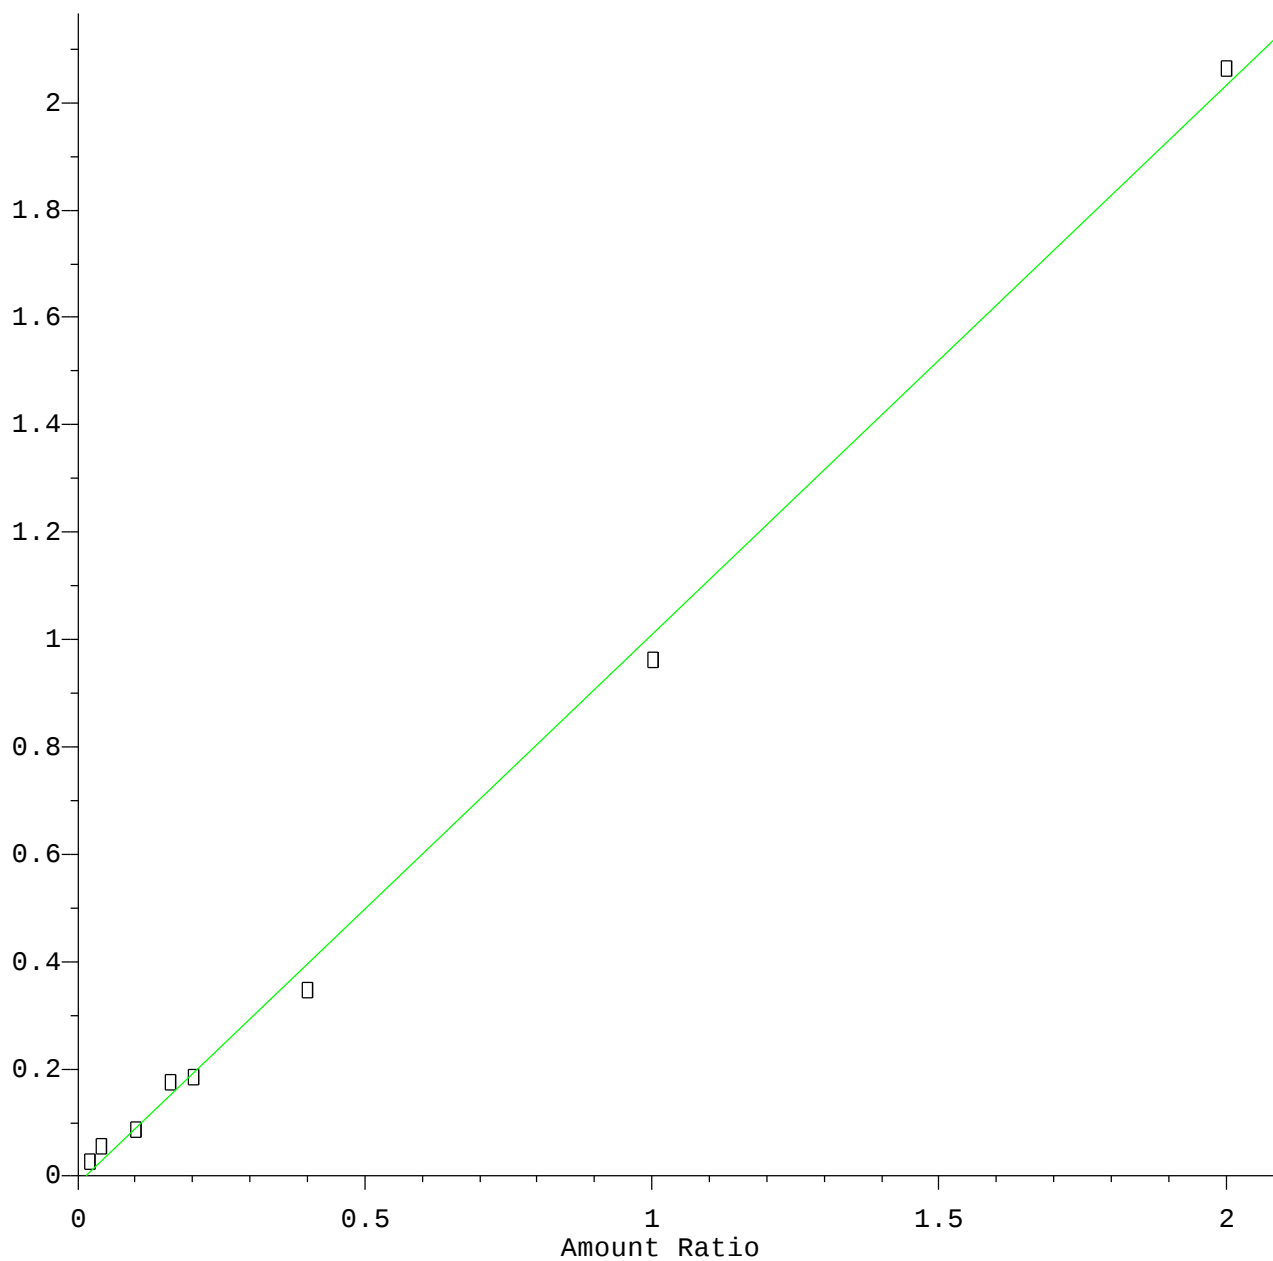


Resp Ratio = 1.02×10^0 * Amt - 1.46×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015


bis(2-Chloroethyl)ether

Response Ratio

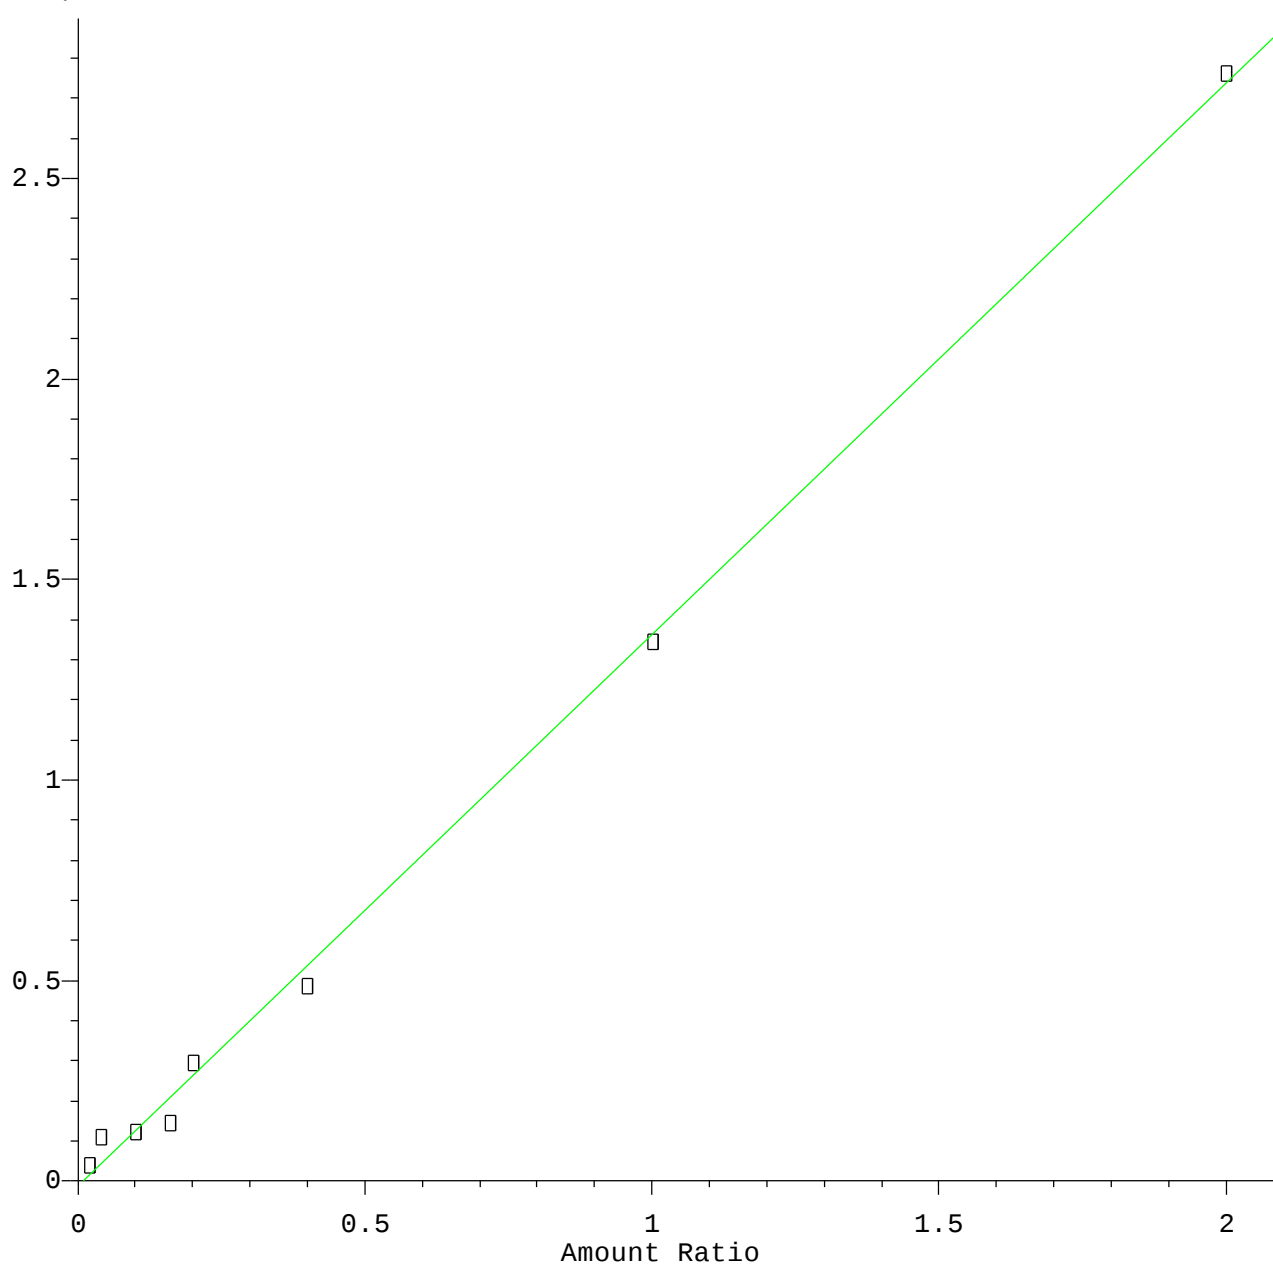


Resp Ratio = 1.37e+000 * Amt - 1.21e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

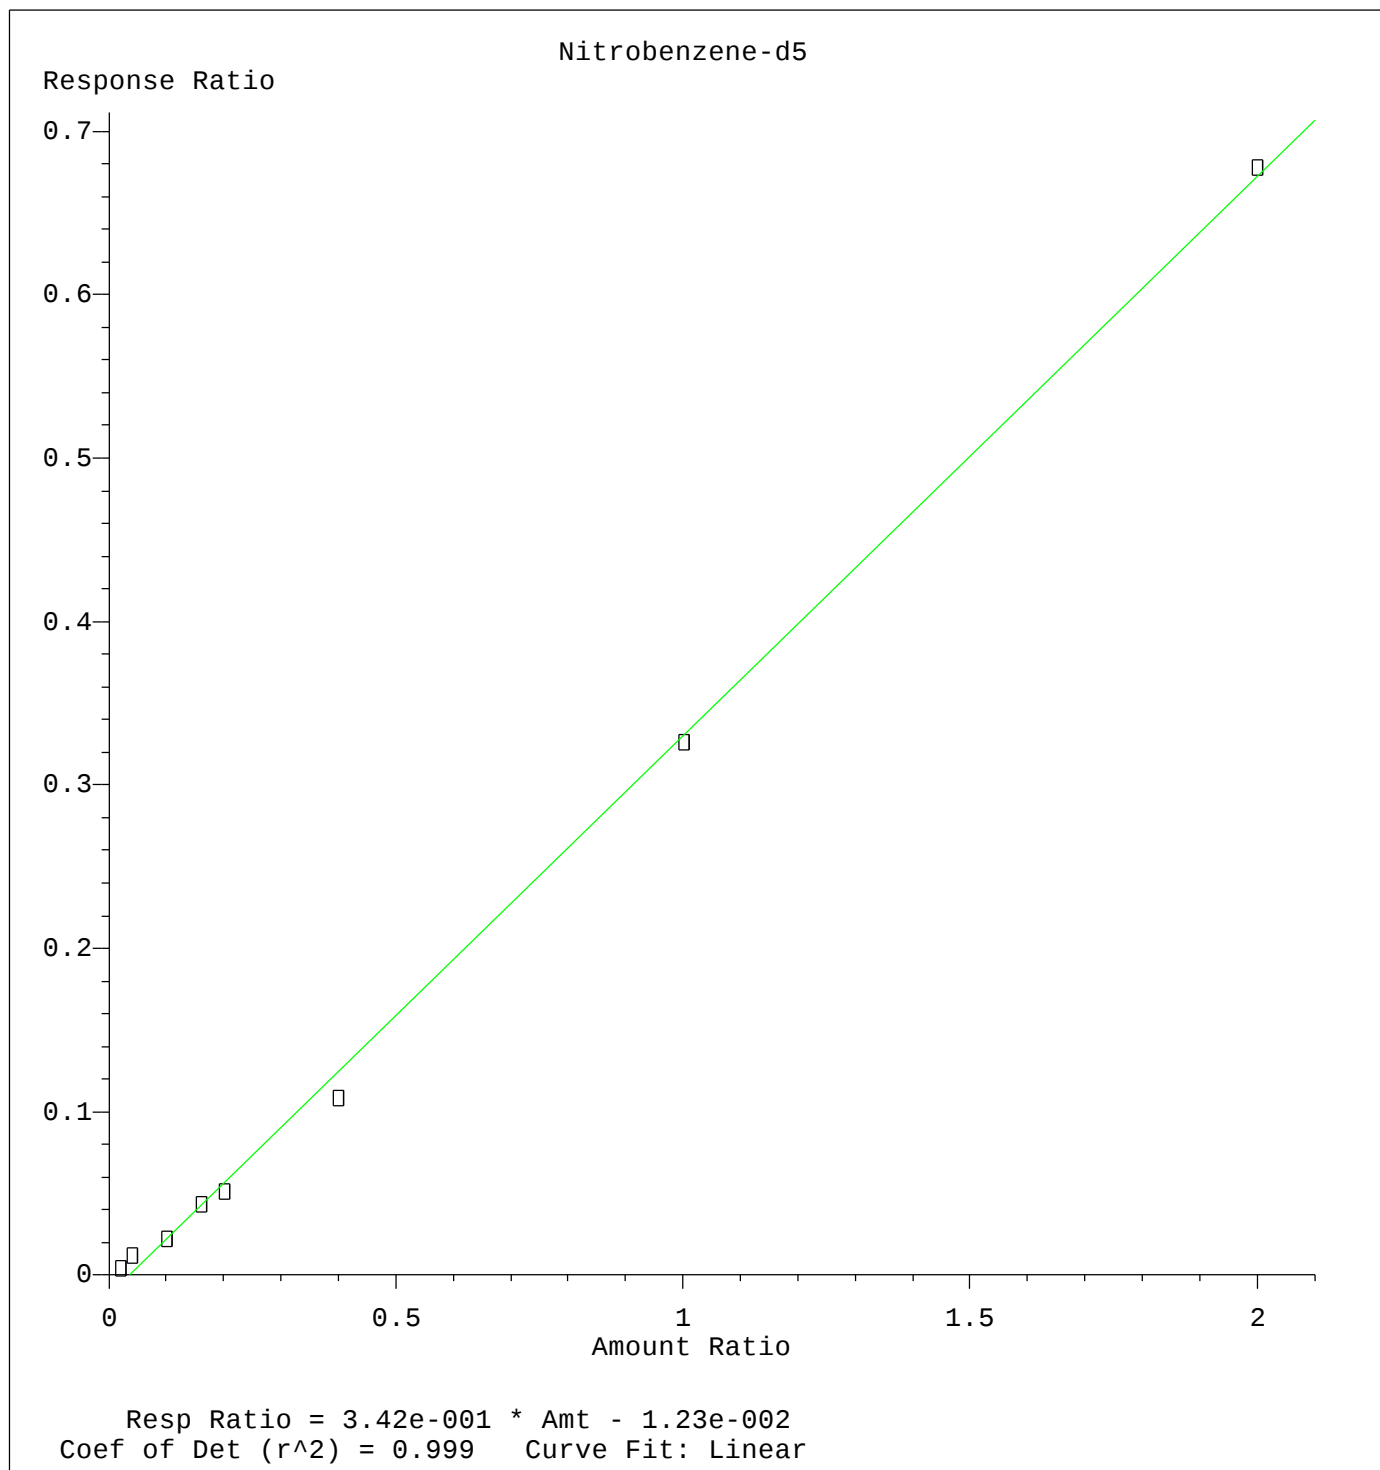


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

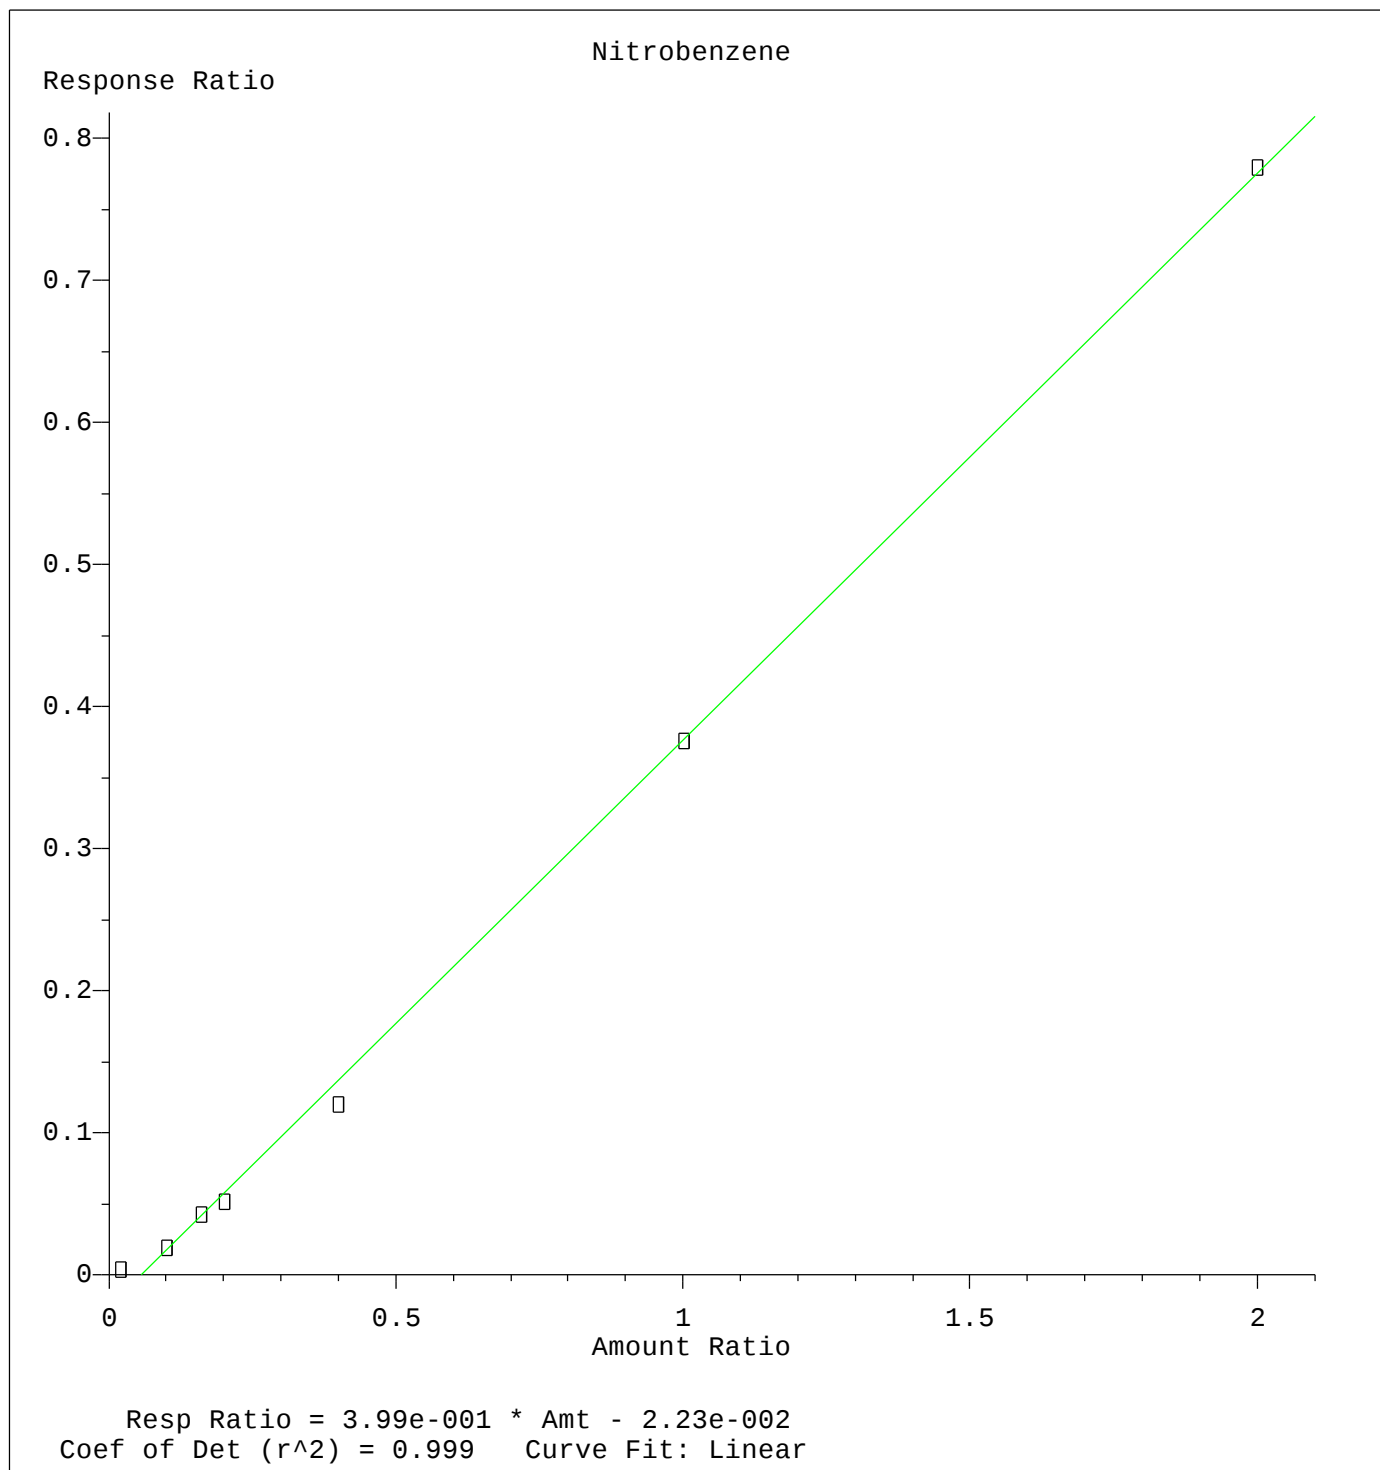


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

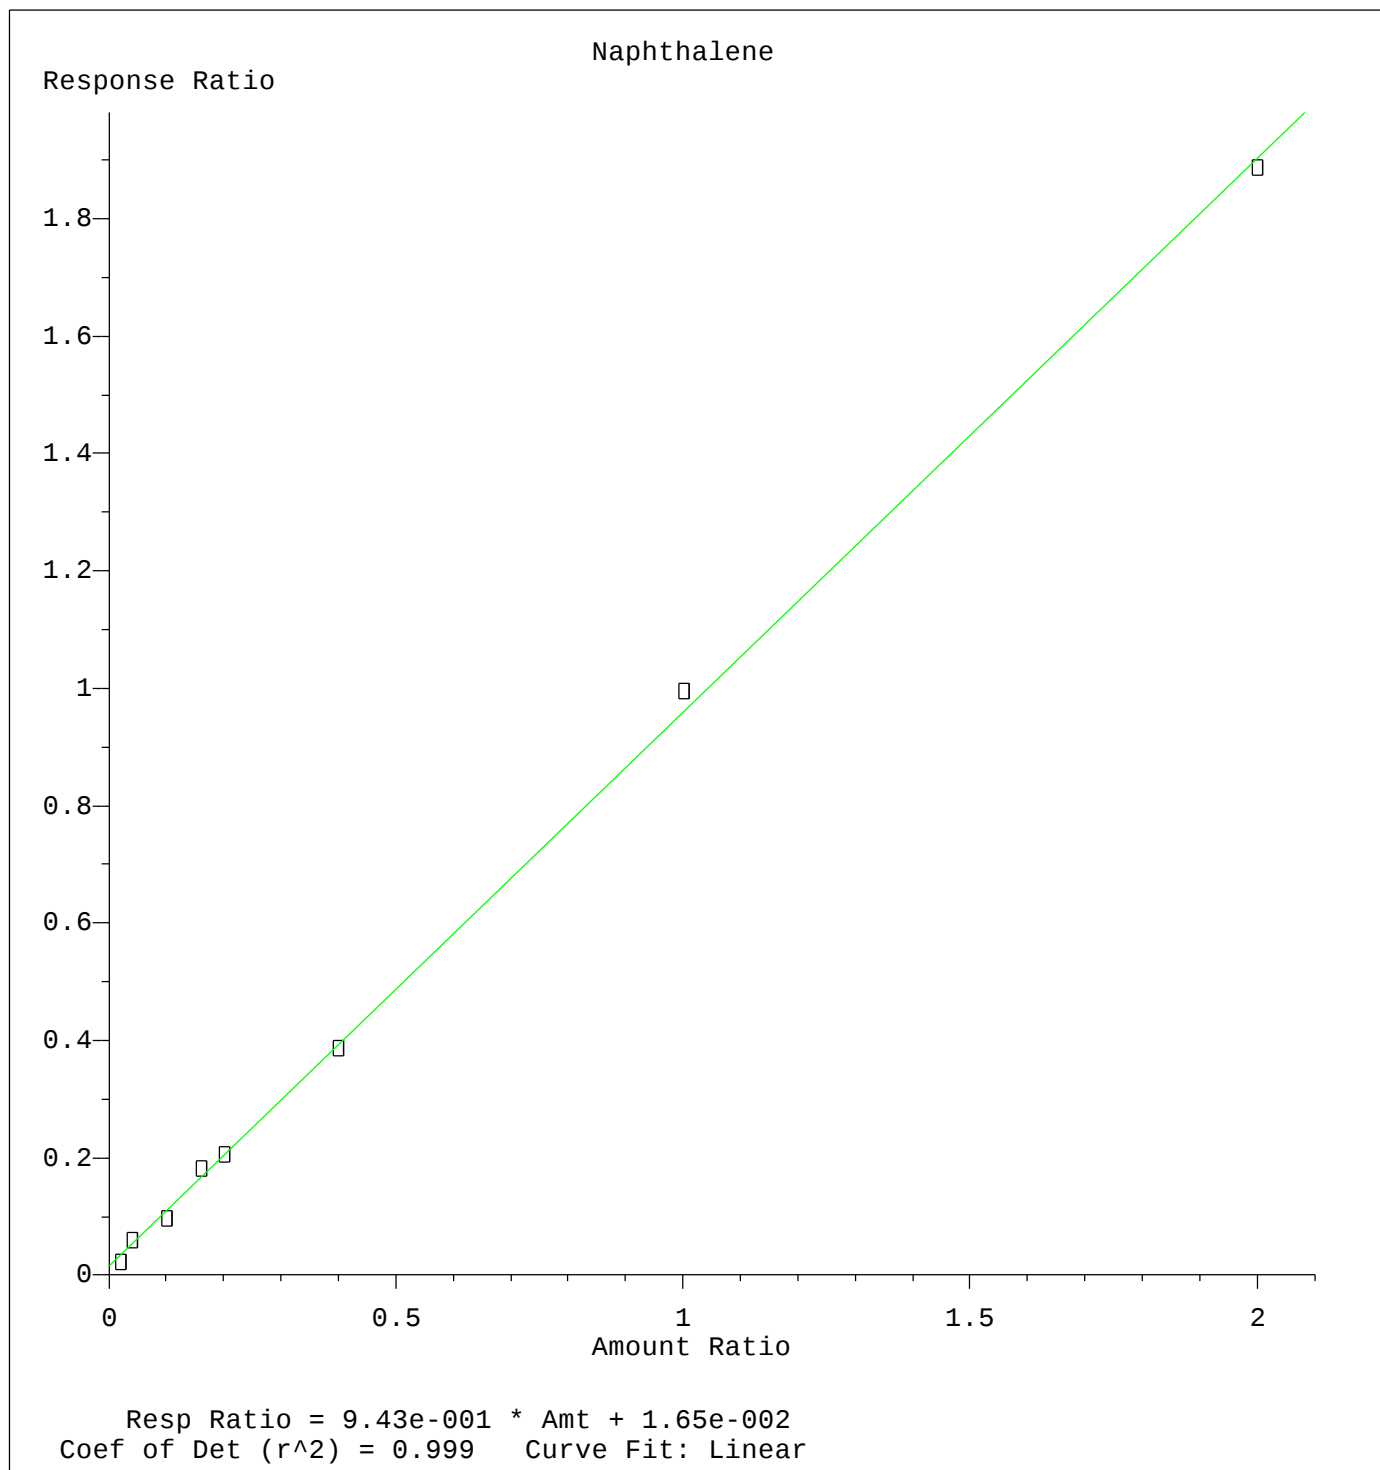

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

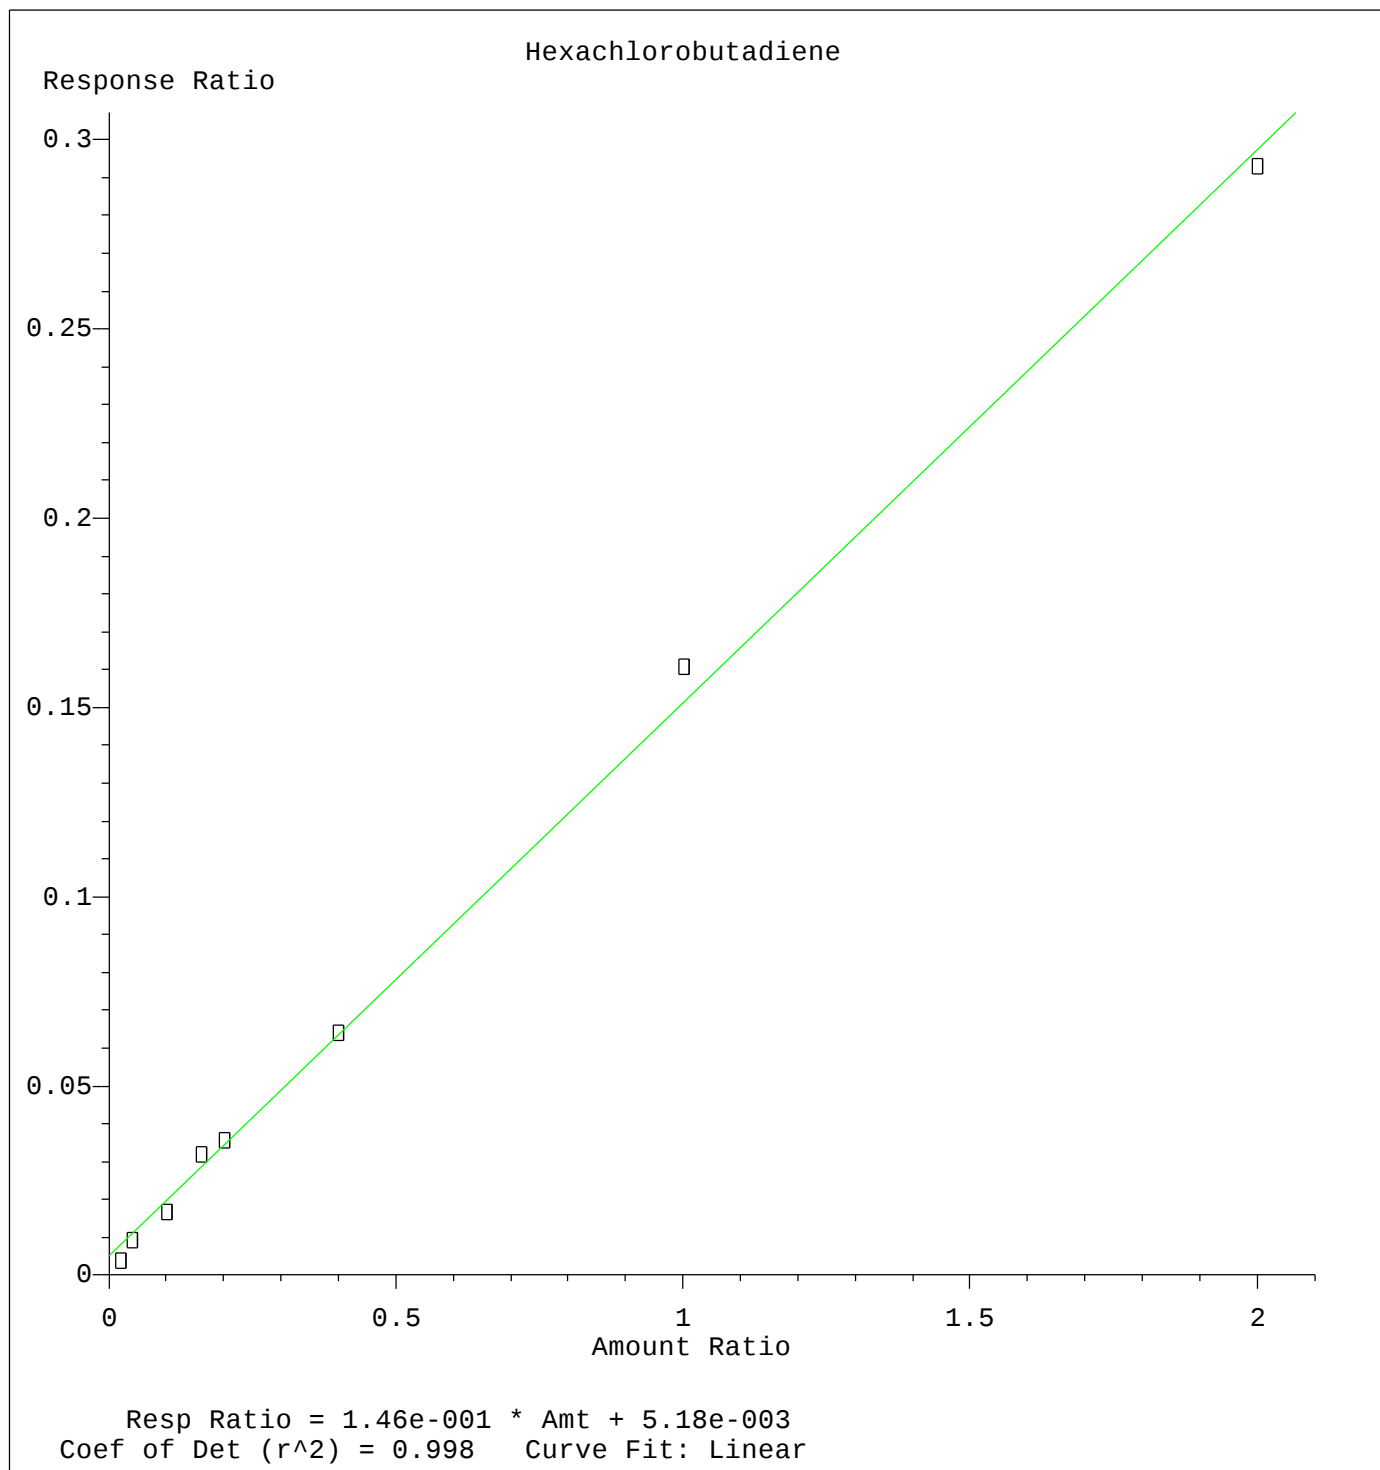


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

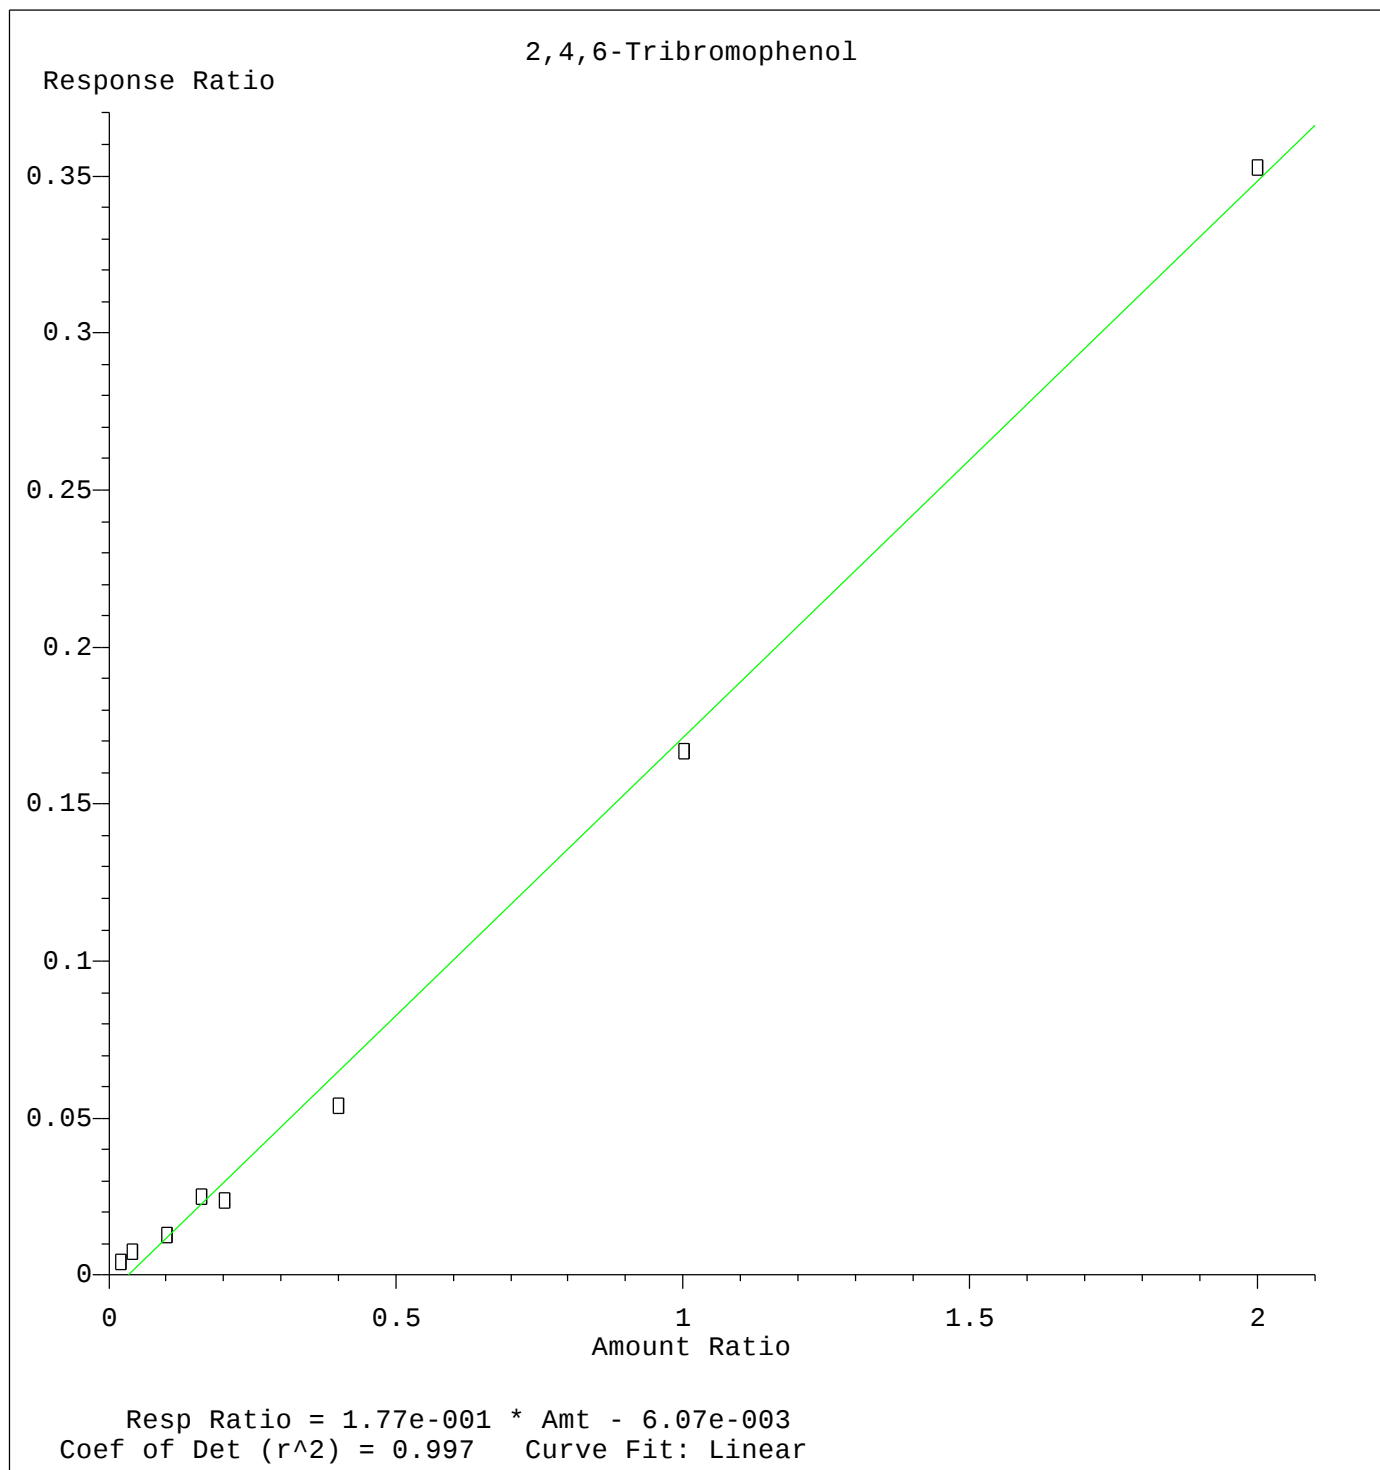

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015


Hexachlorobenzene

Response Ratio

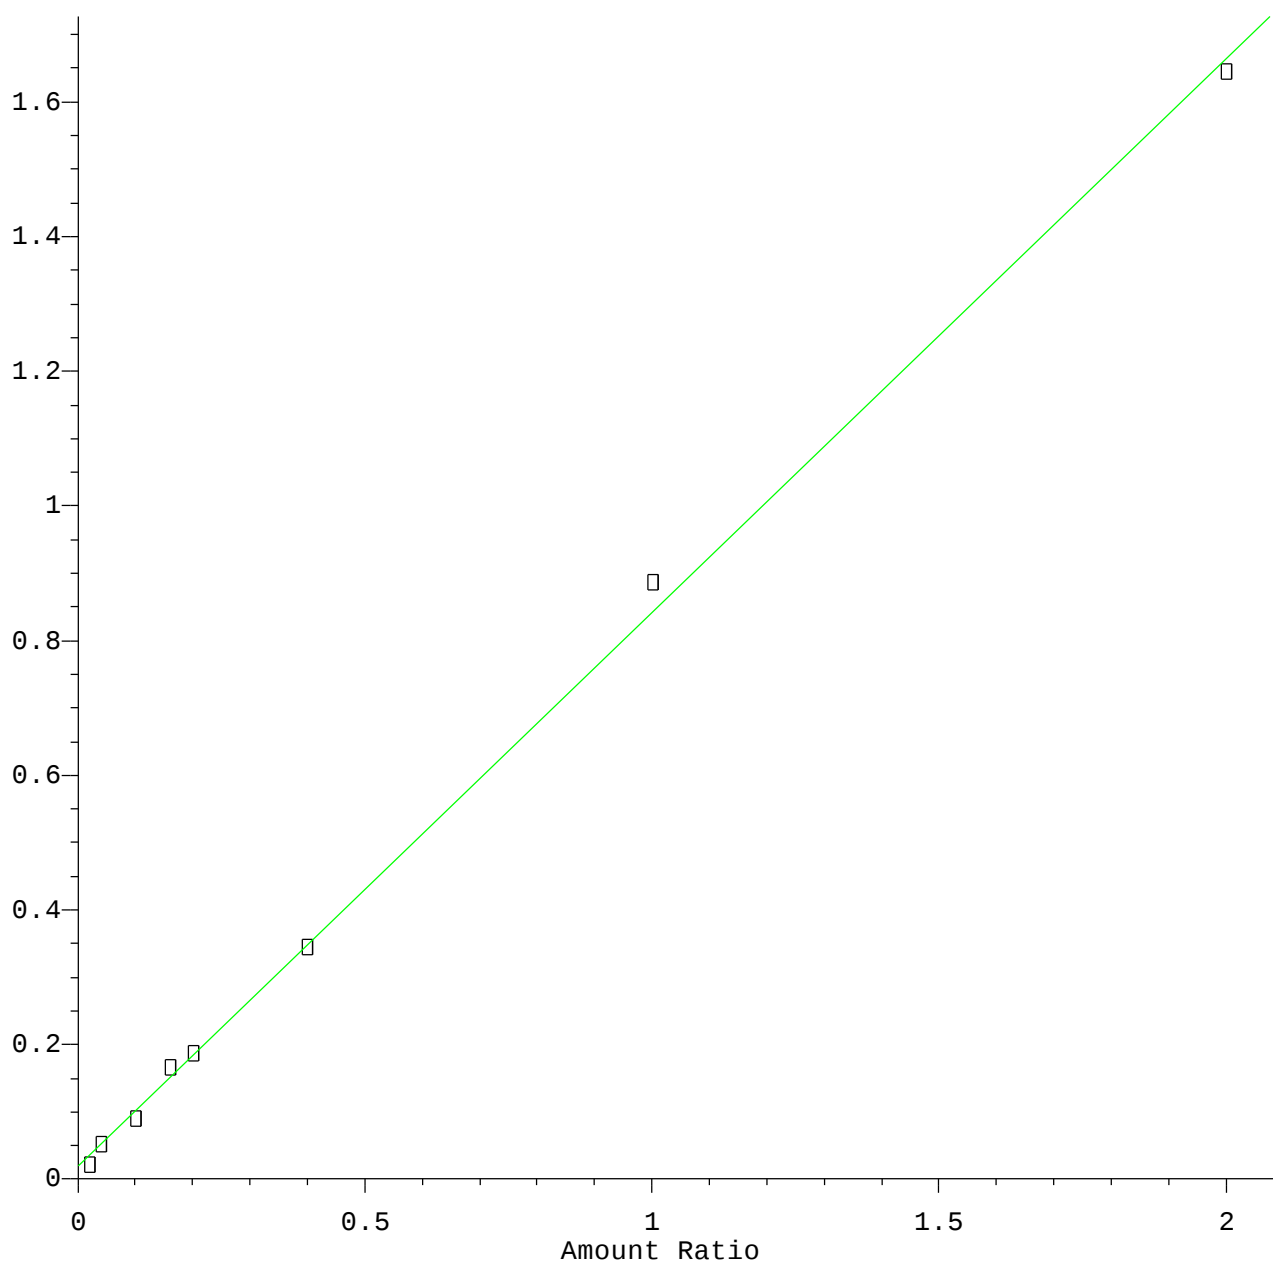

Resp Ratio = $8.22 \times 10^{-1} \times \text{Amt} + 2.02 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015

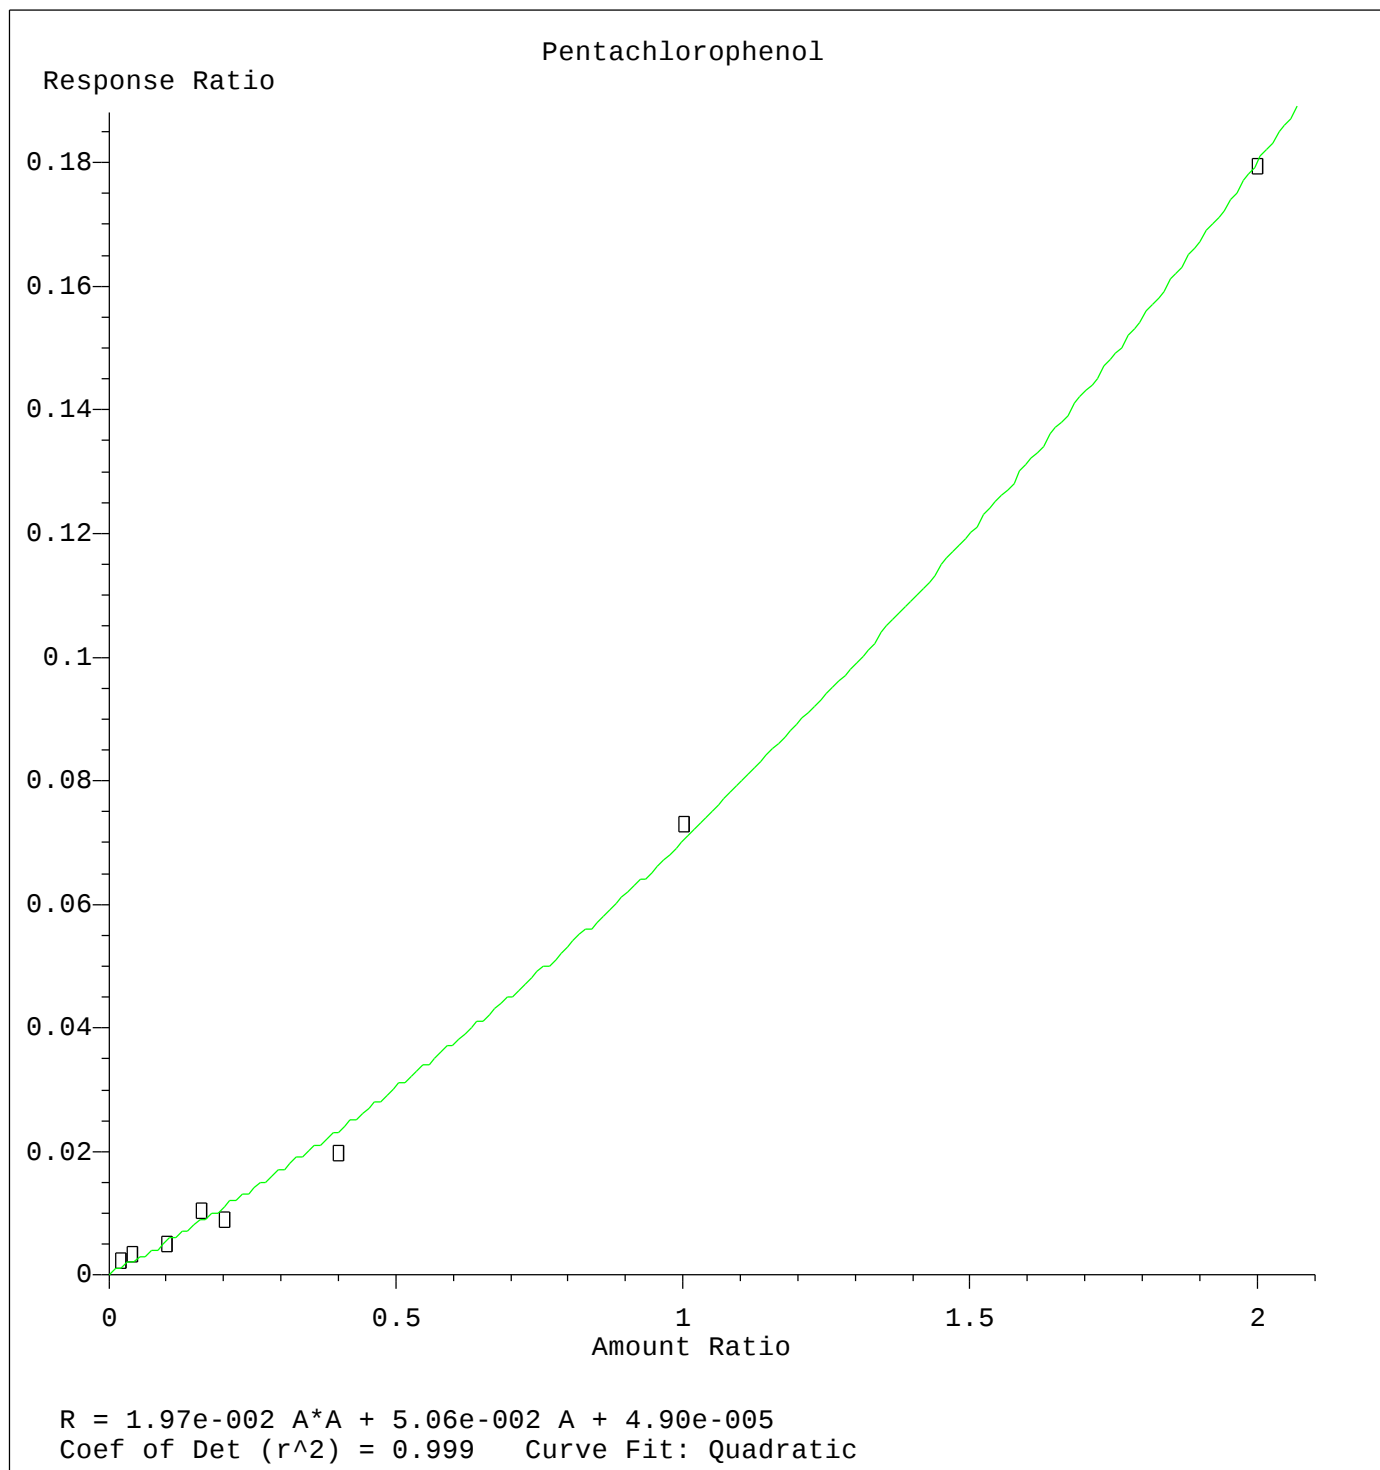

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Tue Sep 29 07:30:21 2015