


1,4-Dioxane

Response Ratio

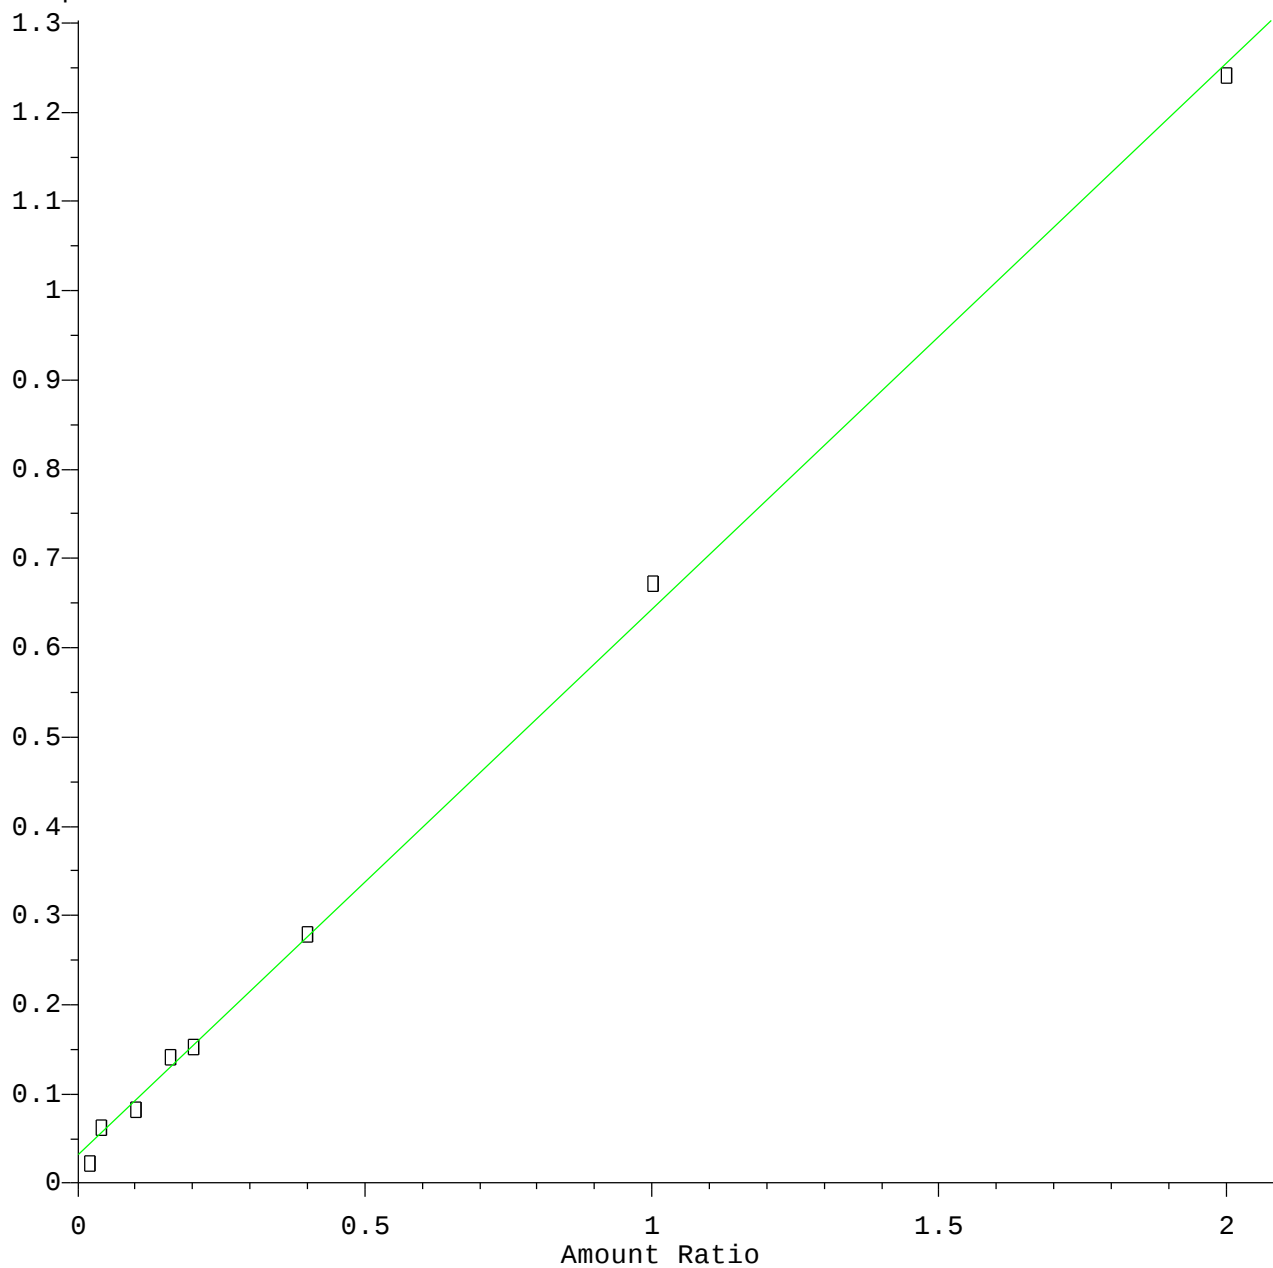


Resp Ratio = $6.12 \times 10^{-1} \times \text{Amt} + 3.12 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015


n-Nitrosodimethylamine

Response Ratio

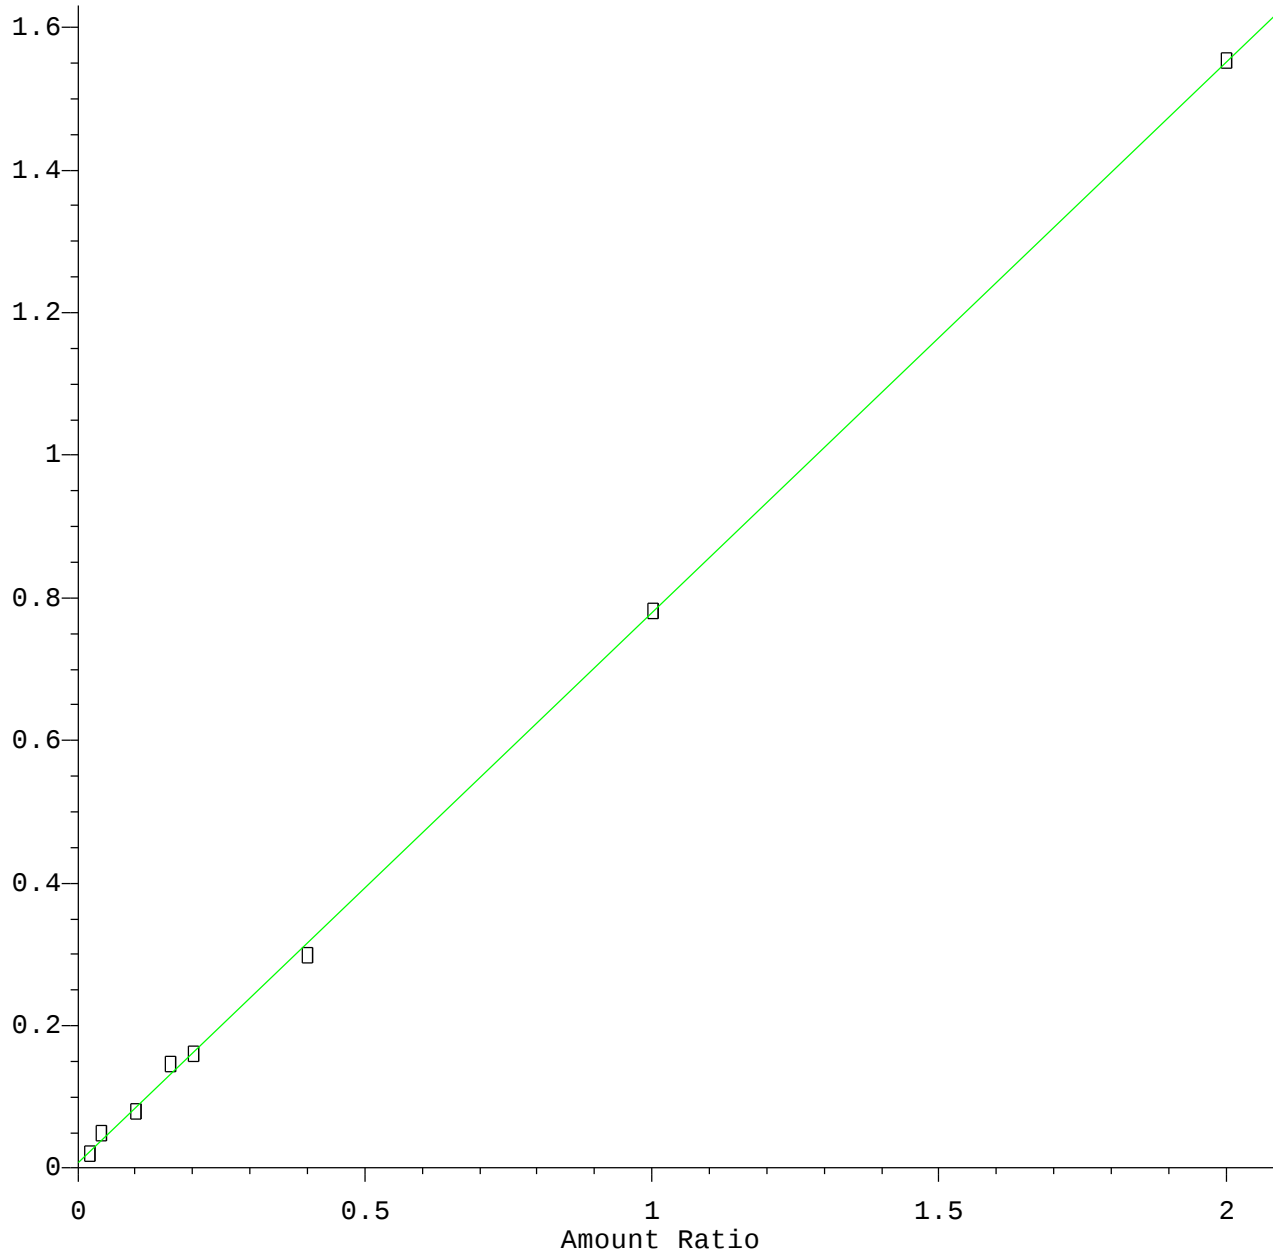

Resp Ratio = $7.72 \times 10^{-1} \times \text{Amt} + 7.44 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

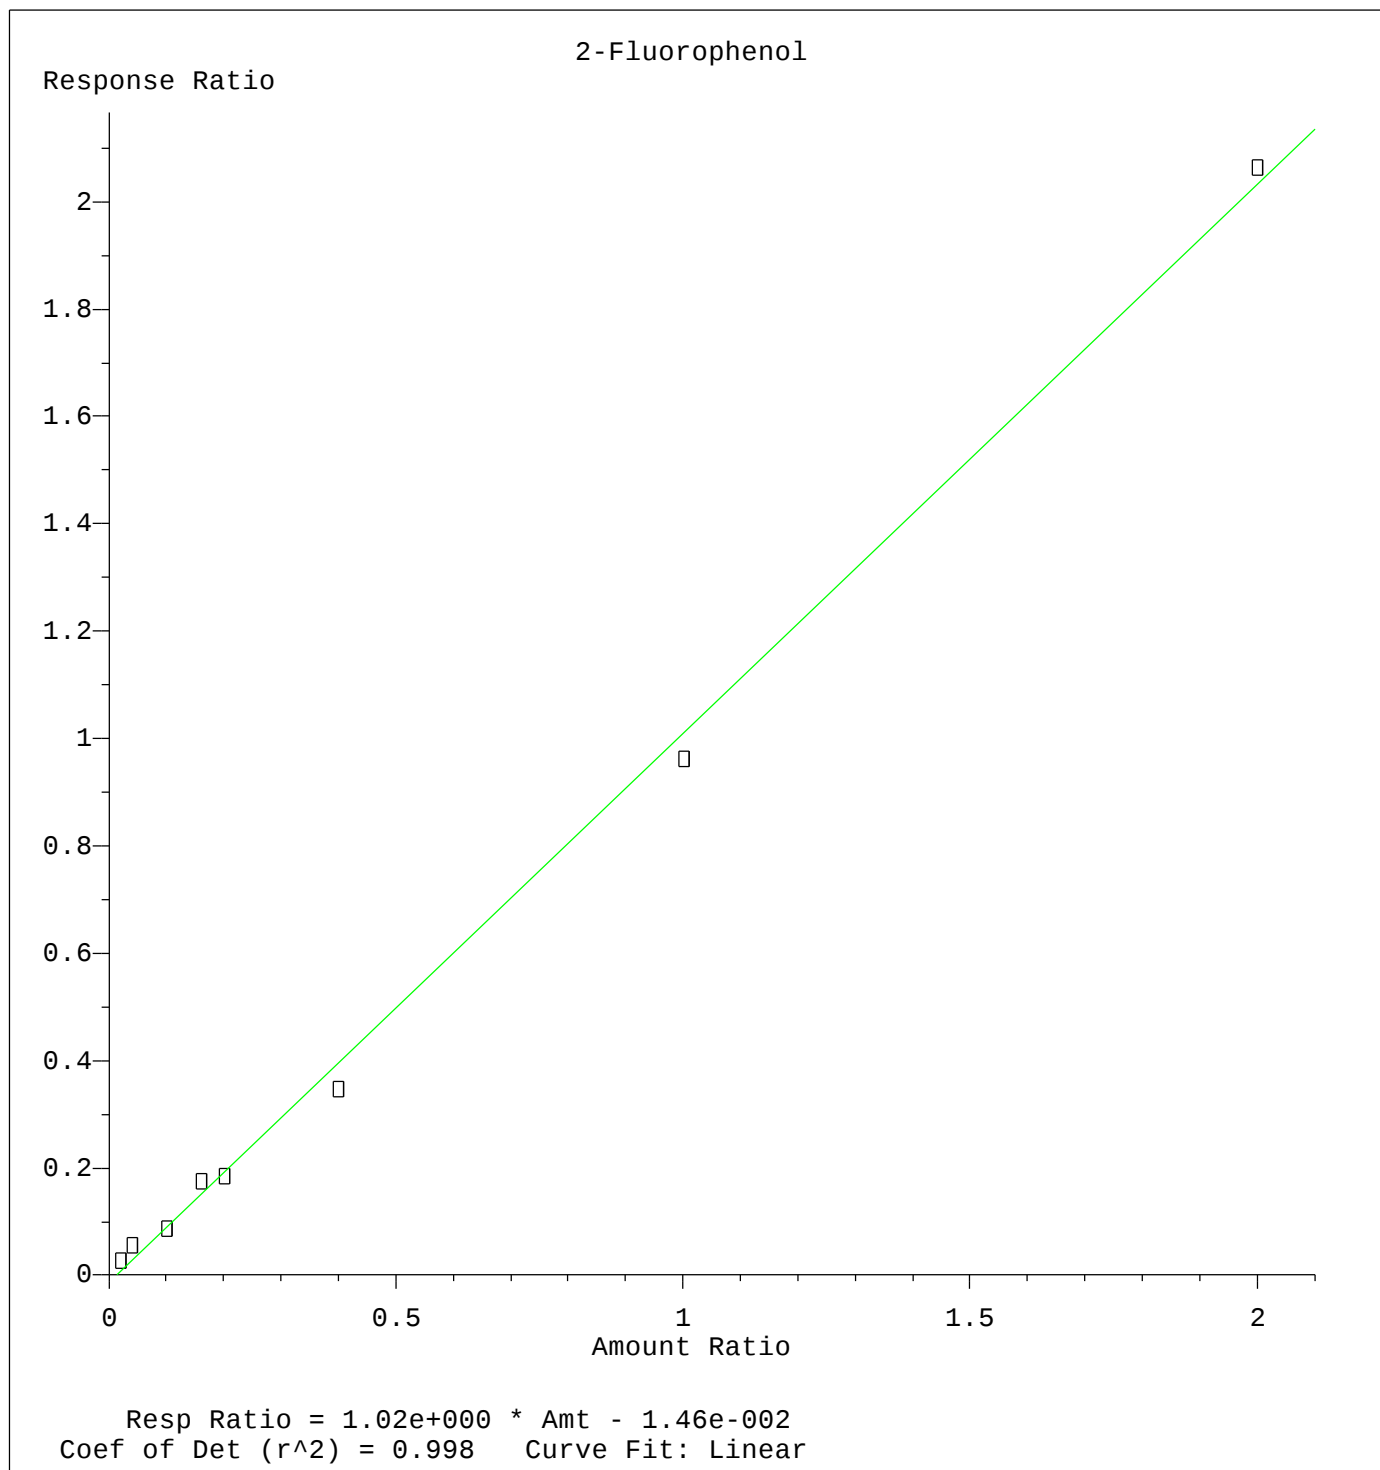

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015


bis(2-Chloroethyl)ether

Response Ratio

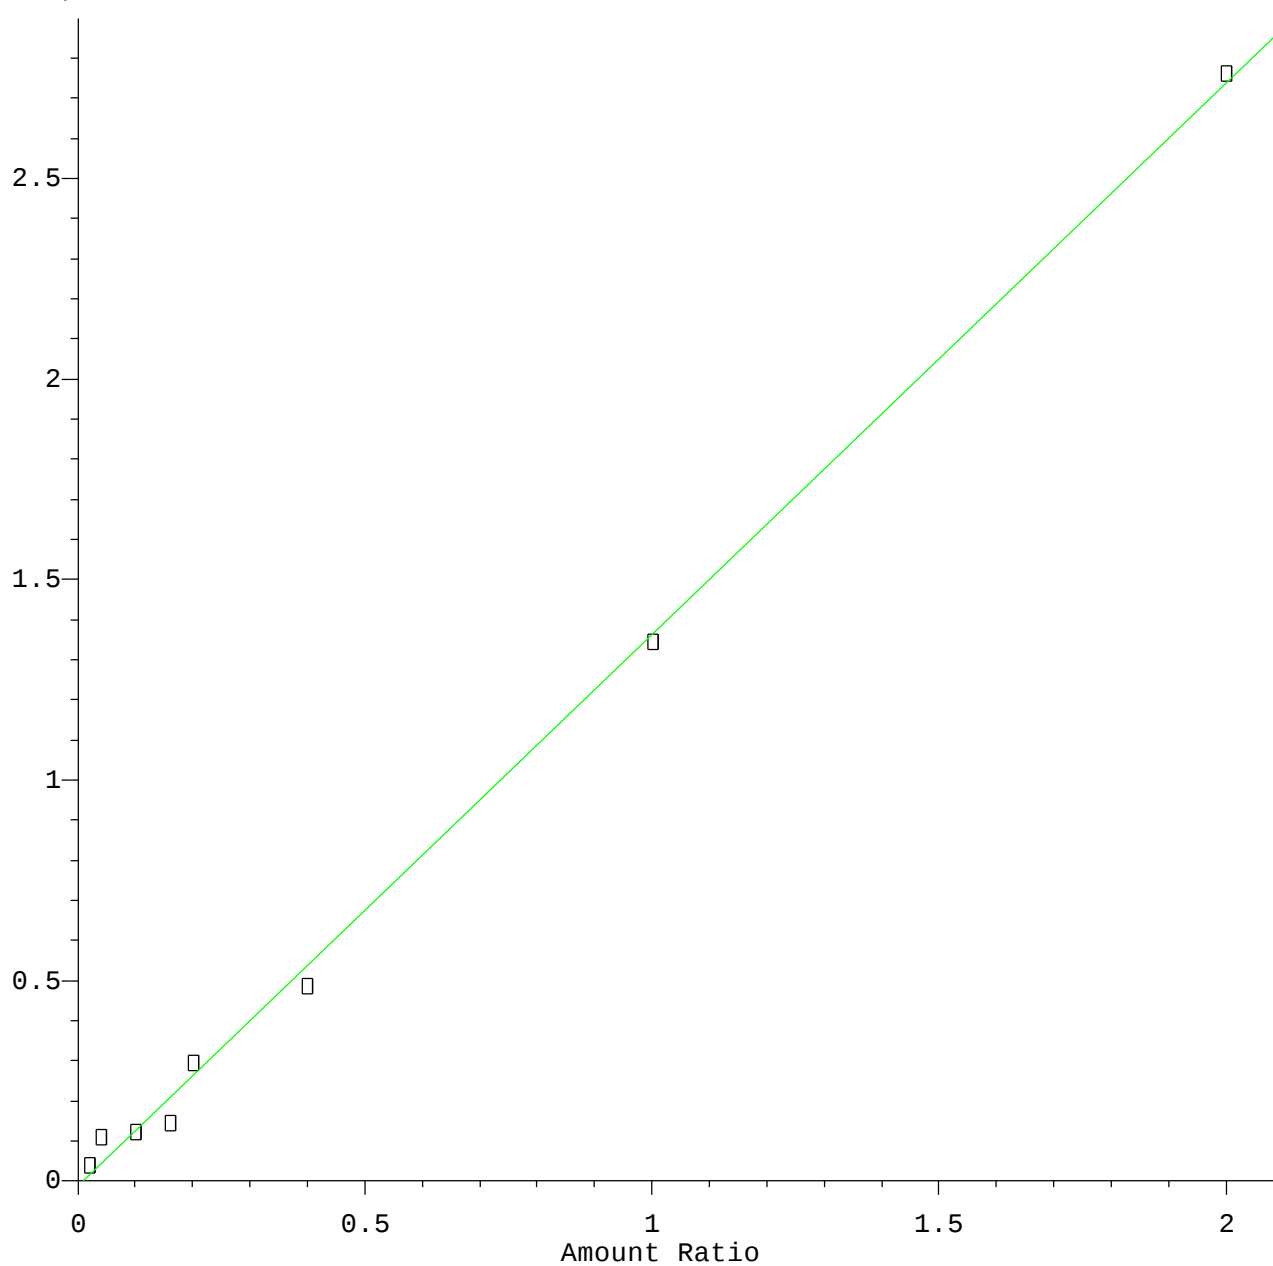


Resp Ratio = 1.37e+000 * Amt - 1.21e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

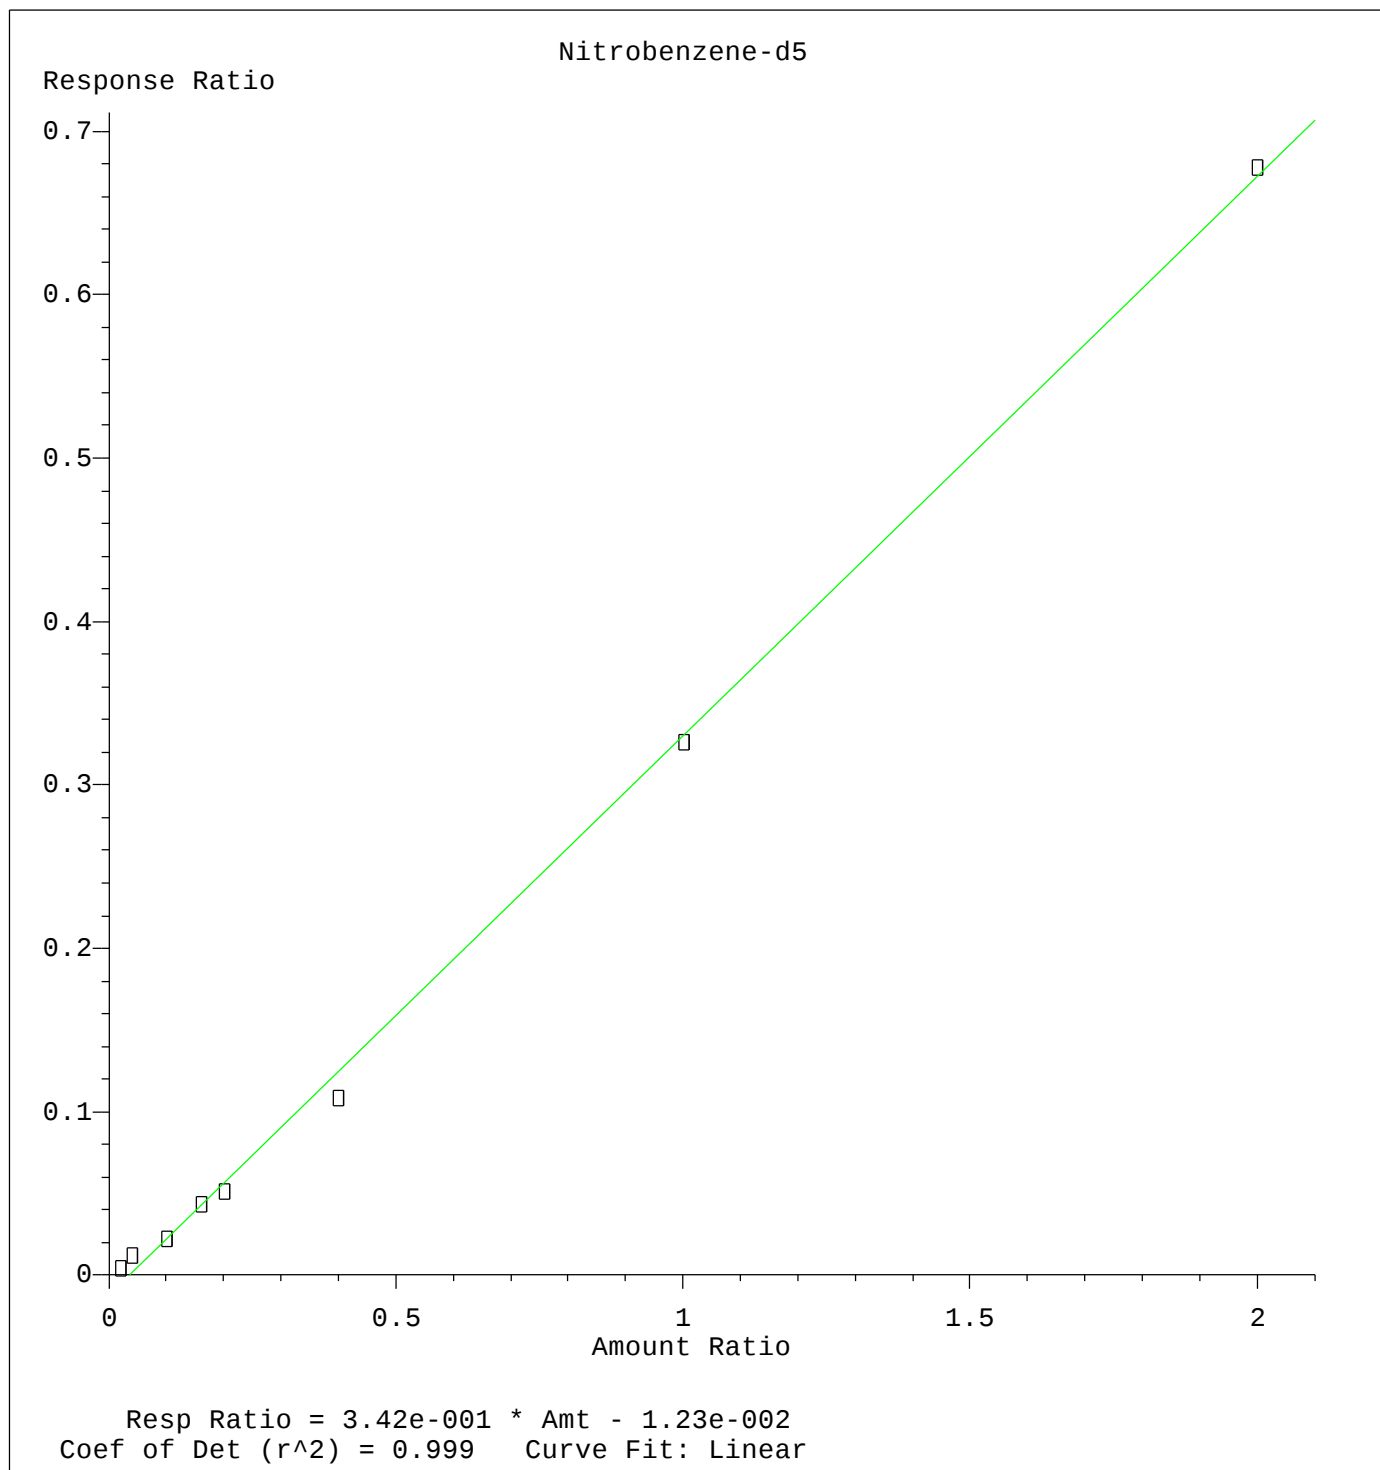


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

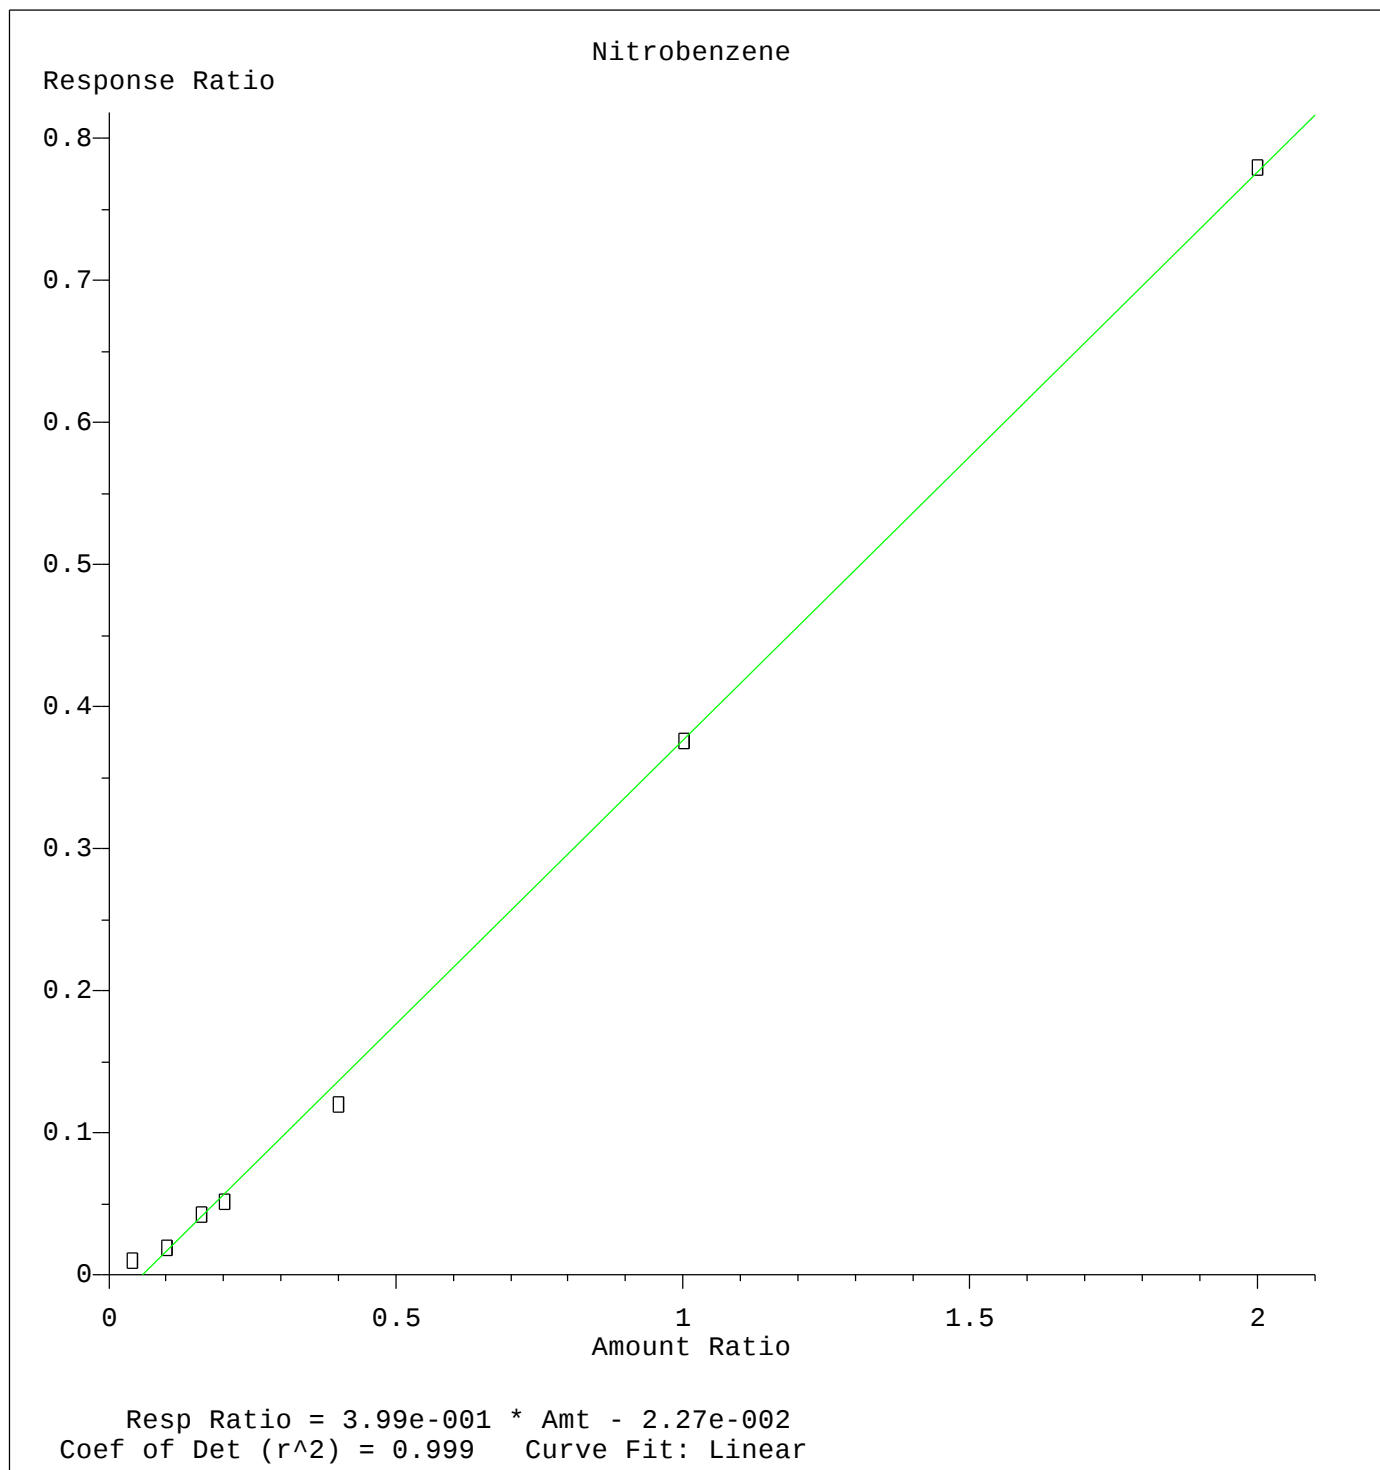


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

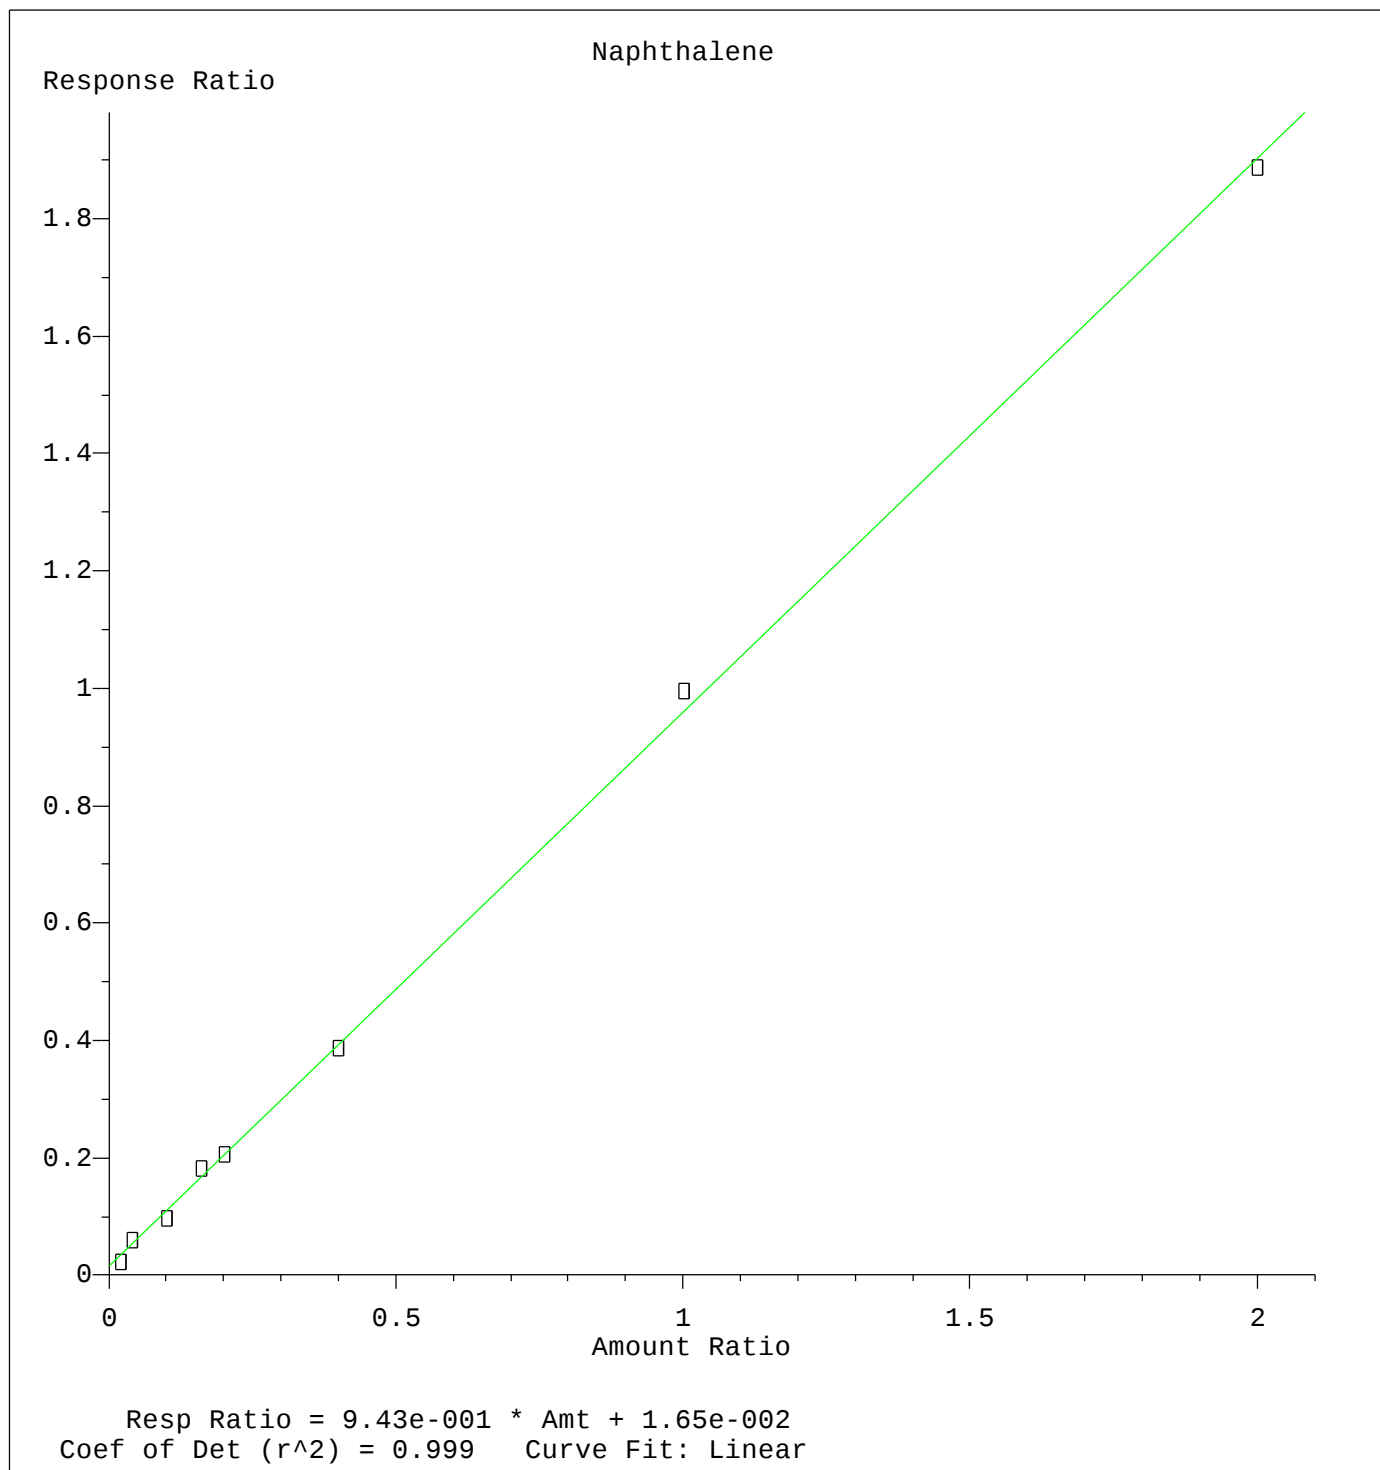

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

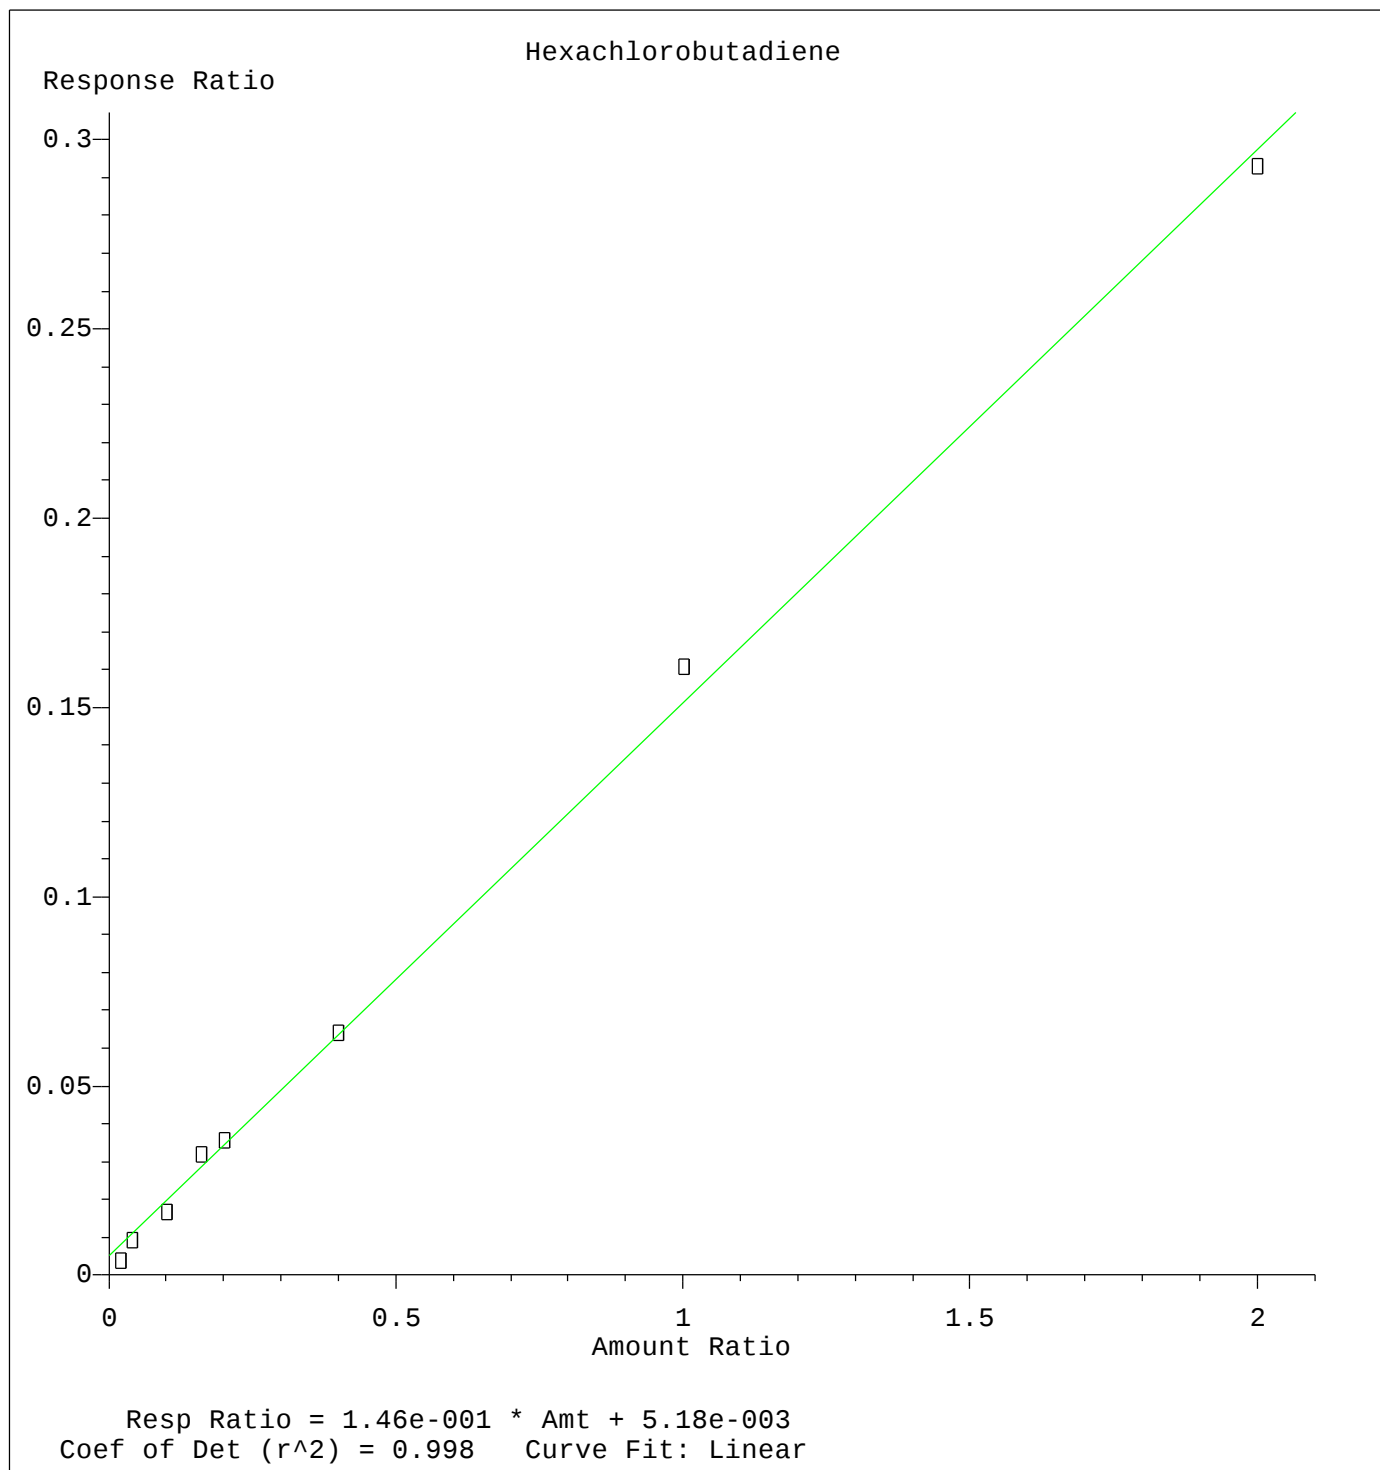


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

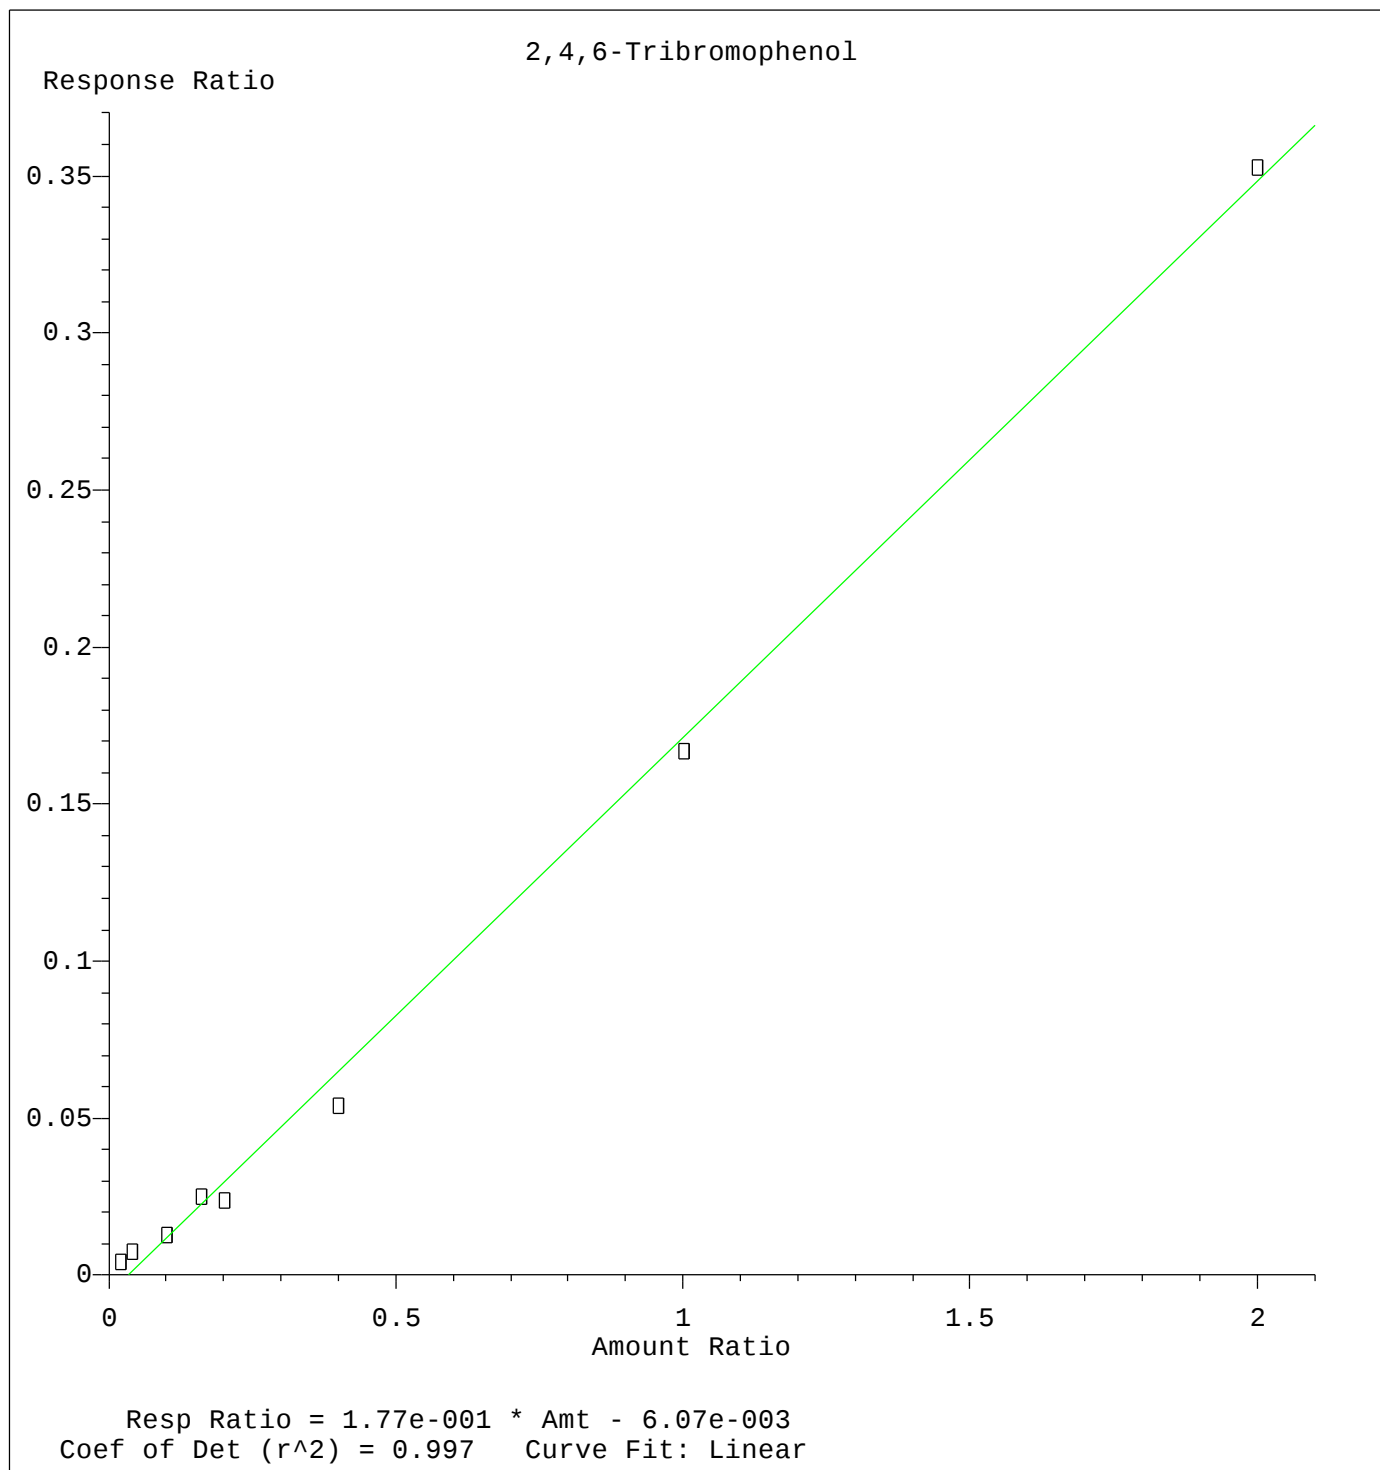

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015


Hexachlorobenzene

Response Ratio

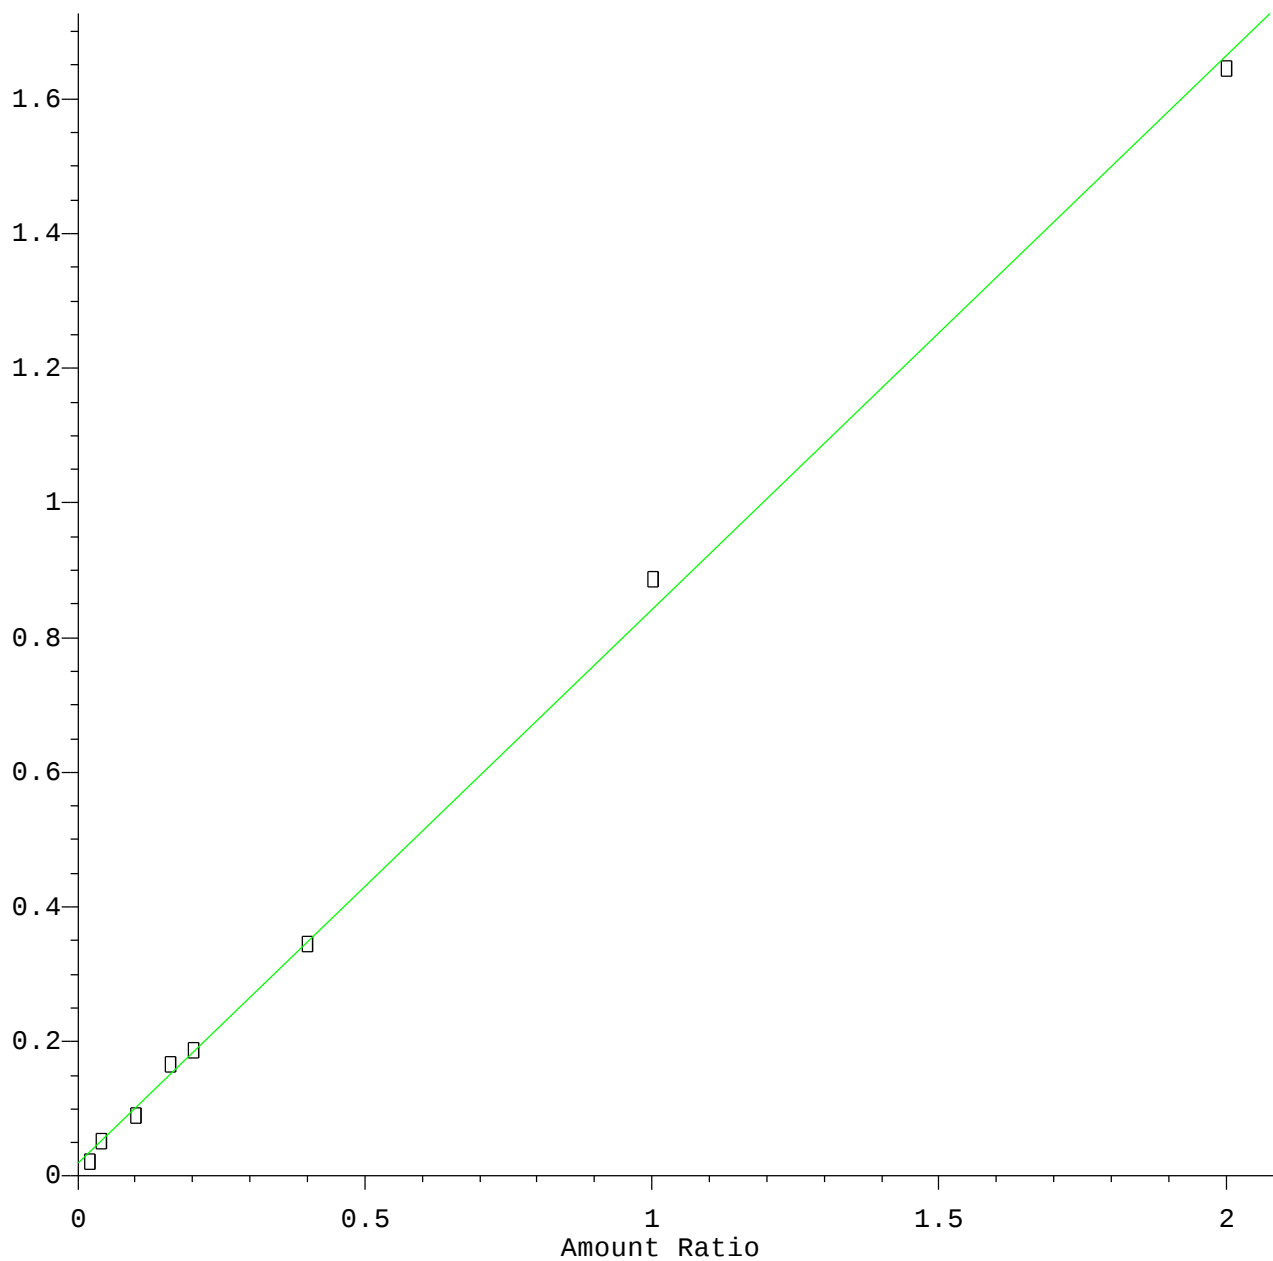


Resp Ratio = $8.22 \times 10^{-1} \times \text{Amt} + 2.02 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

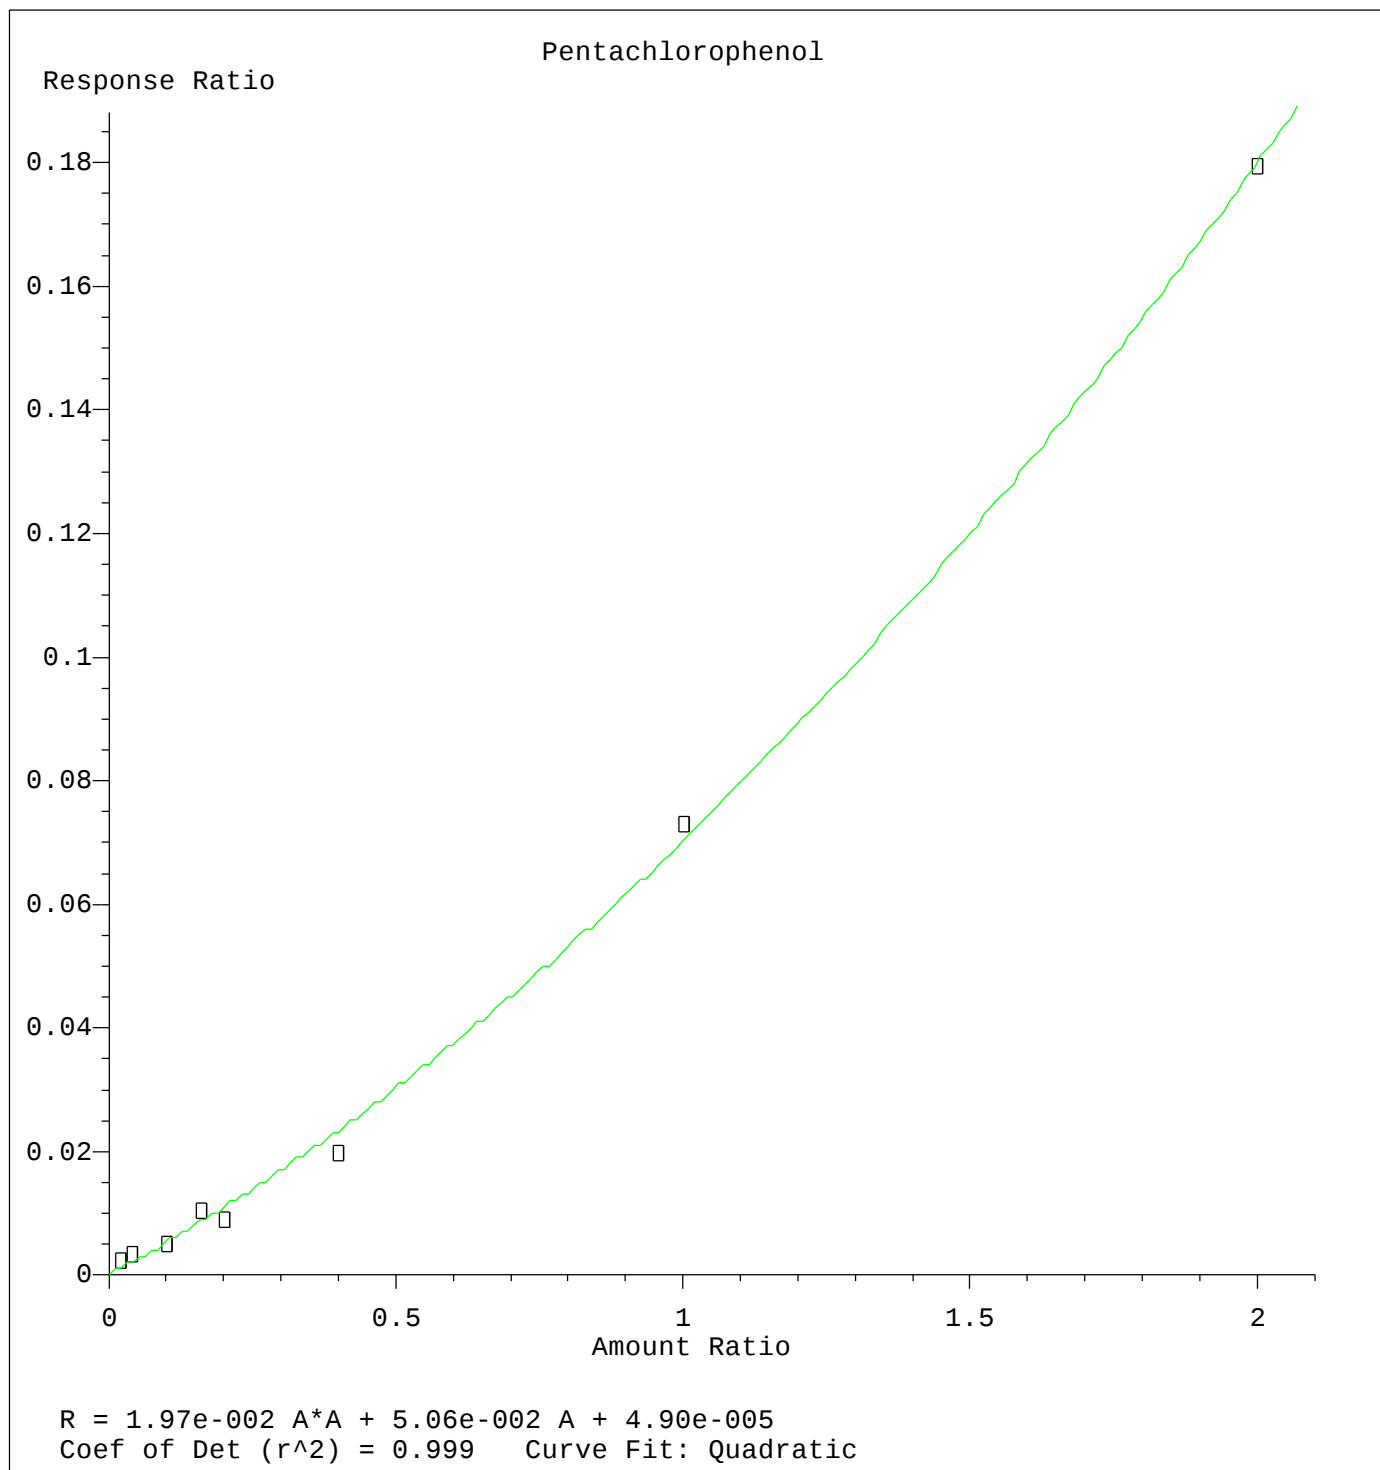


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

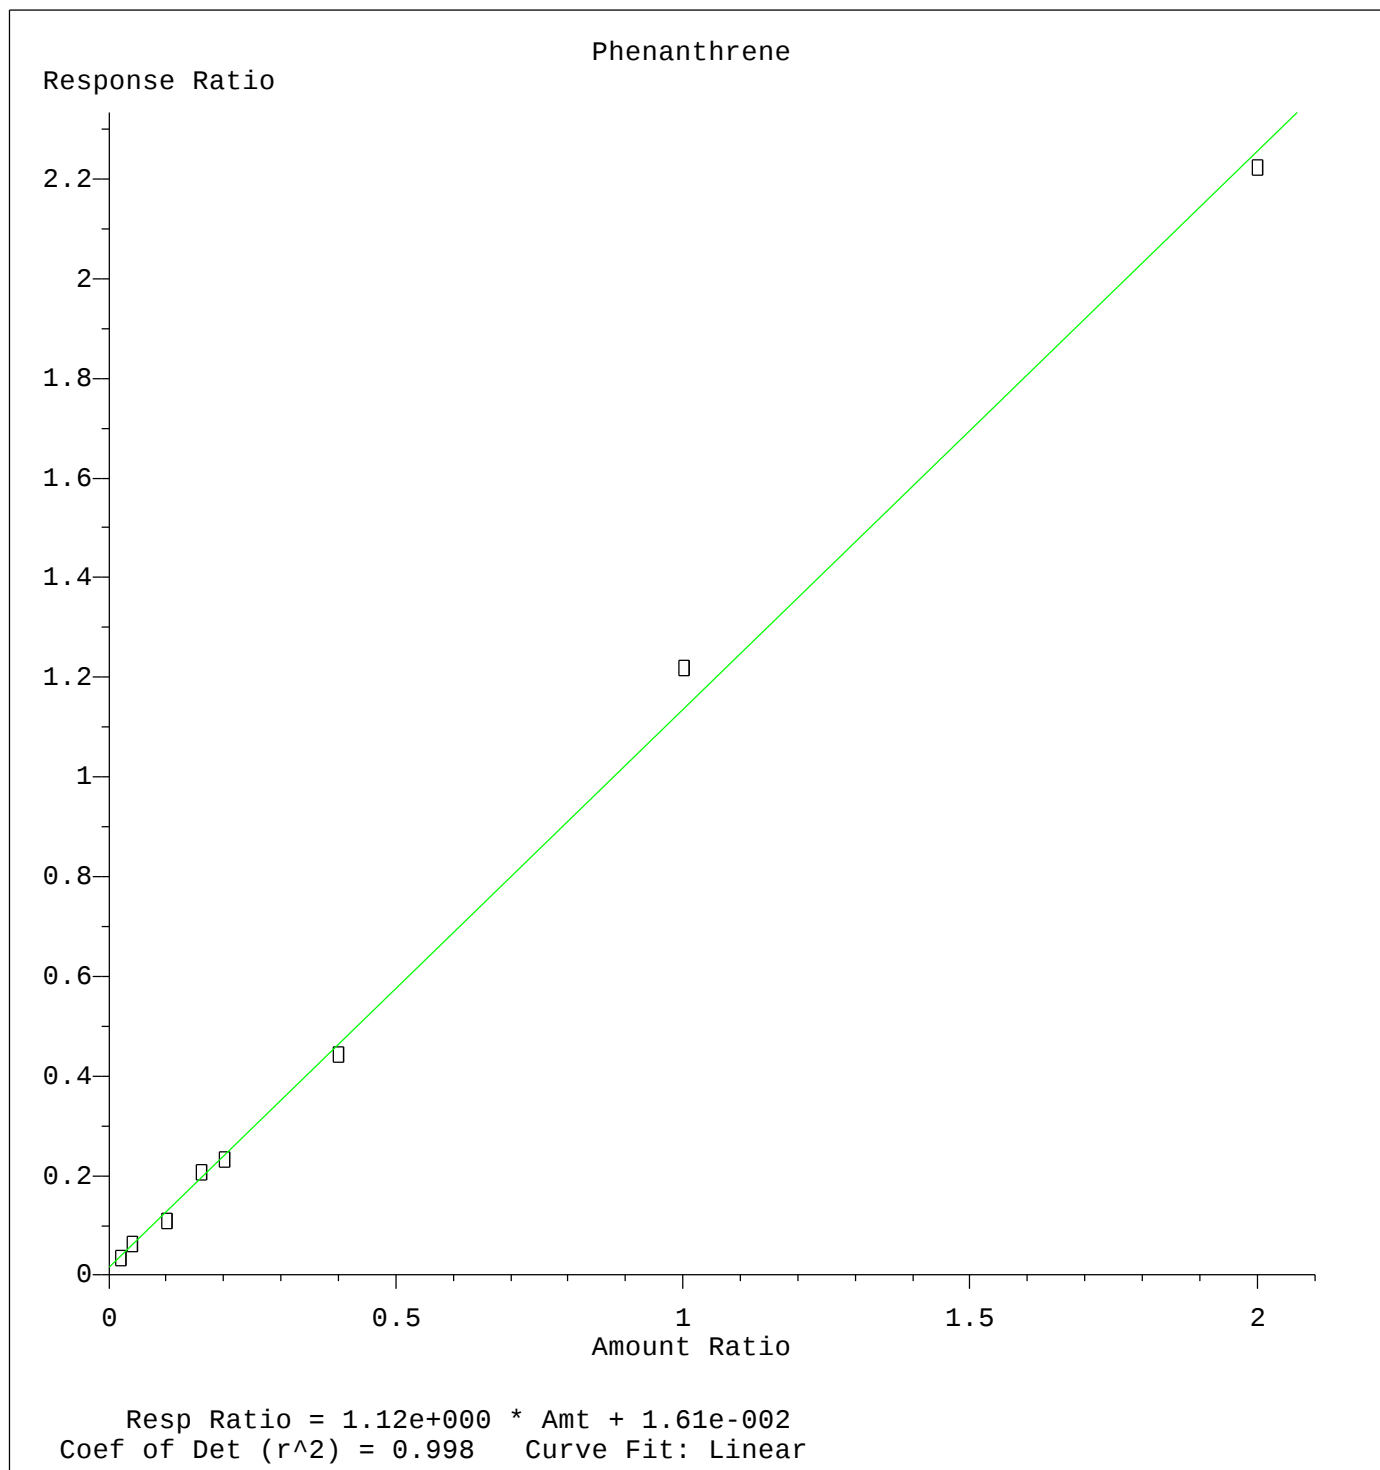


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

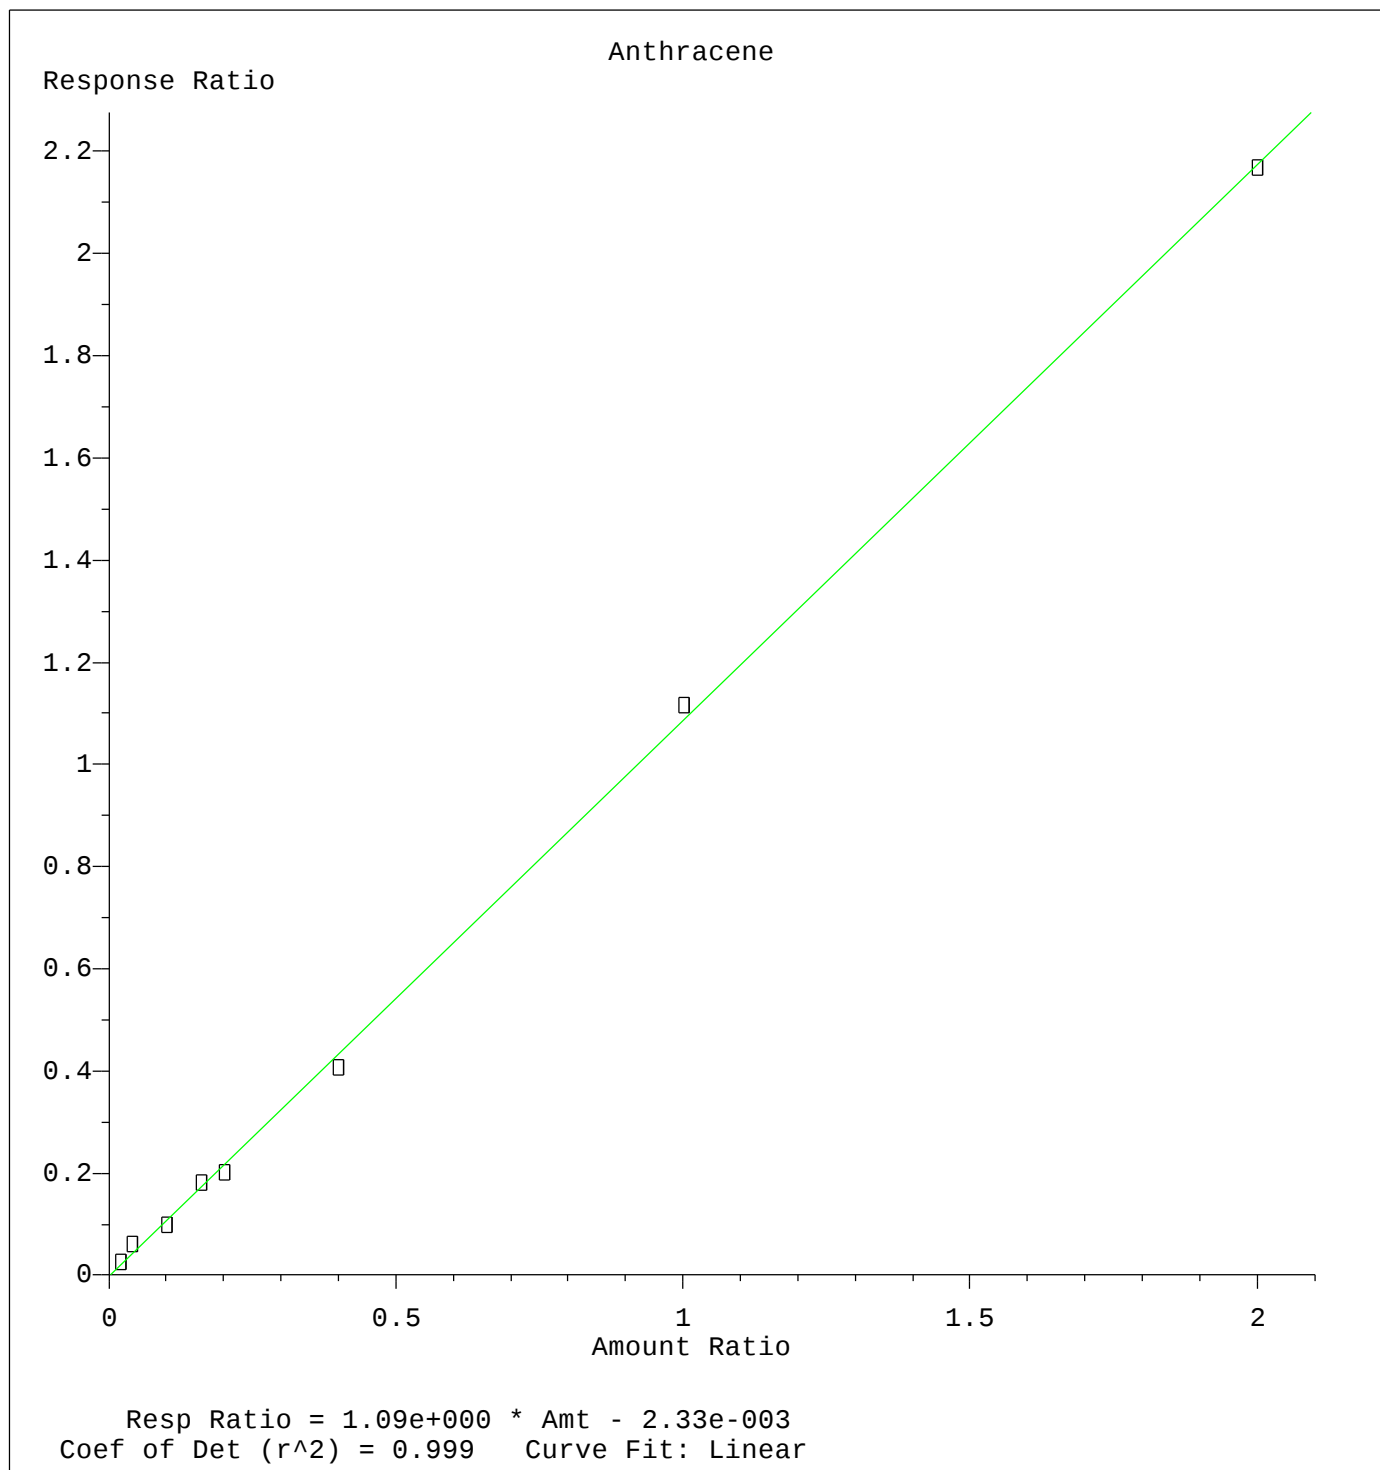


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

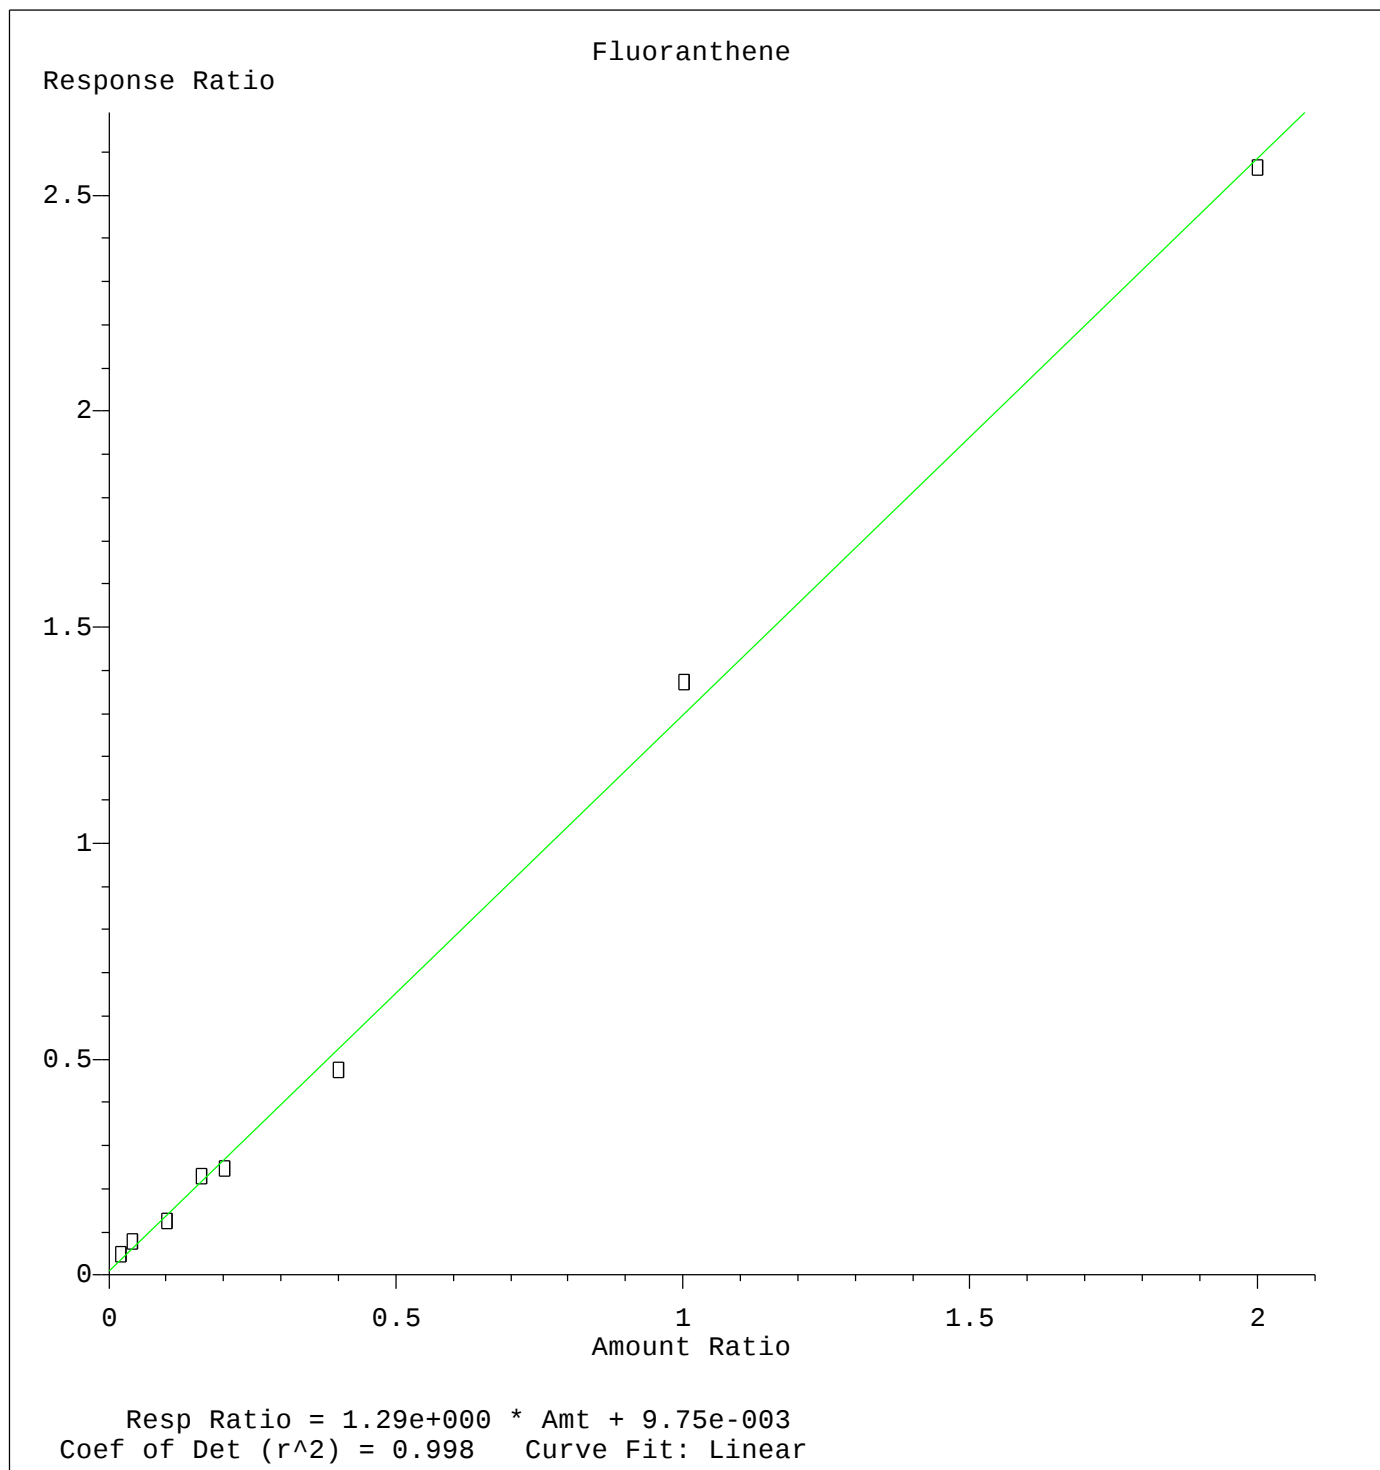


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

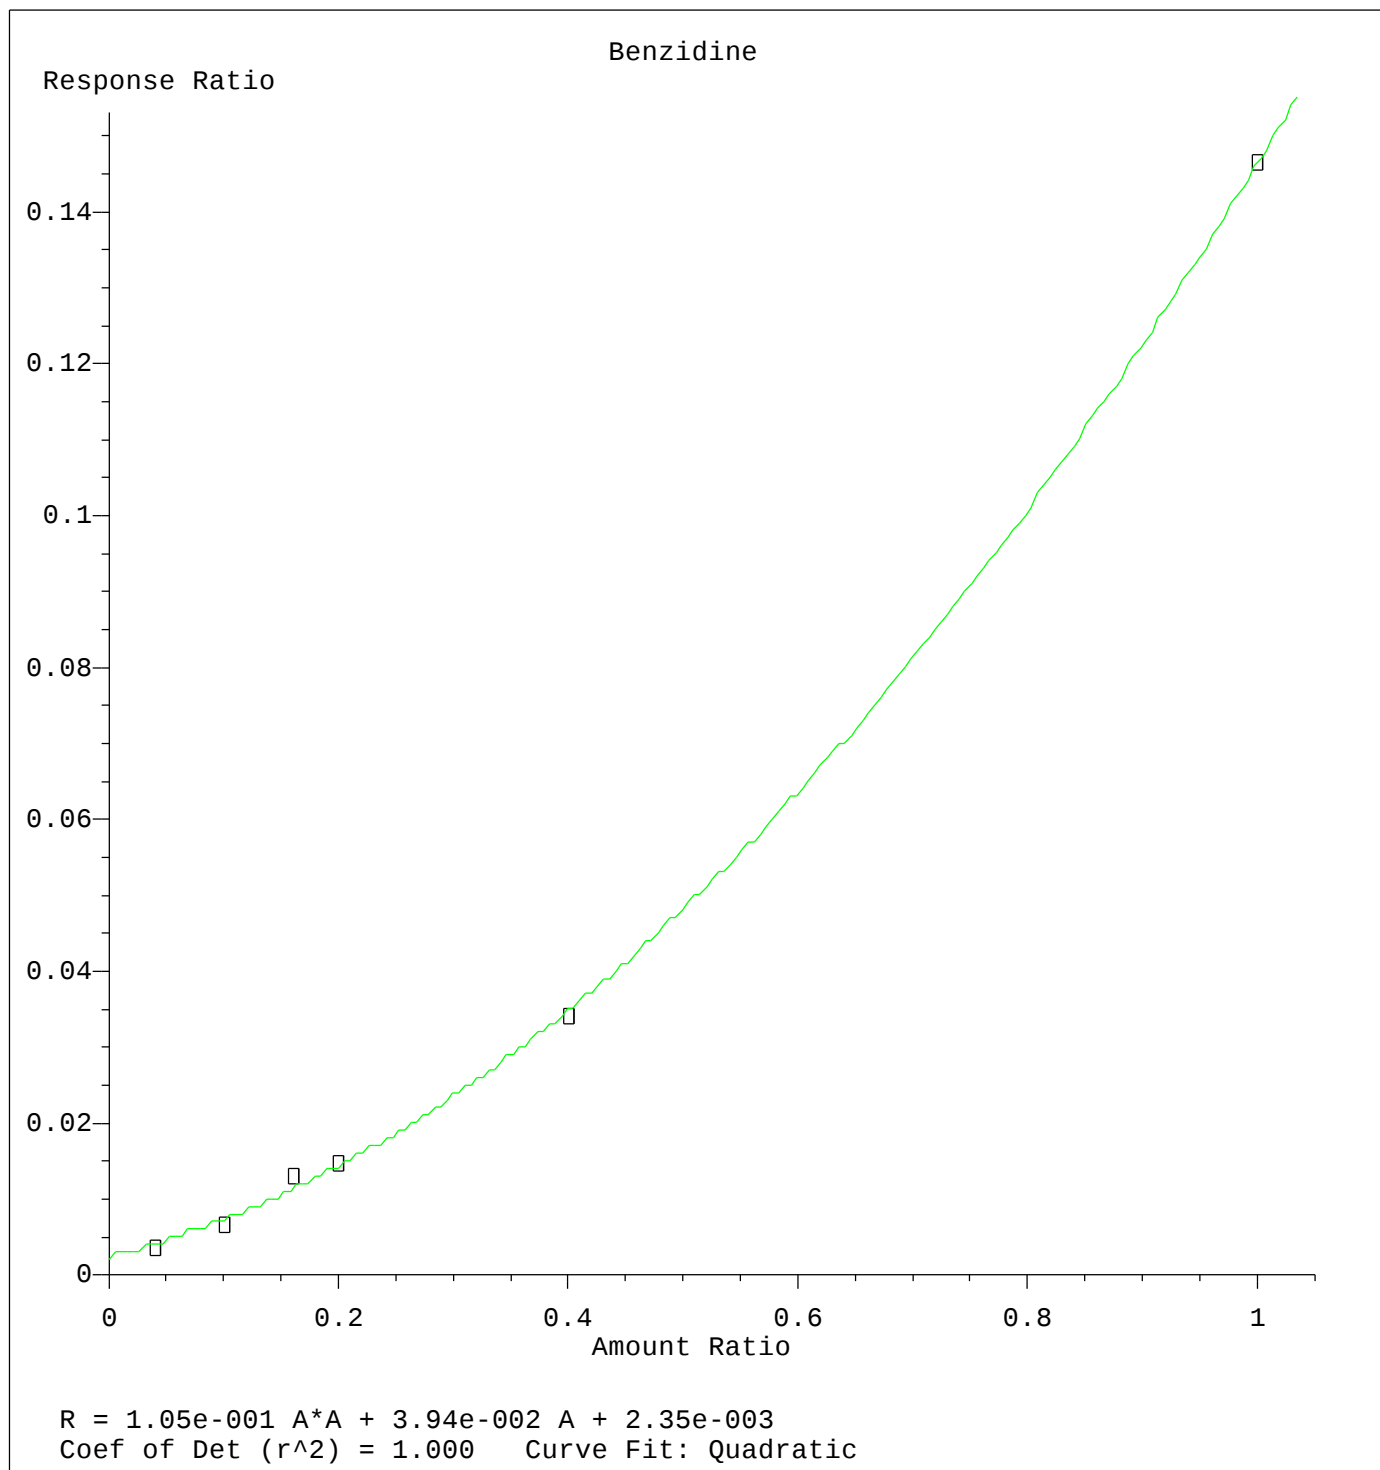


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

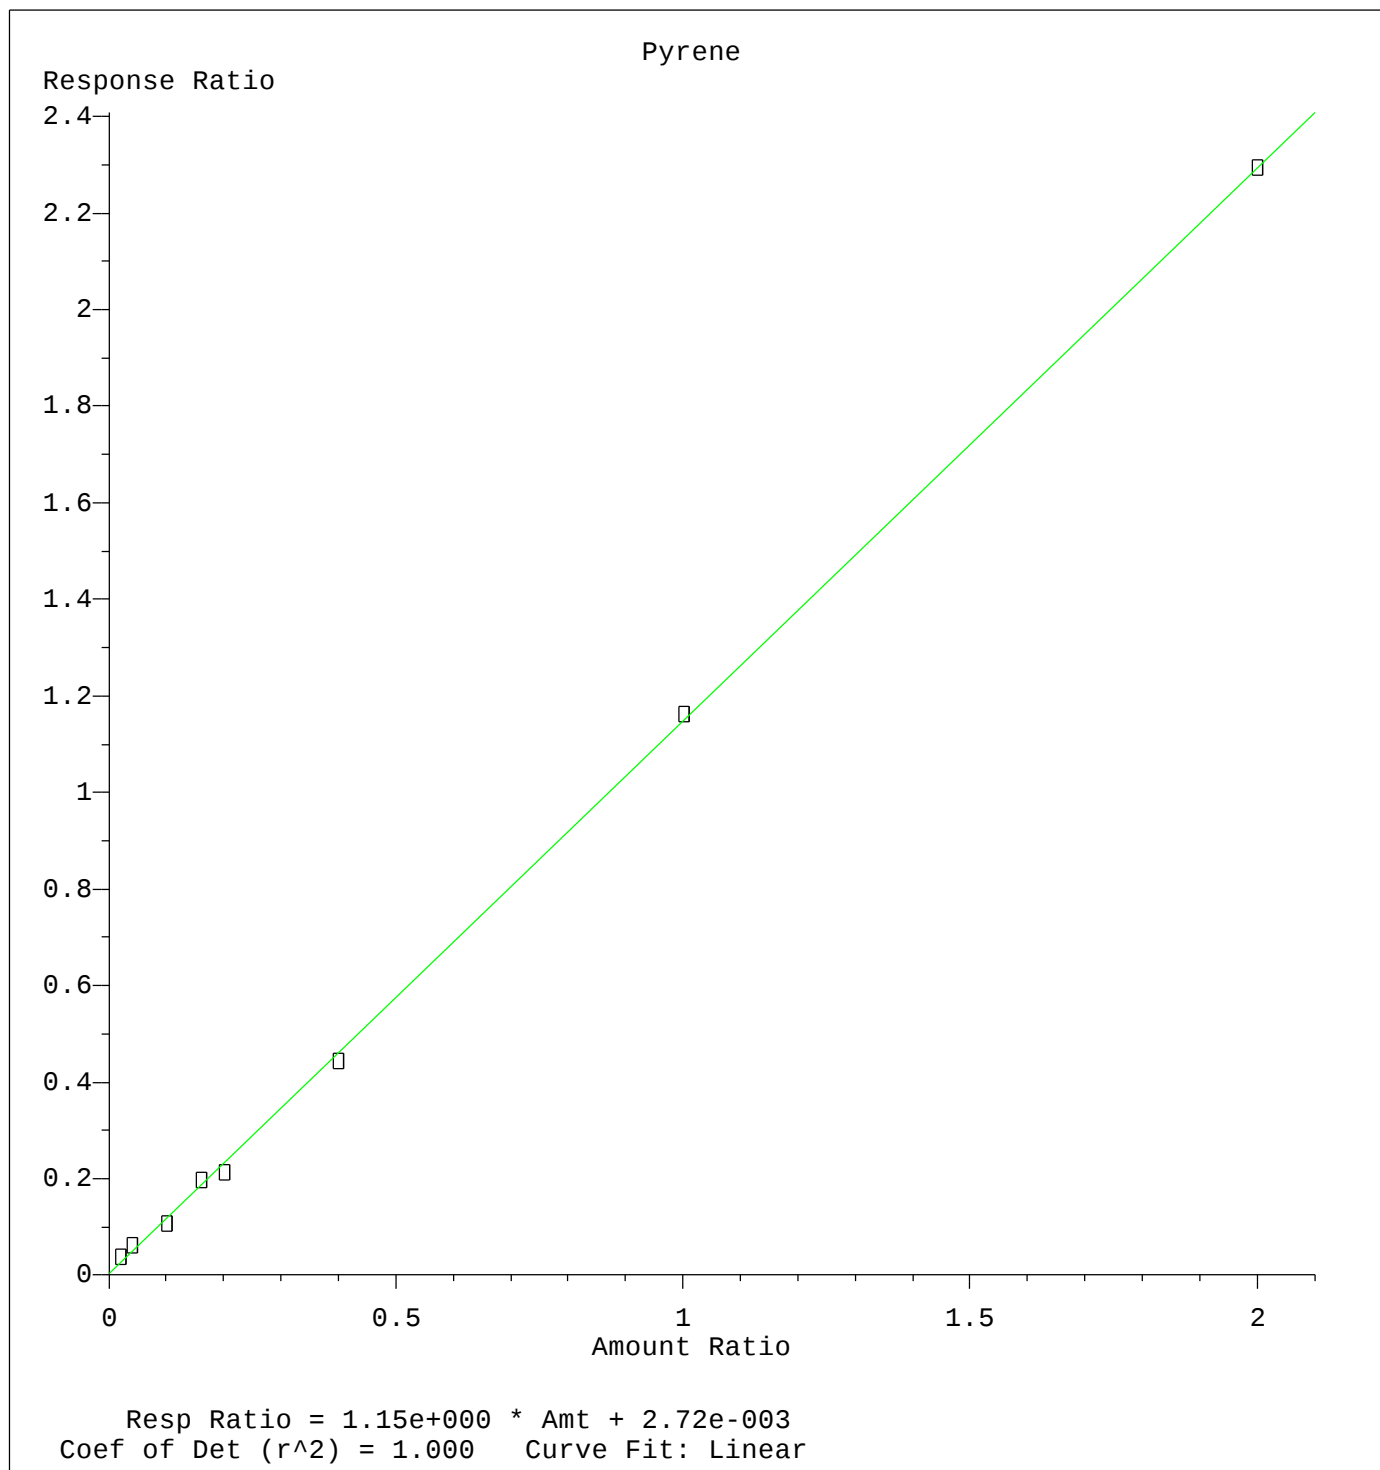

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

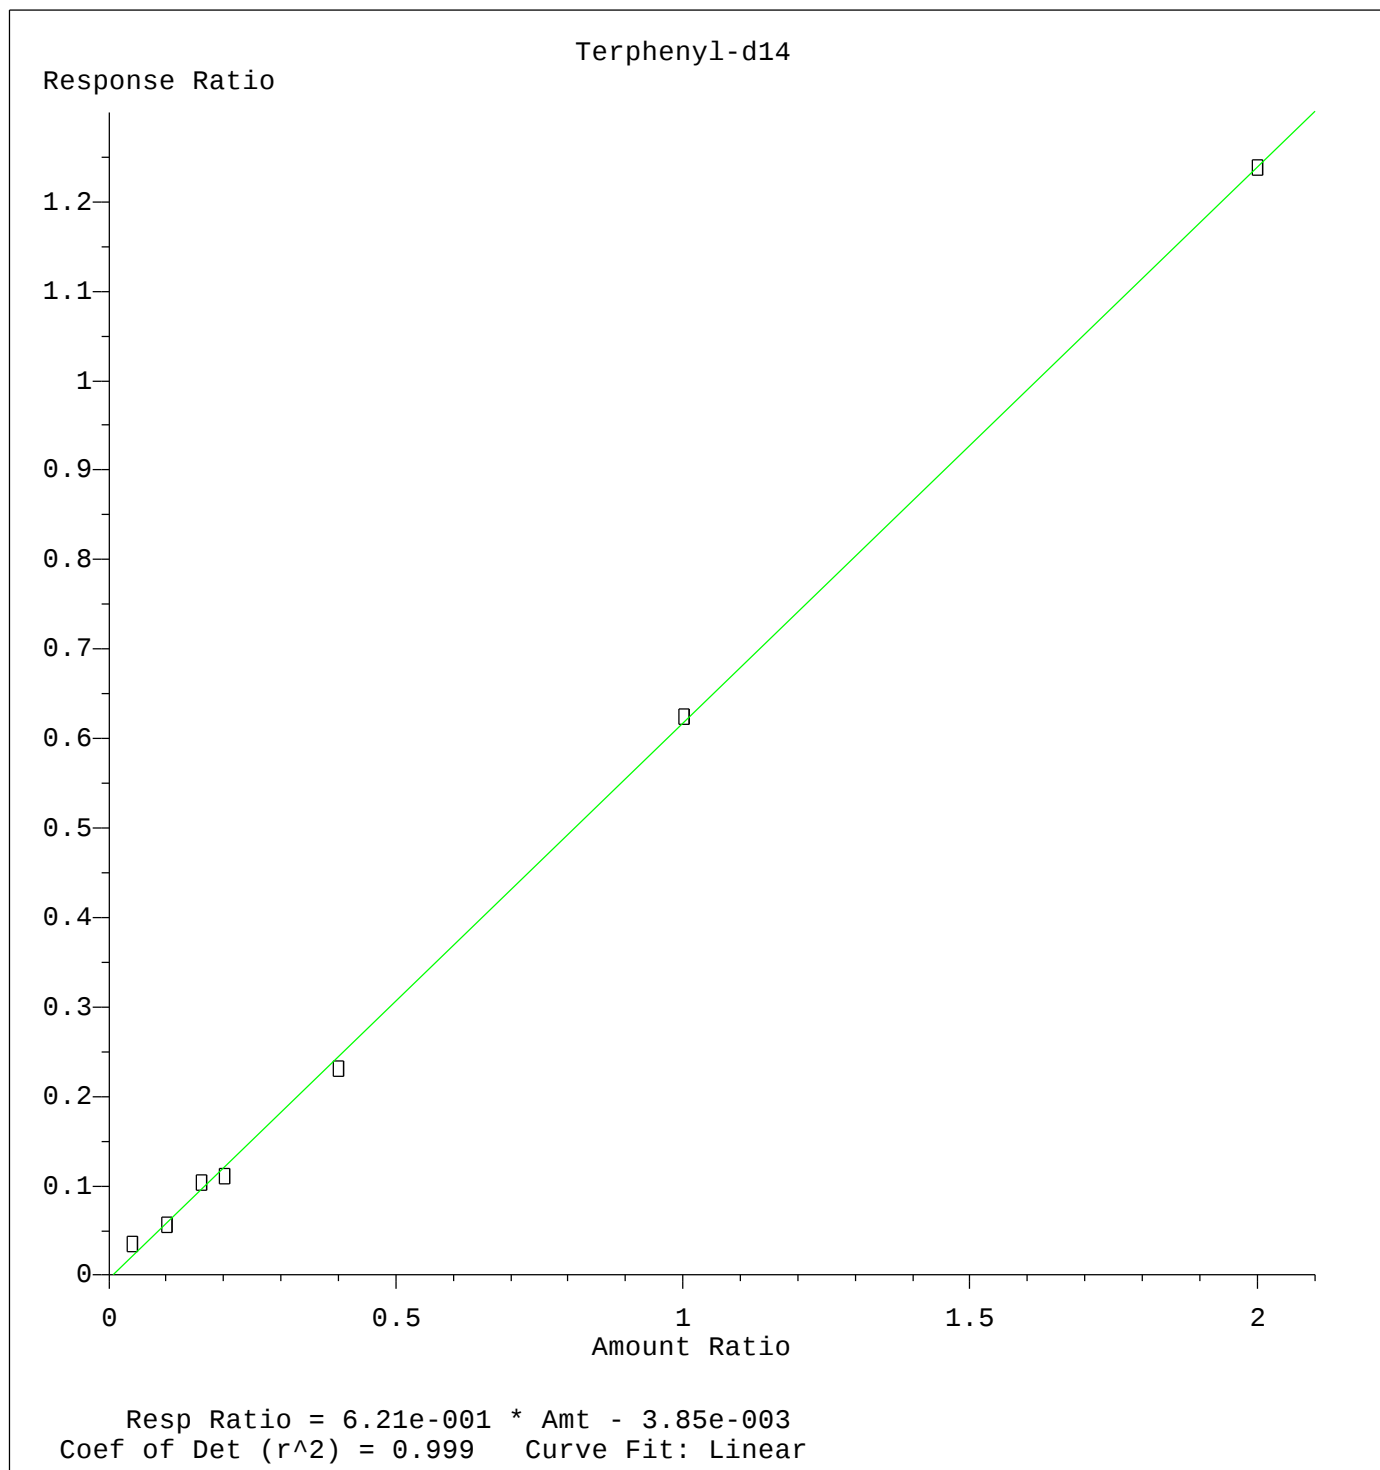


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

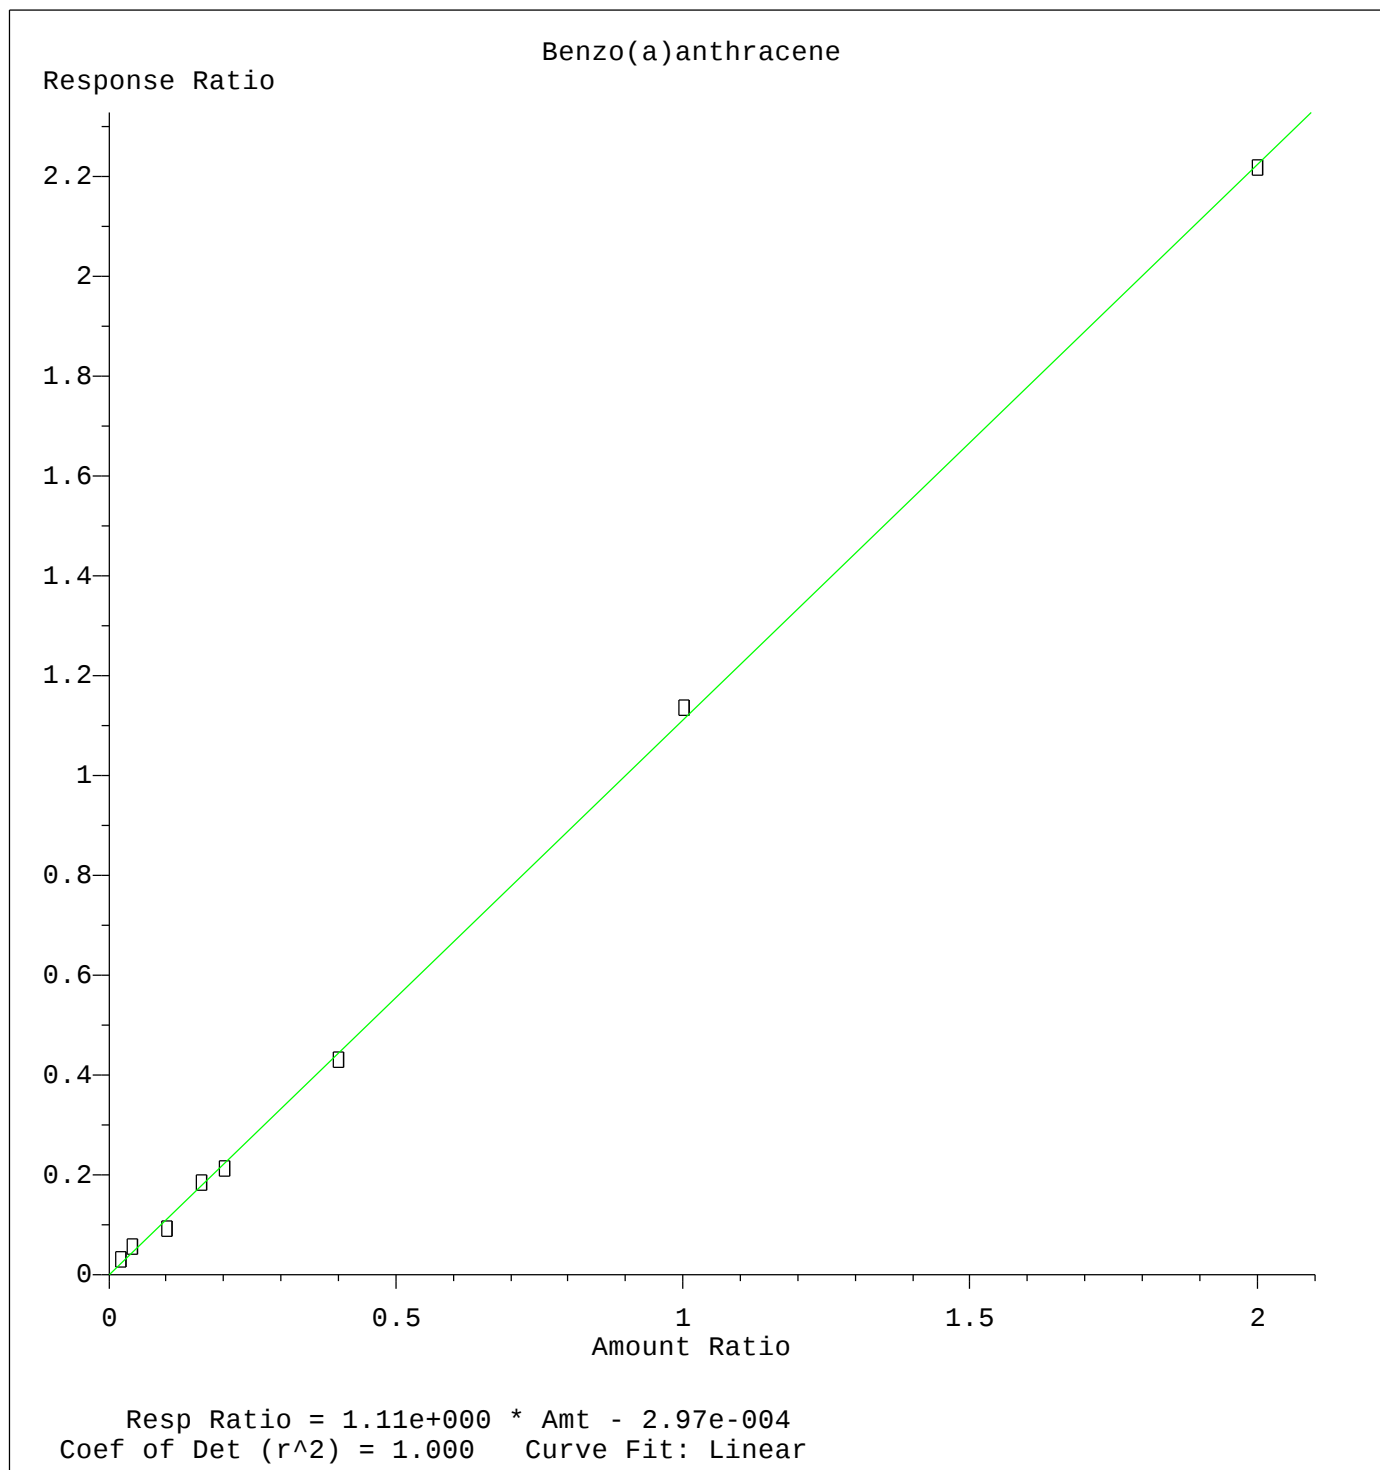

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015


3,3'-Dichlorobenzidine

Response Ratio

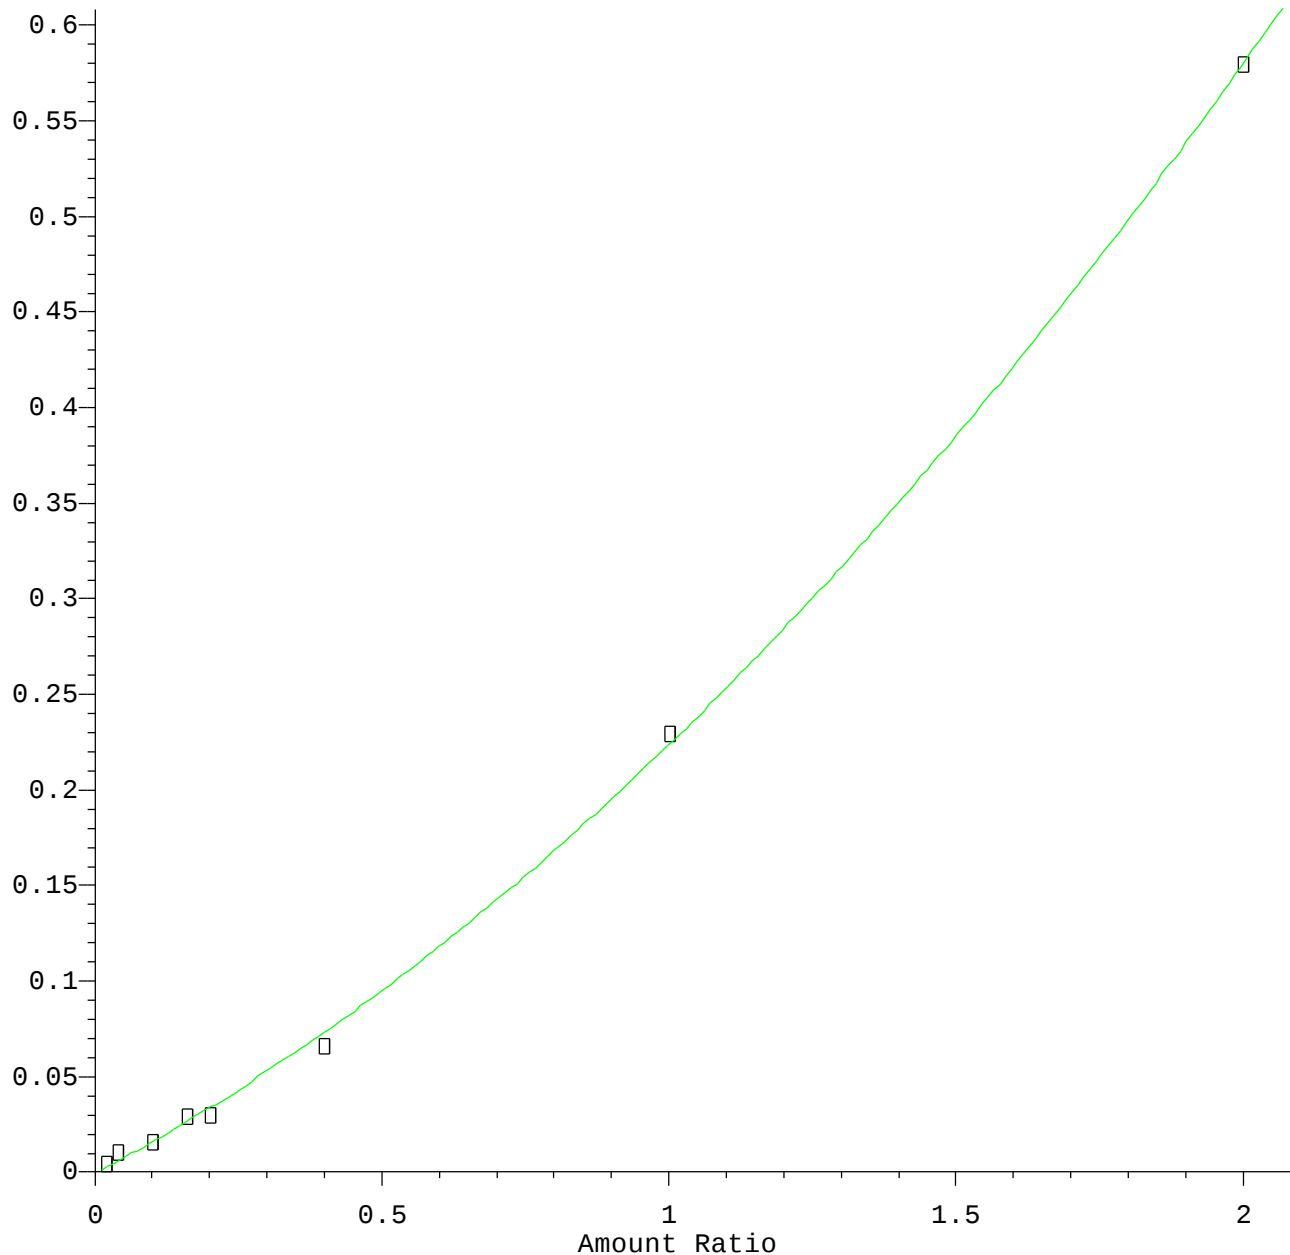

$R = 6.60e-002 A^2 + 1.58e-001 A - 6.99e-004$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

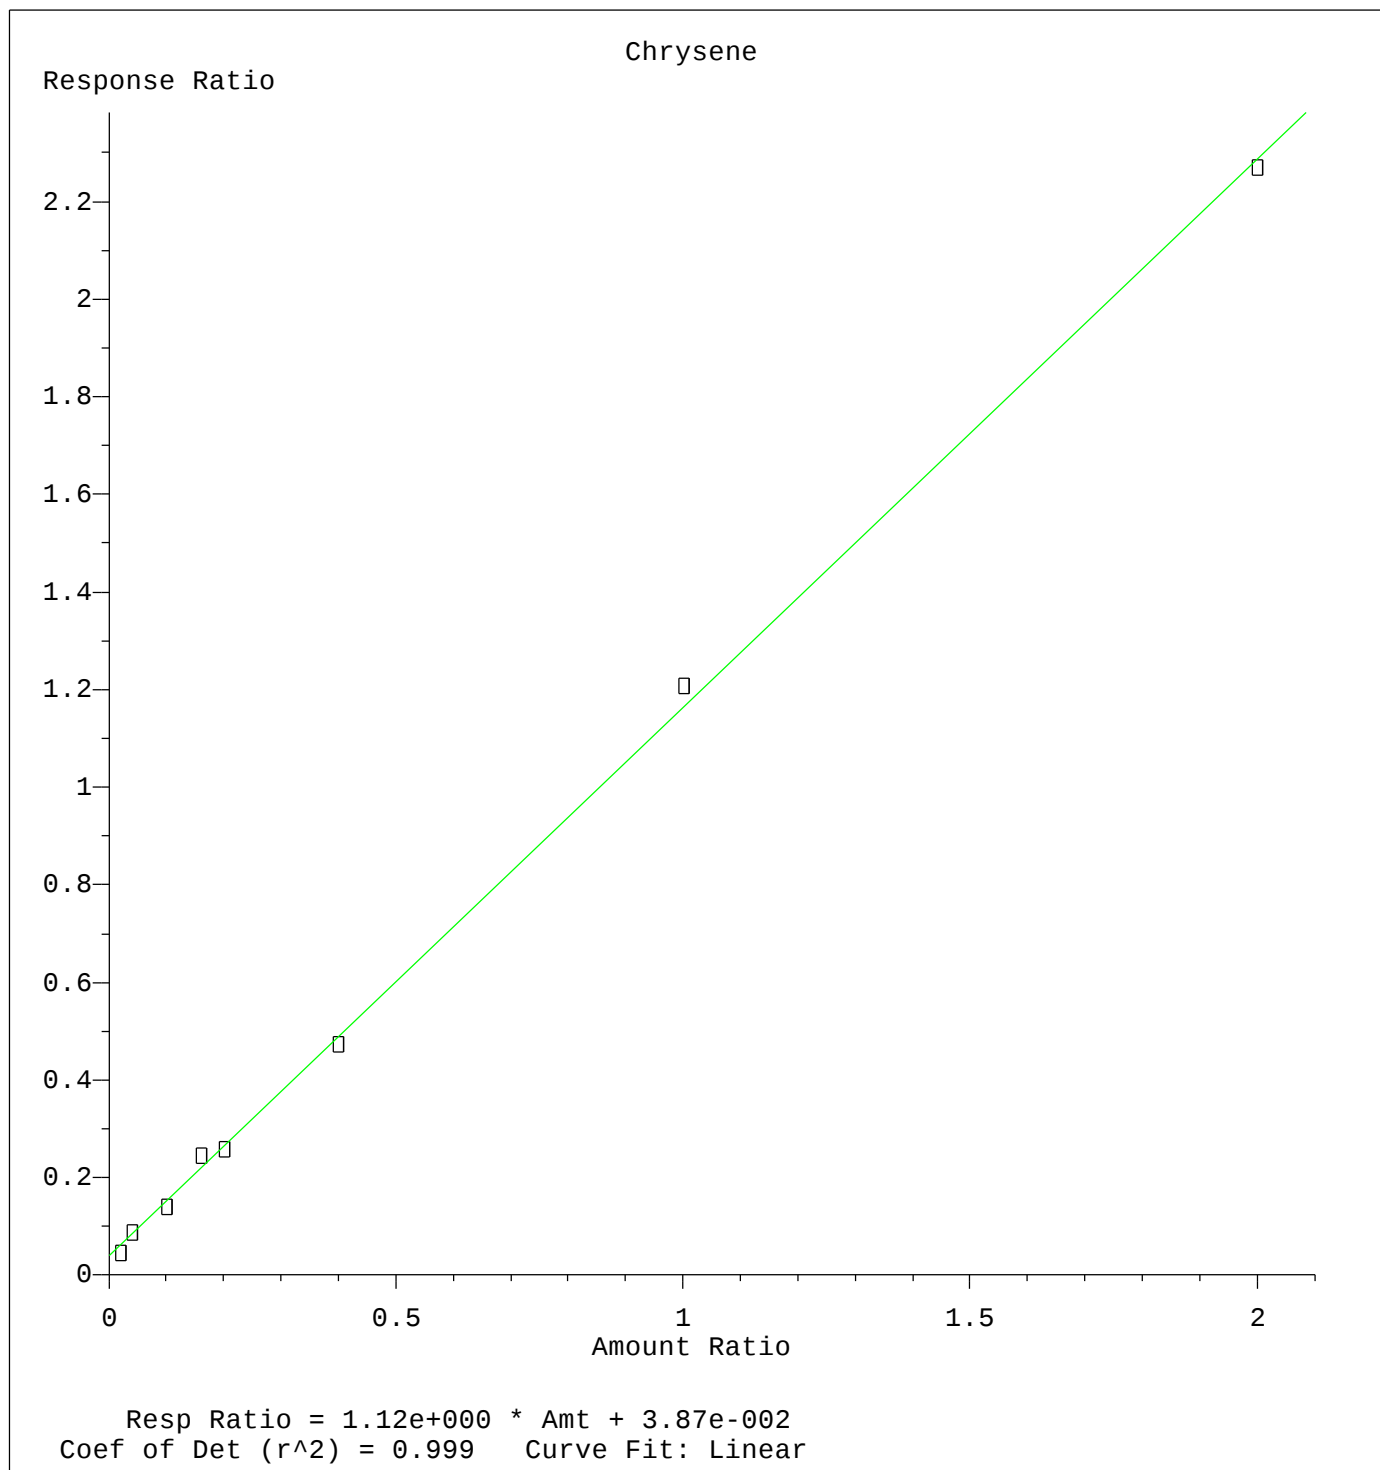

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

Bis(2-ethylhexyl)phthalate

Response Ratio

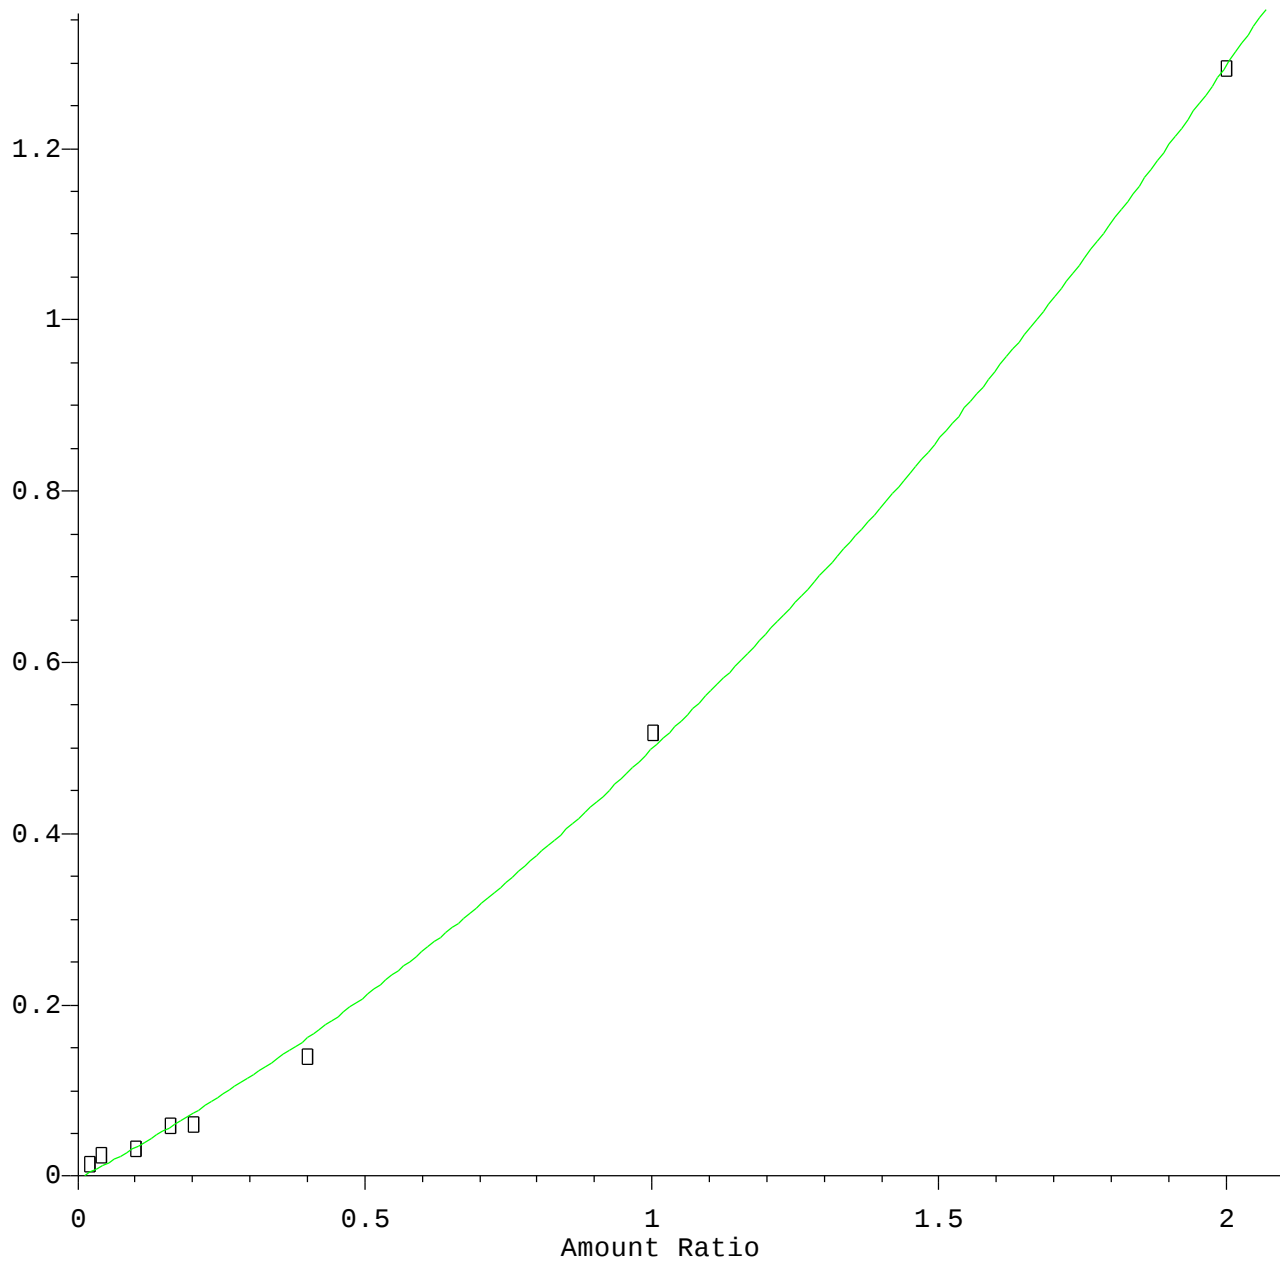


$R = 1.48e-001 A^2 + 3.54e-001 A - 3.56e-003$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015


Indeno(1,2,3-cd)pyrene

Response Ratio

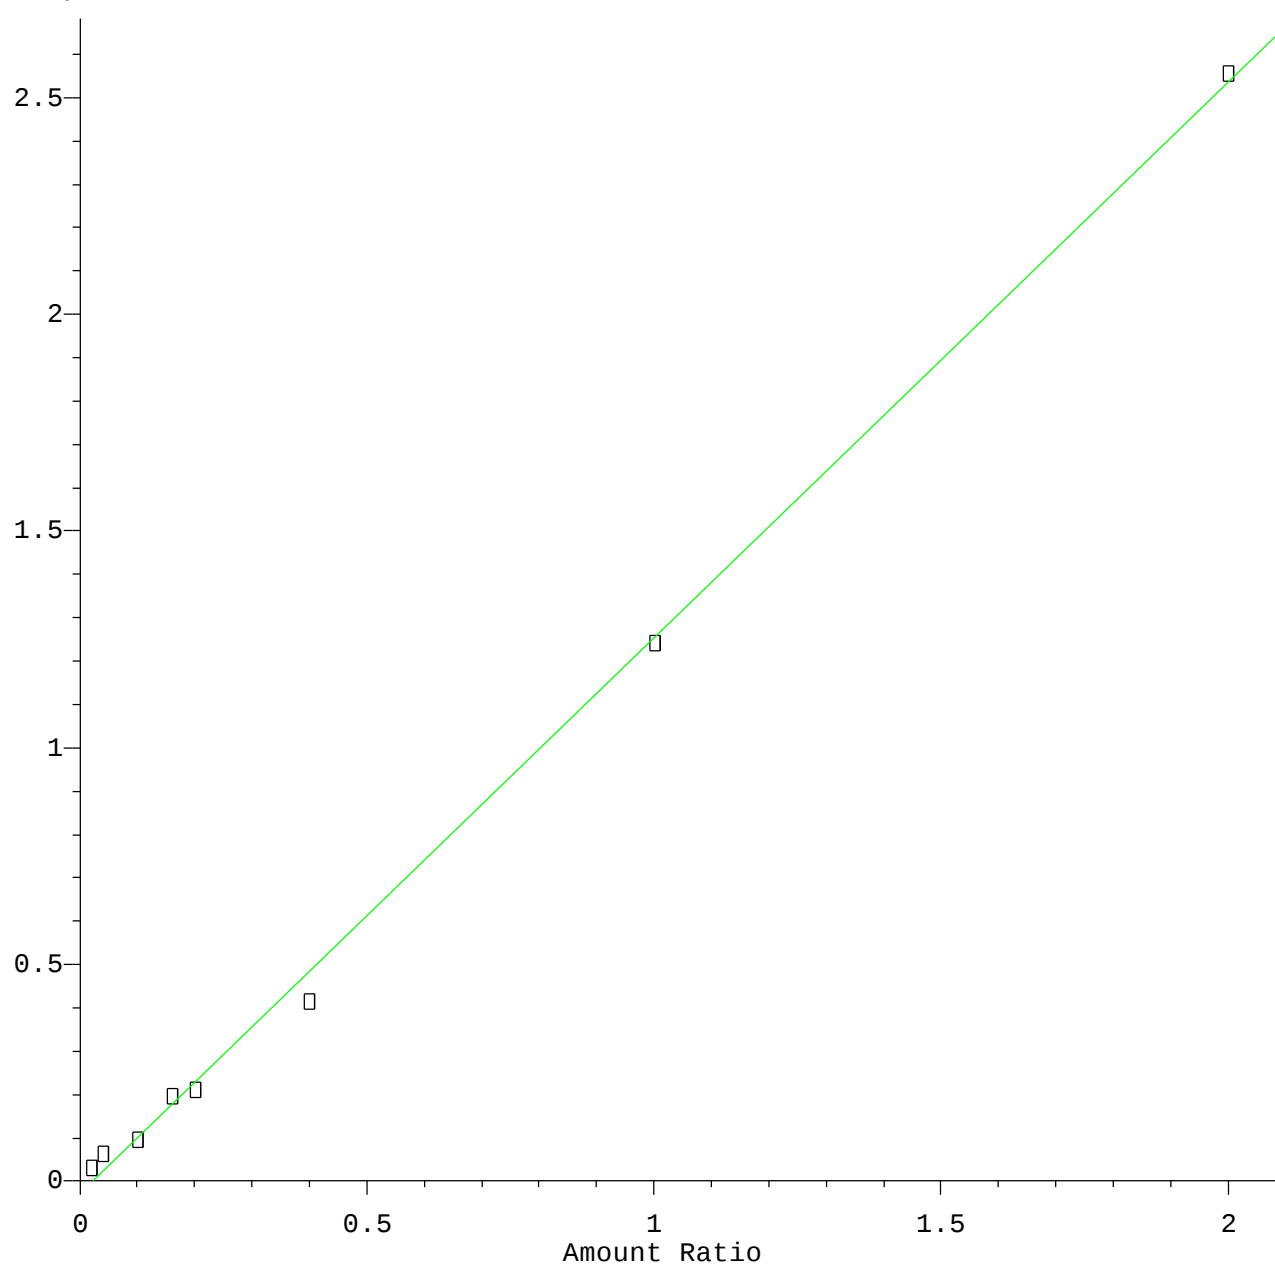

Resp Ratio = 1.28e+000 * Amt - 2.83e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

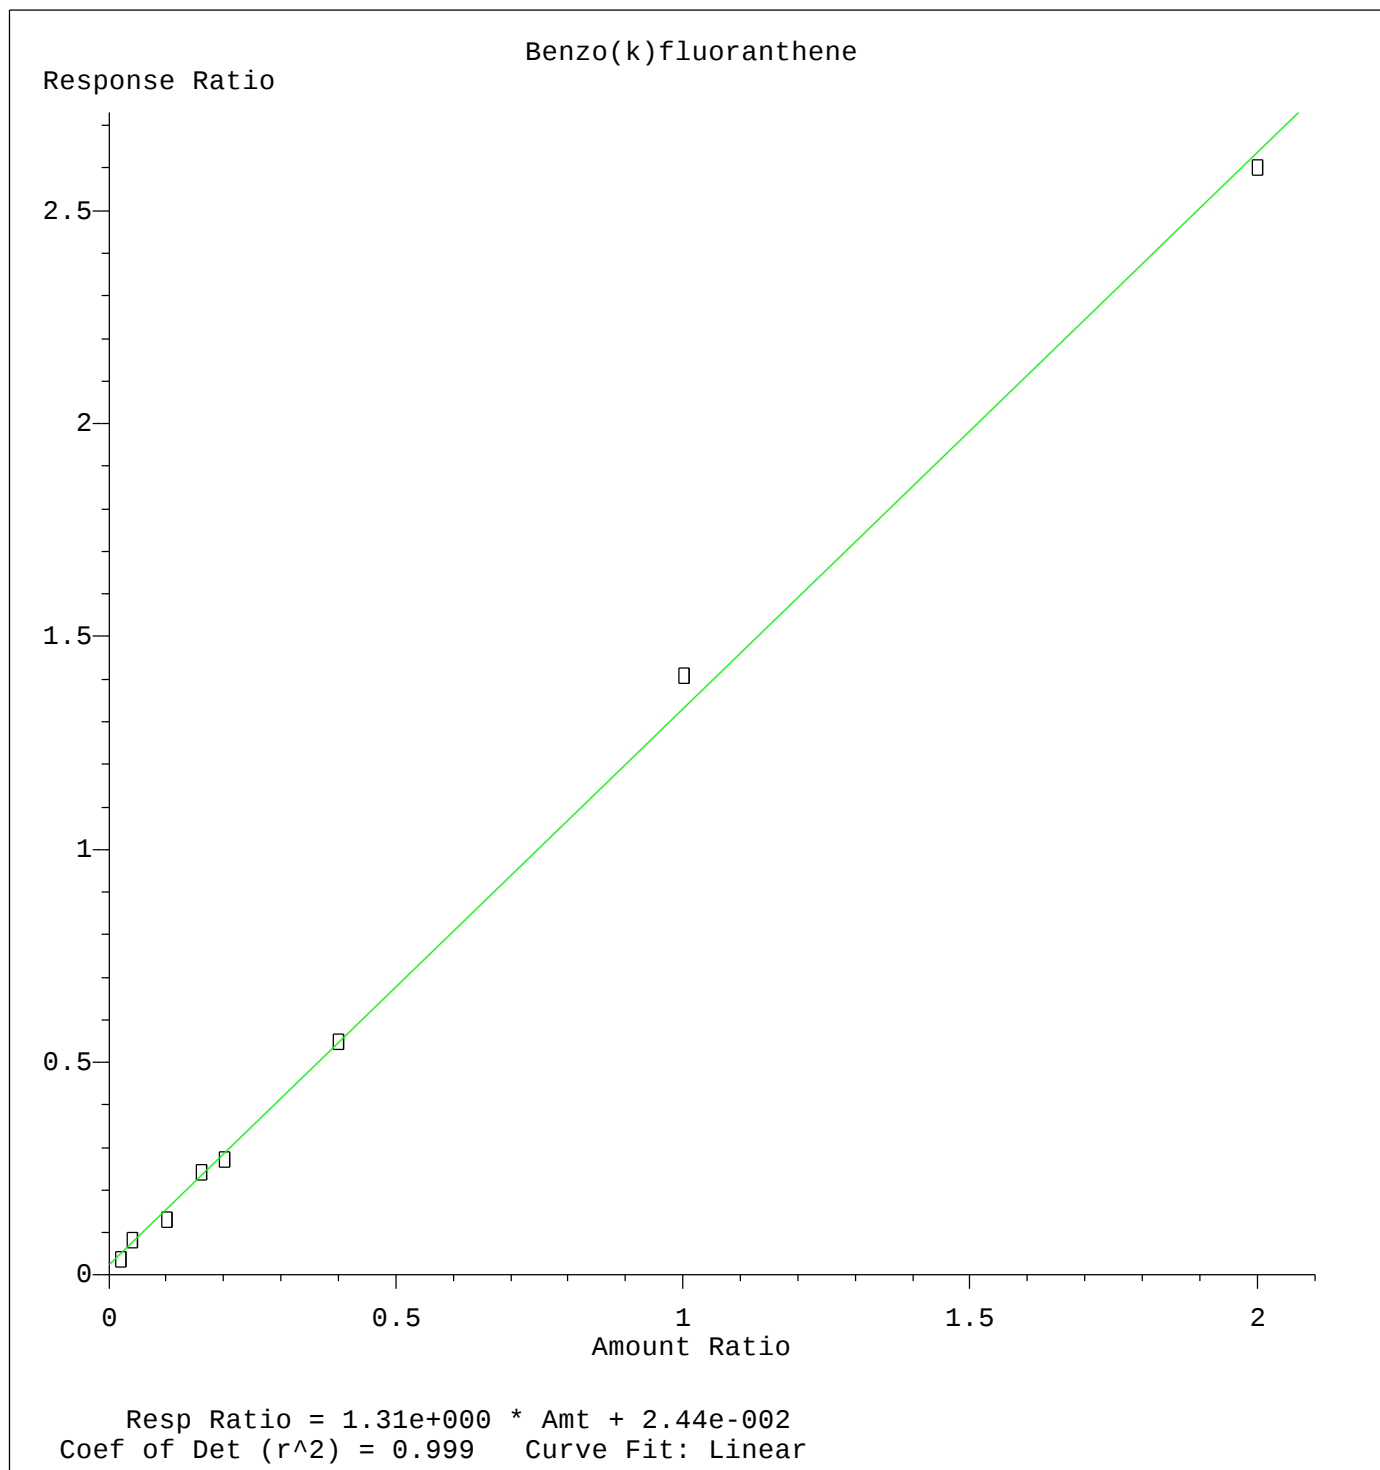

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Calibration Table Last Updated: Wed Sep 30 16:01:03 2015

Method Path : Z:\HPCHEM1\BNA_E\METHODS\
 Method File : 8270-SIM-BE092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 30 16:01:03 2015
 Response Via : Initial Calibration

Calibration Files

0.1 =BE090969.D 0.2 =BE090970.D 0.5 =BE090971.D
 0.8 =BE090972.D 1 =BE090973.D 2 =BE090974.D

	Compound	0.1	0.2	0.5	0.8	1	2	Avg	%RSD

1) I	1,4-Dichlorobenzene-d	-----ISTD-----							
2)	1,4-Dioxane	1.101	1.556	0.819	0.876	0.763	0.695	0.888	34.79
3)	n-Nitrosodimethyl	1.012	1.233	0.784	0.907	0.796	0.747	0.879	19.09
4) S	2-Fluorophenol	1.255	1.393	0.852	1.082	0.918	0.866	1.045	18.41
5) S	Phenol-d6	1.123	1.492	1.065	1.315	1.145	1.210	1.280	13.11
6)	bis(2-Chloroethyl	1.942	2.749	1.204	0.896	1.472	1.209	1.524	37.83
7) I	Naphthalene-d8	-----ISTD-----							
8) S	Nitrobenzene-d5	0.186	0.293	0.221	0.267	0.255	0.270	0.270	18.83
9)	Nitrobenzene		0.245	0.193	0.263	0.259	0.299	0.289	24.71
10)	Naphthalene	1.140	1.449	0.953	1.133	1.024	0.962	1.075	15.78
11)	Hexachlorobutadie	0.190	0.232	0.166	0.199	0.178	0.160	0.179	15.28
12)	2-Methylnaphthale	0.609	0.779	0.541	0.667	0.597	0.594	0.634	11.07
13) I	Acenaphthene-d10	-----ISTD-----							
14) S	2,4,6-Tribromophe	0.203	0.184	0.125	0.155	0.119	0.135	0.158	18.96
15) S	2-Fluorobiphenyl	1.401	1.747	1.150	1.421	1.262	1.240	1.355	13.39
16)	Acenaphthylene	0.848	1.065	0.731	0.866	0.765	0.771	0.835	E1 12.36
17)	Acenaphthene	1.358	1.785	1.206	1.414	1.255	1.210	1.334	14.83
18)	Fluorene	1.781	2.085	1.424	1.708	1.540	1.555	1.649	12.73
19) I	Phenanthrene-d10	-----ISTD-----							
20)	4-Bromophenyl-phe	0.228	0.220	0.160	0.194	0.174	0.170	0.189	12.78
21)	Hexachlorobenzene	1.063	1.286	0.887	1.032	0.927	0.858	0.970	15.71
22)	Pentachlorophenol	0.110	0.081	0.050	0.064	0.045	0.049	0.070	32.41
23)	Phenanthrene	1.643	1.519	1.080	1.290	1.152	1.107	1.265	16.53
24)	Anthracene	1.244	1.503	0.965	1.121	0.999	1.016	1.131	15.38
25)	Fluoranthene	2.354	1.948	1.230	1.435	1.223	1.184	1.503	28.09
26) I	Chrysene-d12	-----ISTD-----							
27)	Benzidine		0.089	0.066	0.081	0.073	0.085	0.090	31.85
28)	Pyrene	1.891	1.544	1.071	1.230	1.064	1.108	1.277	22.88
29) S	Terphenyl-d14		0.847	0.559	0.645	0.549	0.575	0.631	16.10
30)	Benzo(a)anthracen	1.556	1.388	0.925	1.157	1.058	1.076	1.176	17.11
31)	3,3'-Dichlorobenz	0.196	0.252	0.152	0.179	0.147	0.164	0.201	25.55
32)	Chrysene	2.182	2.136	1.382	1.531	1.286	1.182	1.505	28.09
33)	Bis(2-ethylhexyl)	0.685	0.582	0.309	0.364	0.298	0.348	0.469	33.59
34)	Indeno(1,2,3-cd)p	1.406	1.528	0.957	1.213	1.047	1.030	1.212	16.14
35) I	Perylene-d12	-----ISTD-----							
36)	Benzo(b)fluoranth	1.289	1.210	0.865	1.081	0.989	1.036	1.102	12.39
37)	Benzo(k)fluoranth	1.867	2.023	1.302	1.497	1.360	1.370	1.515	18.17
38) C	Benzo(a)pyrene	1.046	1.187	0.797	1.114	0.884	0.935	1.022	13.24
39)	Dibenzo(a,h)anthr	1.046	1.114	0.808	0.984	0.850	0.930	1.009	13.92
40)	Benzo(g,h,i)peryl	1.196	1.314	0.900	1.100	0.952	0.992	1.096	12.68

(#) = Out of Range ### Number of calibration levels exceeded format ###