
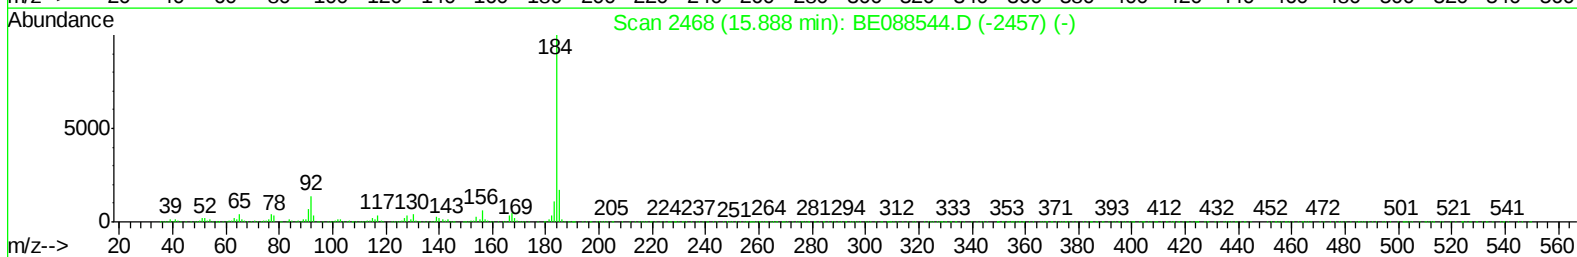
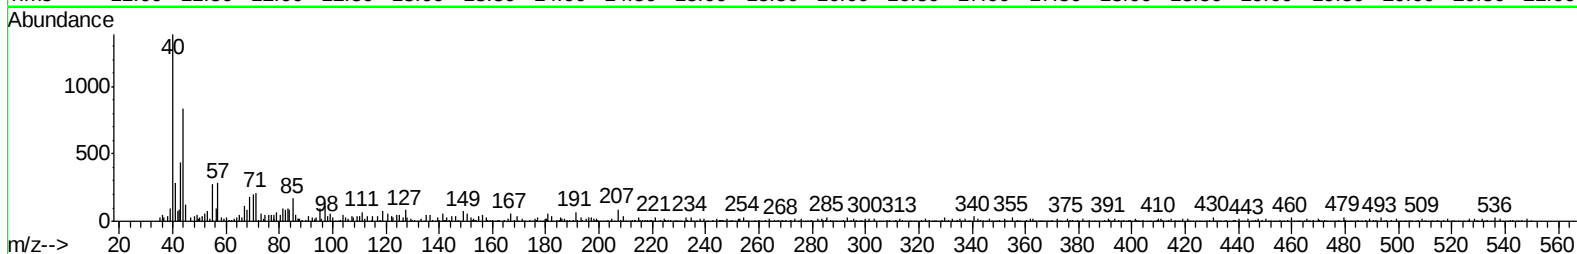


Data Path : Z:\HPCHEM1\BNA E\Data\BE092815\
 Data File : BE090968.D
 Acq On : 28 Sep 2015 15:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 08:44:42 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 06 14:19:16 2014
 Response via : Initial Calibration

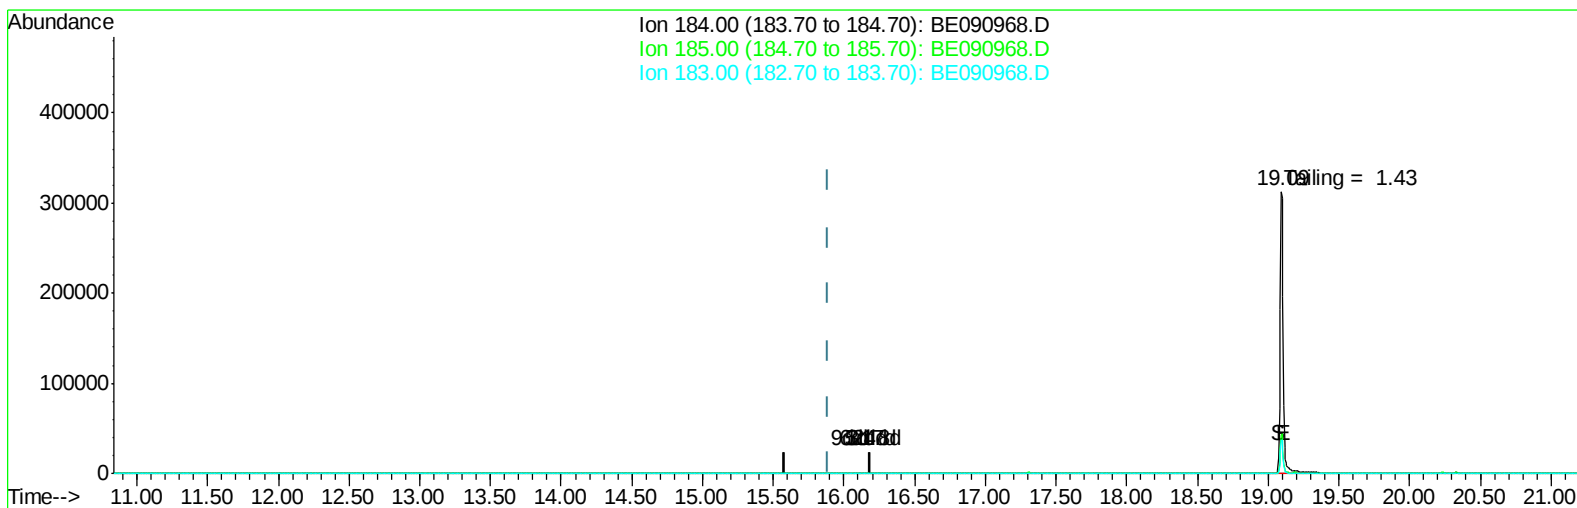

TIC: BE090968.D

(76) Benzidine




16.177min (+0.289) 4.82ng

response 10

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	375.00#
183.00	10.70	33.33#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE092815\
 Data File : BE090968.D
 Acq On : 28 Sep 2015 15:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 08:44:42 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-BE110514.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 06 14:19:16 2014
 Response via : Initial Calibration

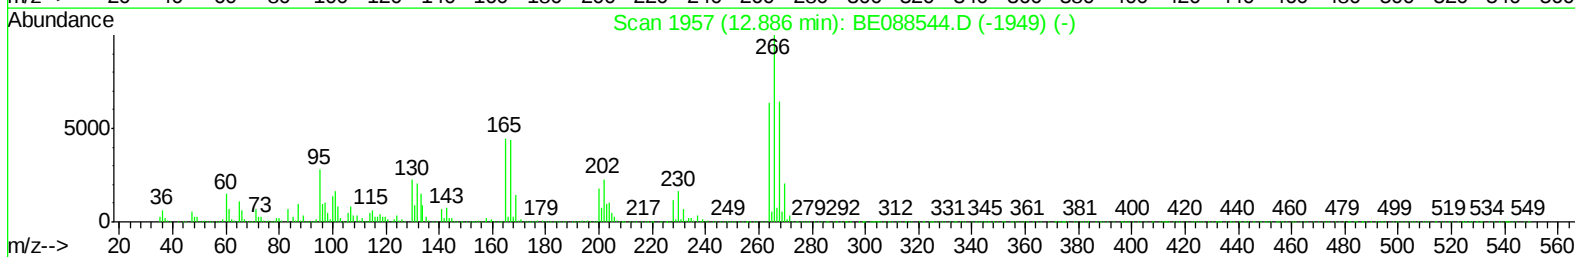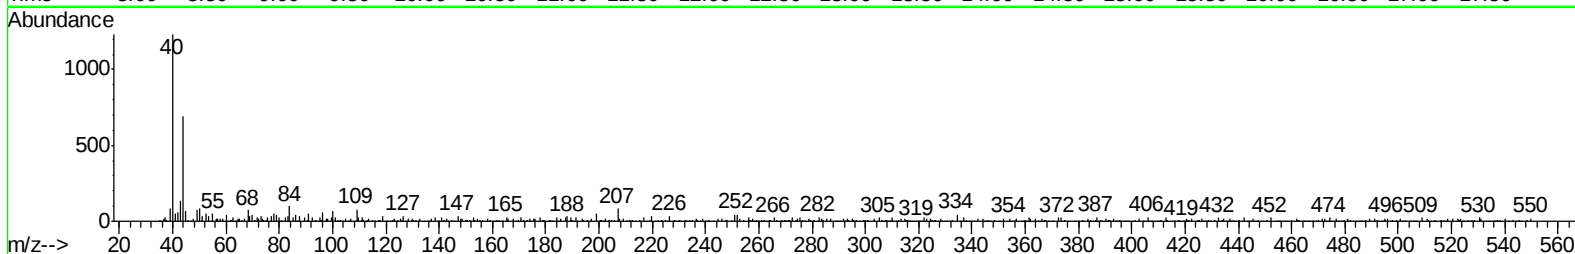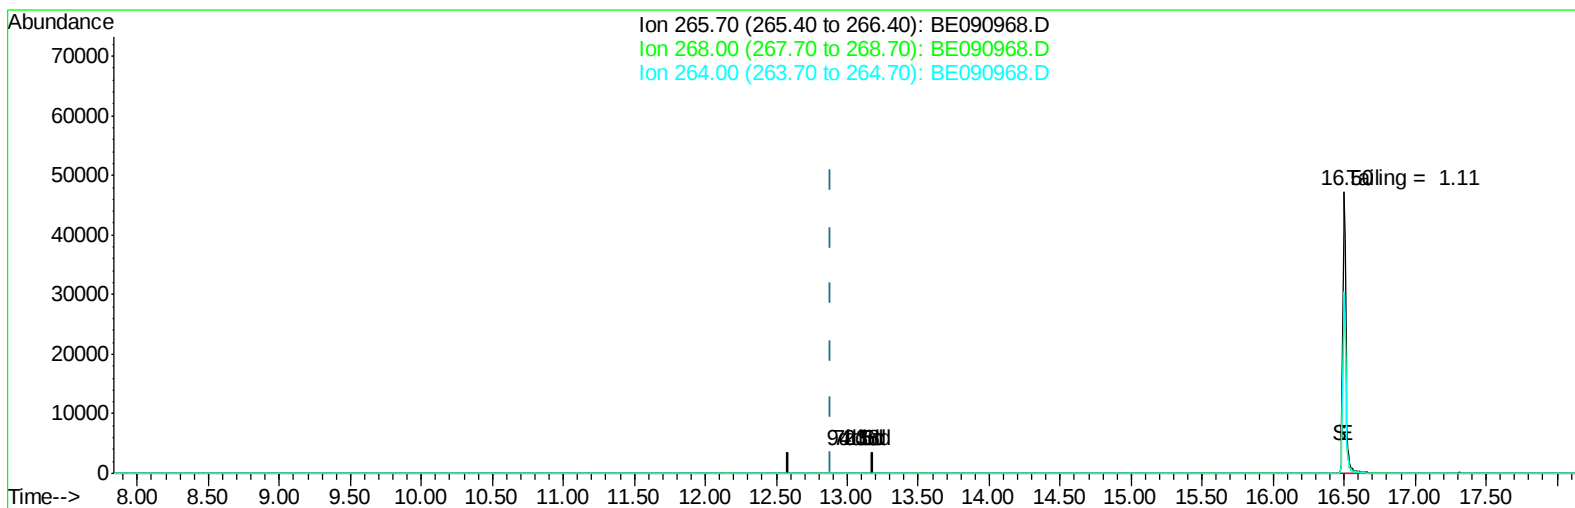

TIC: BE090968.D

(69) Pentachlorophenol (C)

13.122min (+0.236) 74.27ng

response 7

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	13.04#
264.00	63.70	65.22
0.00	0.00	0.00