


Data Path : Z:\HPCHEM1\BNA E\DATA\BE092815\
 Data File : BE090968.D
 Acq On : 28 Sep 2015 15:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 29 07:30:21 2015

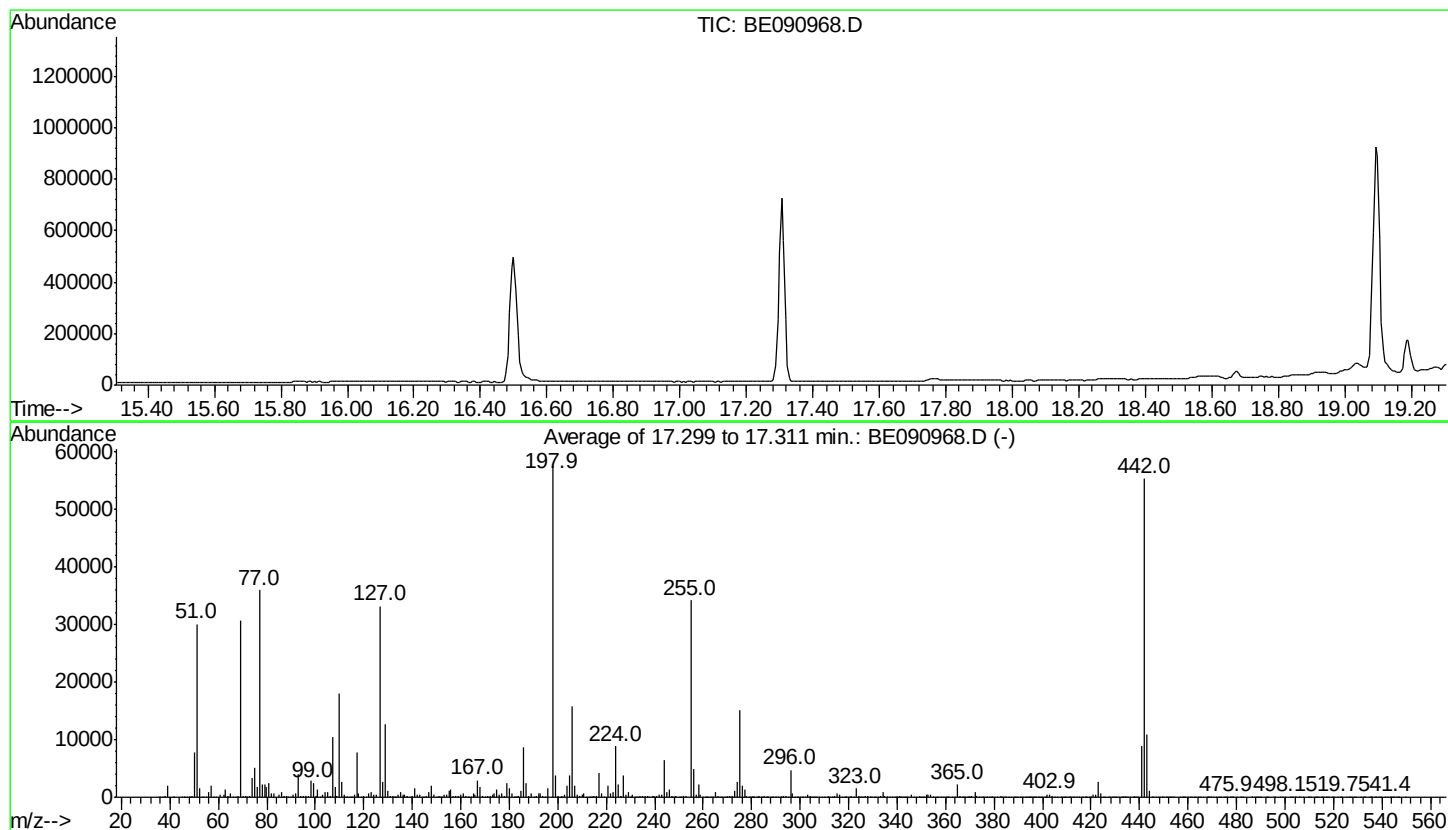

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.2	30045	PASS
68	69	0.00	2	1.1	337	PASS
69	198	0.00	100	53.2	30641	PASS
70	69	0.00	2	0.5	147	PASS
127	198	10	80	57.7	33197	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57576	PASS
199	198	5	9	6.6	3786	PASS
275	198	10	60	26.2	15057	PASS
365	198	1	100	3.8	2182	PASS
441	442	0.01	24	16.3	8981	PASS
442	198	50	100	96.0	55248	PASS
443	442	15	24	19.7	10905	PASS