




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094144.D
Acq On : 29 Sep 2017 9:46
Operator : SJ/JU
Sample : PB102704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:15 PM

Quant Time: Sep 29 14:19:13 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

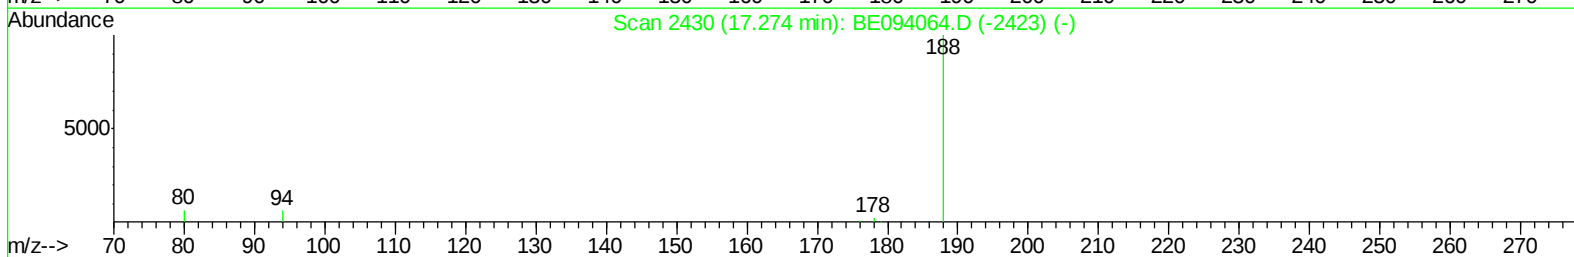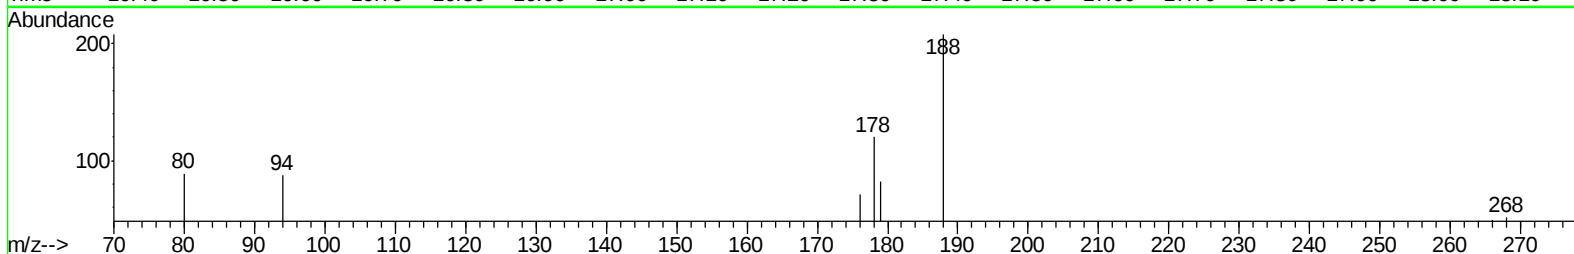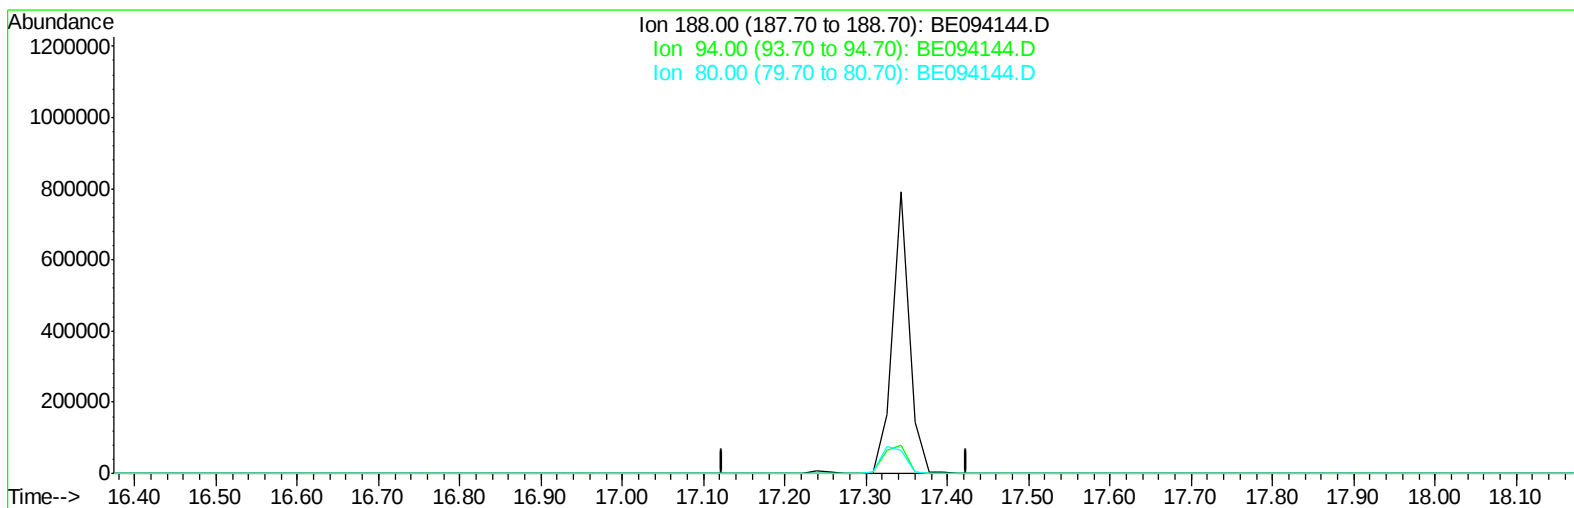

TIC: BE094144.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094144.D
Acq On : 29 Sep 2017 9:46
Operator : SJ/JU
Sample : PB102704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:15 PM

Quant Time: Sep 29 14:19:13 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

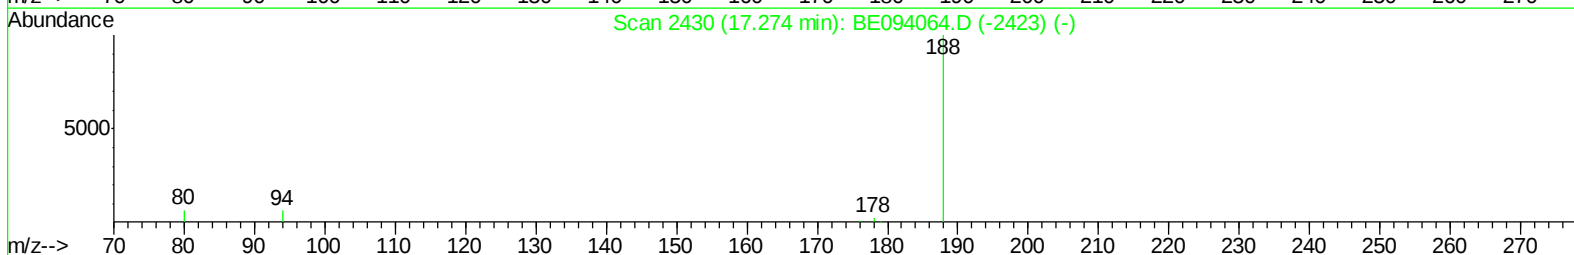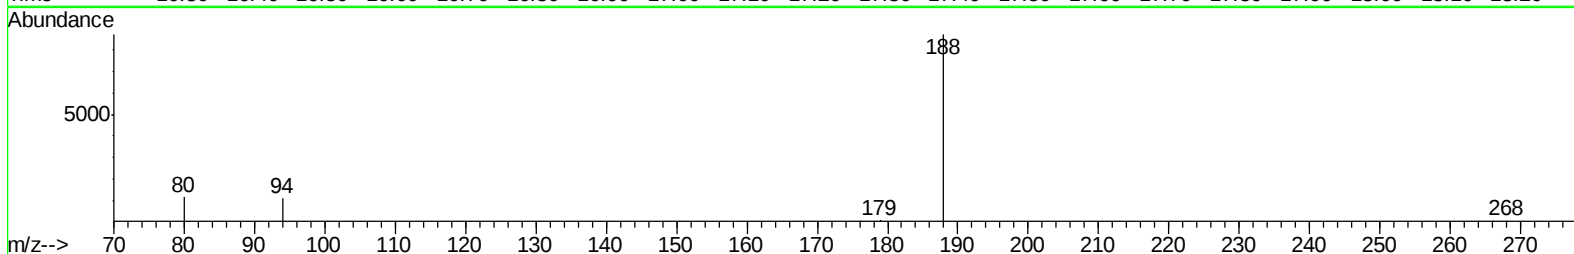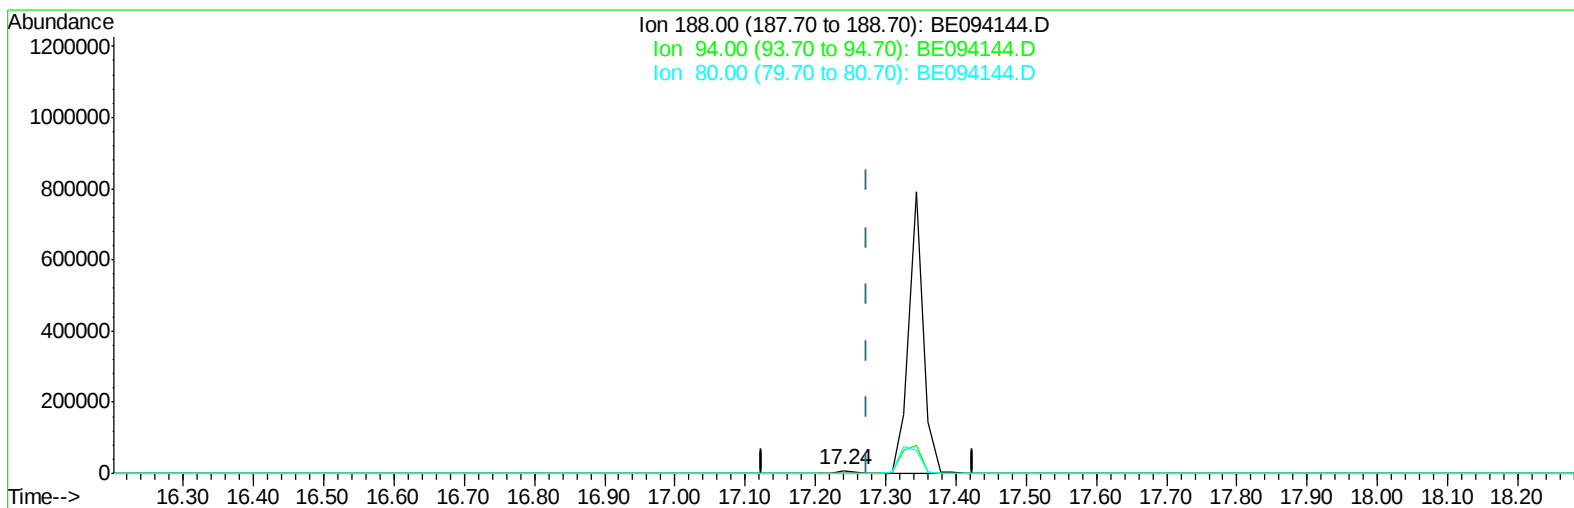

TIC: BE094144.D

(10) Phenanthrene-d10 (I)

17.240min (-0.034) 0.40ng/ul m

response 14546

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.62
80.00	11.80	13.36
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094144.D
Acq On : 29 Sep 2017 9:46
Operator : SJ/JU
Sample : PB102704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:15 PM

Quant Time: Sep 29 14:20:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

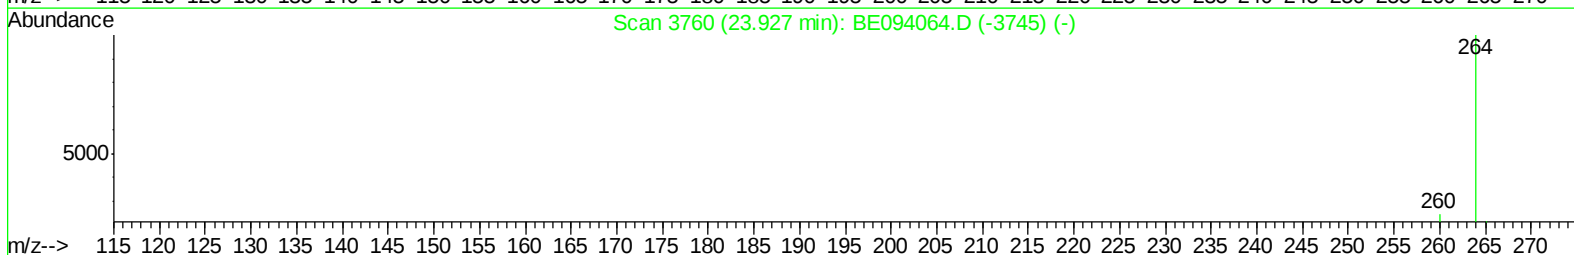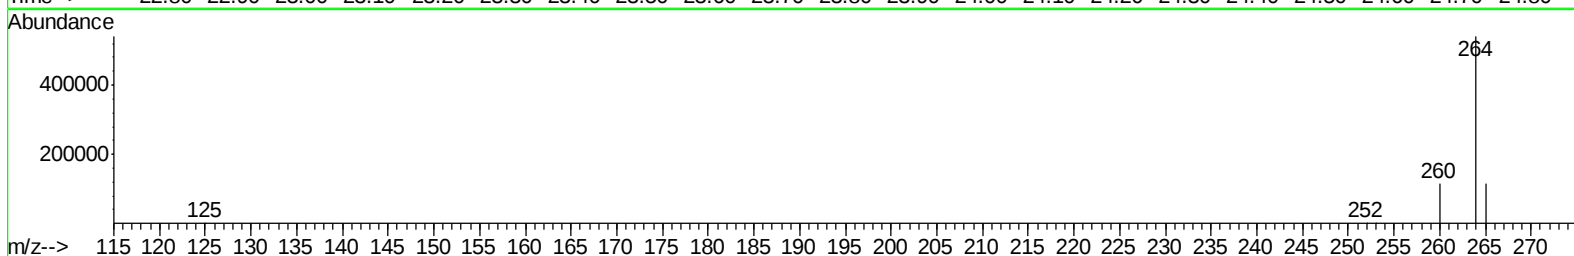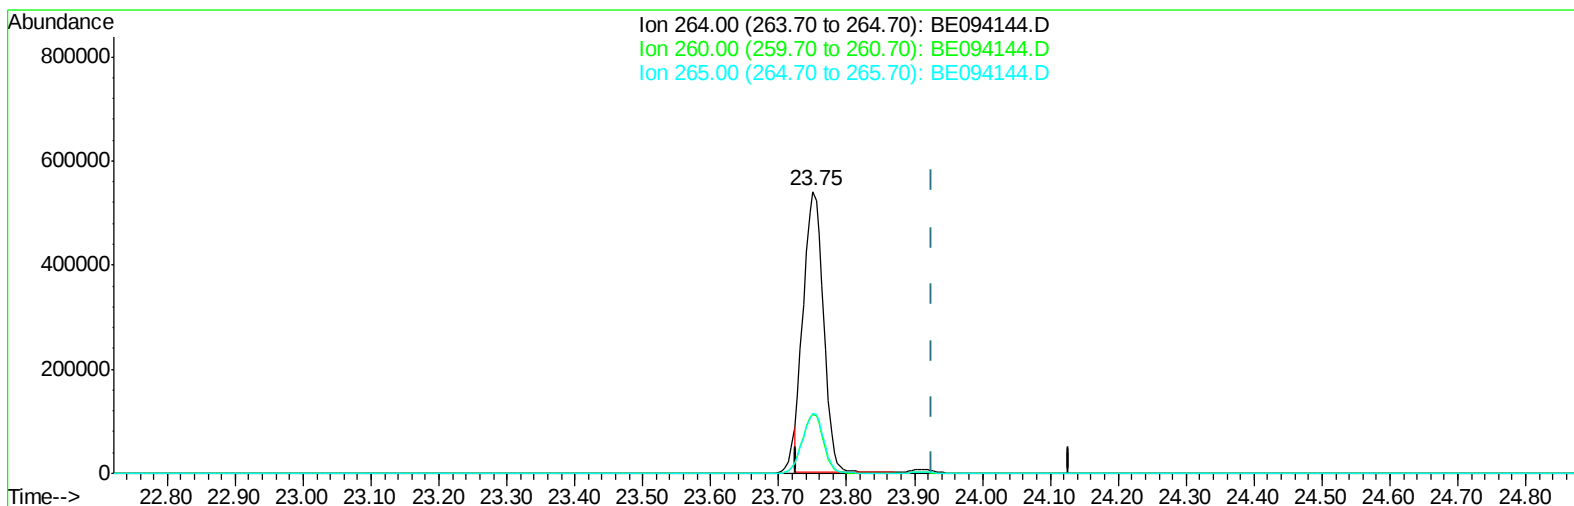

TIC: BE094144.D

(20) Perylene-d12 (I)

23.750min (-0.177) 0.40ng/ul

response 1106928

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.10#
265.00	103.50	21.47#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094144.D
Acq On : 29 Sep 2017 9:46
Operator : SJ/JU
Sample : PB102704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:15 PM

Quant Time: Sep 29 14:20:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

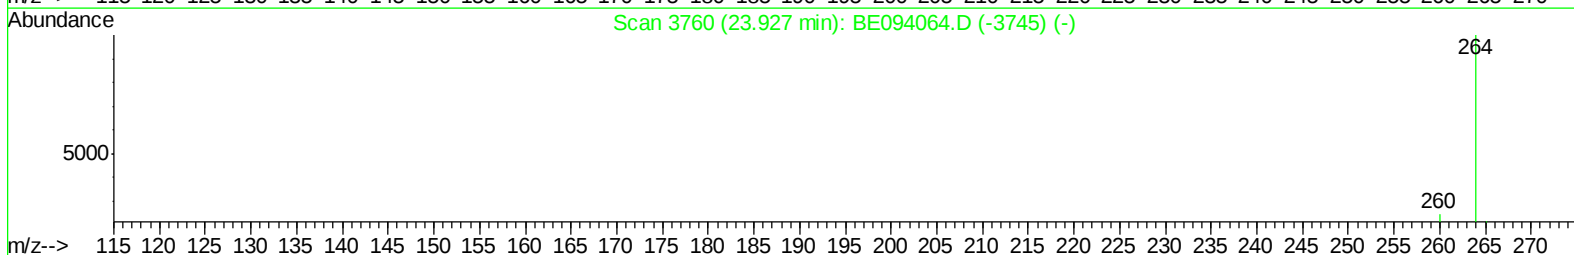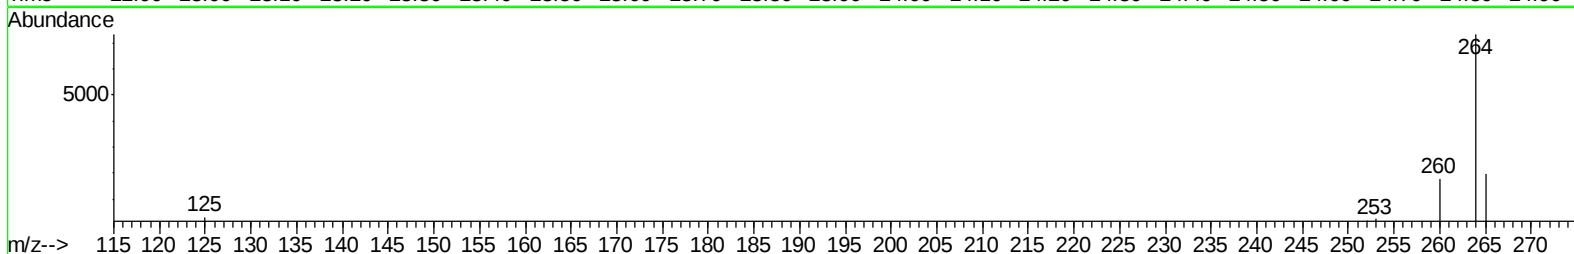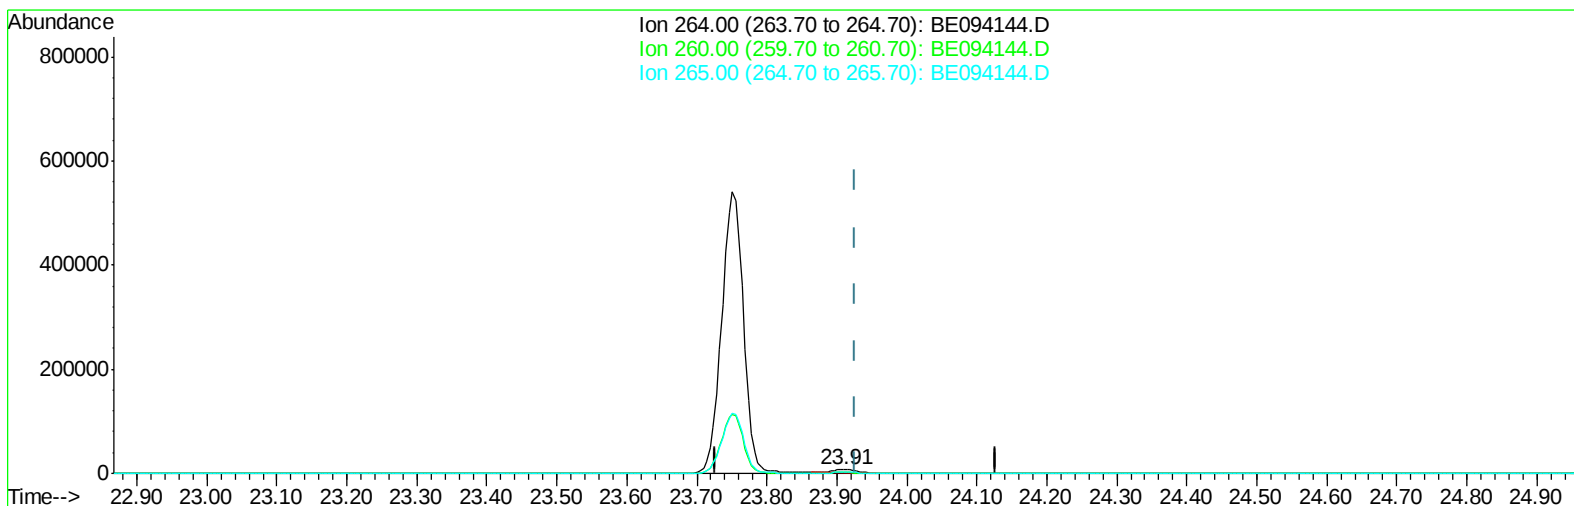

TIC: BE094144.D

(20) Perylene-d12 (I)

23.910min (-0.017) 0.40ng/ul m

response 13333

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.62
265.00	103.50	27.25#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094144.D
Acq On : 29 Sep 2017 9:46
Operator : SJ/JU
Sample : PB102704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:15 PM

Quant Time: Sep 29 14:22:35 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1592	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	8336	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5910	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.24	188	14546m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.41	240	14718	0.40	ng/ul	-0.01
20) Perylene-d12	23.91	264	13333m	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	4348	0.34	ng/ul	-0.01
14) Fluoranthene-d10	19.27	212	14269	0.29	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094144.D
Acq On : 29 Sep 2017 9:46
Operator : SJ/JU
Sample : PB102704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:15 PM

Quant Time: Sep 29 14:22:35 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

