




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
 Data File : BE094145.D
 Acq On : 29 Sep 2017 10:24
 Operator : SJ/JU
 Sample : I5505-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B0AD4

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:37:18 PM

Quant Time: Sep 29 14:25:59 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 29 14:23:42 2017
 Response via : Initial Calibration

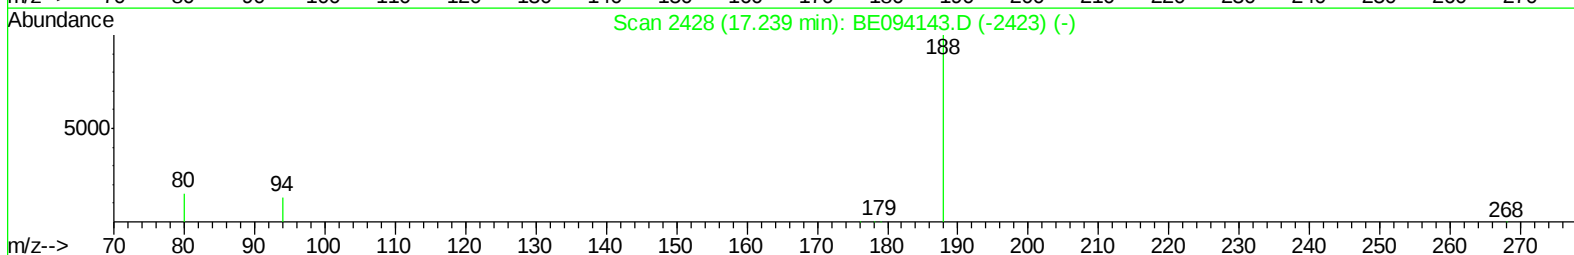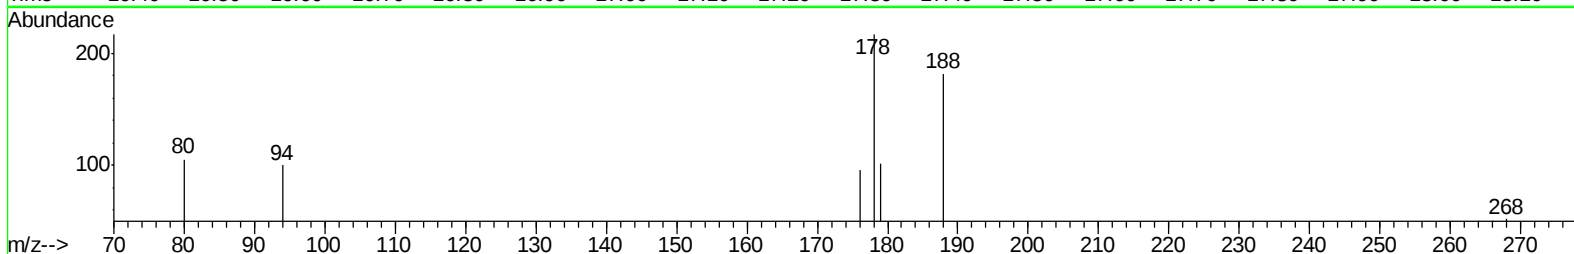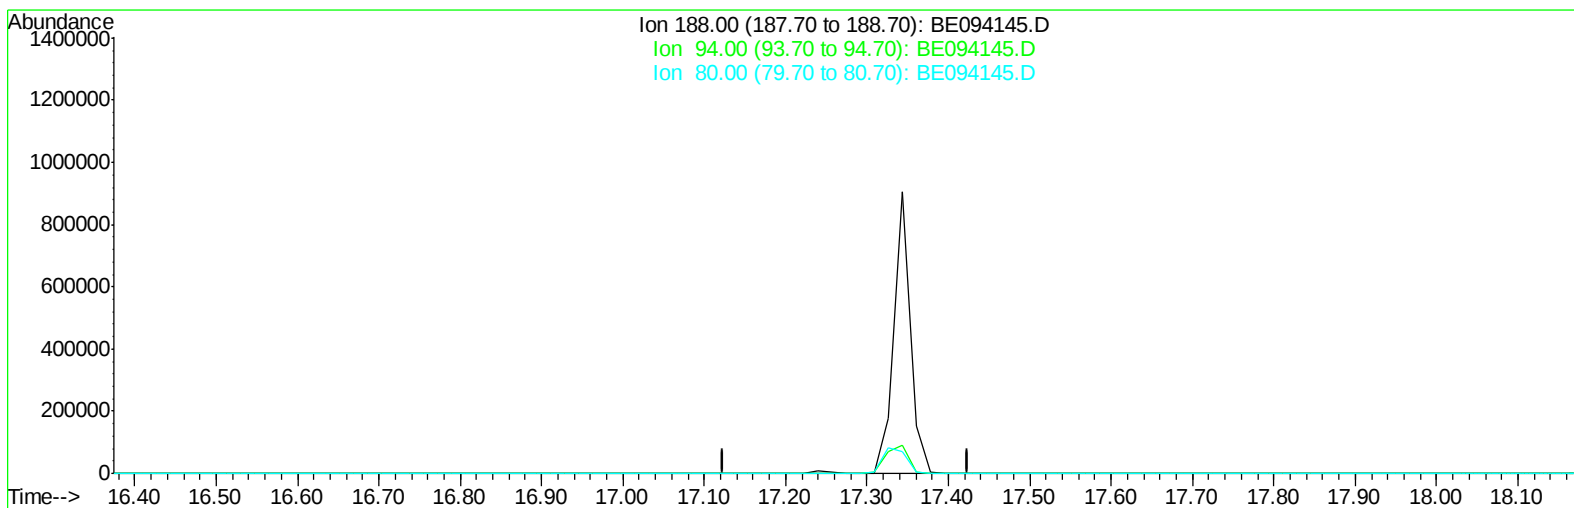

TIC: BE094145.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094145.D
Acq On : 29 Sep 2017 10:24
Operator : SJ/JU
Sample : I5505-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B0AD4

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:18 PM

Quant Time: Sep 29 14:25:59 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 29 14:23:42 2017
Response via : Initial Calibration

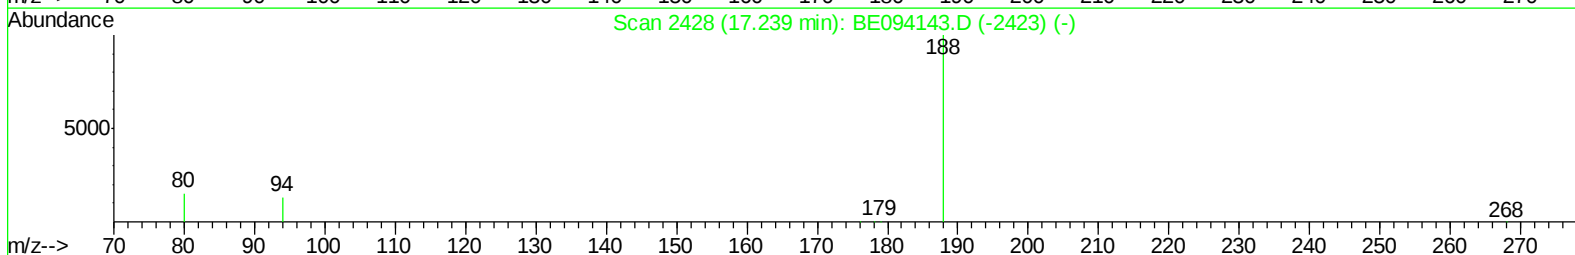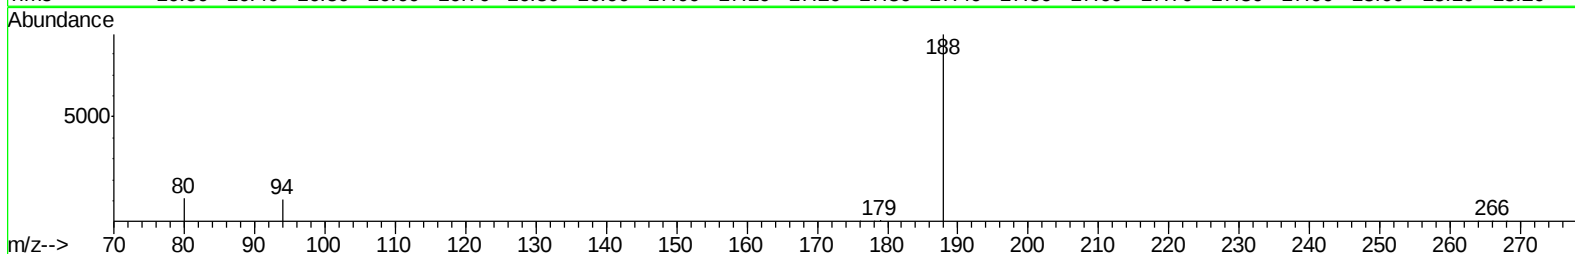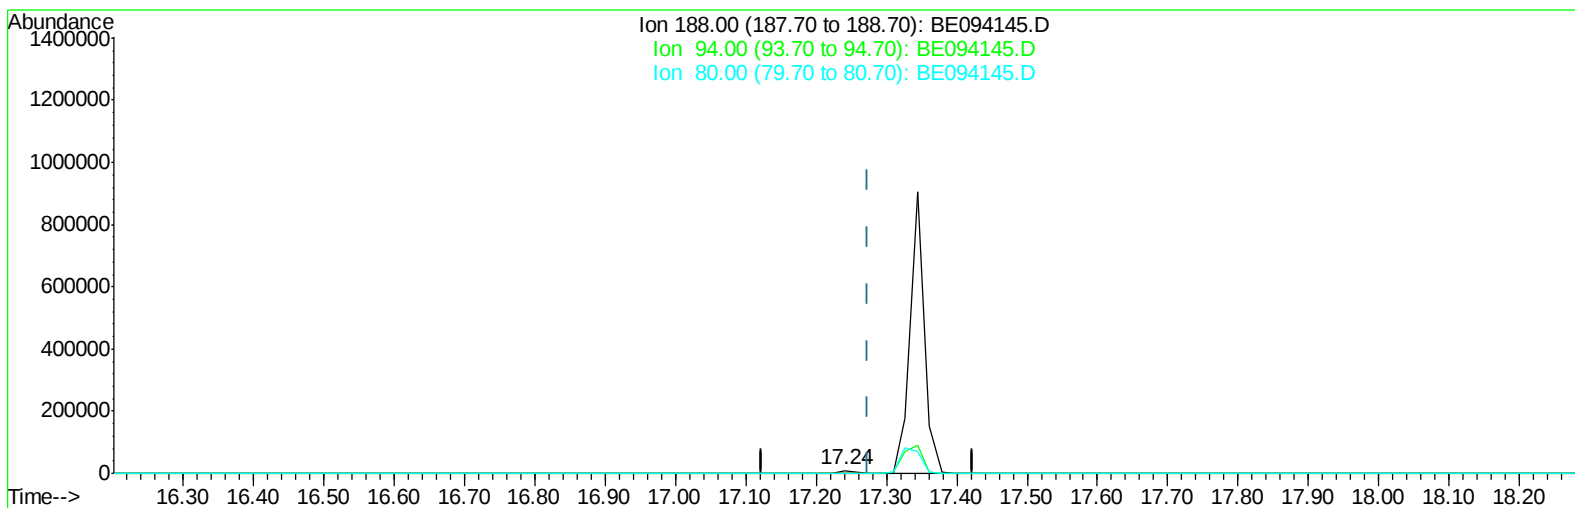

TIC: BE094145.D

(10) Phenanthrene-d10 (I)

17.240min (-0.034) 0.40ng/ul m

response 14073

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.91
80.00	11.80	12.77
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094145.D
Acq On : 29 Sep 2017 10:24
Operator : SJ/JU
Sample : I5505-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B0AD4

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:18 PM

Quant Time: Sep 29 14:26:45 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 29 14:23:42 2017
Response via : Initial Calibration

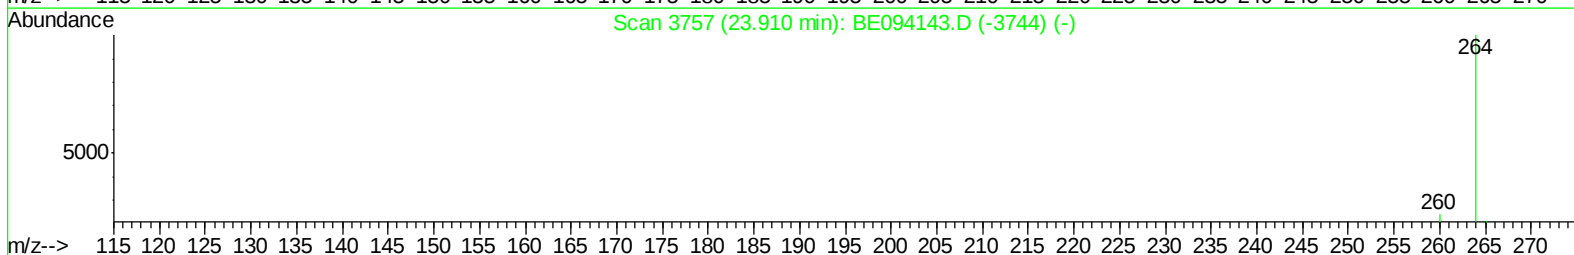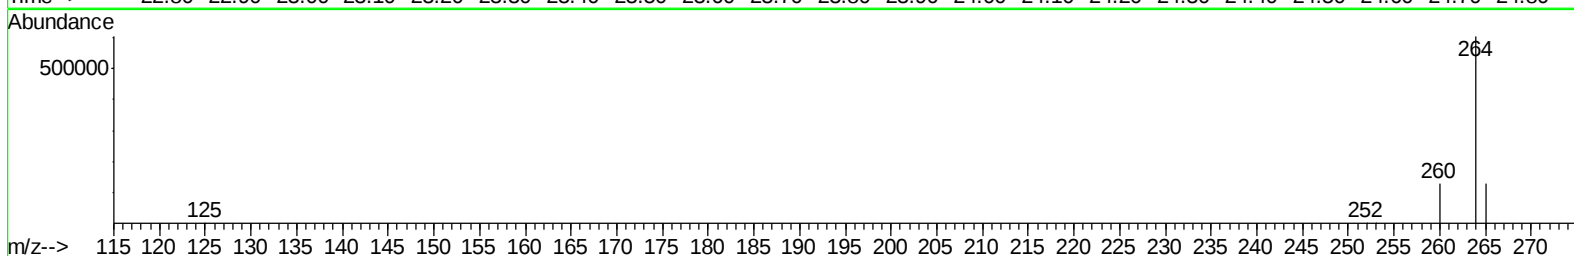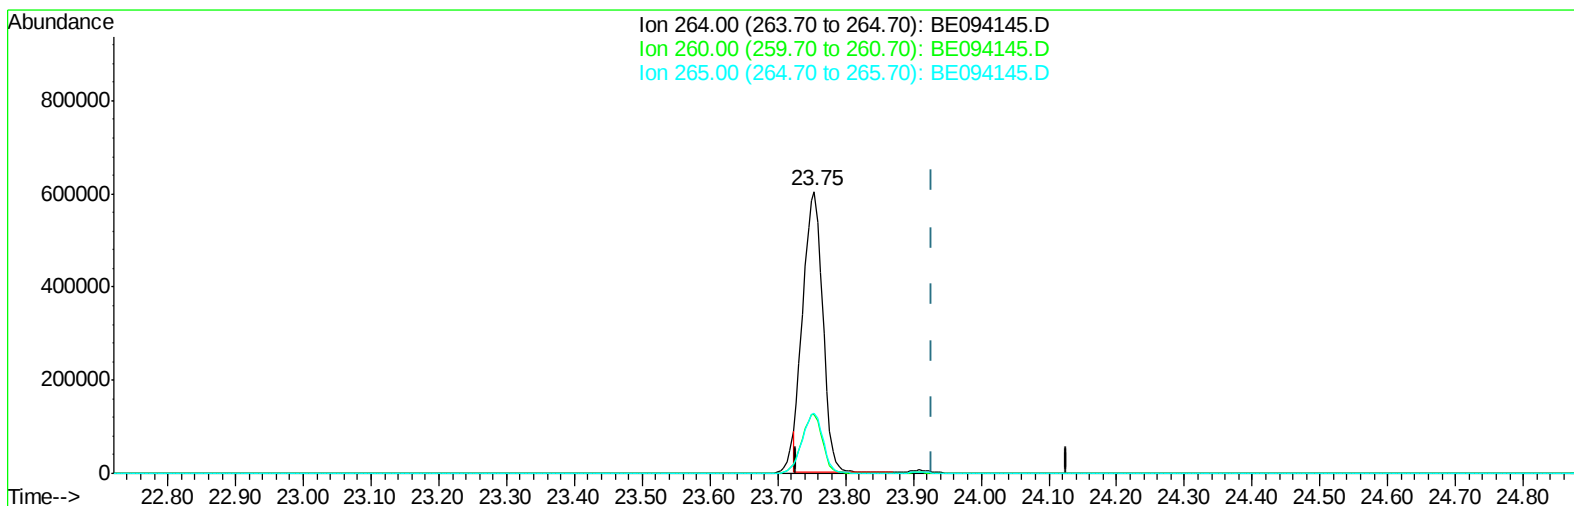

TIC: BE094145.D

(20) Perylene-d12 (I)

23.754min (-0.173) 0.40ng/ul

response 1233373

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.08#
265.00	103.50	21.55#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094145.D
Acq On : 29 Sep 2017 10:24
Operator : SJ/JU
Sample : I5505-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B0AD4

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:18 PM

Quant Time: Sep 29 14:26:45 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 29 14:23:42 2017
Response via : Initial Calibration

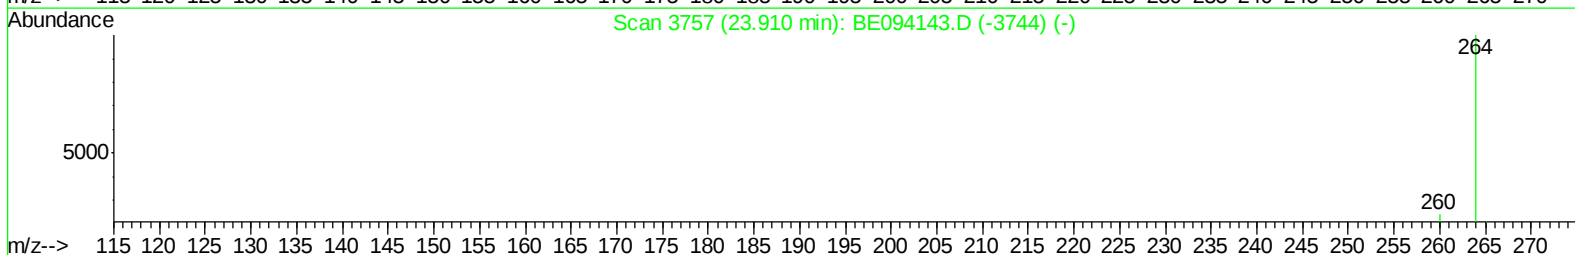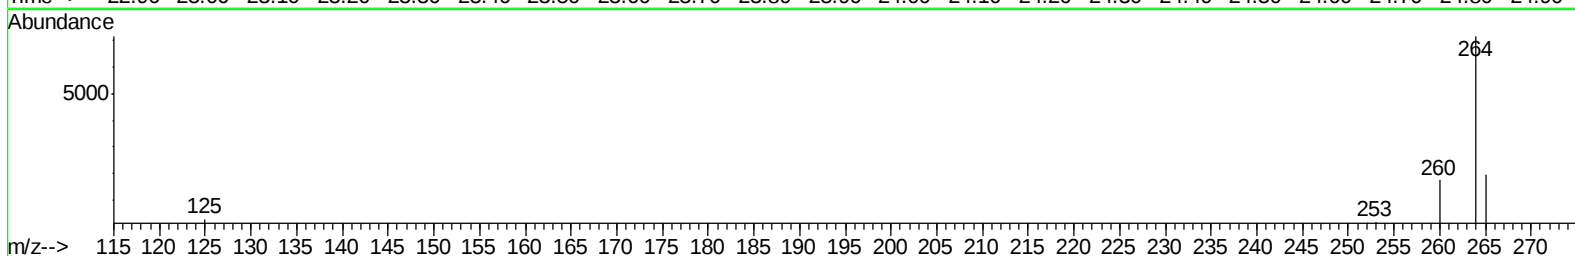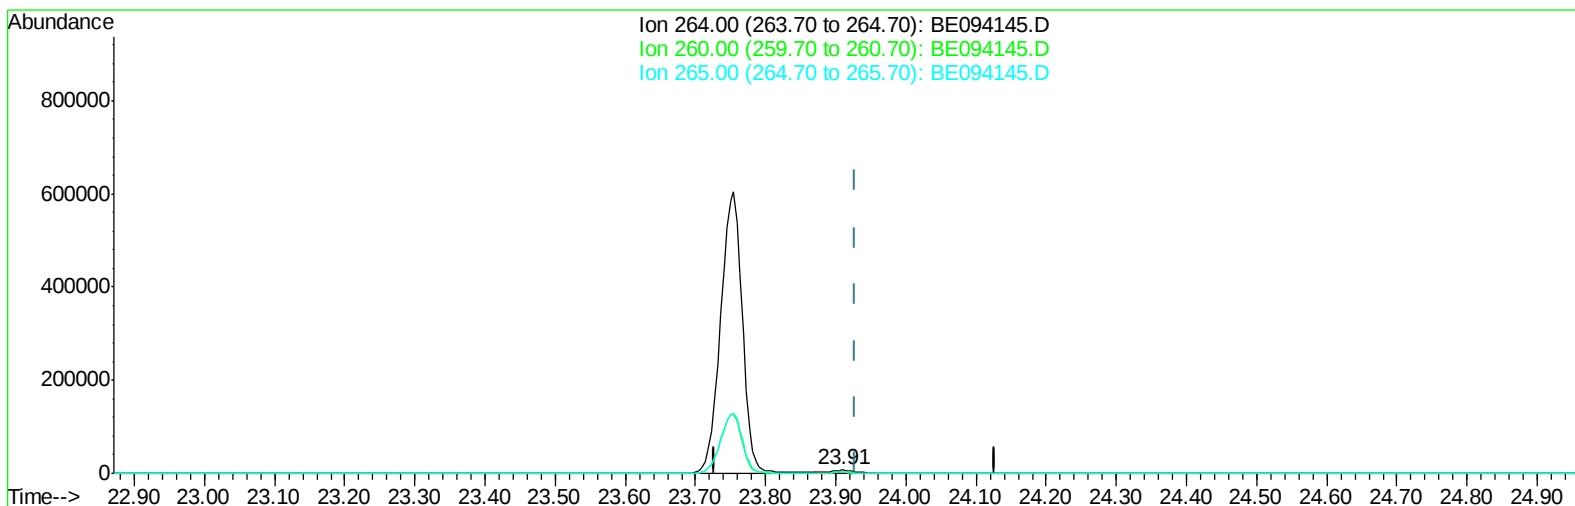

TIC: BE094145.D

(20) Perylene-d12 (I)

23.909min (-0.018) 0.40ng/ul m

response 12401

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.91
265.00	103.50	27.98#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
 Data File : BE094145.D
 Acq On : 29 Sep 2017 10:24
 Operator : SJ/JU
 Sample : I5505-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B0AD4

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:37:18 PM

Quant Time: Sep 29 14:27:48 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 29 14:23:42 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1616	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	8361	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5815	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.24	188	14073m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.40	240	14060	0.40	ng/ul	-0.01
20) Perylene-d12	23.91	264	12401m	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	5043	0.39	ng/ul	-0.02
14) Fluoranthene-d10	19.27	212	16361	0.35	ng/ul	-0.02

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE092917\
Data File : BE094145.D
Acq On : 29 Sep 2017 10:24
Operator : SJ/JU
Sample : I5505-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B0AD4

Manual Integrations
APPROVED

Sohil
10/2/2017 5:37:18 PM

Quant Time: Sep 29 14:27:48 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 29 14:23:42 2017
Response via : Initial Calibration

