


Data Path : Z:\HPCHEM1\BNA E\DATA\BE093015\
Data File : BE090978.D
Acq On : 30 Sep 2015 11:24
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 30 16:01:03 2015

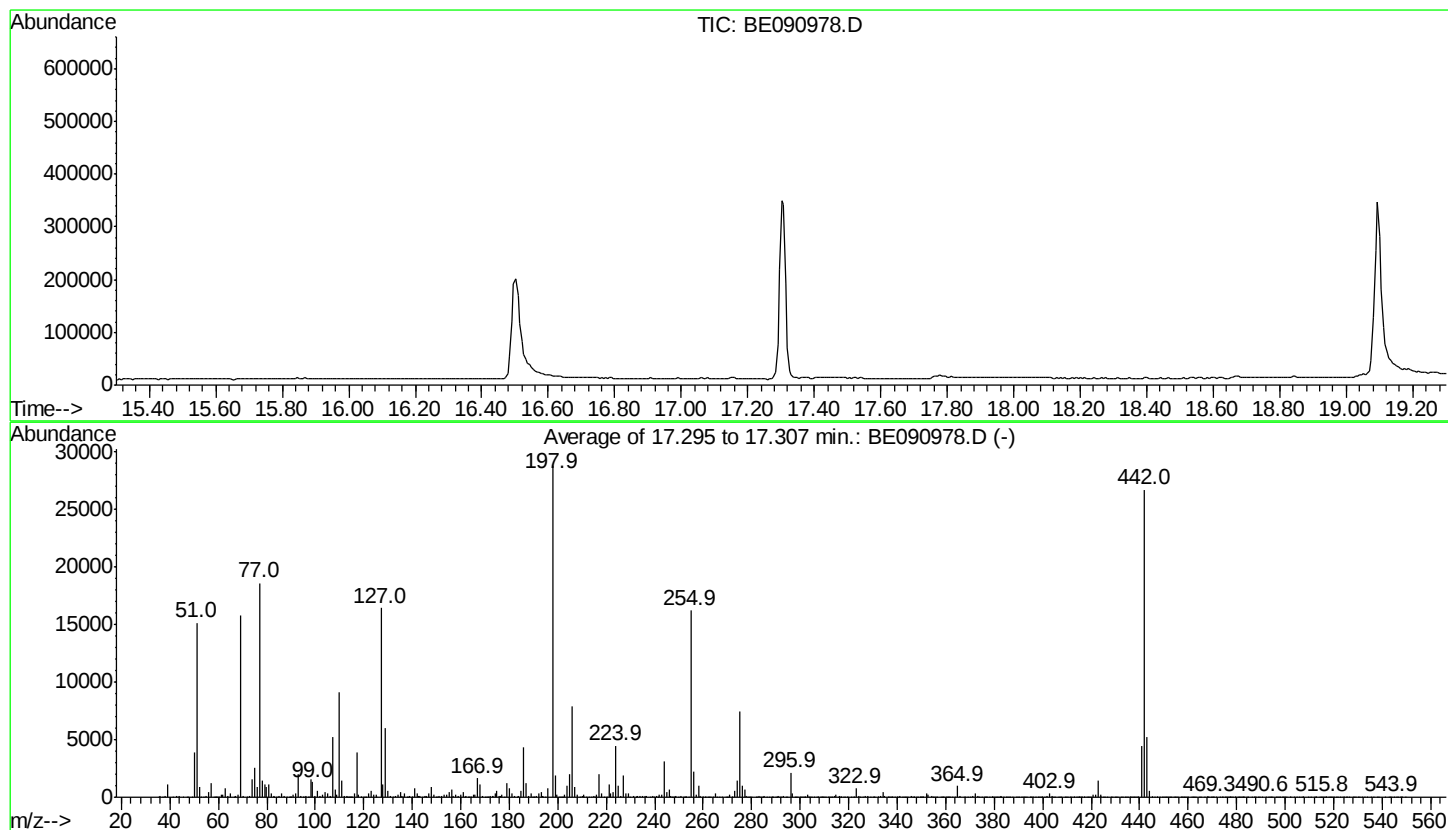

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	15119	PASS
68	69	0.00	2	1.8	278	PASS
69	198	0.00	100	54.9	15782	PASS
70	69	0.00	2	0.6	93	PASS
127	198	10	80	57.0	16370	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28733	PASS
199	198	5	9	6.6	1897	PASS
275	198	10	60	25.9	7453	PASS
365	198	1	100	3.4	980	PASS
441	442	0.01	24	16.7	4454	PASS
442	198	50	100	92.8	26658	PASS
443	442	15	24	19.4	5173	PASS