


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE093016\
 Data File : BE092431.D
 Acq On : 30 Sep 2016 10:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 22 18:25:56 2016

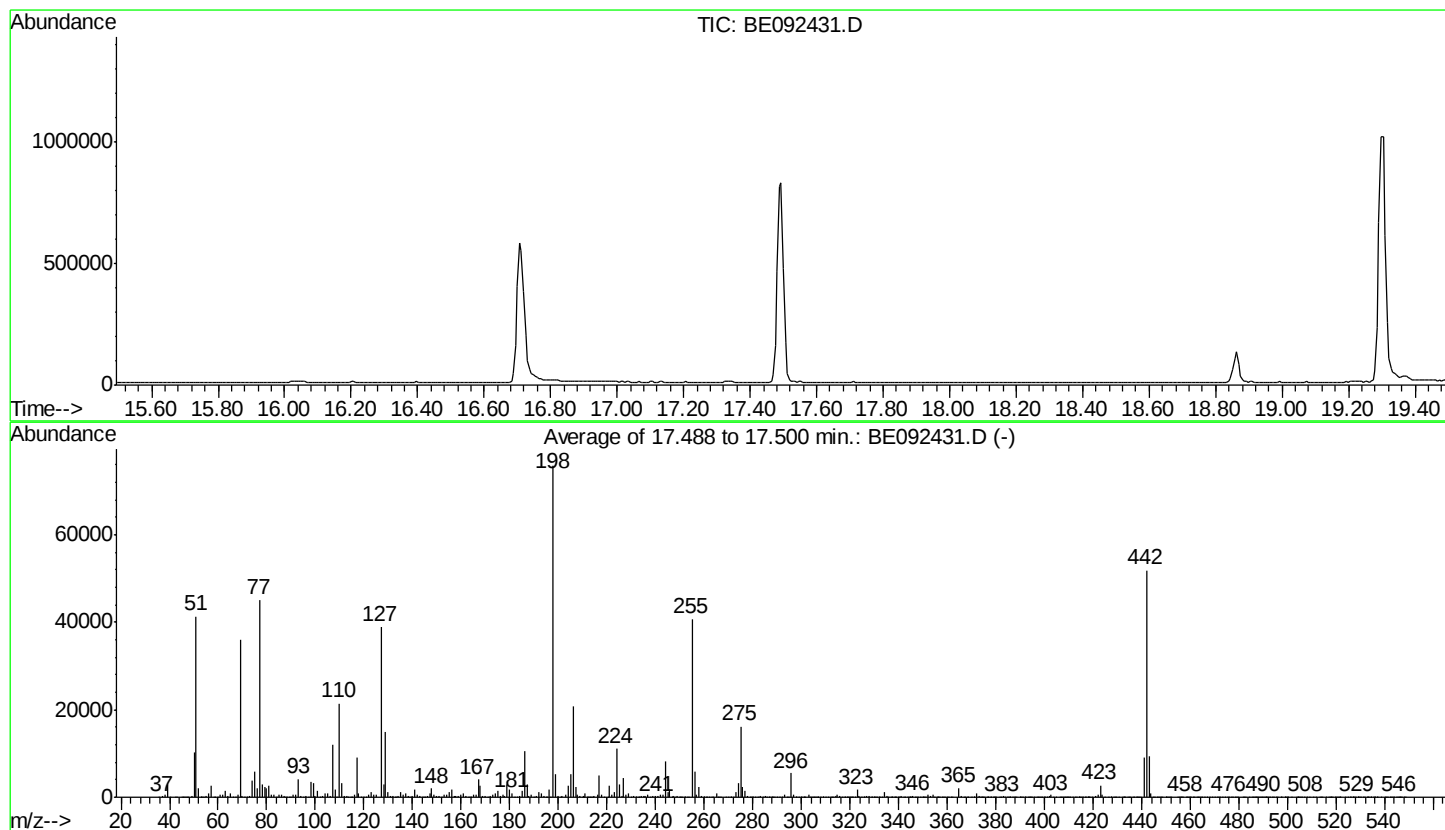

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2525

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	41281	PASS
68	69	0.00	2	1.6	581	PASS
69	198	0.00	100	47.4	35922	PASS
70	69	0.00	2	0.6	222	PASS
127	198	10	80	51.4	38931	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75792	PASS
199	198	5	9	6.9	5261	PASS
275	198	10	60	21.3	16176	PASS
365	198	1	100	2.9	2195	PASS
441	442	0.01	24	17.4	8995	PASS
442	198	50	100	68.4	51805	PASS
443	442	15	24	17.9	9278	PASS