

Data Path : Z:\HPCHEM1\BNA E\DATA\BE093017\
 Data File : BE094154.D
 Acq On : 30 Sep 2017 11:21
 Operator : SJ/JU
 Sample : PB102758BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 30 21:56:22 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1863	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	10589	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	7286	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.24	188	17801	0.40	ng/ul	-0.04
16) Chrysene-d12	21.40	240	17773	0.40	ng/ul	-0.01
20) Perylene-d12	23.75	264	828765	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3457	0.21	ng/ul	-0.01
14) Fluoranthene-d10	19.27	212	10399	0.18	ng/ul	-0.02
Target Compounds						
9) Fluorene	15.51	166	1166	0.043	ng/ul#	21
17) Pyrene	19.63	202	1418	0.029	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE093017\
Data File : BE094154.D
Acq On : 30 Sep 2017 11:21
Operator : SJ/JU
Sample : PB102758BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 30 21:56:22 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration




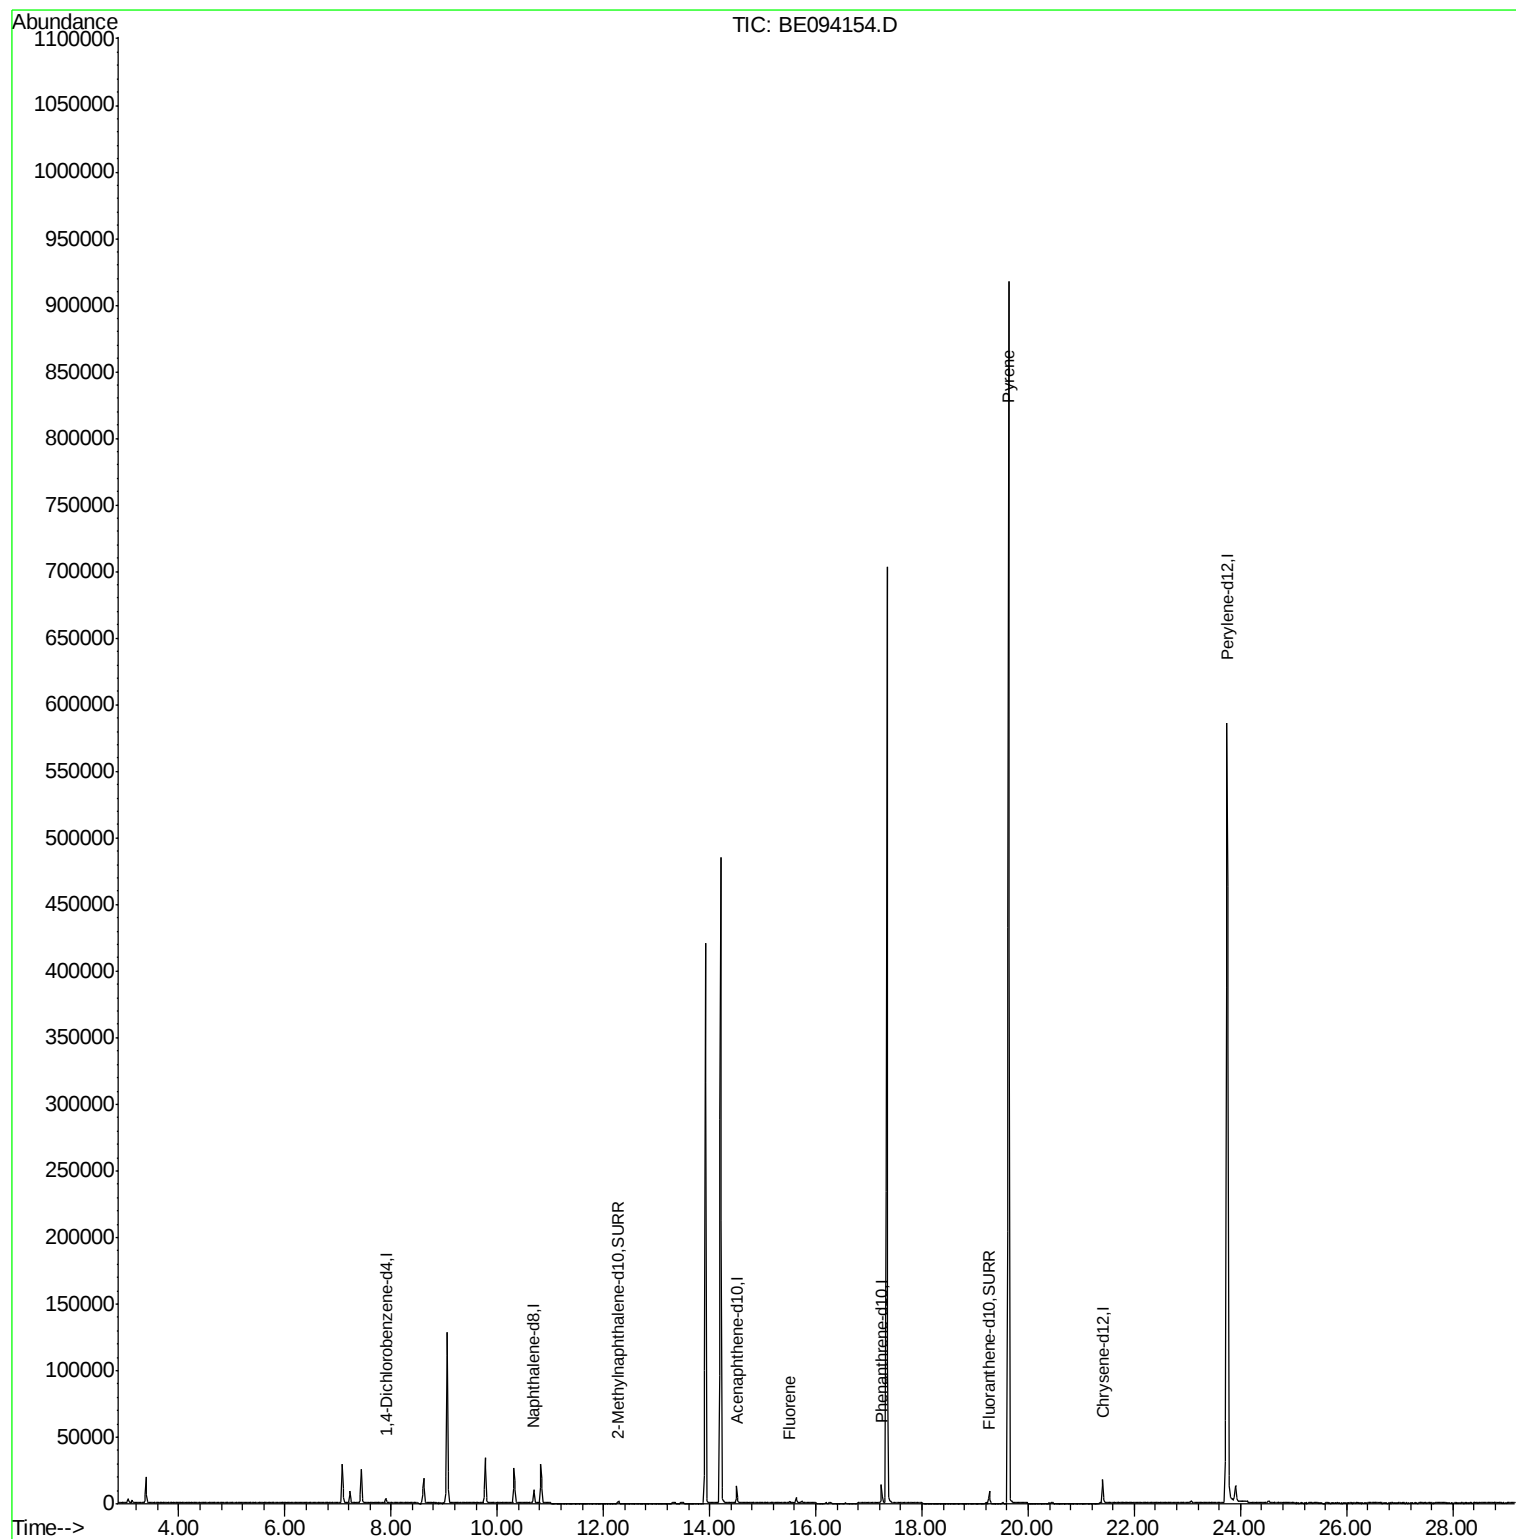


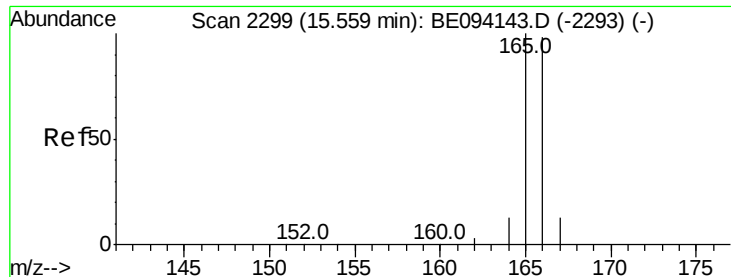

#9
Fluorene
 Concen: 0.043 ng/ul
 RT: 15.51 min Scan# 2291
 Delta R.T. -0.08 min
 Lab File: BE094154.D
 Acq: 30 Sep 2017 11:21

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
166	100		
165	10.4	73.4	110.2#
167	38.3	14.6	22.0#

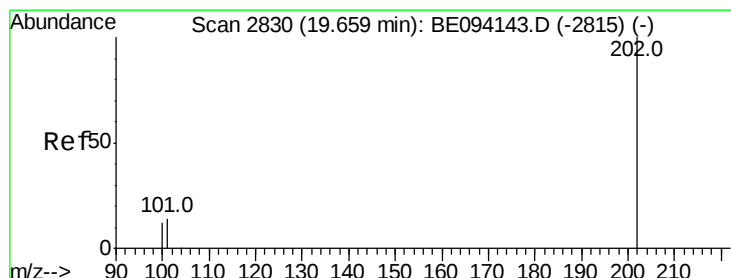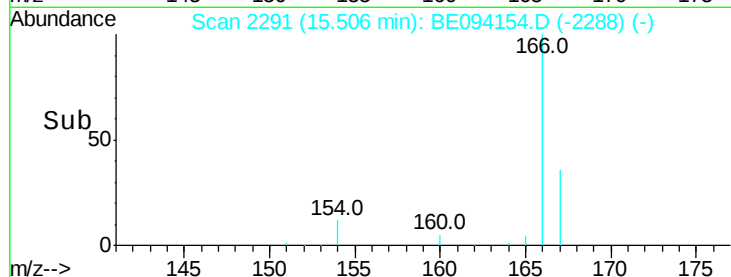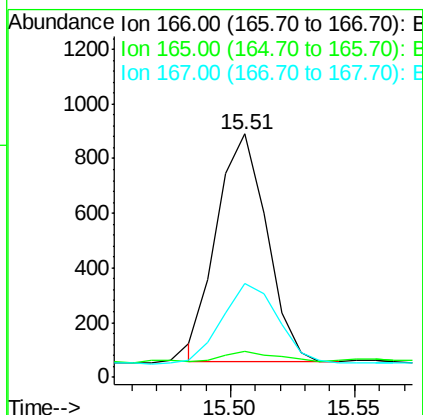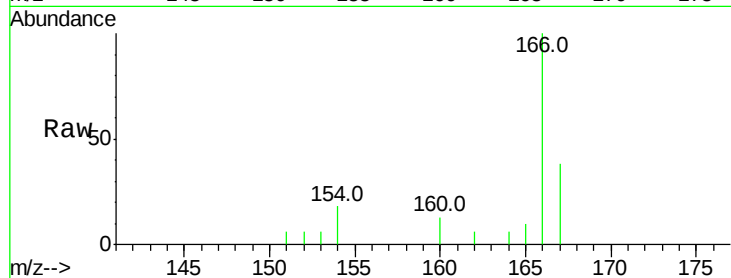

#17
Pyrene
 Concen: 0.029 ng/ul
 RT: 19.63 min Scan# 2823
 Delta R.T. -0.04 min
 Lab File: BE094154.D
 Acq: 30 Sep 2017 11:21

Tgt Ion	Ratio	Lower	Upper
202	100		
101	171.7	18.2	27.4#
100	940.2	15.6	23.4#

