

Data Path : Z:\HPCHEM1\BNA E\DATA\BE093017\
 Data File : BE094155.D
 Acq On : 30 Sep 2017 11:57
 Operator : SJ/JU
 Sample : I5505-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 30 21:56:27 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1801	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	9493	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	6405	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.40	240	16332	0.40	ng/ul	-0.01
20) Perylene-d12	23.75	264	775381	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	3313	0.23	ng/ul	-0.01
14) Fluoranthene-d10	19.26	212	10929	0.00	ng/ul	-0.02
Target Compounds						
17) Pyrene	19.65	202	2222	0.049	ng/ul	95
18) Benzo(a)anthracene	21.39	228	966	0.022	ng/ul#	83
19) Chrysene	21.44	228	1114	0.022	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE093017\
Data File : BE094155.D
Acq On : 30 Sep 2017 11:57
Operator : SJ/JU
Sample : I5505-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 30 21:56:27 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration




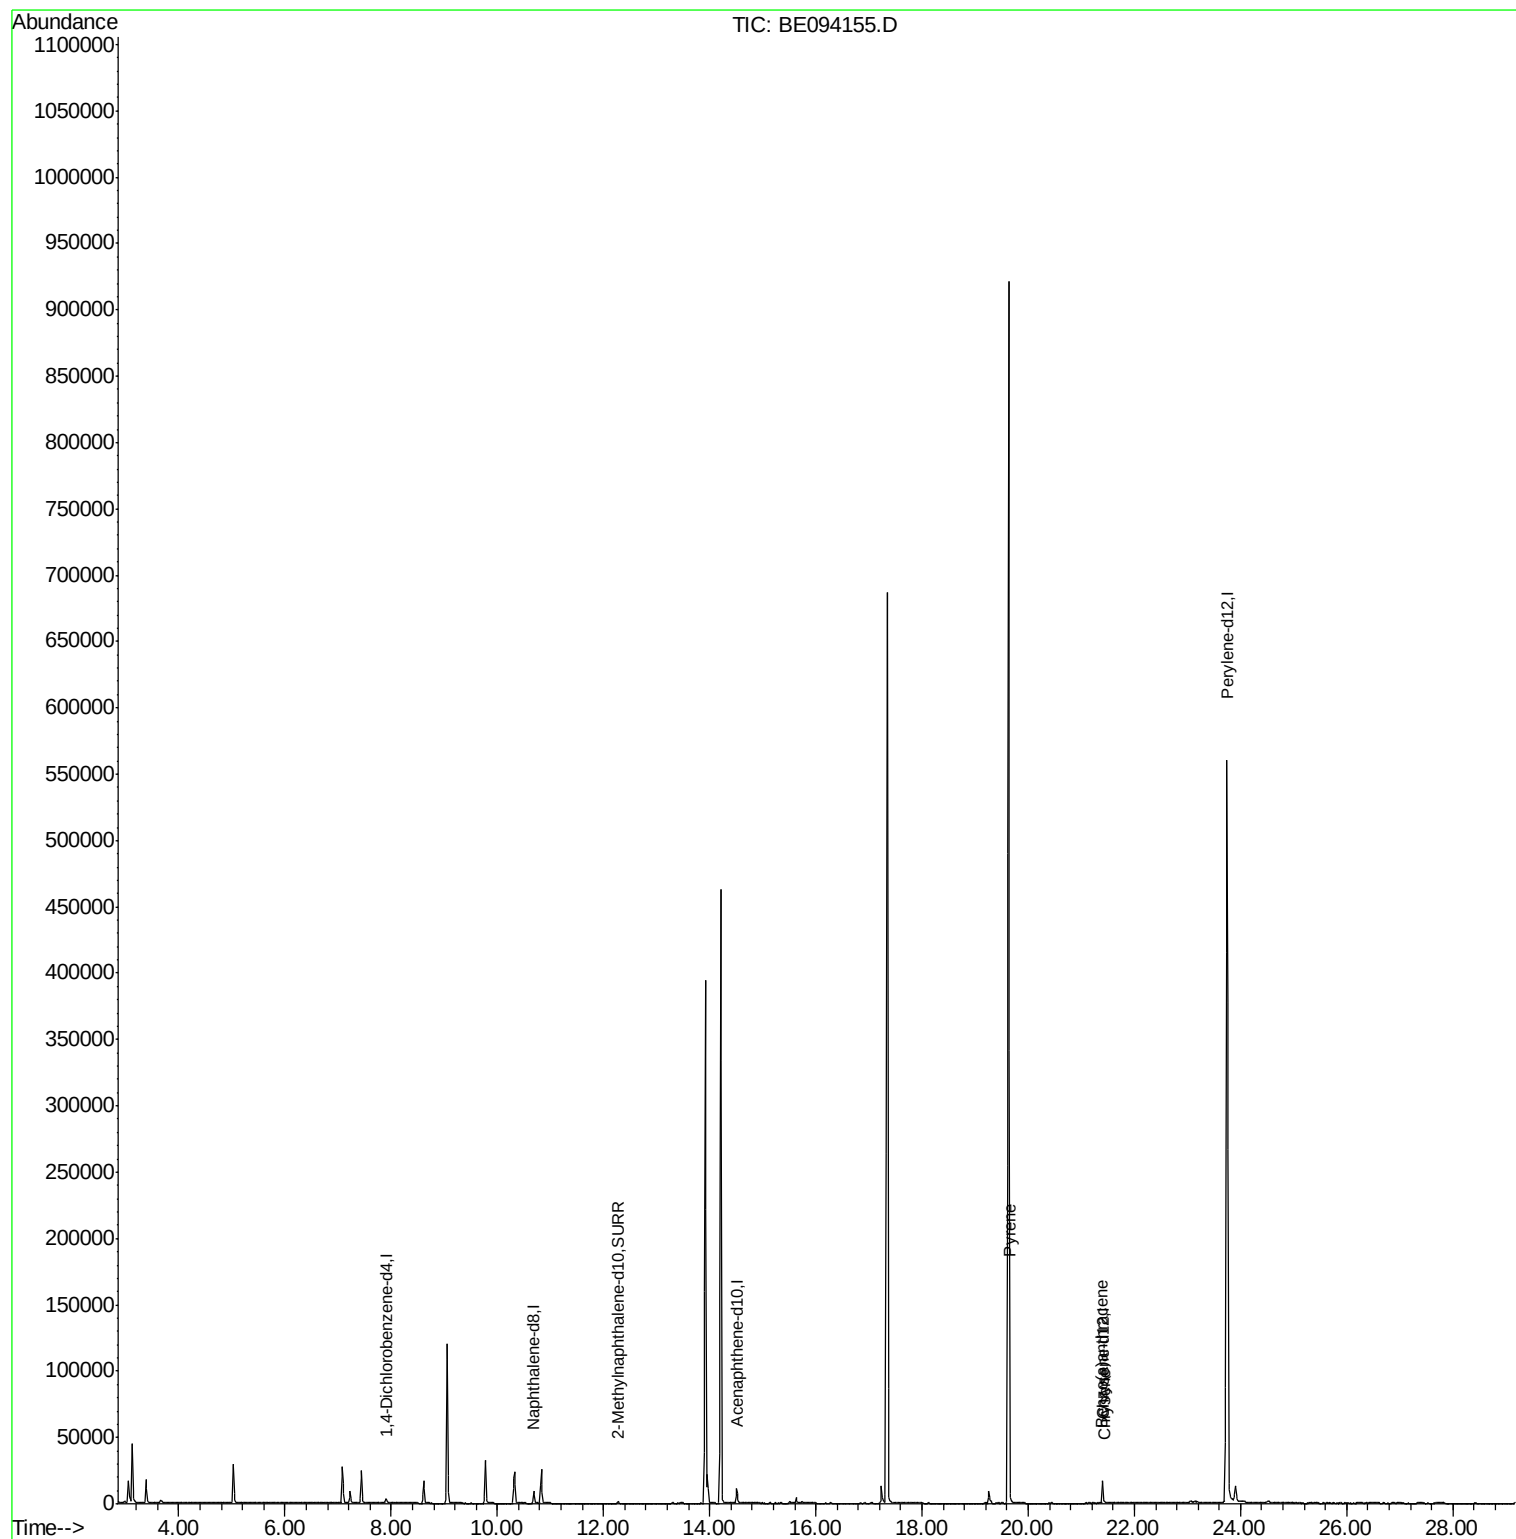


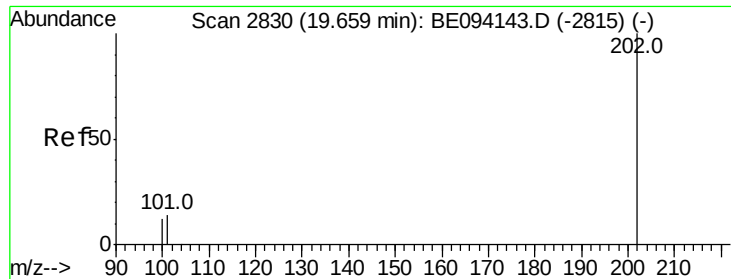

#17
Pvrene
Concen: 0.049 ng/ul
RT: 19.65 min Scan# 2829
Delta R.T. -0.02 min
Lab File: BE094155.D
Acq: 30 Sep 2017 11:57




Instrument :
BNA_E
ClientSampleId :




Tot Ion:202 Resp: 2222
Ion Ratio Lower Upper
202 100
101 18.7 18.2 27.4
100 19.3 15.6 23.4

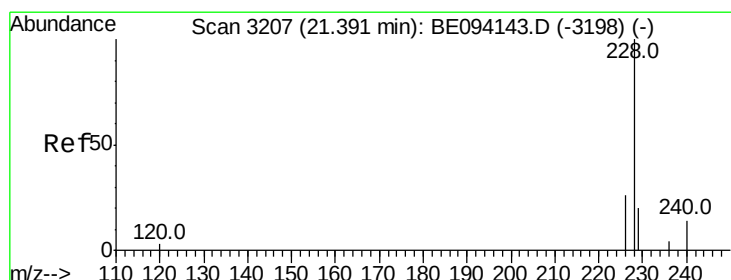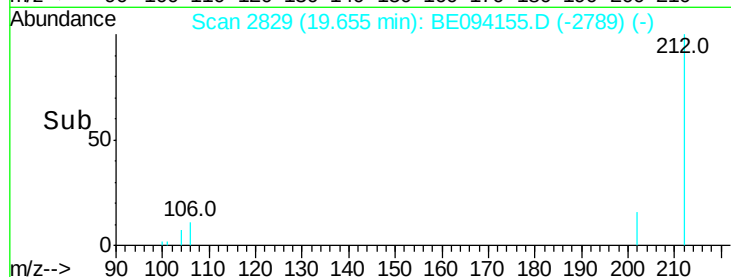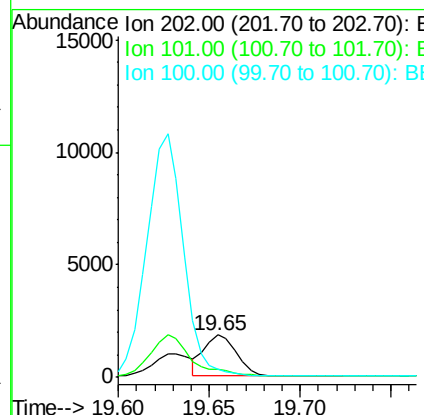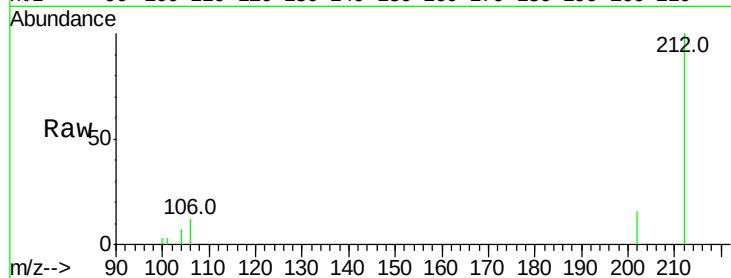

#18
Benzo(a)anthracene
Concen: 0.022 ng/ul
RT: 21.39 min Scan# 3206
Delta R.T. -0.02 min
Lab File: BE094155.D
Acq: 30 Sep 2017 11:57

Tgt Ion:228 Resp: 966
Ion Ratio Lower Upper
228 100
229 30.6 22.8 34.2
226 37.2 17.0 25.6#

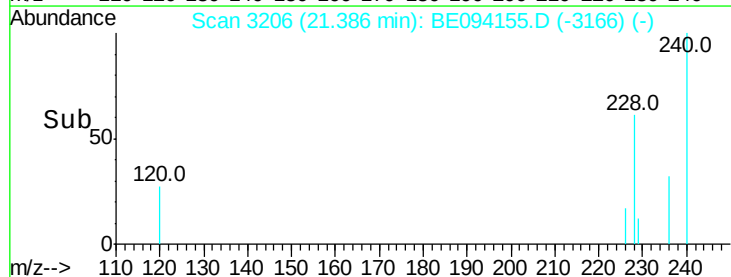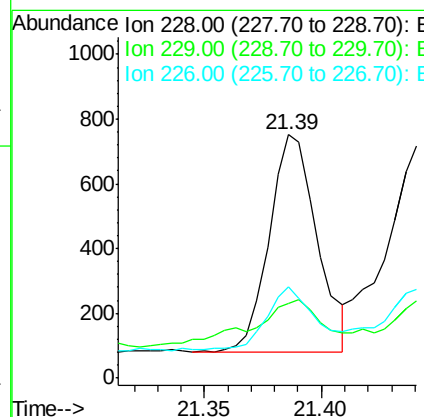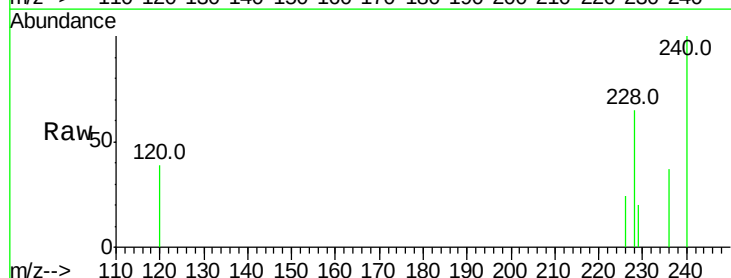

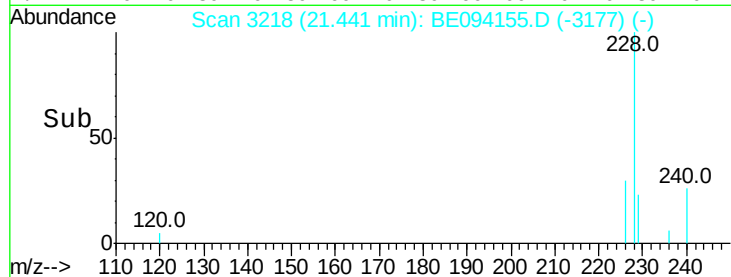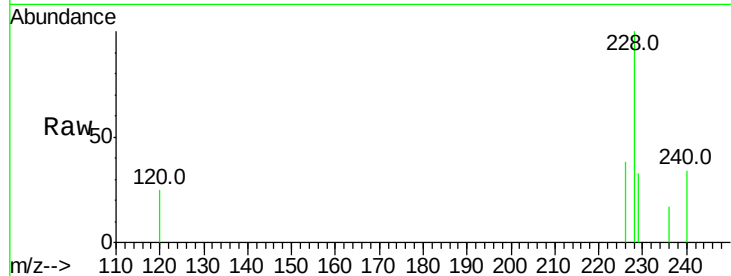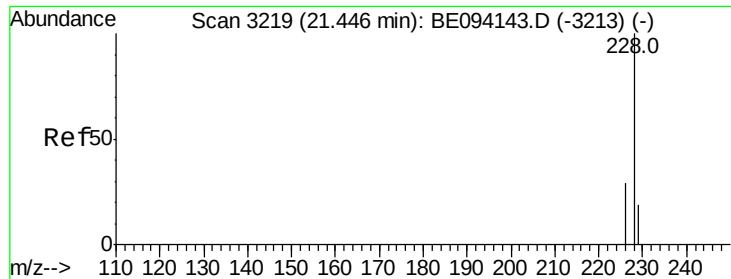

#19

Chrysene

Concen: 0.022 ng/ul

RT: 21.44 min Scan# 3218

Delta R.T. -0.01 min

Lab File: BE094155.D

Acq: 30 Sep 2017 11:57

Instrument :

BNA_E

ClientSampleId :

Tot Ion:228 Resp: 1114

Ion Ratio Lower Upper

228 100

226 38.3 23.4 35.0#

229 33.3 17.7 26.5#

