




Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
Data File : BE094154.D
Acq On : 30 Sep 2017 11:21
Operator : SJ/JU
Sample : PB102758BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK58

Manual Integrations
APPROVED

Sohil
10/2/2017 5:42:44 PM

Quant Time: Sep 30 23:57:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

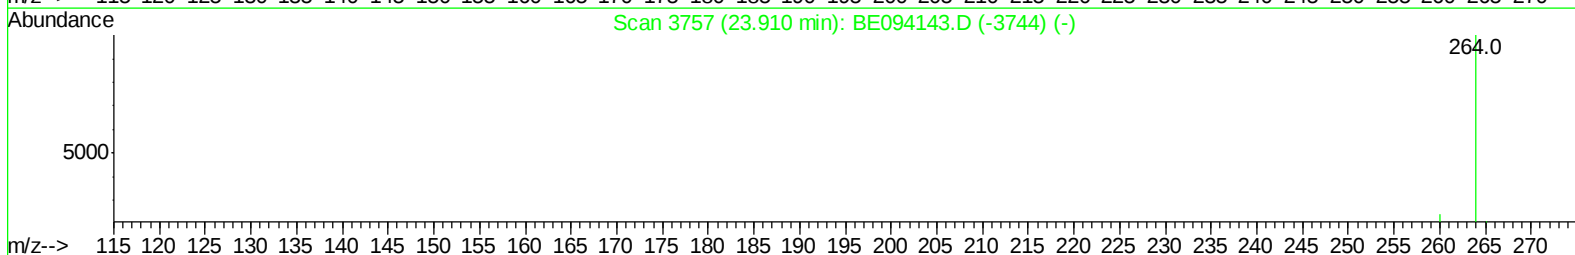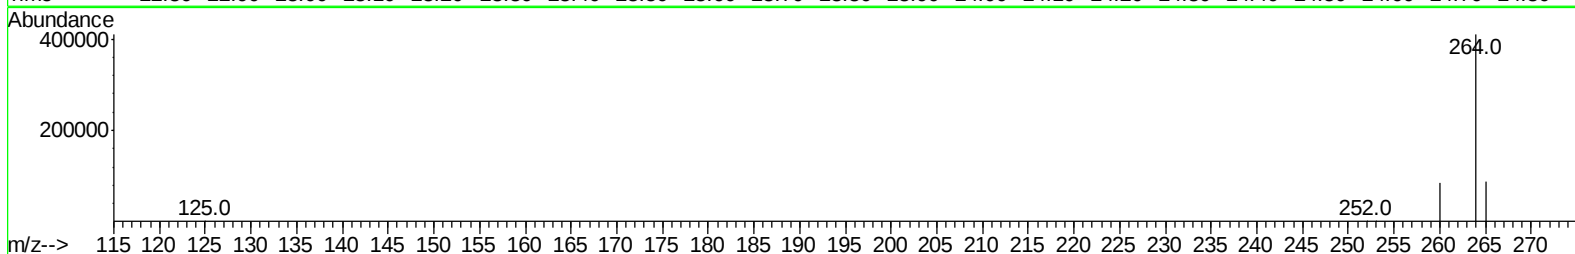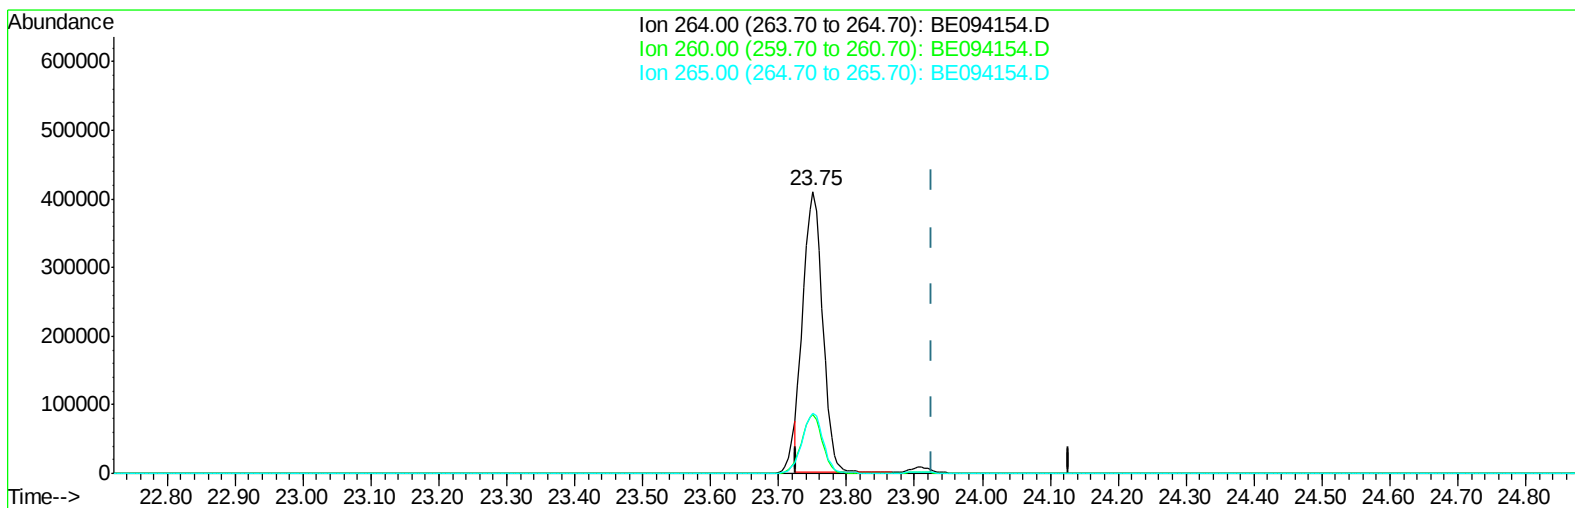

TIC: BE094154.D

(20) Perylene-d12 (I)

23.751min (-0.177) 0.40ng/ul

response 828765

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.93#
265.00	103.50	21.32#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
Data File : BE094154.D
Acq On : 30 Sep 2017 11:21
Operator : SJ/JU
Sample : PB102758BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK58

Manual Integrations
APPROVED

Sohil
10/2/2017 5:42:44 PM

Quant Time: Sep 30 23:57:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

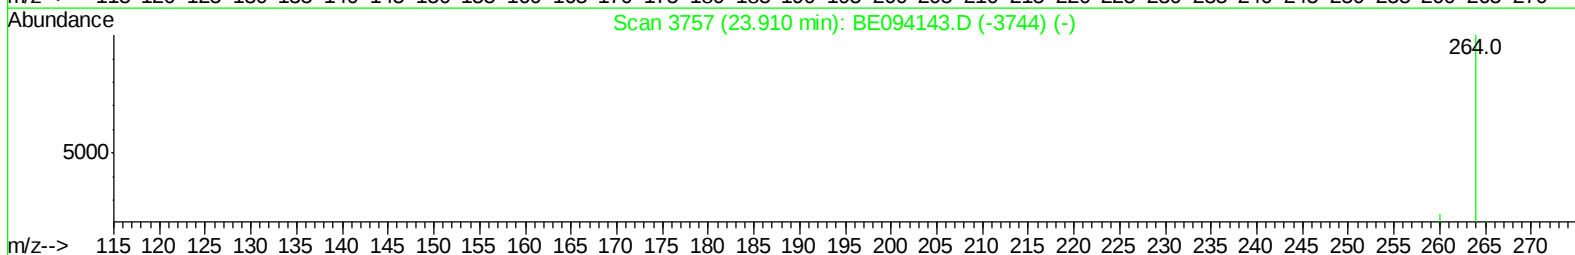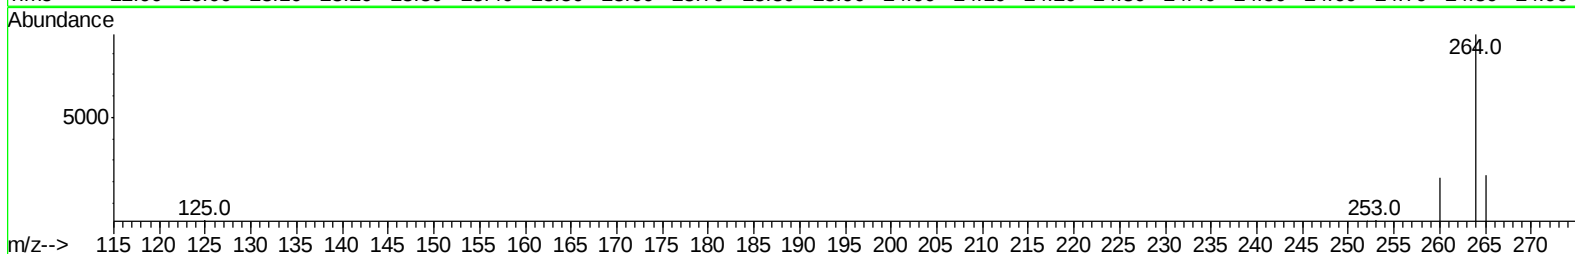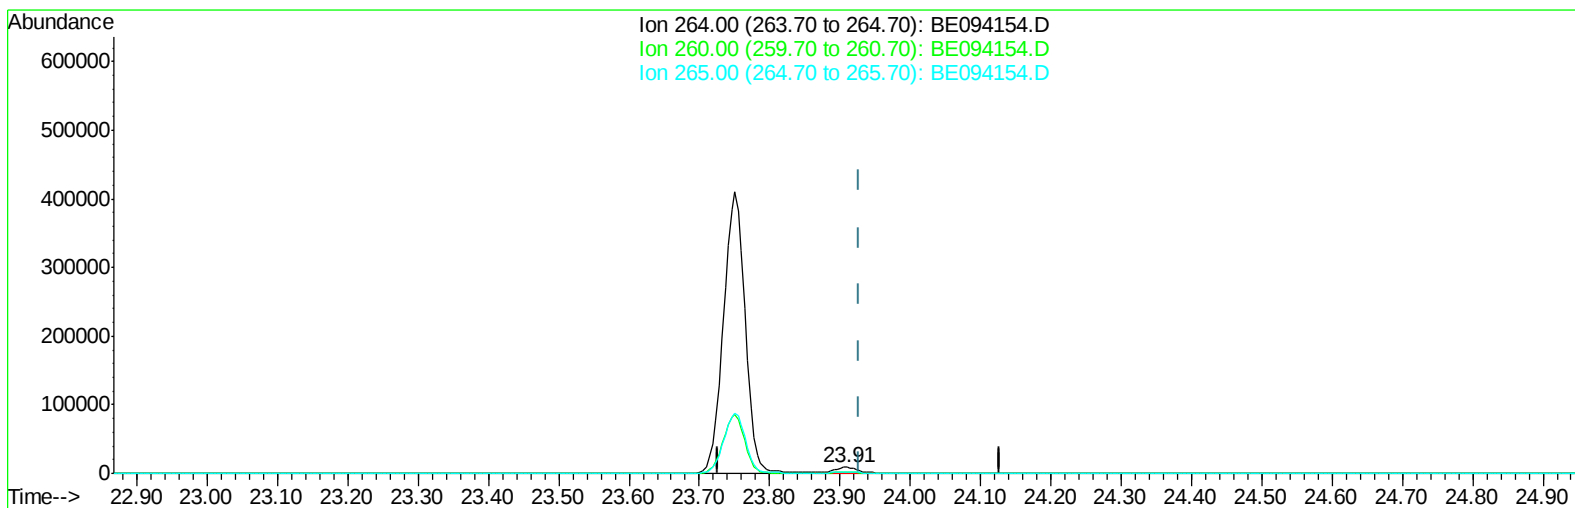

TIC: BE094154.D

(20) Perylene-d12 (I)

23.910min (-0.017) 0.40ng/ul m

response 17842

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.44
265.00	103.50	25.89#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
 Data File : BE094154.D
 Acq On : 30 Sep 2017 11:21
 Operator : SJ/JU
 Sample : PB102758BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK58

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:42:44 PM

Quant Time: Sep 30 23:58:40 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1863	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	10589	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	7286	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.24	188	17801	0.40	ng/ul	-0.04
16) Chrysene-d12	21.40	240	17773	0.40	ng/ul	-0.01
20) Perylene-d12	23.91	264	17842m	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3457	0.21	ng/ul	-0.01
14) Fluoranthene-d10	19.27	212	10399	0.18	ng/ul	-0.02

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
Data File : BE094154.D
Acq On : 30 Sep 2017 11:21
Operator : SJ/JU
Sample : PB102758BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK58

Manual Integrations
APPROVED

Sohil
10/2/2017 5:42:44 PM

Quant Time: Sep 30 23:58:40 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

