




Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
Data File : BE094156.D
Acq On : 30 Sep 2017 12:35
Operator : SJ/JU
Sample : I5505-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B0AD8

Manual Integrations
APPROVED

Sohil
10/2/2017 5:42:48 PM

Quant Time: Oct 01 00:05:16 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

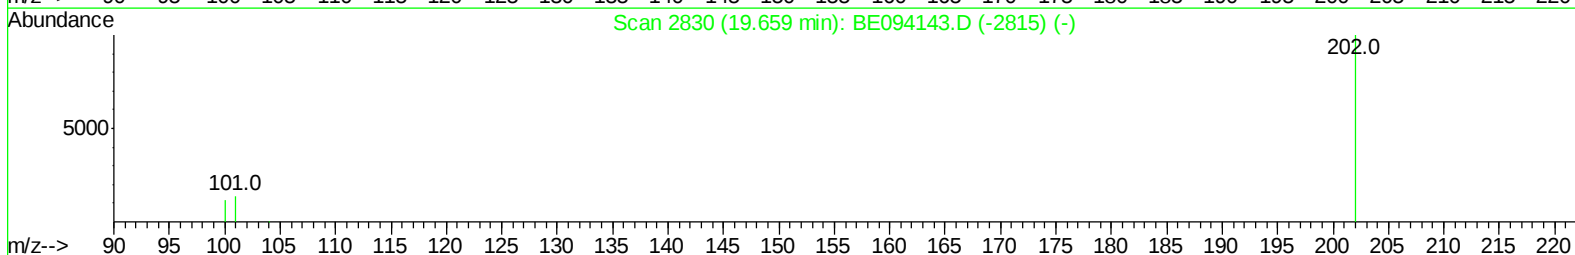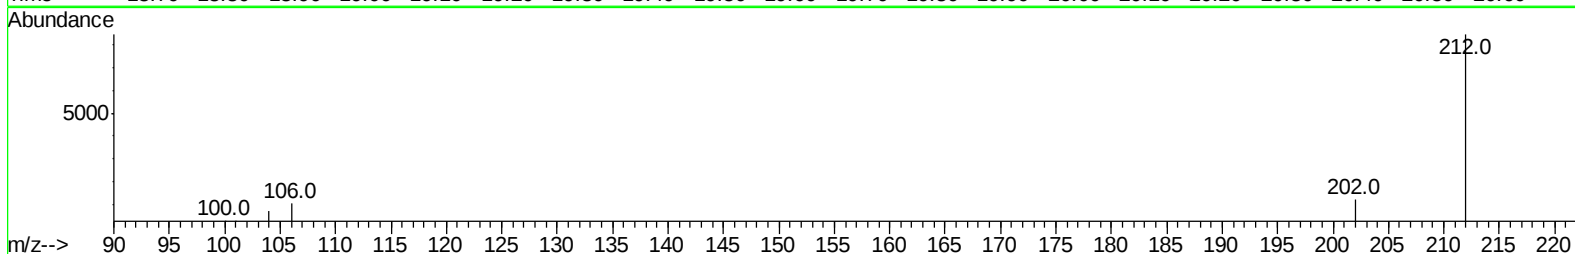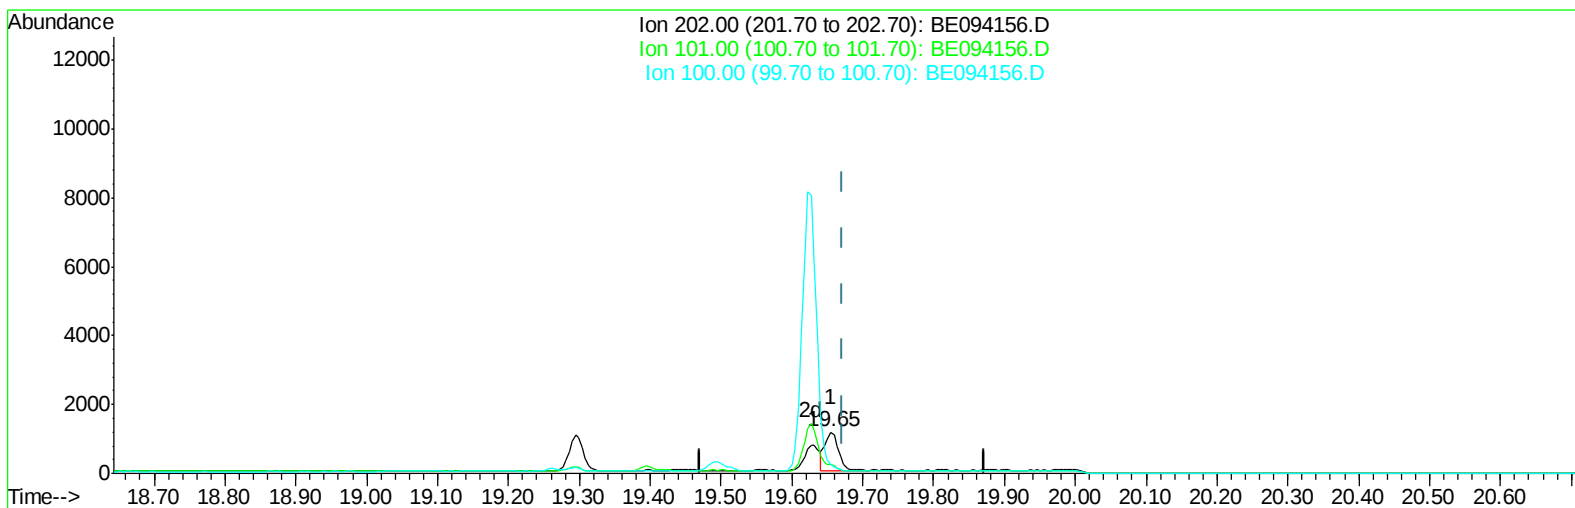

TIC: BE094156.D

(17) Pyrene

19.655min (-0.017) 0.03ng/ul

response 1394

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	21.00
100.00	19.50	22.51
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
 Data File : BE094156.D
 Acq On : 30 Sep 2017 12:35
 Operator : SJ/JU
 Sample : I5505-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B0AD8

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:42:48 PM

Quant Time: Oct 01 00:05:16 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

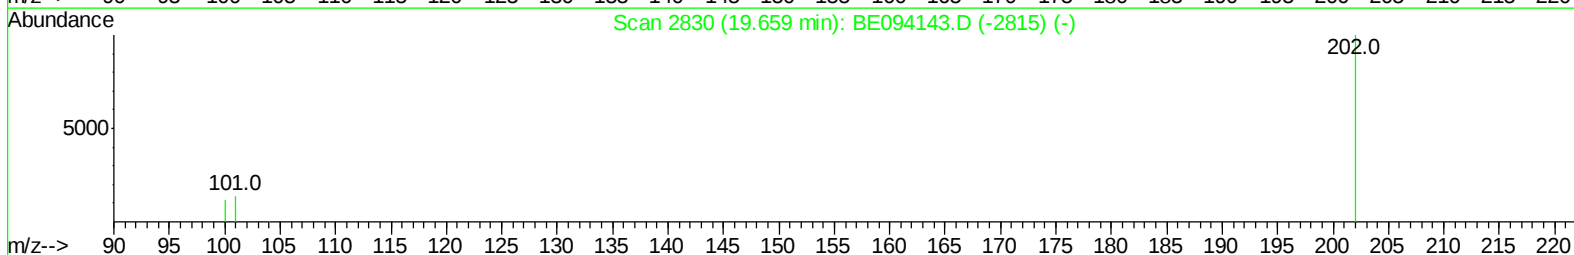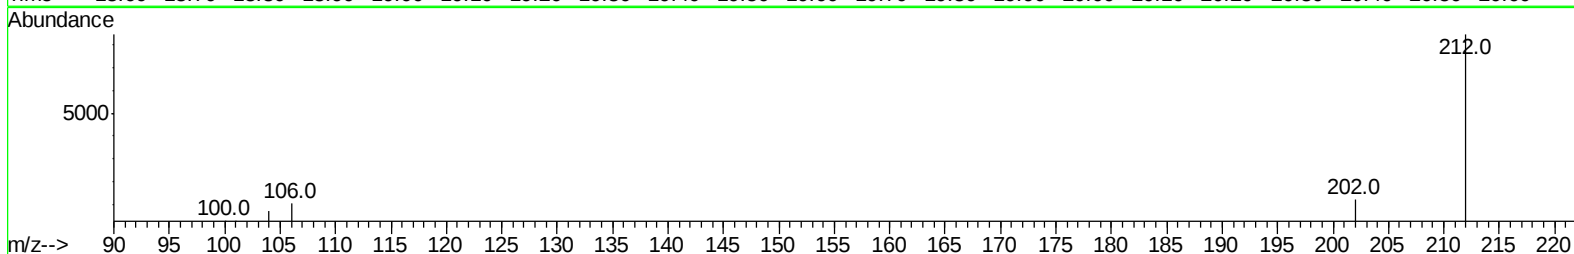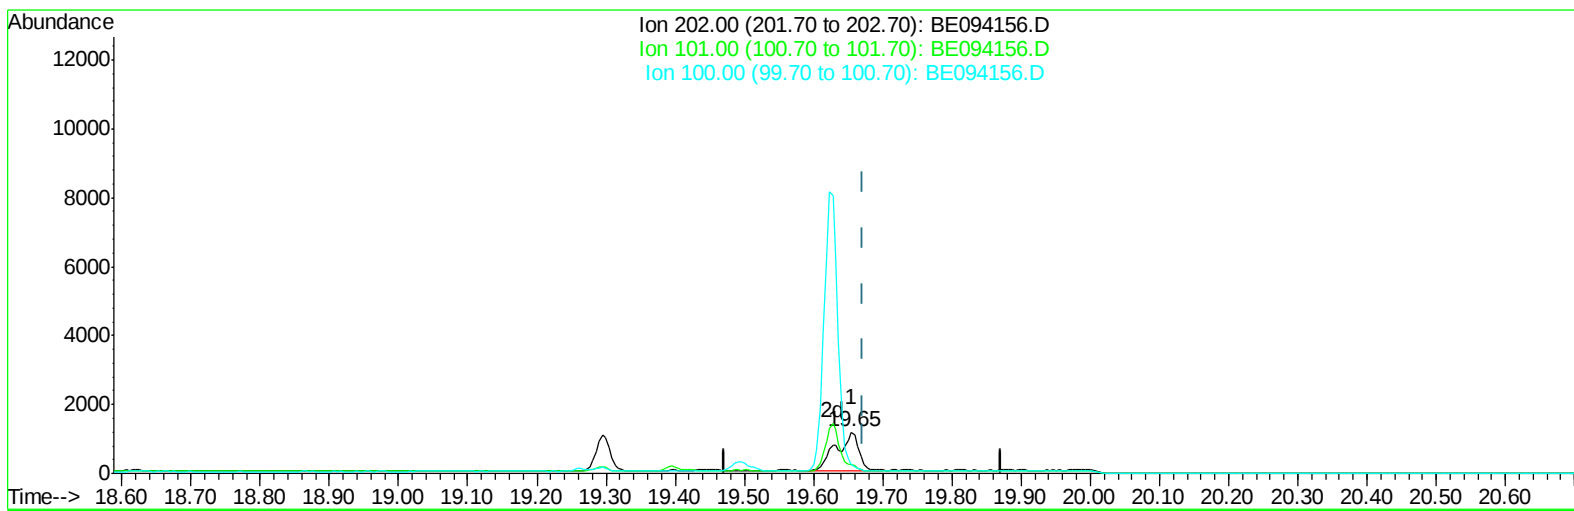

TIC: BE094156.D

(17) Pyrene

19.655min (-0.017) 0.06ng/ul m

response 2621

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	21.00
100.00	19.50	22.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
 Data File : BE094156.D
 Acq On : 30 Sep 2017 12:35
 Operator : SJ/JU
 Sample : I5505-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B0AD8

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:42:48 PM

Quant Time: Oct 01 00:06:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1739	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	9116	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	6078	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.24	188	15343	0.40	ng/ul	-0.04
16) Chrysene-d12	21.40	240	15713	0.40	ng/ul	-0.01
20) Perylene-d12	23.91	264	18025	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	2580	0.18	ng/ul	-0.02
14) Fluoranthene-d10	19.26	212	8488	0.17	ng/ul	-0.02
Target Compounds						
17) Pyrene	19.65	202	2621m	0.060	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\Data\BE093017\
Data File : BE094156.D
Acq On : 30 Sep 2017 12:35
Operator : SJ/JU
Sample : I5505-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B0AD8

Manual Integrations
APPROVED

Sohil
10/2/2017 5:42:48 PM

Quant Time: Oct 01 00:06:50 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

