

Data Path : Z:\HPCHEM1\BNA E\DATA\BE093017\
 Data File : BE094156.D
 Acq On : 30 Sep 2017 12:35
 Operator : SJ/JU
 Sample : I5505-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B0AD8

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:42:48 PM

Quant Time: Oct 01 00:06:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1739	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	9116	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	6078	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.24	188	15343	0.40	ng/ul	-0.04
16) Chrysene-d12	21.40	240	15713	0.40	ng/ul	-0.01
20) Perylene-d12	23.91	264	18025	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	2580	0.18	ng/ul	-0.02
14) Fluoranthene-d10	19.26	212	8488	0.17	ng/ul	-0.02
Target Compounds						
17) Pyrene	19.65	202	2621m	0.060	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE093017\
Data File : BE094156.D
Acq On : 30 Sep 2017 12:35
Operator : SJ/JU
Sample : I5505-07
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
B0AD8

Manual Integrations
APPROVED

Sohil
10/2/2017 5:42:48 PM

Quant Time: Oct 01 00:06:50 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

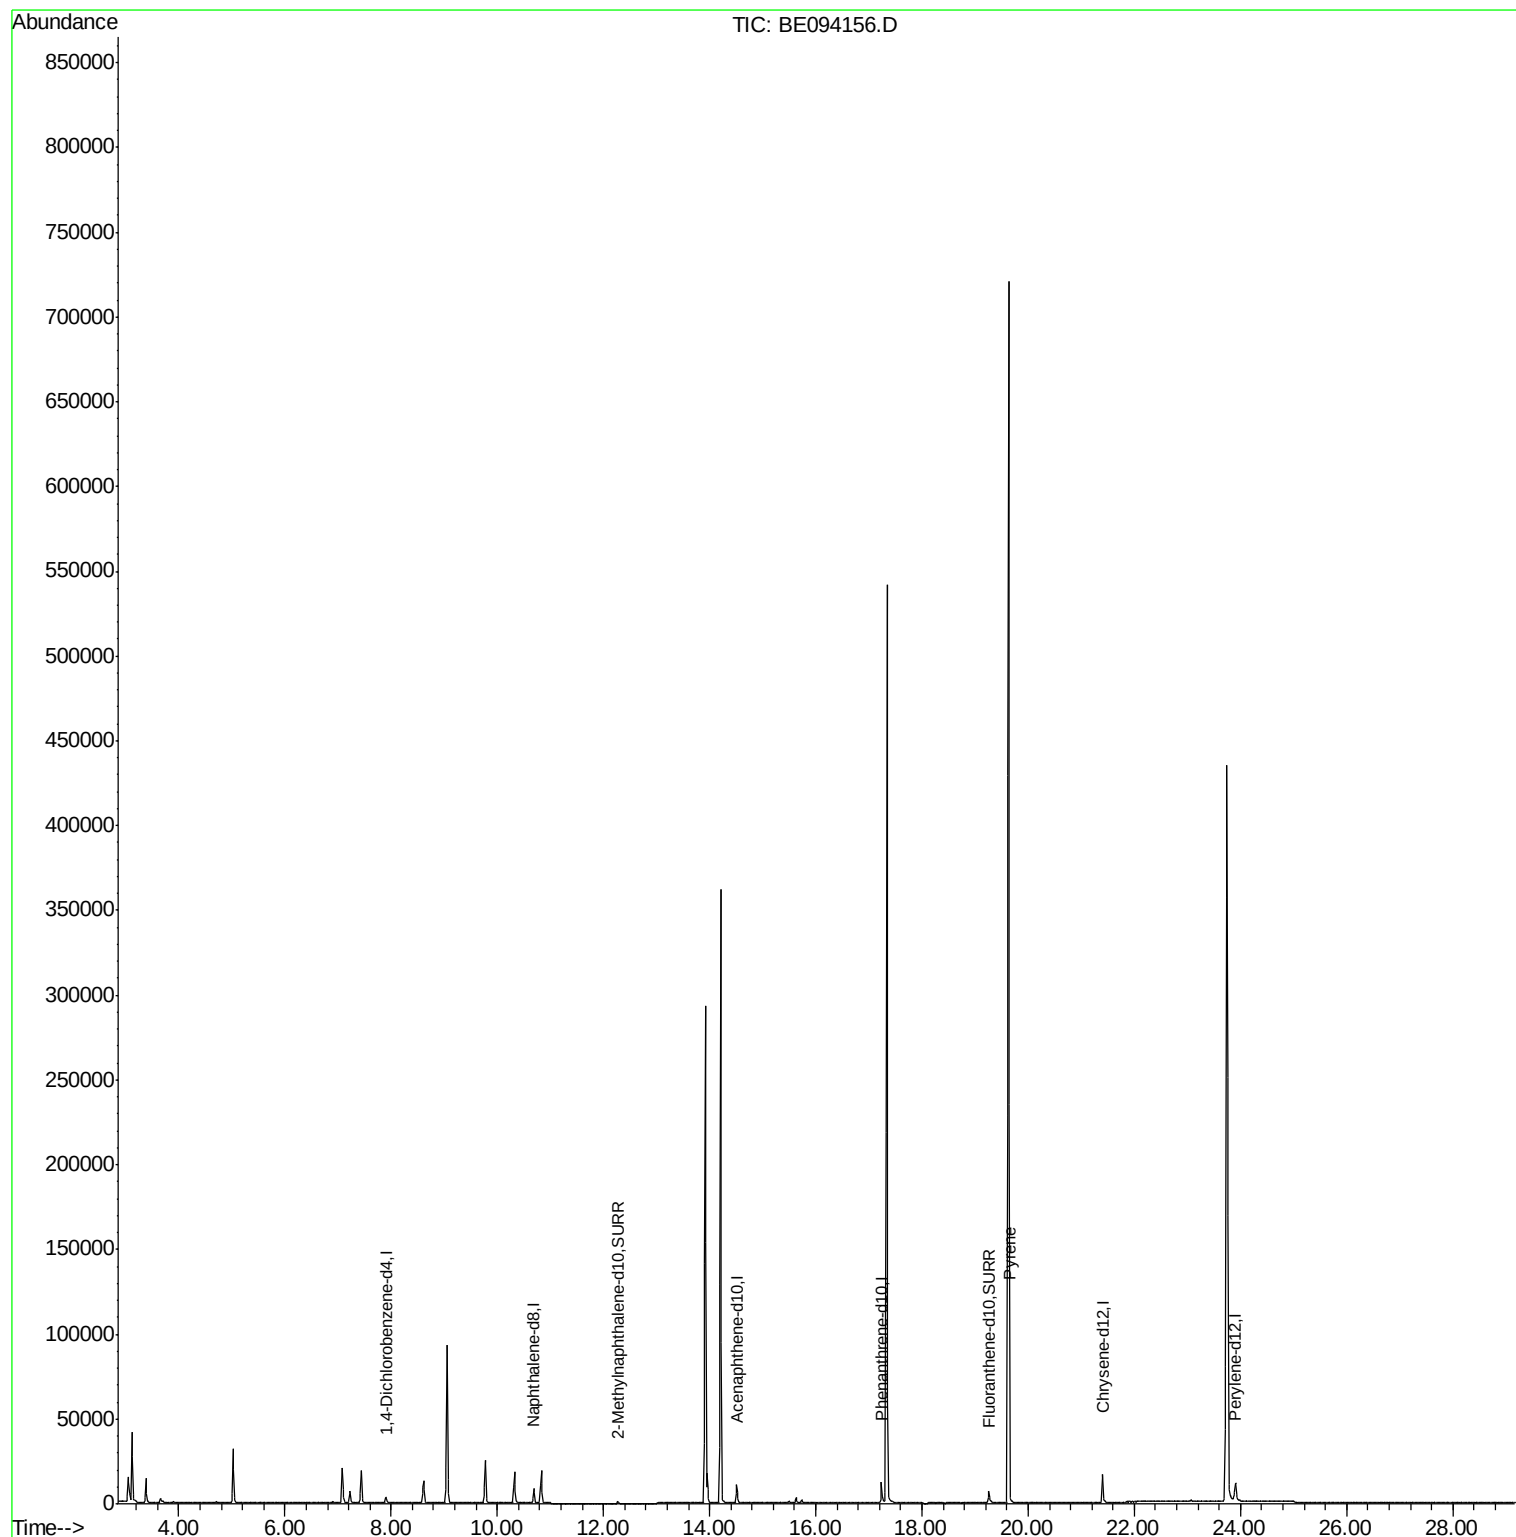

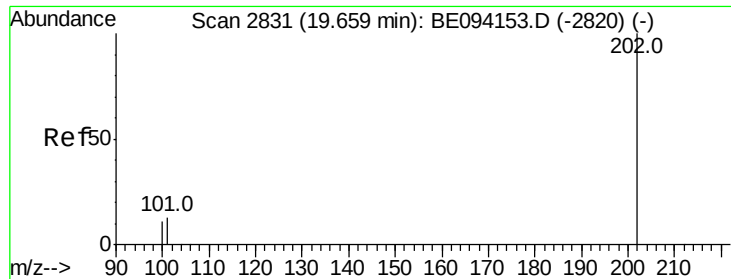

#17
 Pvrene
 Concen: 0.060 ng/ul m
 RT: 19.65 min Scan# 2829
 Delta R.T. -0.02 min
 Lab File: BE094156.D
 Acq: 30 Sep 2017 12:35

Instrument :
 BNA_E
 ClientSampleId :
 B0AD8

Tot Ion:	202	Resp:	2621
Ion Ratio	Lower	Upper	
202	100		
101	21.0	18.2	27.4
100	22.5	15.6	23.4

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:42:48 PM

