


Data Path : Z:\HPCHEM1\BNA E\Data\BE100317\
Data File : BE094158.D
Acq On : 3 Oct 2017 17:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 29 13:57:50 2017

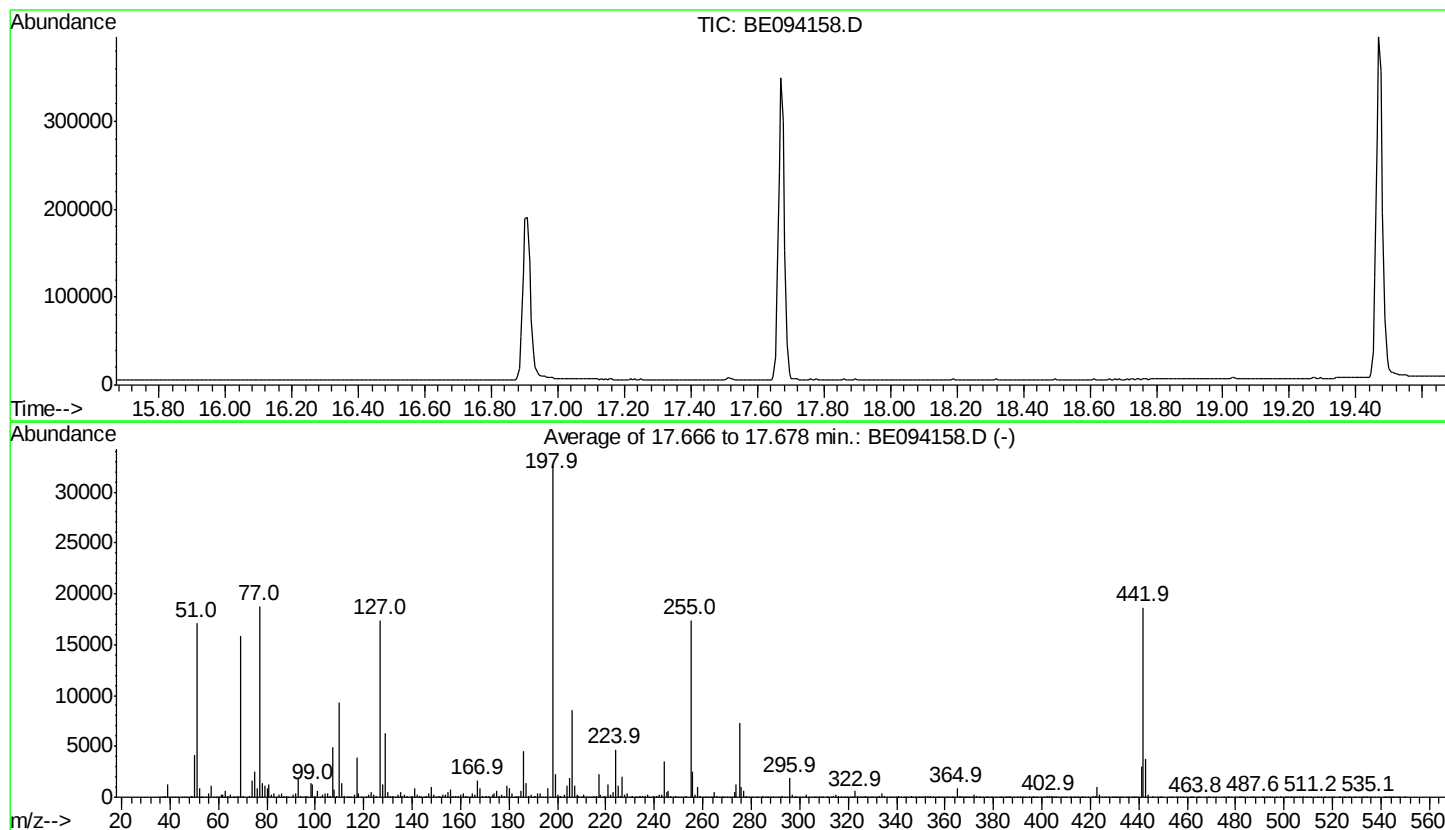

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.7	17175	PASS
68	69	0.00	2	1.1	170	PASS
69	198	0.00	100	48.6	15839	PASS
70	69	0.00	2	0.6	91	PASS
127	198	10	80	53.3	17383	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32591	PASS
199	198	5	9	7.0	2283	PASS
275	198	10	60	22.6	7362	PASS
365	198	1	100	2.7	887	PASS
441	442	0.01	24	16.3	3040	PASS
442	198	50	100	57.3	18681	PASS
443	442	15	24	19.9	3721	PASS