

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100417\  
 Data File : BE094171.D  
 Acq On : 4 Oct 2017 19:40  
 Operator : SJ/JU  
 Sample : I5496-04  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 2

Instrument :  
 BNA\_E  
 ClientSampleId :  
 PAMT-COMP-E

Quant Time: Oct 04 20:38:22 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE092517.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Sep 29 13:57:50 2017  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4      | 7.91  | 152  | 3029     | 0.80  | ng    | 0.00     |
| 7) Naphthalene-d8              | 10.69 | 136  | 15405    | 0.80  | ng    | 0.00     |
| 13) Acenaphthene-d10           | 14.51 | 164  | 9516     | 0.80  | ng    | 0.00     |
| 19) Phenanthrene-d10           | 17.23 | 188  | 26475    | 0.80  | ng    | 0.00     |
| 27) Chrysene-d12               | 21.40 | 240  | 23638    | 0.80  | ng    | 0.00     |
| 34) Perylene-d12               | 23.90 | 264  | 22179    | 0.80  | ng    | -0.01    |
| System Monitoring Compounds    |       |      |          |       |       |          |
| 4) 2-Fluorophenol              | 5.50  | 112  | 56586    | 9.86  | ng    | 0.00     |
| 5) Phenol-d6                   | 7.08  | 99   | 69186    | 8.68  | ng    | 0.00     |
| 8) Nitrobenzene-d5             | 9.04  | 82   | 194003   | 26.03 | ng    | -0.02    |
| 11) 2-Methylnaphthalene-d10    | 12.25 | 152  | 22       | 0.00  | ng    | -0.02    |
| 14) 2,4,6-Tribromophenol       | 16.00 | 330  | 38261    | 15.41 | ng    | 0.00     |
| 15) 2-Fluorobiphenyl           | 13.13 | 172  | 370661   | 23.58 | ng    | 0.00     |
| 25) Fluoranthene-d10           | 19.30 | 212  | 472      | 0.00  | ng    | 0.03     |
| 29) Terphenyl-d14              | 19.84 | 244  | 481054   | 22.31 | ng    | 0.00     |
| Target Compounds               |       |      |          |       |       |          |
| 23) Phenanthrene               | 17.27 | 178  | 2398     | 0.071 | ng    | # 82     |
| 26) Fluoranthene               | 19.29 | 202  | 2222     | 0.059 | ng    | # 90     |
| 28) Pyrene                     | 19.65 | 202  | 4785     | 0.128 | ng    | # 95     |
| 30) Benzo(a)anthracene         | 21.38 | 228  | 1683     | 0.042 | ng    | # 76     |
| 31) Chrysene                   | 21.44 | 228  | 2003     | 0.052 | ng    | # 82     |
| 32) Bis(2-ethylhexyl)phthalate | 21.29 | 149  | 161836   | 1.214 | ng    | 100      |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100417\  
Data File : BE094171.D  
Acq On : 4 Oct 2017 19:40  
Operator : SJ/JU  
Sample : I5496-04  
Misc :  
ALS Vial : 3 Sample Multiplier: 2

Instrument :  
BNA\_E  
ClientSampleId :  
PAMT-COMP-E

Quant Time: Oct 04 20:38:22 2017  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE092517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 29 13:57:50 2017  
Response via : Initial Calibration

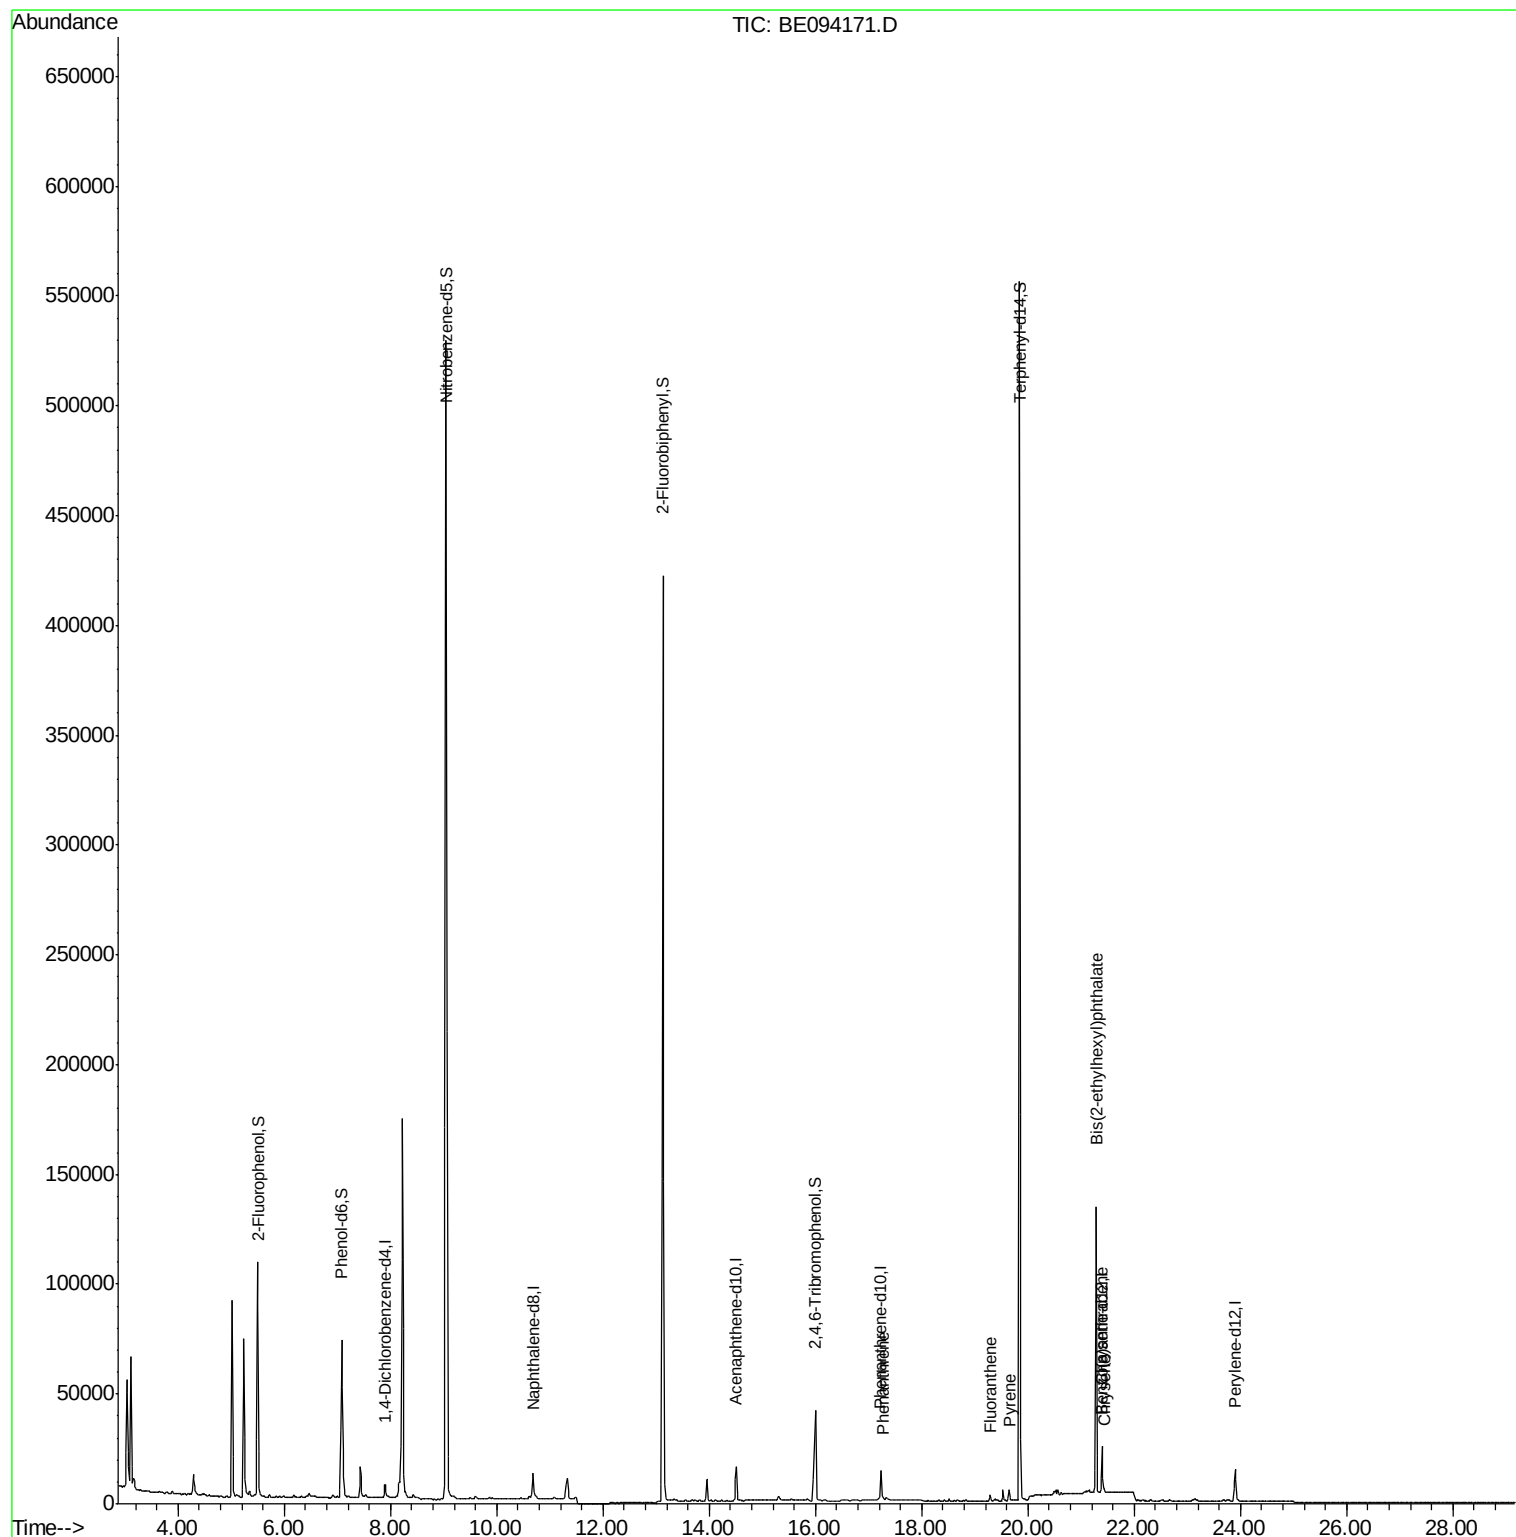

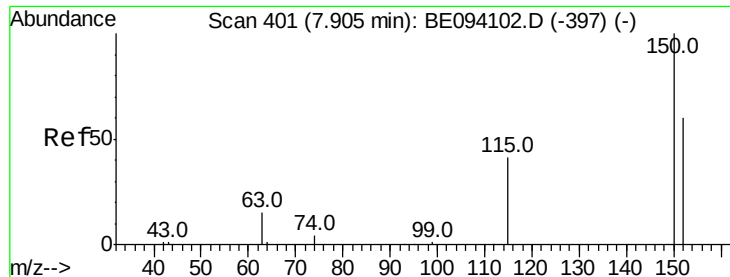


#1




1,4-Dichlorobenzene-d4  
Concen: 0.800 ng  
RT: 7.91 min Scan# 401  
Delta R.T. 0.00 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40

Instrument :  
BNA\_E  
ClientSampleId :  
PAMT-COMP-E

Tot Ion:152 Resp: 3029  
Ion Ratio Lower Upper  
152 100  
150 151.4 117.2 175.8  
115 65.6 57.0 85.6

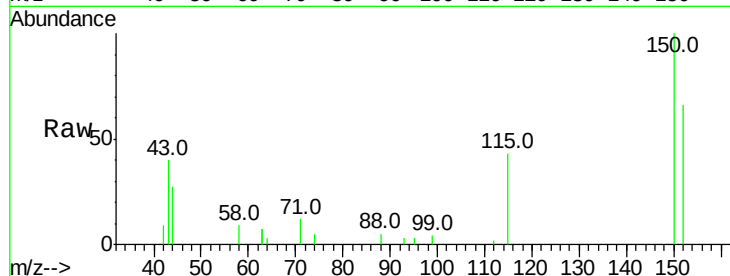


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

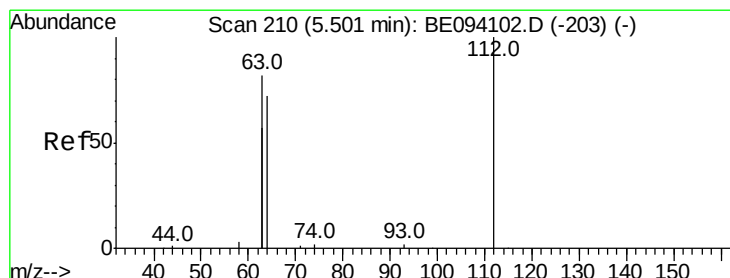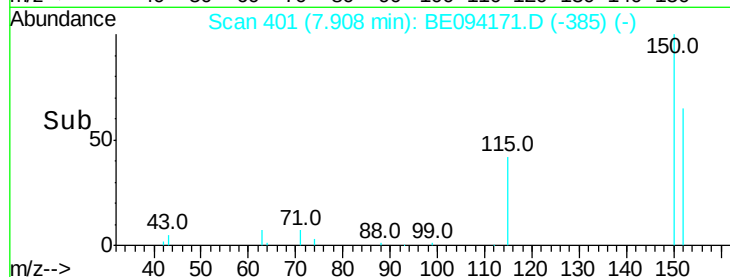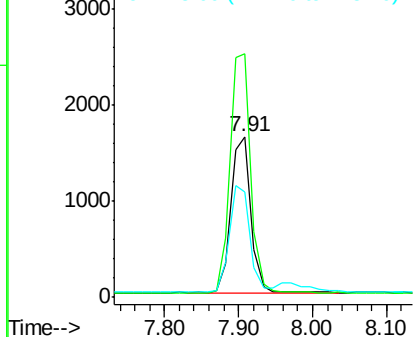



#4


2-Fluorophenol  
Concen: 9.856 ng  
RT: 5.50 min Scan# 210  
Delta R.T. 0.00 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40

Tgt Ion:112 Resp: 56586  
Ion Ratio Lower Upper  
112 100  
64 75.5 60.1 90.1  
63 149.5 116.8 175.2

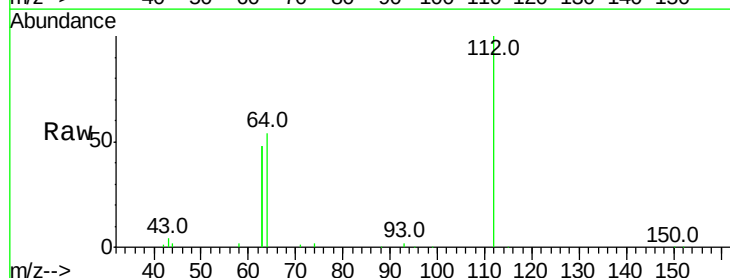

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BE0  
Ion 63.00 (62.70 to 63.70): BE0

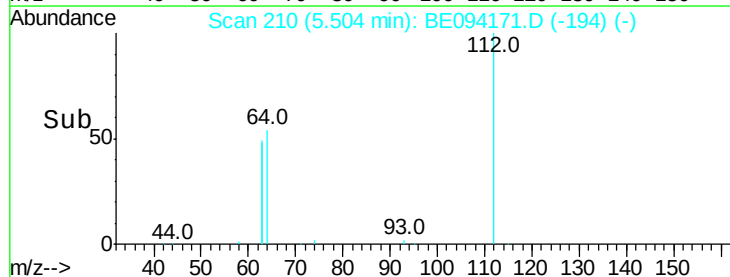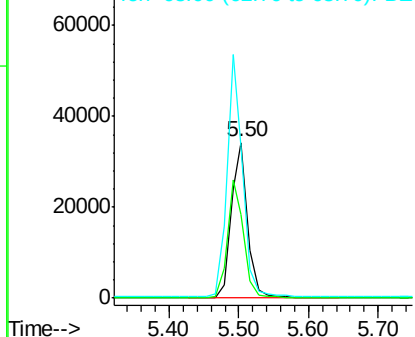

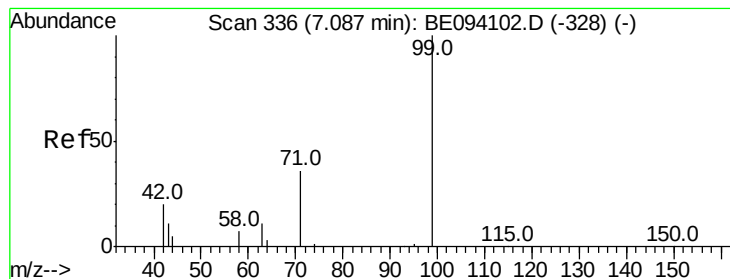

#5

Phenol-d6

Concen: 8.676 ng

RT: 7.08 min Scan# 335

Delta R.T. -0.01 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40

Instrument :

BNA\_E

ClientSampleId :

PAMT-COMP-E


Tot Ion: 99 Resp: 69186

Ion Ratio Lower Upper




99 100

42 21.2 20.2 30.2

71 35.2 28.4 42.6

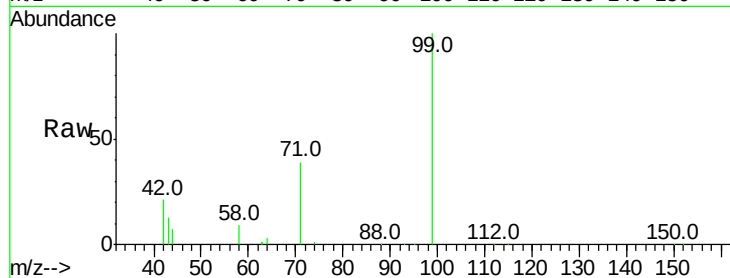

Abundance Ion 99.00 (98.70 to 99.70): BE0  
Ion 42.00 (41.70 to 42.70): BE0  
Ion 71.00 (70.70 to 71.70): BE0

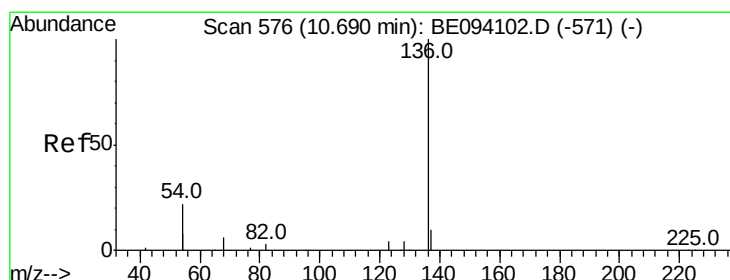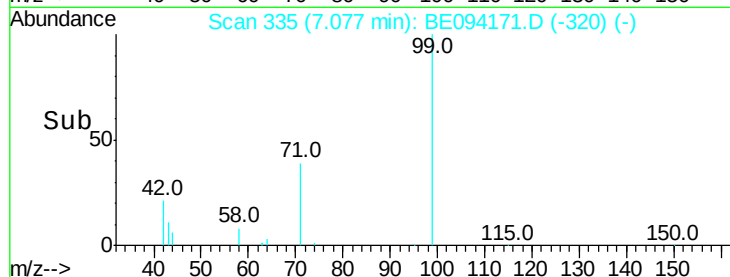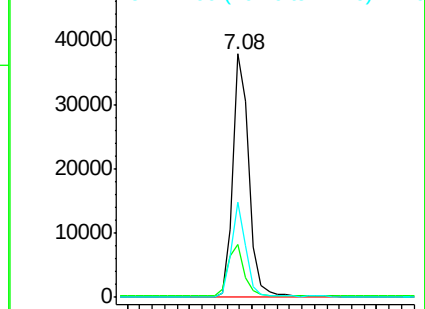

#7

Naphthalene-d8

Concen: 0.800 ng

RT: 10.69 min Scan# 576

Delta R.T. -0.00 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40

Tgt Ion: 136 Resp: 15405


Ion Ratio Lower Upper

136 100



137 11.3 9.5 14.3


54 26.2 29.1 43.7#

68 5.6 6.2 9.2#

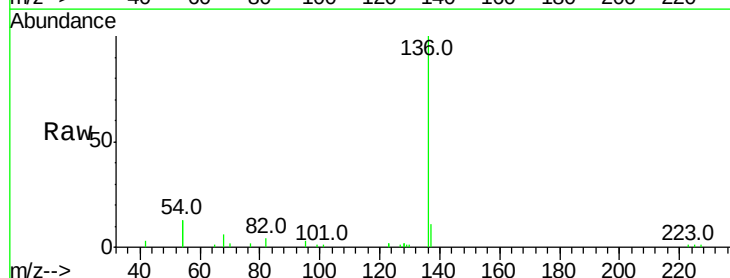

Abundance Ion 136.00 (135.70 to 136.70): E  
Ion 137.00 (136.70 to 137.70): E  
Ion 54.00 (53.70 to 54.70): BE0  
Ion 68.00 (67.70 to 68.70): BE0

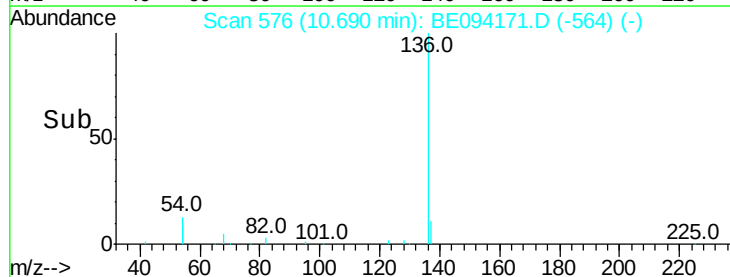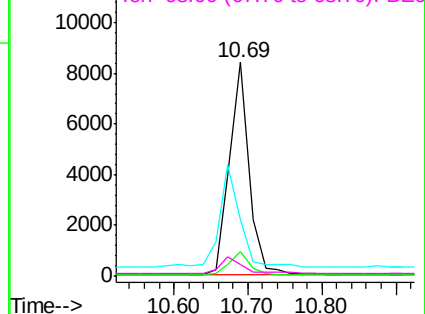



#8

Nitrobenzene-d5

Concen: 26.027 ng

RT: 9.04 min Scan# 478

Delta R.T. -0.02 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40

Instrument :

BNA\_E

ClientSampleId :

PAMT-COMP-E





Tot Ion: 82 Resp: 194003

Ion Ratio Lower Upper

82 100

128 118.3 150.0 225.0#

54 215.8 154.2 231.4

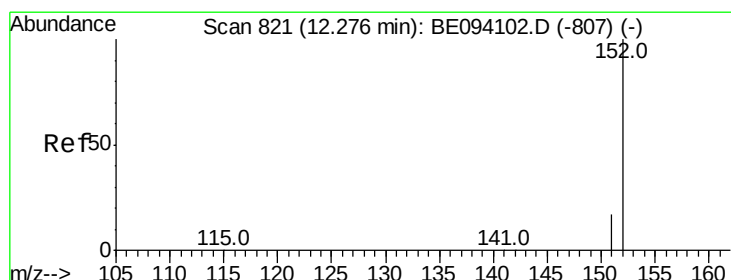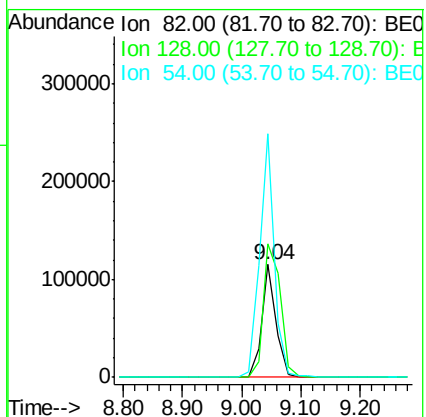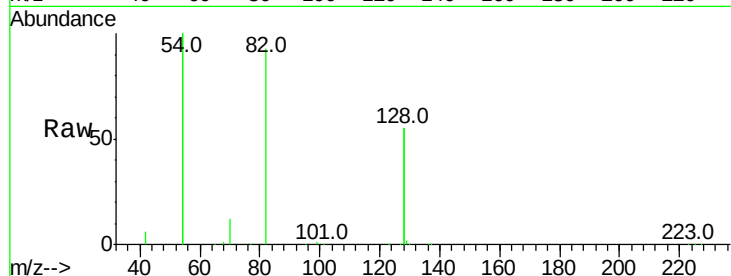

#11

2-Methylnaphthalene-d10

Concen: 0.002 ng

RT: 12.25 min Scan# 815

Delta R.T. -0.02 min

Lab File: BE094171.D




Acq: 4 Oct 2017 19:40


Tgt Ion: 152 Resp: 22

Ion Ratio Lower Upper

152 100

151 354.5 15.4 23.0#



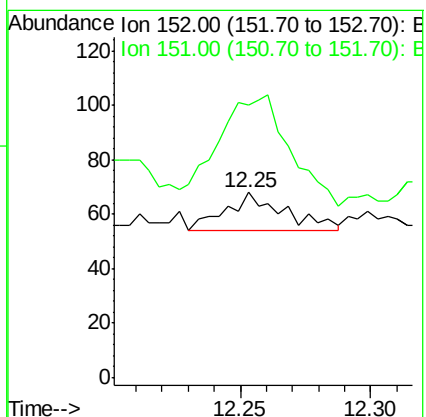





#13  
Acenaphthene-d10  
Concen: 0.800 ng  
RT: 14.51 min Scan# 1111  
Delta R.T. -0.00 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40




Instrument :  
BNA\_E  
ClientSampleId :  
PAMT-COMP-E


Tot Ion:164 Resp: 9516  
Ion Ratio Lower Upper  
164 100  
162 101.6 83.1 124.7  
160 44.3 37.1 55.7

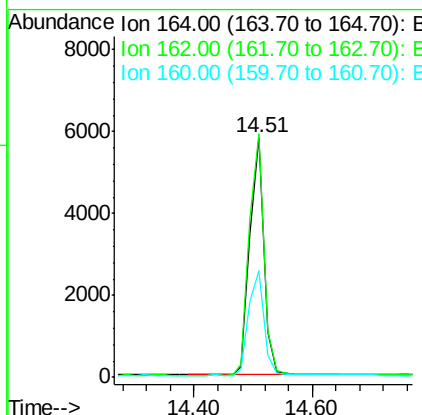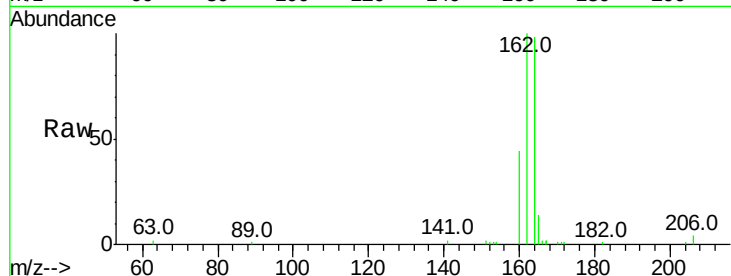

#14  
2,4,6-Tribromophenol  
Concen: 15.415 ng  
RT: 16.00 min Scan# 1205  
Delta R.T. 0.00 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40

Tgt Ion:330 Resp: 38261  
Ion Ratio Lower Upper  
330 100  
332 97.1 152.7 229.1#  
141 0.0 33.7 50.5#


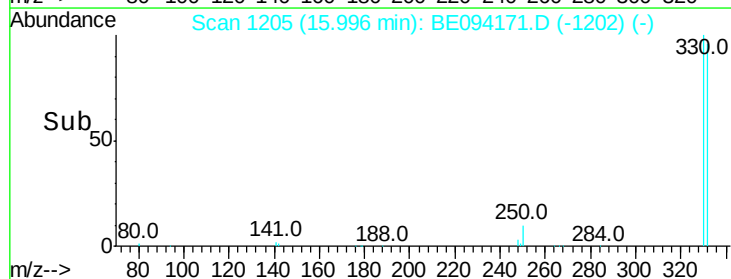
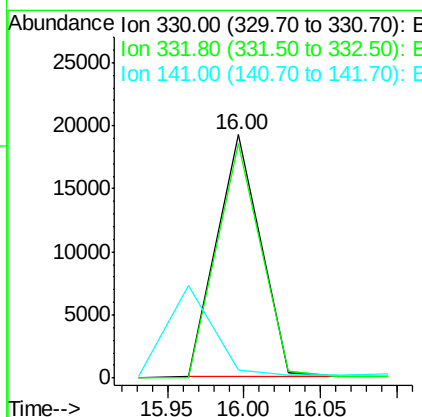



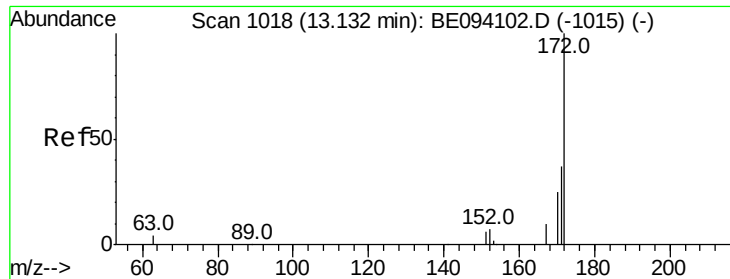

#15  
2-Fluorobiphenyl  
Concen: 23.577 ng  
RT: 13.13 min Scan# 1018  
Delta R.T. -0.00 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40




Instrument :  
BNA\_E  
ClientSampleId :  
PAMT-COMP-E


Tot Ion:172 Resp: 370661  
Ion Ratio Lower Upper  
172 100  
171 35.3 29.9 44.9  
170 23.7 21.8 32.8

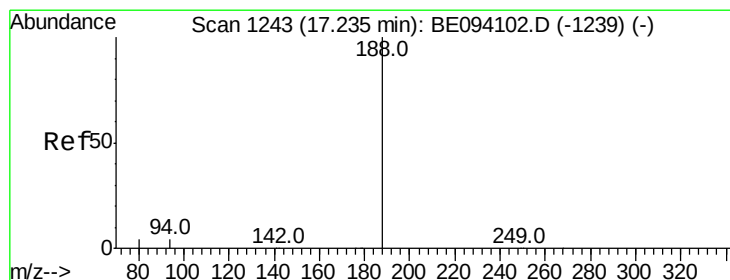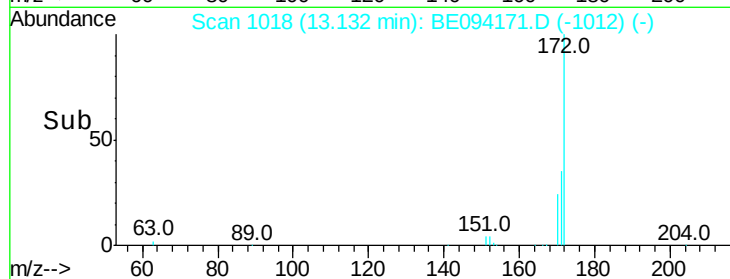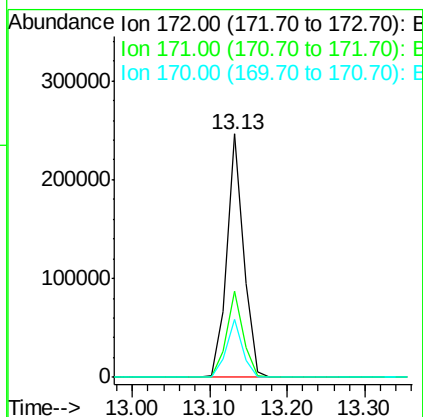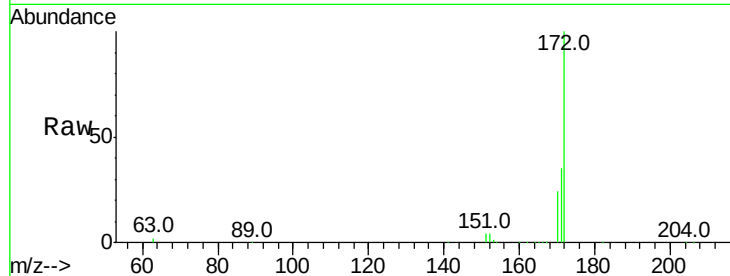

#19  
Phenanthrene-d10  
Concen: 0.800 ng  
RT: 17.23 min Scan# 1243  
Delta R.T. -0.00 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40

Tgt Ion:188 Resp: 26475  
Ion Ratio Lower Upper  
188 100  
94 4.4 3.9 5.9  
80 3.9 3.6 5.4

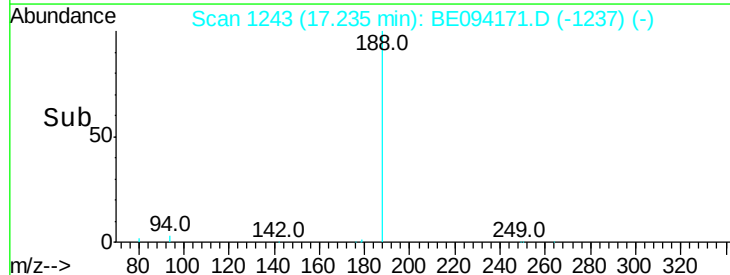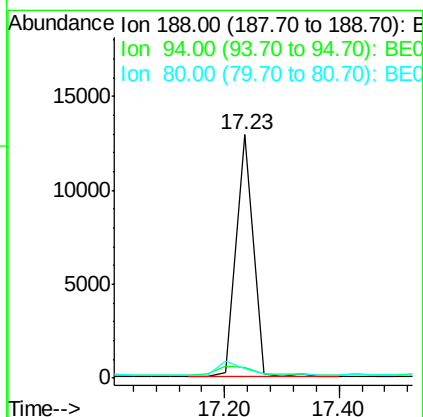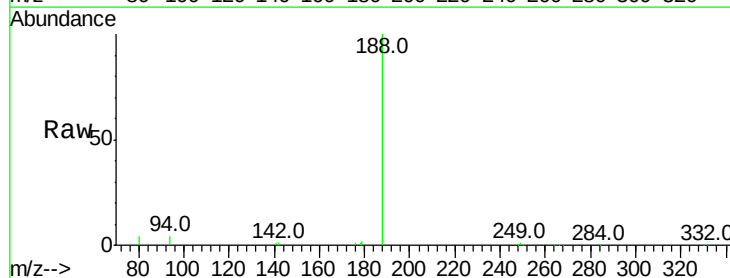



#23

Phenanthrene

Concen: 0.071 ng

RT: 17.27 min Scan# 1244

Delta R.T. -0.00 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40

Instrument :

BNA\_E

ClientSampleId :

PAMT-COMP-E


Tot Ion:178 Resp: 2398

Ion Ratio Lower Upper

178 100

176 21.3 15.1 22.7




179 28.8 11.8 17.6#

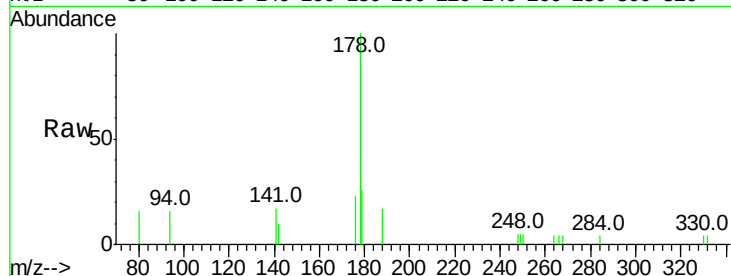

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

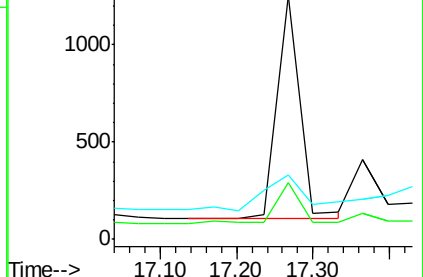

#25

Fluoranthene-d10

Concen: 0.004 ng

RT: 19.30 min Scan# 1435

Delta R.T. 0.03 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40


Tgt Ion:212 Resp: 472

Ion Ratio Lower Upper

212 100

106 10.2 2.8 4.2#



104 0.0 1.6 2.4#




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

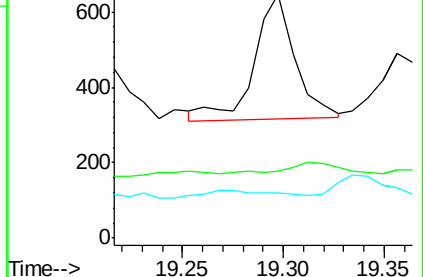







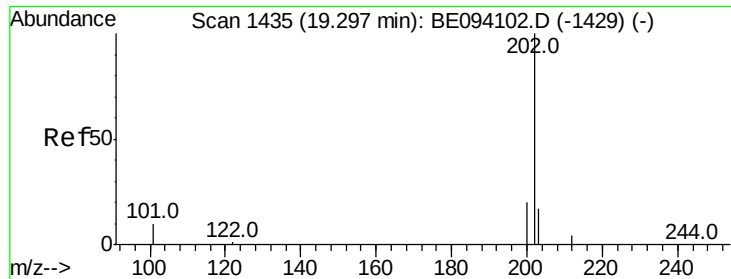

#26  
 Fluoranthene  
 Concen: 0.059 ng  
 RT: 19.29 min Scan# 1434  
 Delta R.T. -0.01 min  
 Lab File: BE094171.D  
 Acq: 4 Oct 2017 19:40




Instrument :  
 BNA\_E  
 ClientSampleId :  
 PAMT-COMP-E


Tot Ion:202 Resp: 2222  
 Ion Ratio Lower Upper  
 202 100  
 101 20.3 9.8 14.8#  
 203 18.4 13.7 20.5

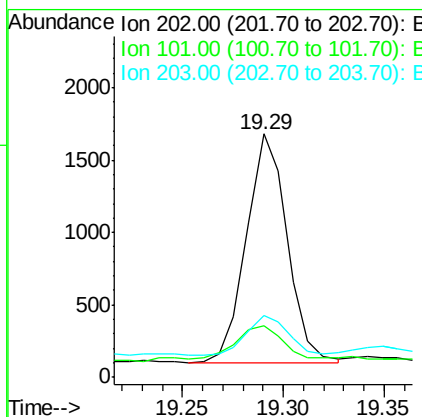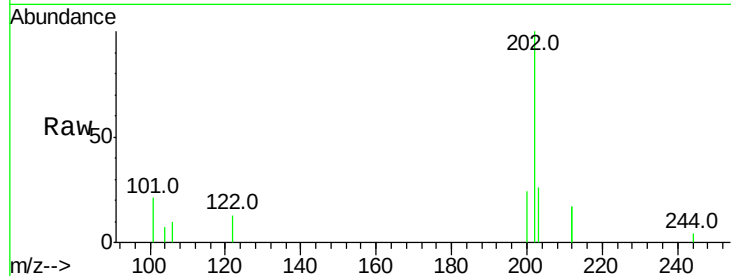

#27  
 Chrysene-d12  
 Concen: 0.800 ng  
 RT: 21.40 min Scan# 1654  
 Delta R.T. -0.00 min  
 Lab File: BE094171.D  
 Acq: 4 Oct 2017 19:40

Tgt Ion:240 Resp: 23638  
 Ion Ratio Lower Upper  
 240 100  
 120 7.8 5.5 8.3  
 236 25.6 20.7 31.1



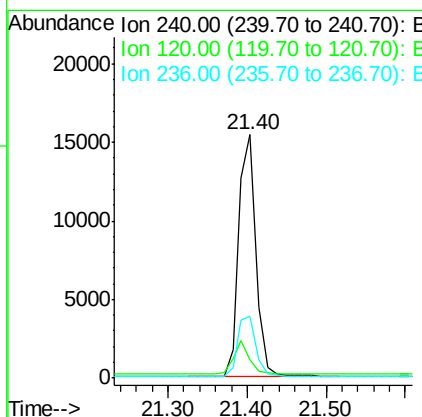



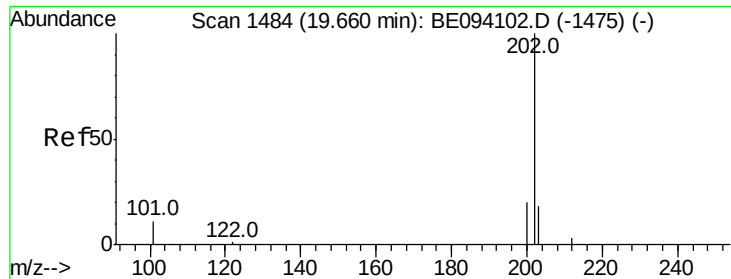

#28  
Pvrene  
Concen: 0.128 ng  
RT: 19.65 min Scan# 1483  
Delta R.T. -0.01 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40




Instrument :  
BNA\_E  
ClientSampleId :  
PAMT-COMP-E


Tot Ion:202 Resp: 4785  
Ion Ratio Lower Upper  
202 100  
200 21.2 16.6 25.0  
203 21.7 13.8 20.8#

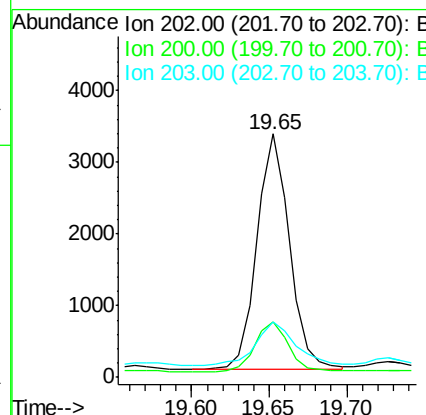

#29  
Terphenyl-d14  
Concen: 22.309 ng  
RT: 19.84 min Scan# 1509  
Delta R.T. -0.01 min  
Lab File: BE094171.D  
Acq: 4 Oct 2017 19:40

Tgt Ion:244 Resp: 481054  
Ion Ratio Lower Upper  
244 100  
212 34.7 25.4 38.0  
122 13.8 8.1 12.1#

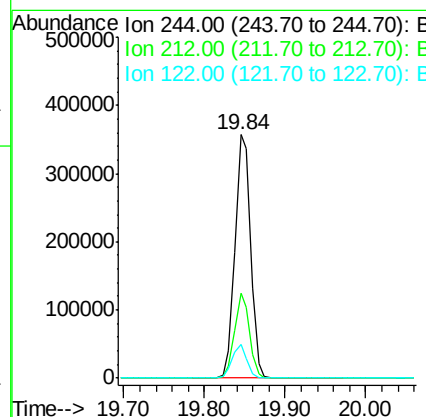



#30

Benzo(a)anthracene

Concen: 0.042 ng

RT: 21.38 min Scan# 1652

Delta R.T. -0.00 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40

Instrument :

BNA\_E

ClientSampleId :

PAMT-COMP-E


Tot Ion:228 Resp: 1683

Ion Ratio Lower Upper

228 100

226 34.8 21.4 32.0#




229 37.0 16.4 24.6#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

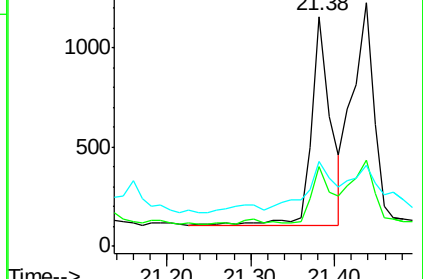

#31

Chrysene

Concen: 0.052 ng

RT: 21.44 min Scan# 1657

Delta R.T. -0.00 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40


Tgt Ion:228 Resp: 2003

Ion Ratio Lower Upper

228 100

226 35.3 23.6 35.4



229 33.4 16.4 24.6#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

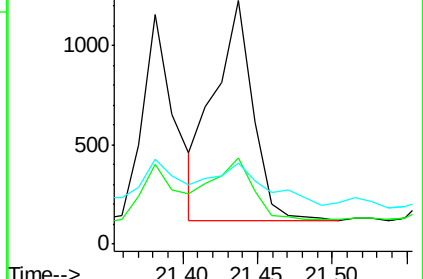



#32

Bis(2-ethylhexyl)phthalate

Concen: 1.214 ng

RT: 21.29 min Scan# 1644

Delta R.T. -0.00 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40

Instrument :

BNA\_E

ClientSampleId :

PAMT-COMP-E


Tot Ion:149 Resp: 161836

Ion Ratio Lower Upper

149 100

167 6.7 5.4 8.0




279 0.9 0.7 1.1



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

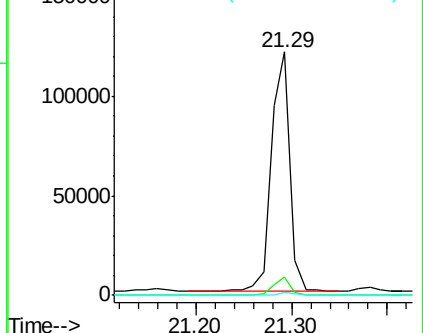

#34

Perylene-d12

Concen: 0.800 ng

RT: 23.90 min Scan# 2120

Delta R.T. -0.01 min

Lab File: BE094171.D

Acq: 4 Oct 2017 19:40


Tgt Ion:264 Resp: 22179

Ion Ratio Lower Upper

264 100

260 24.7 20.5 30.7

265 24.4 22.8 34.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

