


Data Path : Z:\HPCHEM1\BNA E\Data\BE100417\
 Data File : BE094169.D
 Acq On : 4 Oct 2017 16:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 29 13:57:50 2017

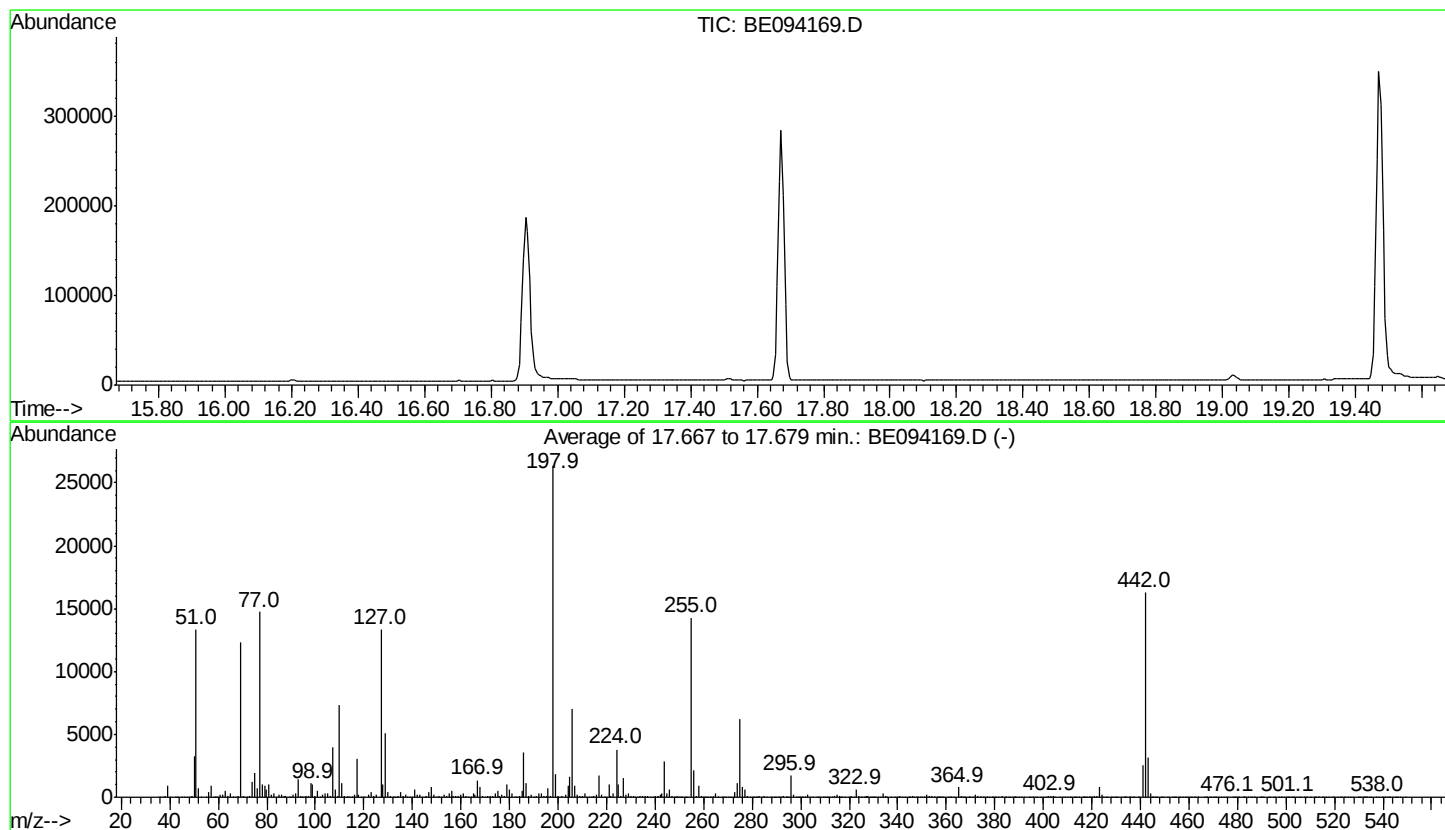

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	13301	PASS
68	69	0.00	2	1.1	136	PASS
69	198	0.00	100	46.9	12360	PASS
70	69	0.00	2	0.5	58	PASS
127	198	10	80	50.5	13327	PASS
197	198	0.00	2	0.3	92	PASS
198	198	100	100	100.0	26373	PASS
199	198	5	9	6.9	1829	PASS
275	198	10	60	23.5	6204	PASS
365	198	1	100	2.9	770	PASS
441	442	0.01	24	15.8	2567	PASS
442	198	50	100	61.6	16243	PASS
443	442	15	24	19.2	3125	PASS