


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100418\
 Data File : BE097719.D
 Acq On : 4 Oct 2018 8:27
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 03 12:17:19 2018

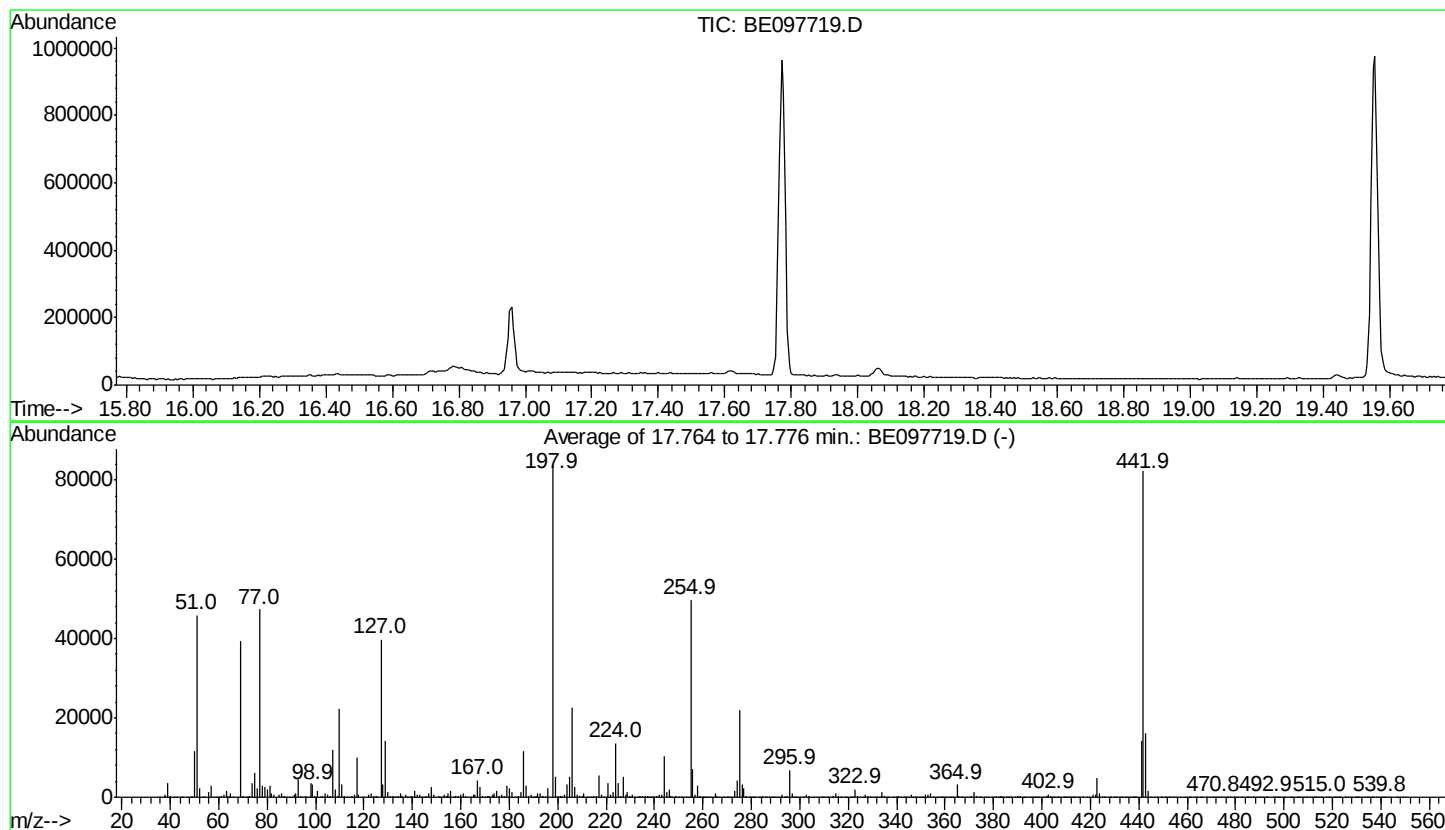

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	45843	PASS
68	69	0.00	2	0.4	162	PASS
69	198	0.00	100	47.2	39476	PASS
70	69	0.00	2	0.5	206	PASS
127	198	10	80	47.6	39752	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83597	PASS
199	198	5	9	6.3	5268	PASS
275	198	10	60	26.3	21982	PASS
365	198	1	100	3.7	3120	PASS
441	198	0.01	100	16.9	14163	PASS
442	198	50	100	98.4	82233	PASS
443	442	15	24	19.7	16221	PASS