


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100418\
 Data File : BE097725.D
 Acq On : 4 Oct 2018 14:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 03 12:17:19 2018

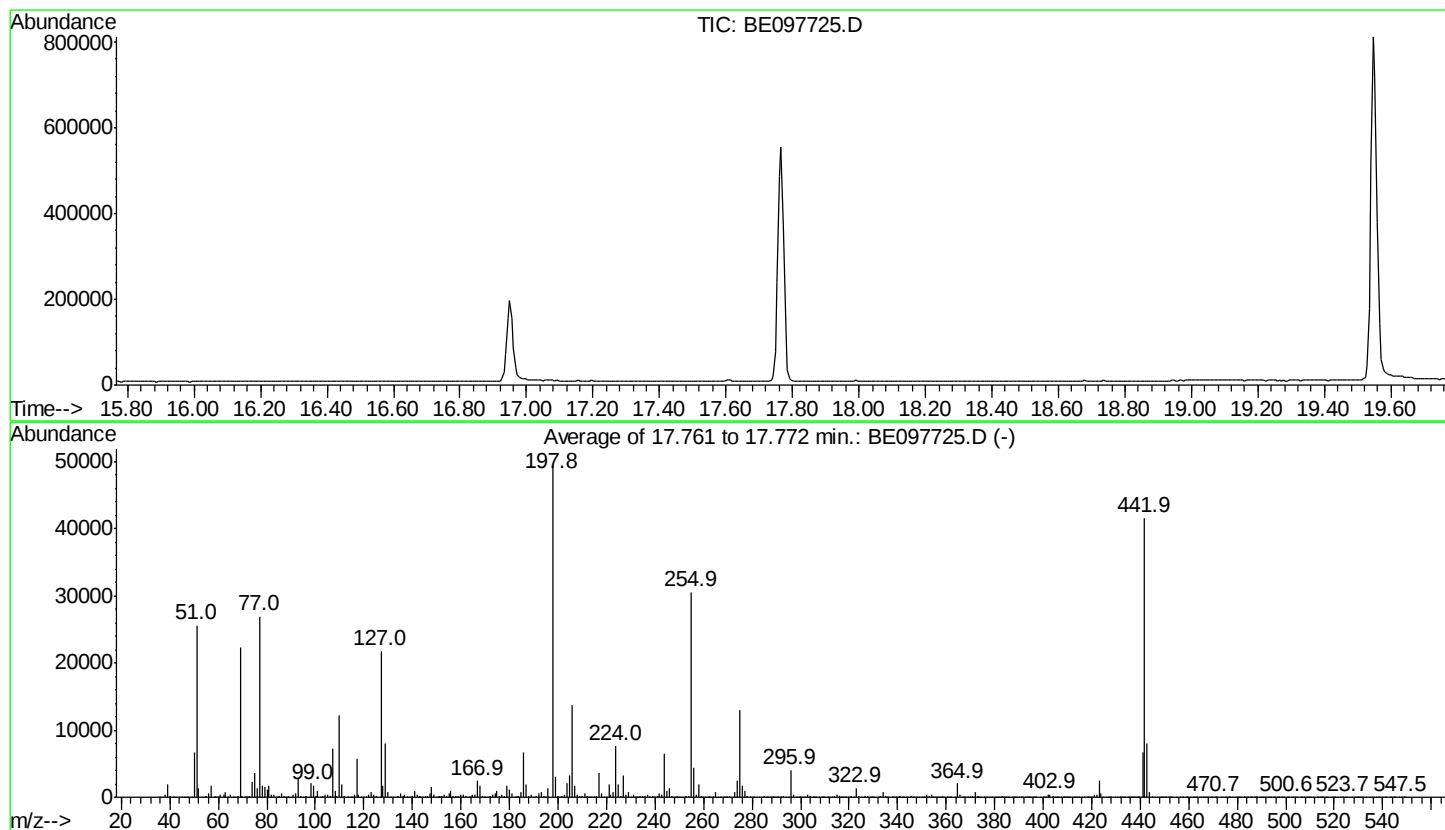

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.8	25579	PASS
68	69	0.00	2	1.3	290	PASS
69	198	0.00	100	45.3	22337	PASS
70	69	0.00	2	0.7	151	PASS
127	198	10	80	44.1	21773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49358	PASS
199	198	5	9	6.3	3102	PASS
275	198	10	60	26.2	12952	PASS
365	198	1	100	4.1	2021	PASS
441	198	0.01	100	13.5	6682	PASS
442	198	50	100	84.2	41584	PASS
443	442	15	24	19.1	7956	PASS