
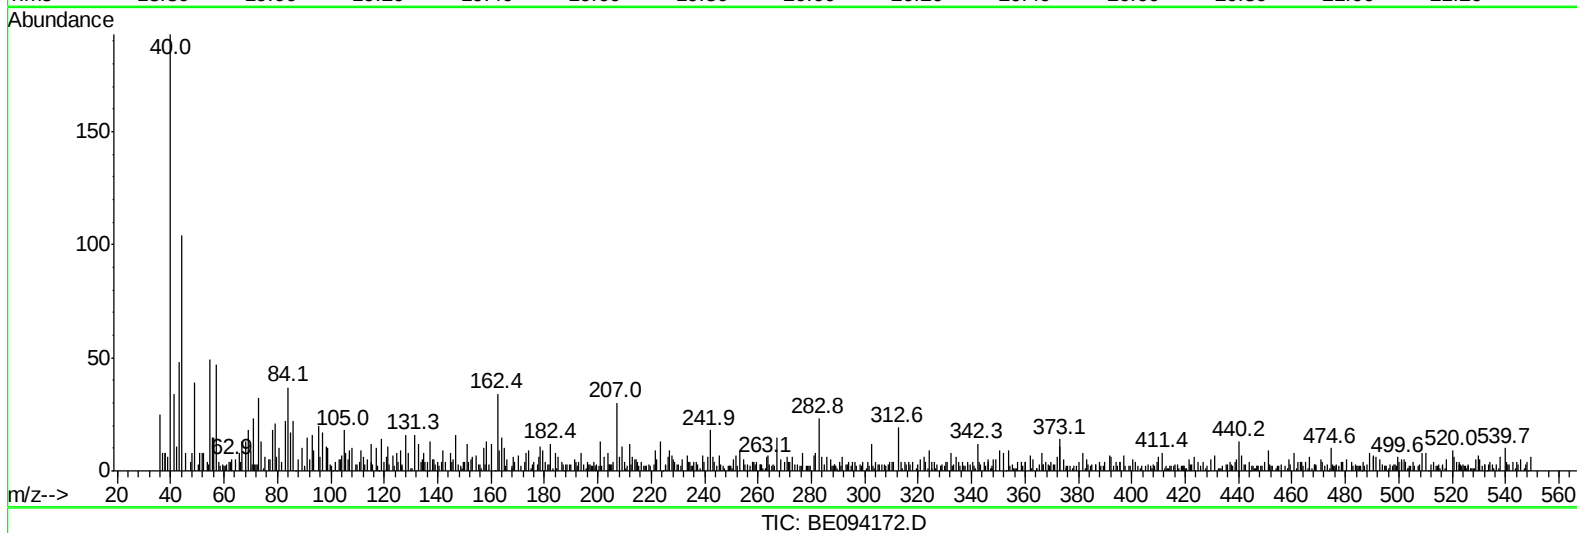


Data Path : Z:\HPCHEM1\BNA E\DATA\BE100617\
Data File : BE094172.D
Acq On : 6 Oct 2017 10:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 02:53:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

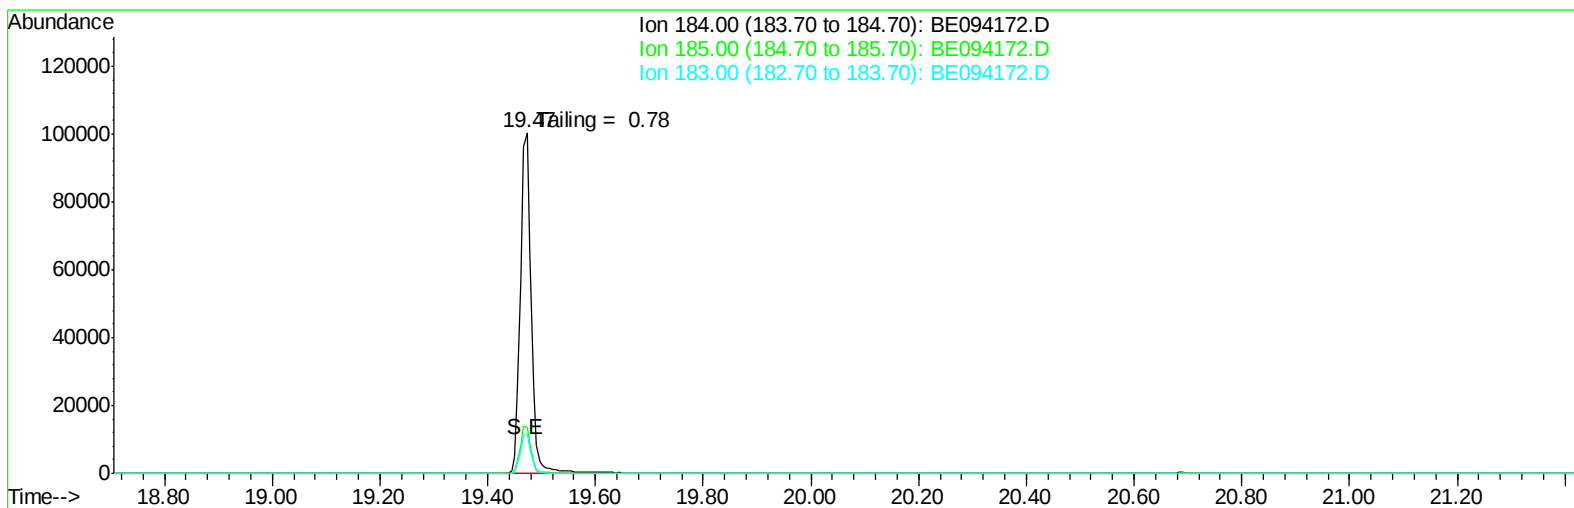

(76) Benzidine



12.658min (-0.070) 60.83ng

response 9

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	66.67#
183.00	11.60	11.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100617\
Data File : BE094172.D
Acq On : 6 Oct 2017 10:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 02:53:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

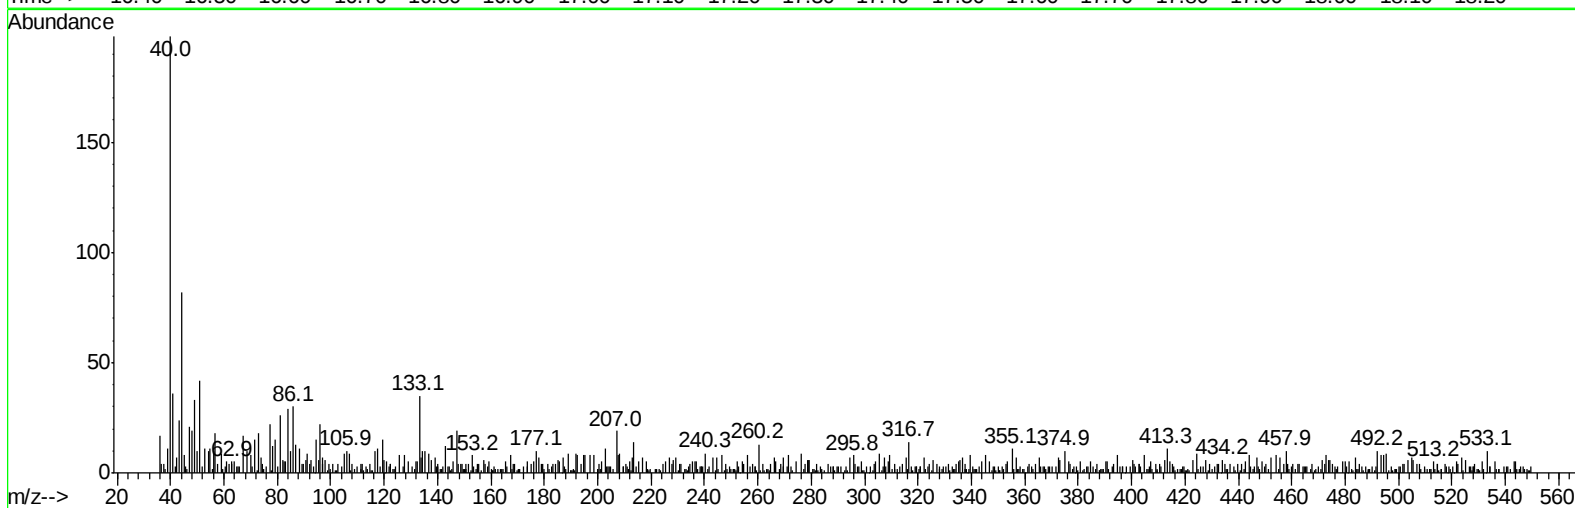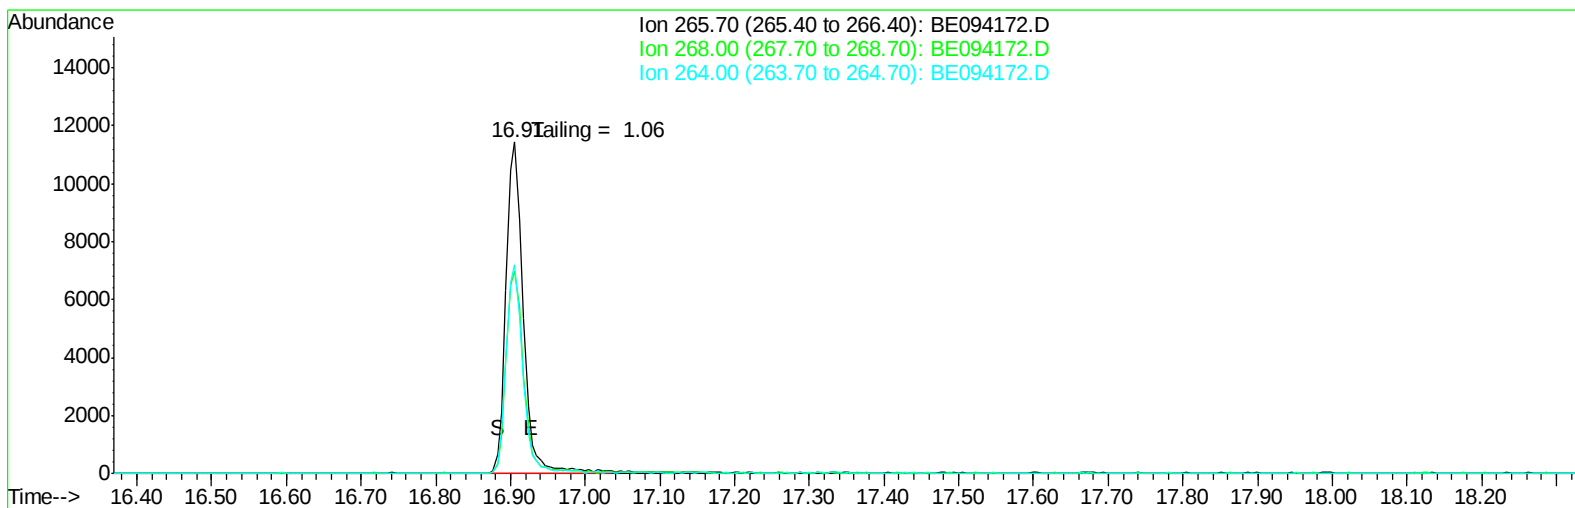

TIC: BE094172.D

(69) Pentachlorophenol (C)

11.148min (-0.050) 384.24ng

response 15

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	85.71#
264.00	61.90	100.00#
0.00	0.00	0.00