


Data Path : Z:\HPCHEM1\BNA E\Data\BE100617\
 Data File : BE094172.D
 Acq On : 6 Oct 2017 10:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 06 15:16:13 2017

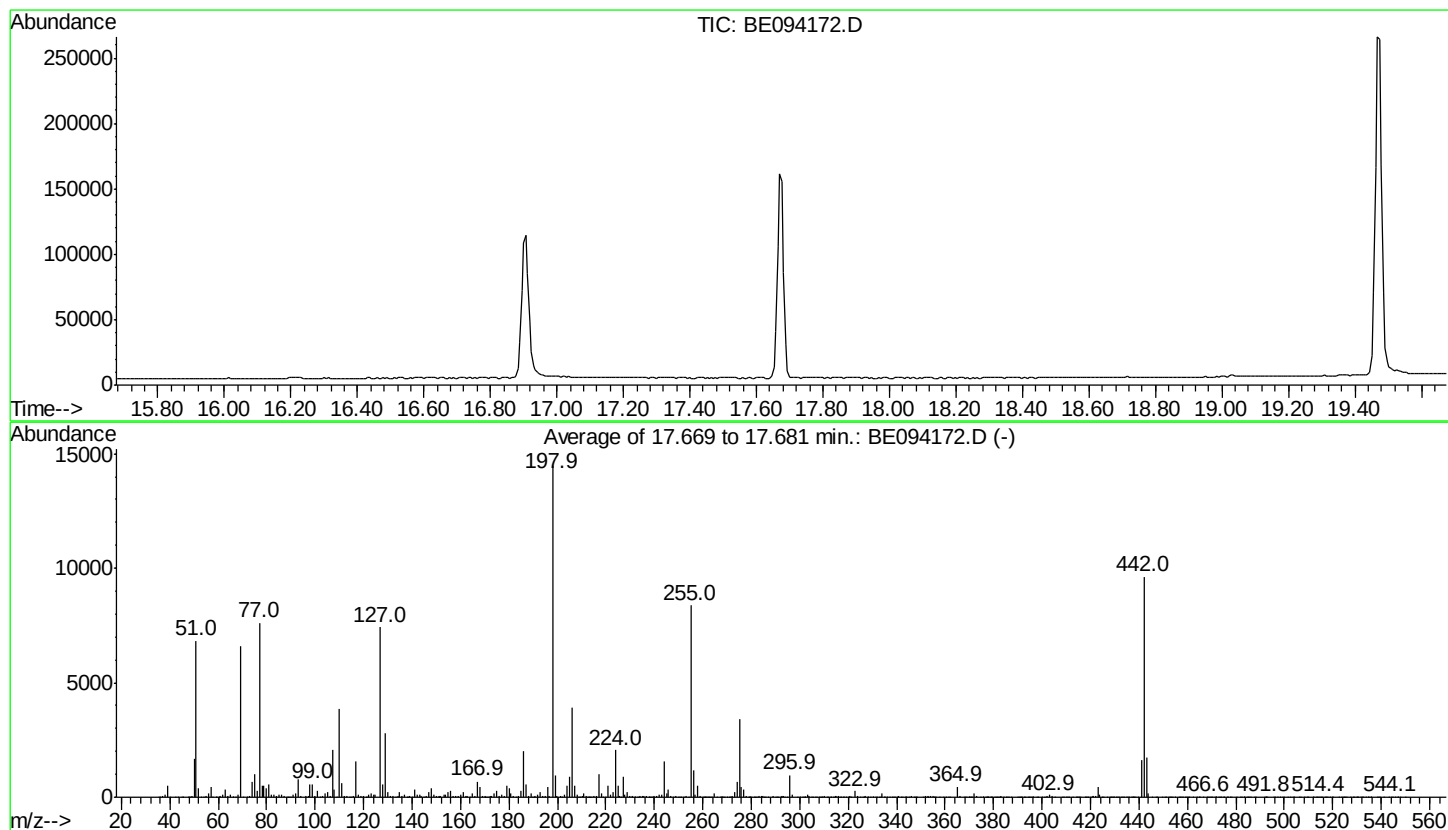

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	6835	PASS
68	69	0.00	2	1.9	126	PASS
69	198	0.00	100	45.6	6607	PASS
70	69	0.00	2	0.0	2	PASS
127	198	10	80	51.2	7418	PASS
197	198	0.00	2	0.2	33	PASS
198	198	100	100	100.0	14477	PASS
199	198	5	9	6.5	938	PASS
275	198	10	60	23.6	3416	PASS
365	198	1	100	3.1	456	PASS
441	442	0.01	24	16.9	1634	PASS
442	198	50	100	66.6	9642	PASS
443	442	15	24	18.1	1744	PASS