
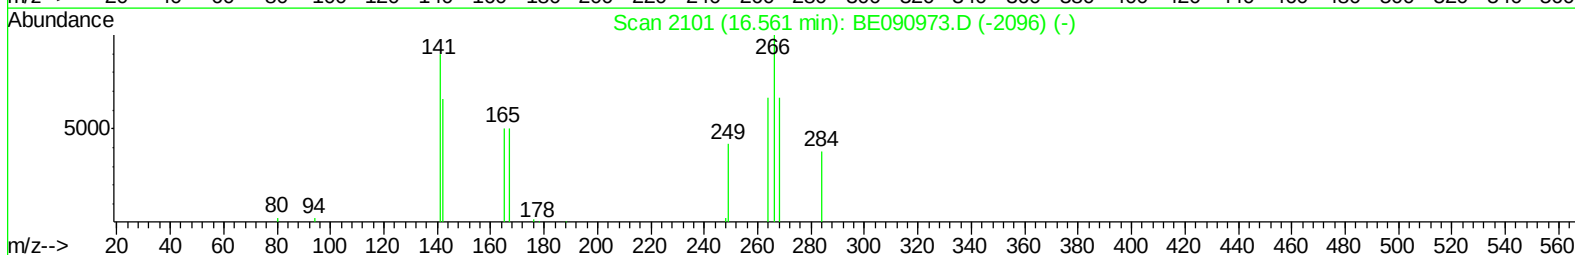
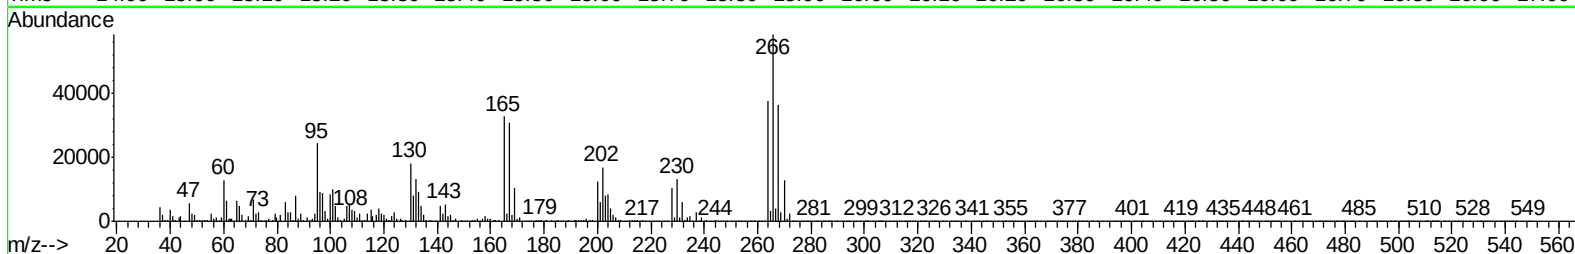


Data Path : Z:\HPCHEM1\BNA E\Data\BE100715\
Data File : BE090986.D
Acq On : 7 Oct 2015 13:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 02:33:14 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 17:11:43 2015
Response via : Initial Calibration

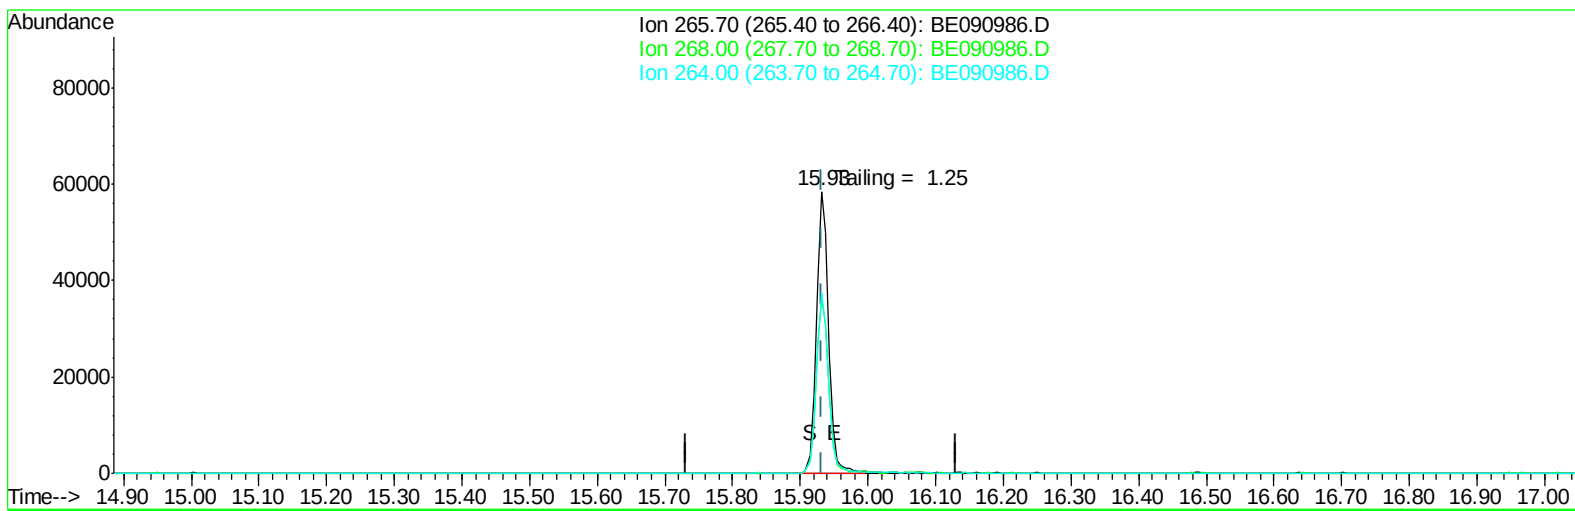

TIC: BE090986.D

(22) Pentachlorophenol




15.931min (-0.000) 1065.99ng

response 75046

Ion	Exp%	Act%
265.70	100	100
268.00	72.70	62.43
264.00	70.30	64.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE100715\
Data File : BE090986.D
Acq On : 7 Oct 2015 13:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 02:33:14 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 17:11:43 2015
Response via : Initial Calibration

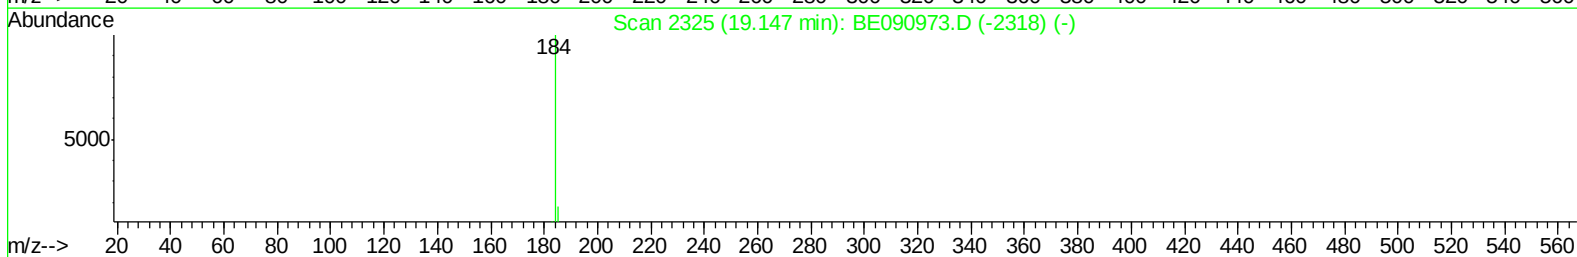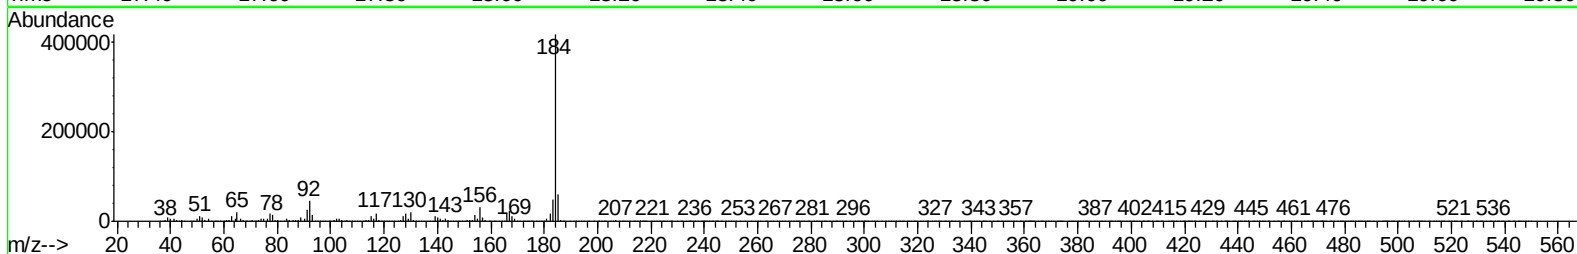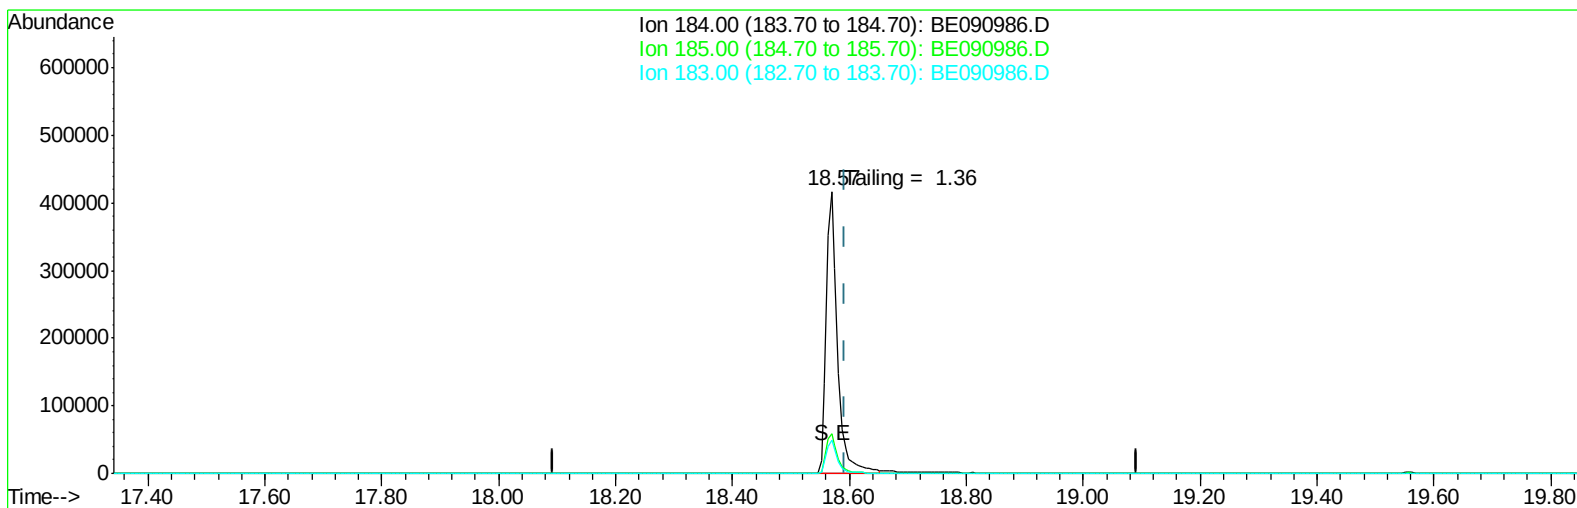

TIC: BE090986.D

(27) Benzidine

18.569min (-0.024) 1522.38ng

response 563112

Ion	Exp%	Act%
184.00	100	100
185.00	27.90	14.27#
183.00	20.50	11.89#
0.00	0.00	0.00