


Data Path : Z:\HPCHEM1\BNA E\DATA\BE100715\
 Data File : BE090986.D
 Acq On : 7 Oct 2015 13:28
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 07 17:11:43 2015

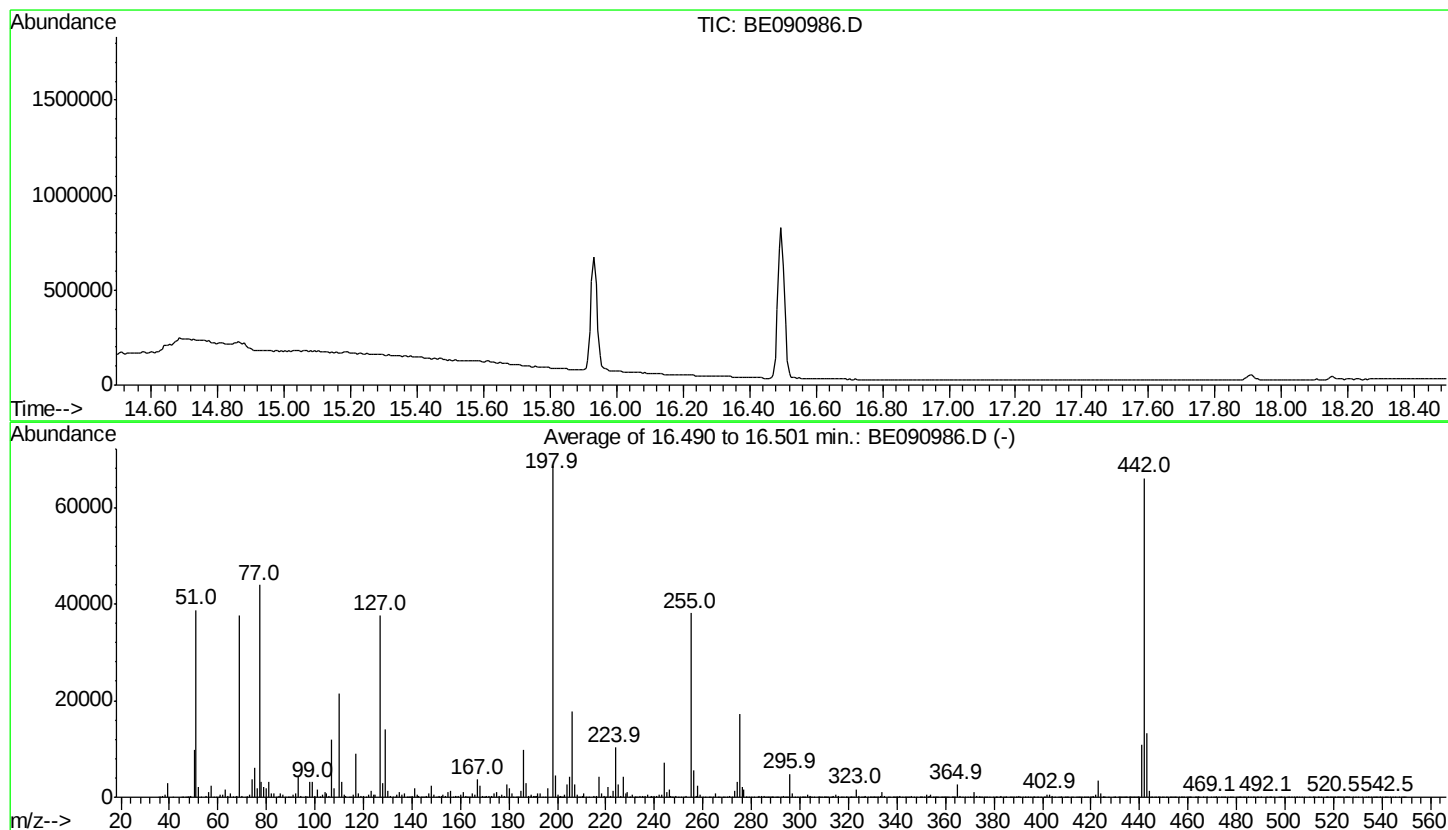

AutoFind: Scans 2366, 2367, 2368; Background Corrected with Scan 2359

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.5	38796	PASS
68	69	0.00	2	1.0	367	PASS
69	198	0.00	100	54.7	37509	PASS
70	69	0.00	2	0.5	184	PASS
127	198	10	80	54.8	37608	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68616	PASS
199	198	5	9	6.8	4640	PASS
275	198	10	60	25.2	17282	PASS
365	198	1	100	3.8	2585	PASS
441	442	0.01	24	16.6	10929	PASS
442	198	50	100	96.1	65965	PASS
443	442	15	24	19.9	13158	PASS